

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
 Data File : PP035484.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2021 17:12
 Operator : DD\AJ
 Sample : M2245-04 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HA-61

Manual Integrations
 APPROVED

Ankita
 5/4/2021 9:56:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 03:02:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	198362	159847	3.907	4.695
2) SA Decachlor...	10.644f	9.461	197953	113582	4.874m	5.861

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
Data File : PP035484.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2021 17:12
Operator : DD\AJ
Sample : M2245-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/4/2021 9:56:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 03:02:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

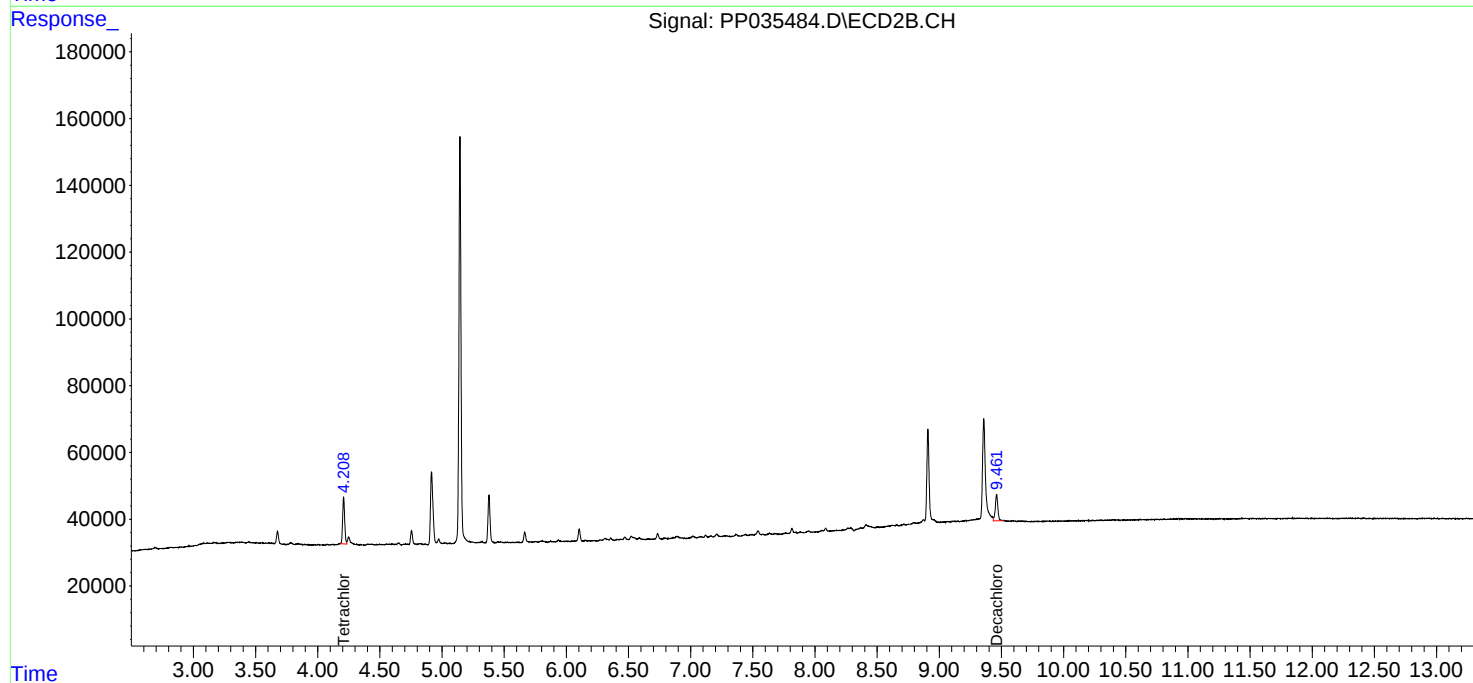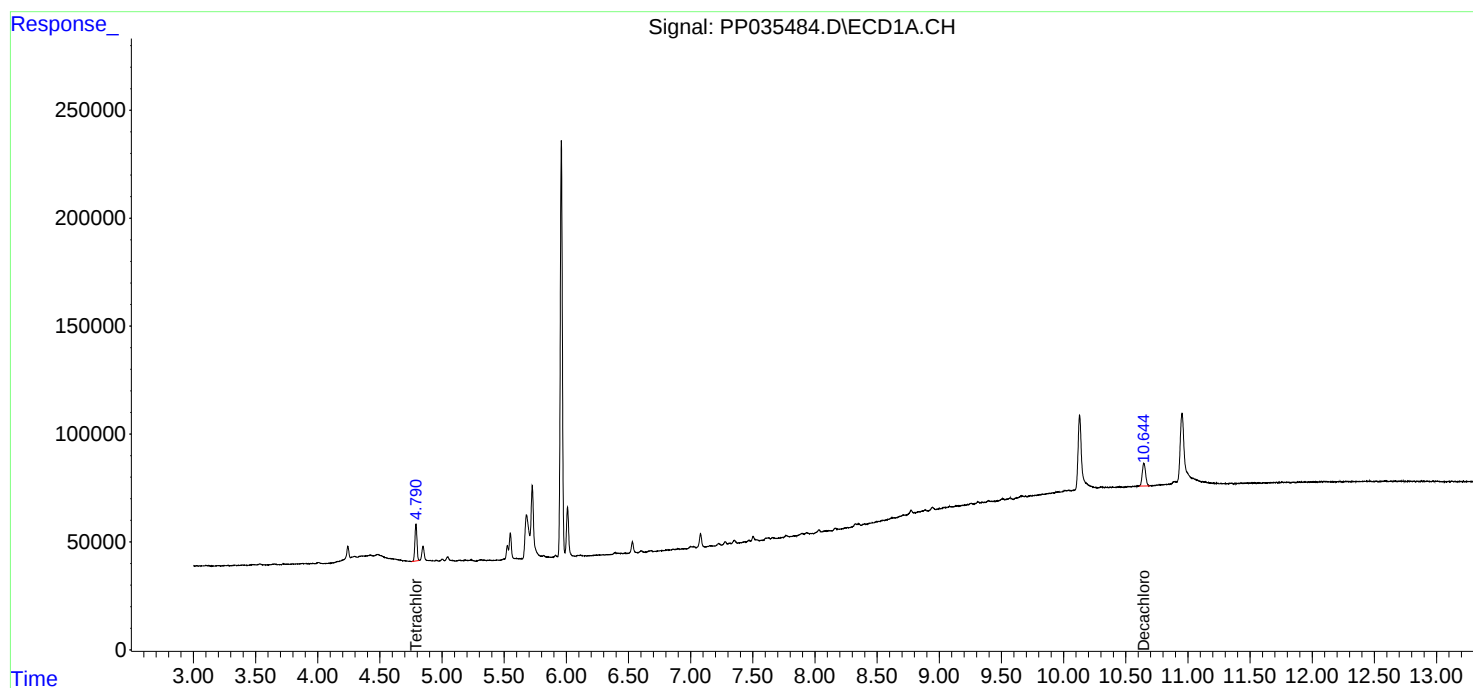

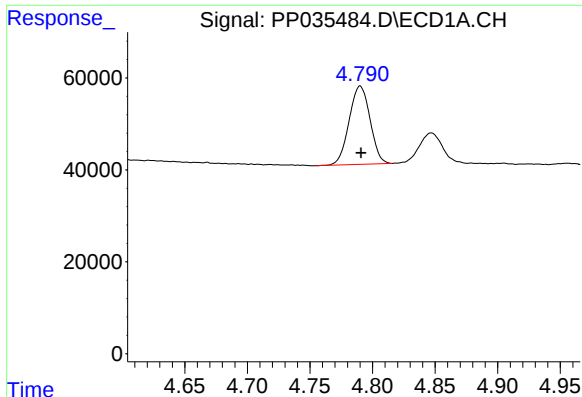


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 198362
Conc: 3.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/4/2021 9:56:39 AM

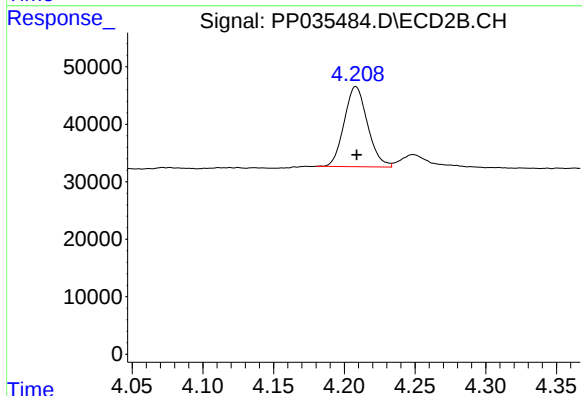


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 159847
Conc: 4.70 ng/ml

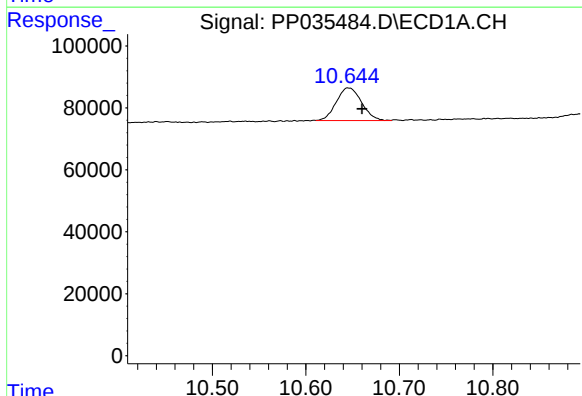

#2 Decachlorobiphenyl

R.T.: 10.644 min
Delta R.T.: -0.016 min
Response: 197953
Conc: 4.87 ng/ml m

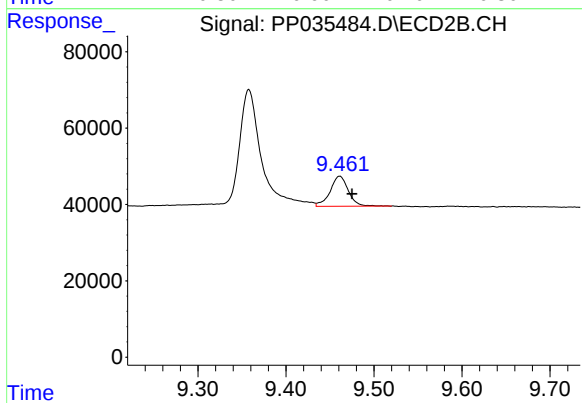

#2 Decachlorobiphenyl

R.T.: 9.461 min
Delta R.T.: -0.014 min
Response: 113582
Conc: 5.86 ng/ml