

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050322\
 Data File : PP046960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 03:15
 Operator : YP\AJ
 Sample : N2643-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 31487

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/04/2022
 Supervised By :mohammad ahmed 05/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 07:59:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 03 11:45:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.852	3.128	67431013	36252207	27.934m	11.051 #
2) SA Decachlor...	9.952f	8.459f	25854359	42523852	17.570	17.827

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050322\
Data File : PP046960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 03:15
Operator : YP\AJ
Sample : N2643-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
31487


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2022
Supervised By :mohammad ahmed 05/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 07:59:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 03 11:45:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

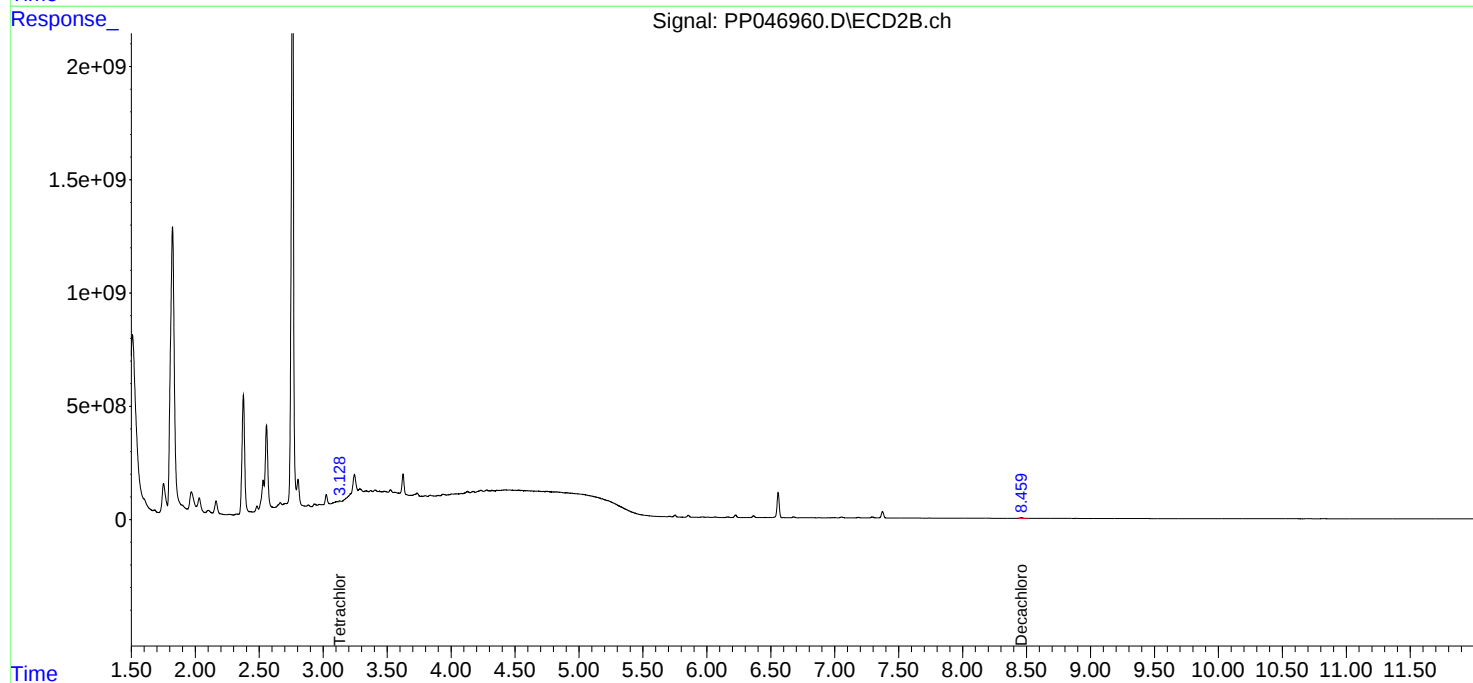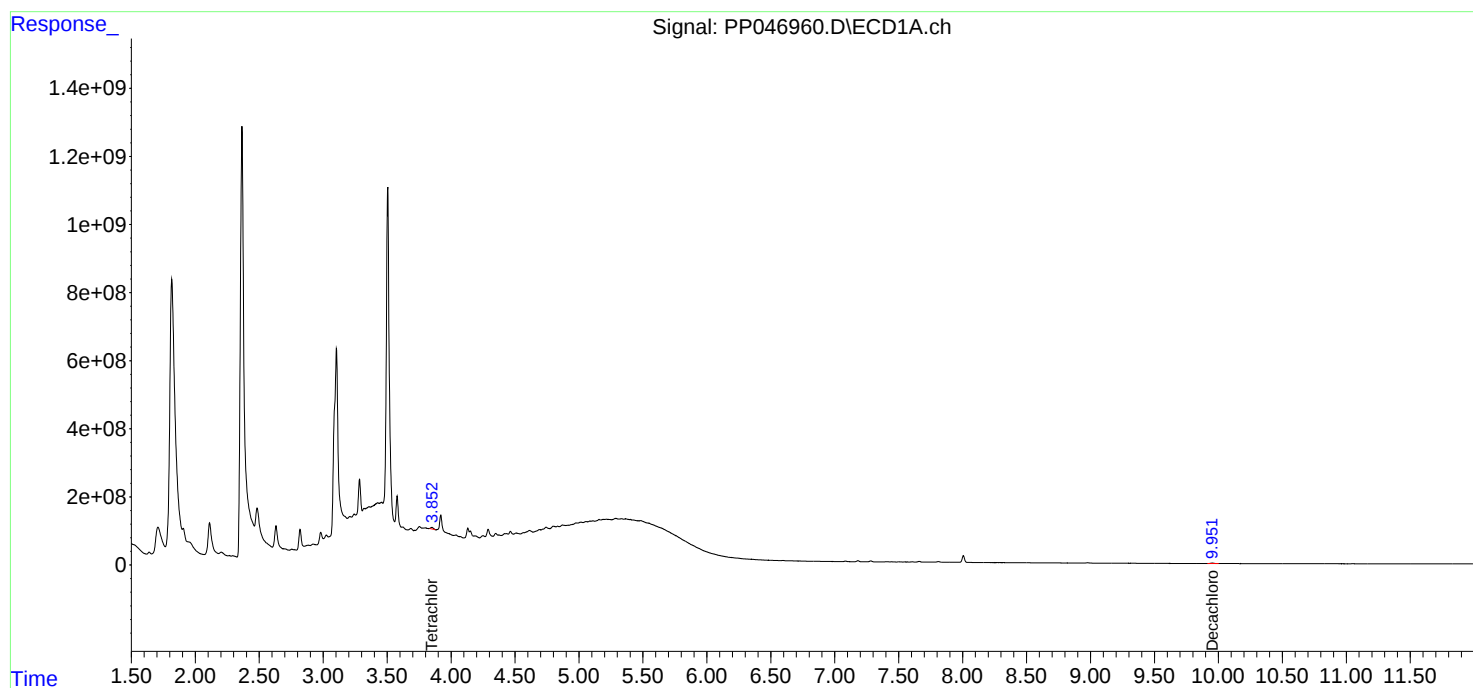

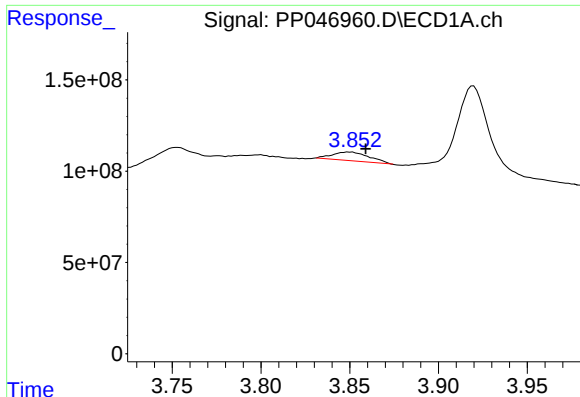


#1 Tetrachloro-m-xylene

R.T.: 3.852 min
Delta R.T.: -0.007 min
Response: 67431013
Conc: 27.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
31487


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2022
Supervised By :mohammad ahmed 05/04/2022

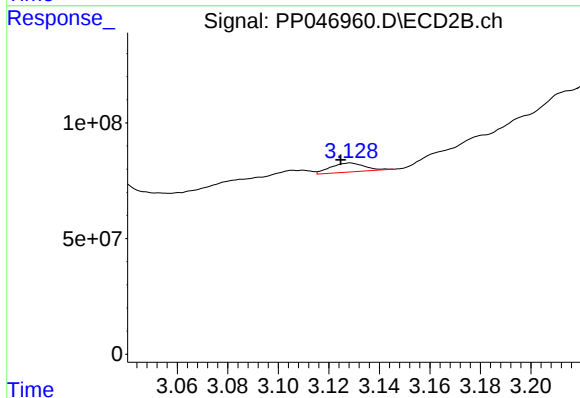


#1 Tetrachloro-m-xylene

R.T.: 3.128 min
Delta R.T.: 0.004 min
Response: 36252207
Conc: 11.05 ng/ml

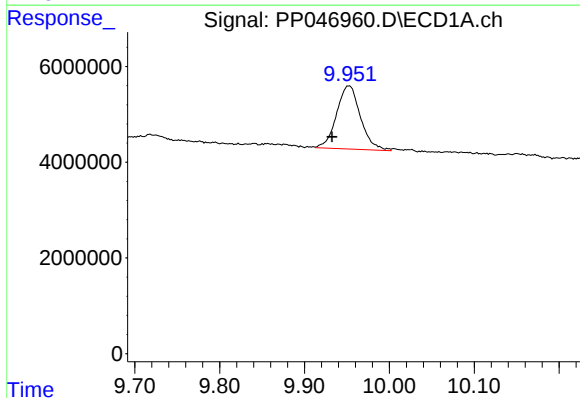

#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: 0.020 min
Response: 25854359
Conc: 17.57 ng/ml

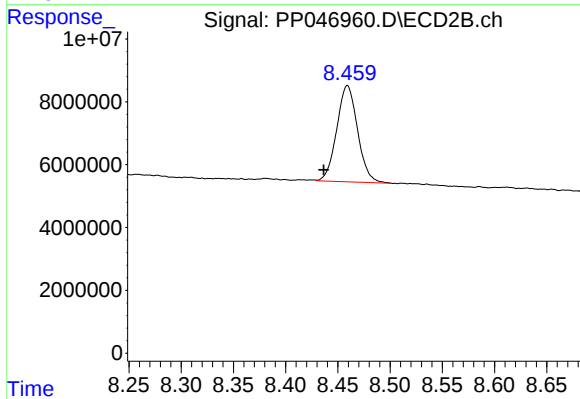

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: 0.023 min
Response: 42523852
Conc: 17.83 ng/ml