

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050323\
 Data File : PP057476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 04:57
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/04/2023
 Supervised By :Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 05:28:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 04 05:28:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.625	11337740	11270699	5.237	5.297
2) SA Decachlor...	10.223	8.691	6229666	13663681	4.904	5.561
Target Compounds						
41) L9 AR-1268-1	8.680	7.571	6177810	13834842	49.339m	56.373
42) L9 AR-1268-2	8.777	7.636	5128264	11884102	46.916	54.378
43) L9 AR-1268-3	9.009	7.846	4700124	10575074	46.859	55.521
44) L9 AR-1268-4	9.445	8.134	1859817	4312259	50.056	56.093
45) L9 AR-1268-5	9.872	8.431	12049020	26372613	47.132	52.106

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050323\
Data File : PP057476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 04:57
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 05:28:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 04 05:28:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

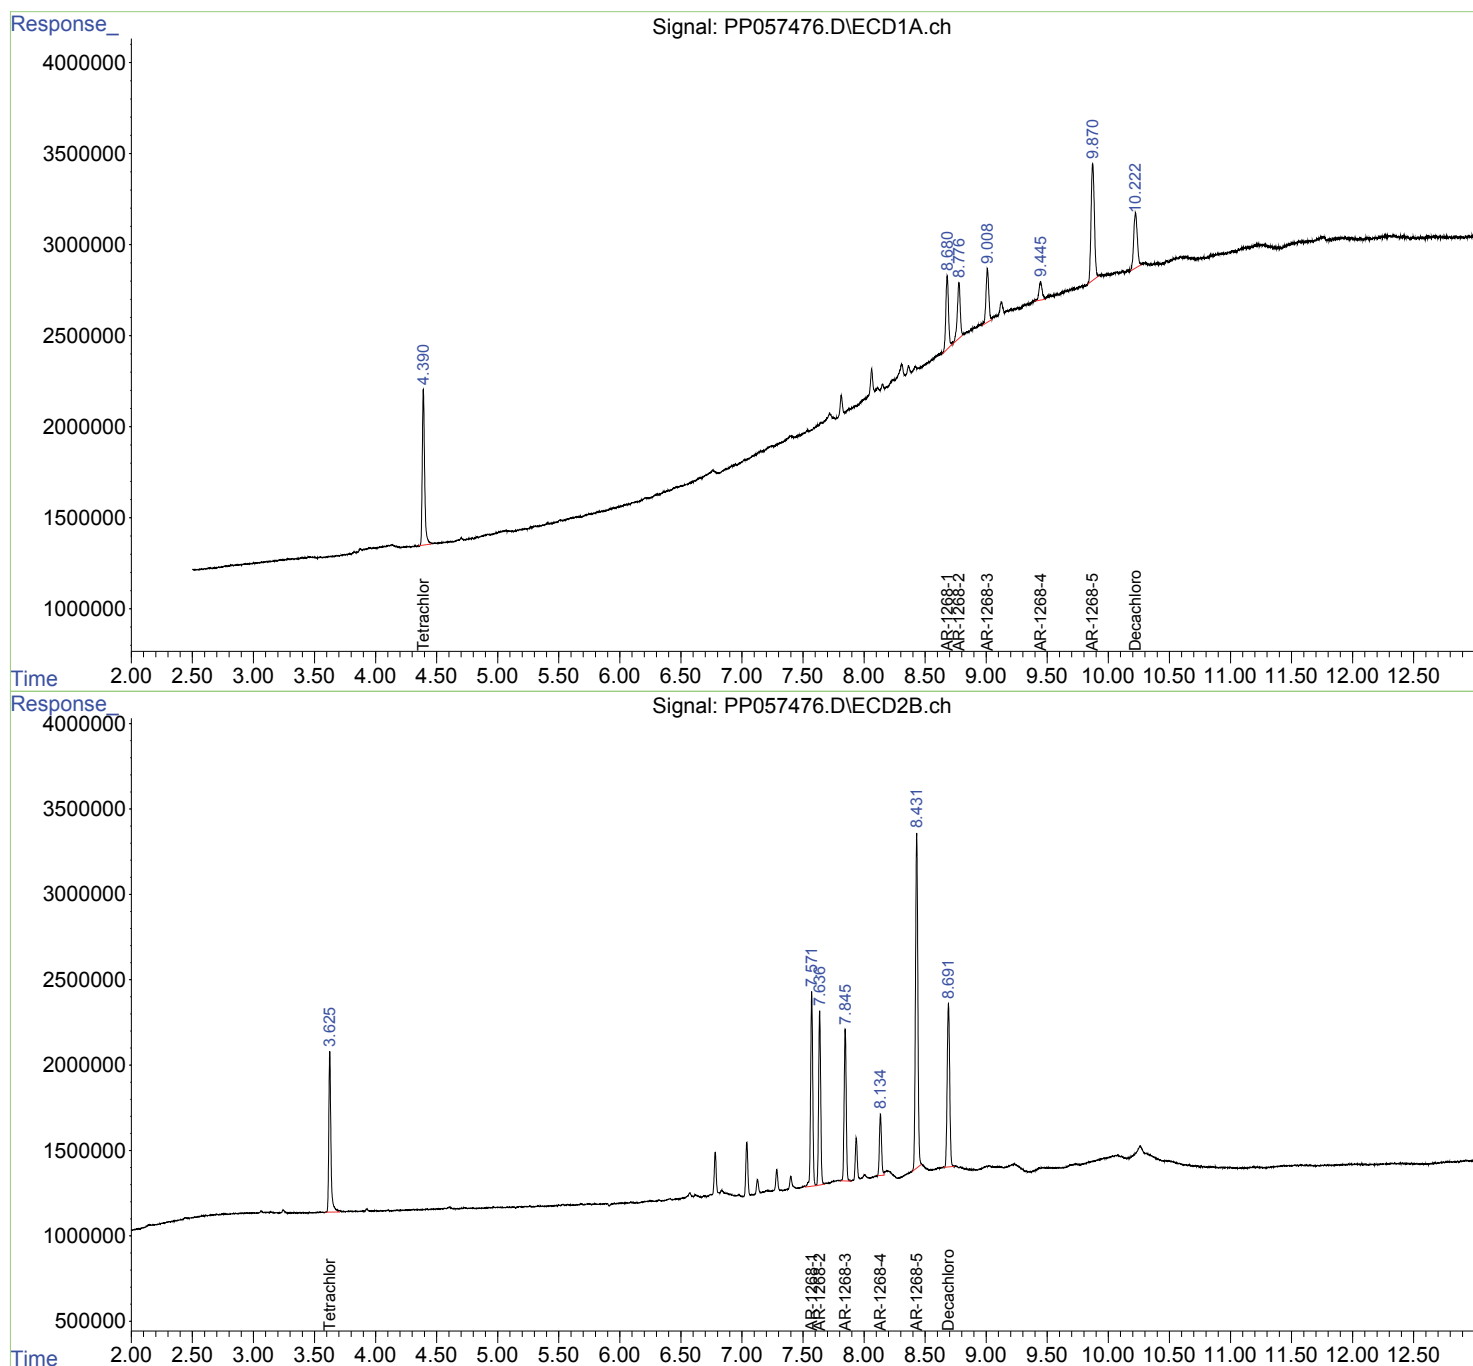

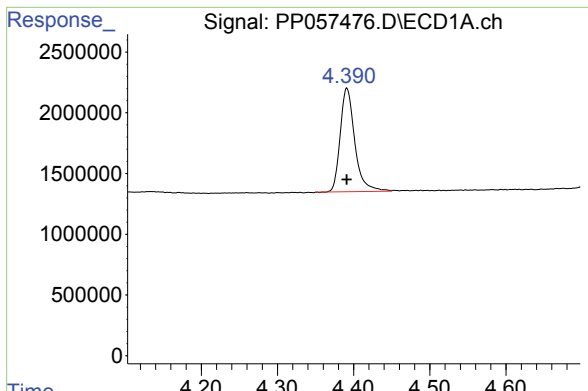


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 11337740
Conc: 5.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

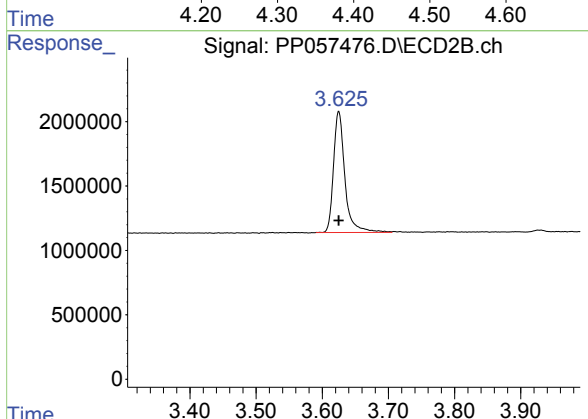


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 11270699
Conc: 5.30 ng/ml

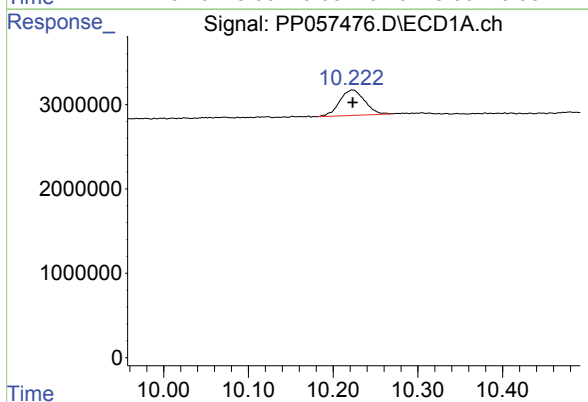


#2 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: 0.000 min
Response: 6229666
Conc: 4.90 ng/ml

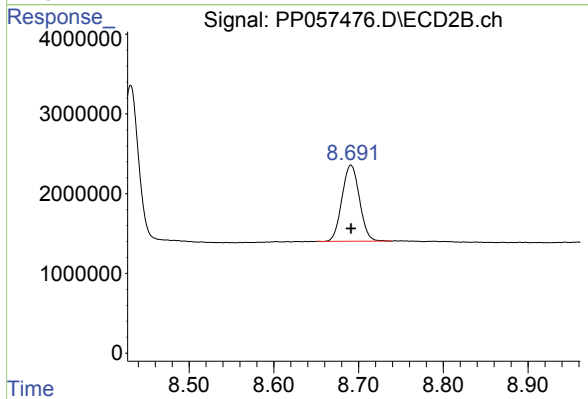

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: 0.000 min
Response: 13663681
Conc: 5.56 ng/ml

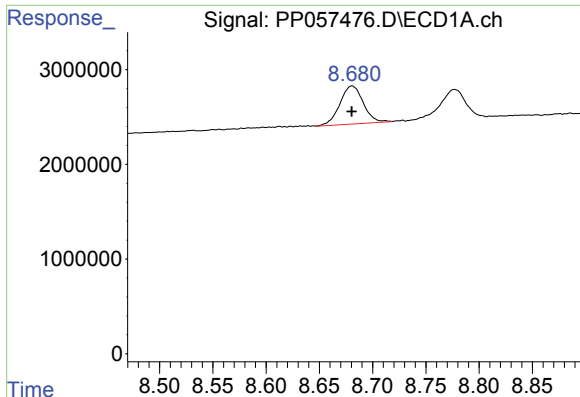


#41 AR-1268-1

R.T.: 8.680 min
Delta R.T.: 0.000 min
Response: 6177810
Conc: 49.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

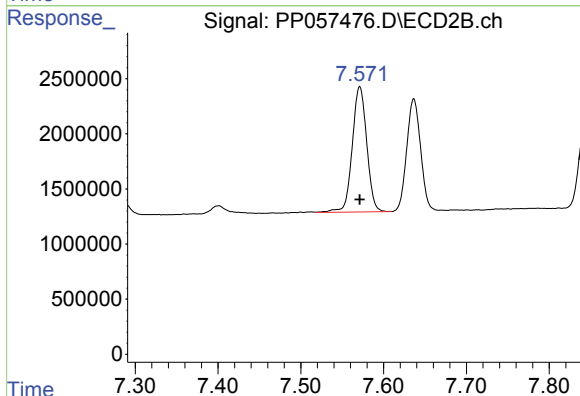


#41 AR-1268-1

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 13834842
Conc: 56.37 ng/ml

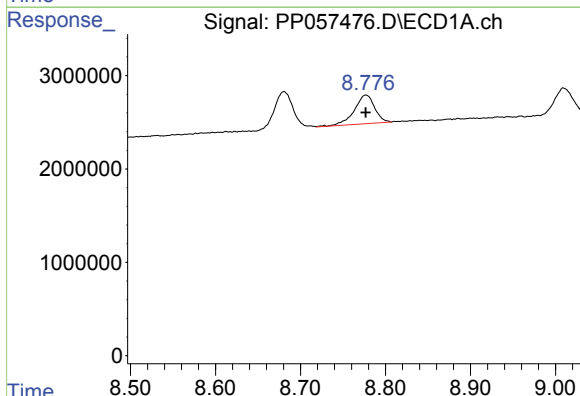


#42 AR-1268-2

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 5128264
Conc: 46.92 ng/ml

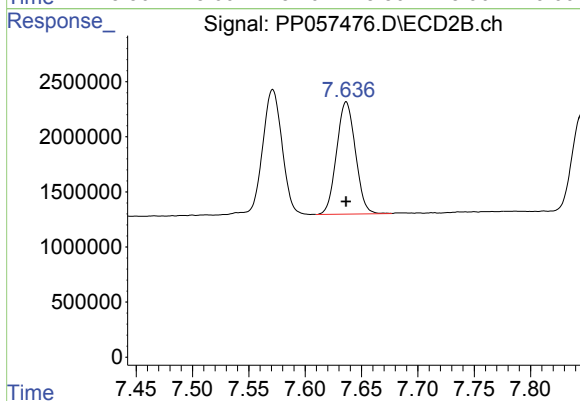

#42 AR-1268-2

R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 11884102
Conc: 54.38 ng/ml

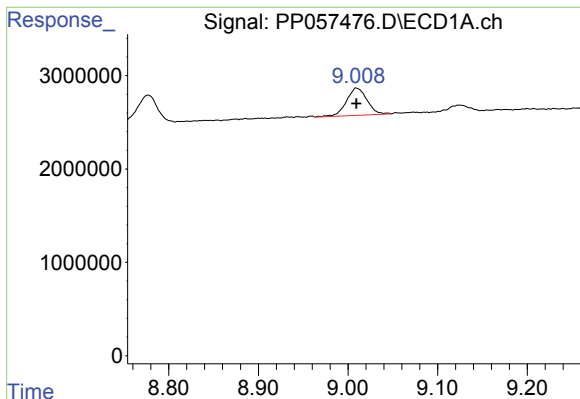


#43 AR-1268-3

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 4700124
Conc: 46.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

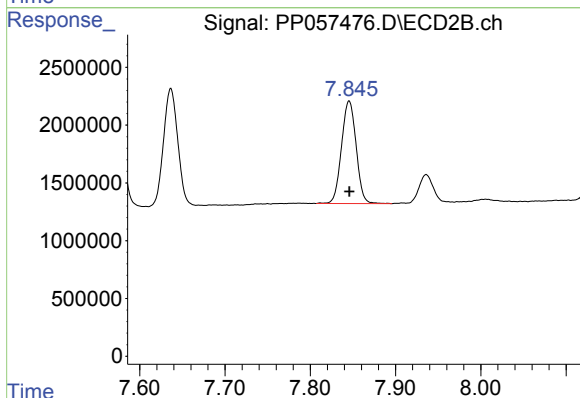


#43 AR-1268-3

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 10575074
Conc: 55.52 ng/ml

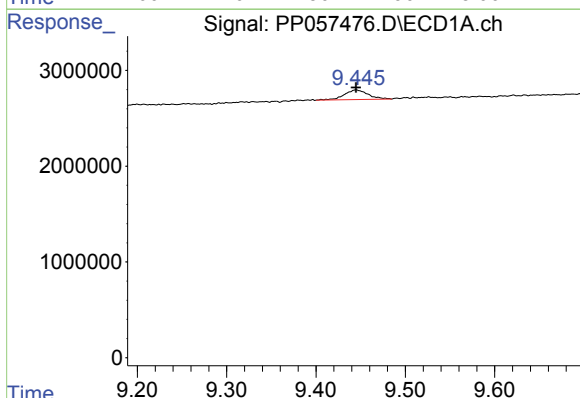


#44 AR-1268-4

R.T.: 9.445 min
Delta R.T.: 0.000 min
Response: 1859817
Conc: 50.06 ng/ml

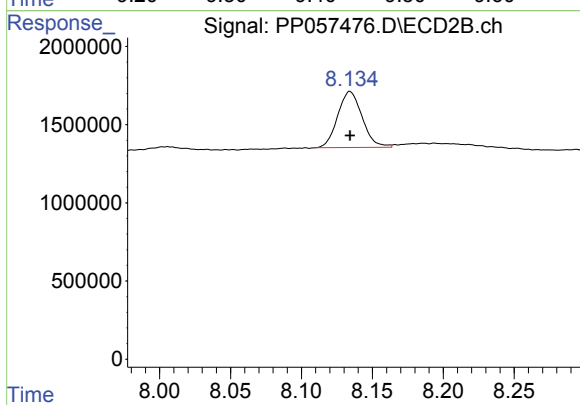

#44 AR-1268-4

R.T.: 8.134 min
Delta R.T.: 0.000 min
Response: 4312259
Conc: 56.09 ng/ml

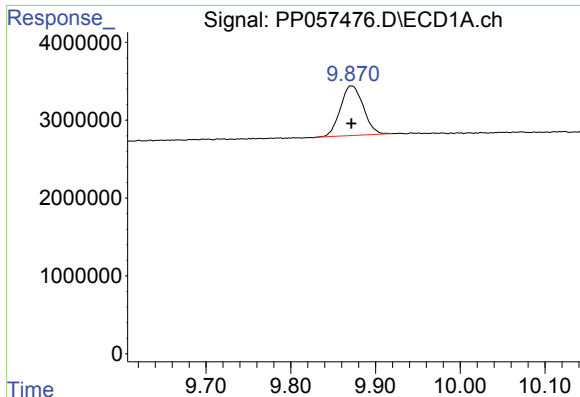

#45 AR-1268-5

R.T.: 9.872 min
Delta R.T.: 0.000 min
Response: 12049020
Conc: 47.13 ng/ml

Instrument :

ECD_P

ClientSampleId :


AR1268ICC050

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2023

Supervised By :Ankita Jodhani 05/04/2023

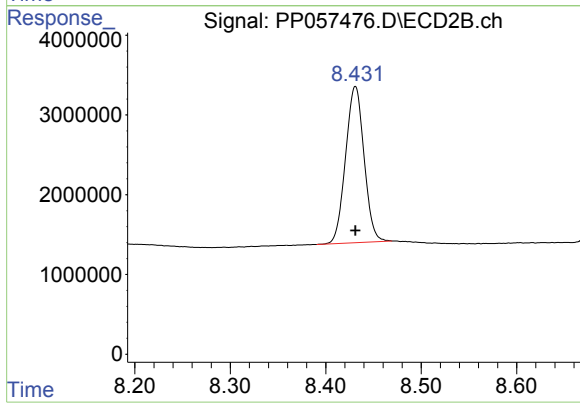

#45 AR-1268-5

R.T.: 8.431 min
Delta R.T.: 0.000 min
Response: 26372613
Conc: 52.11 ng/ml