

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035490.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 9:59
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:28:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.790	4.208	1056728	754127	20.813	22.151
2)	SA Decachlor...	10.647	9.460	909098	497999	22.386	25.699
Target Compounds							
20)	L4 AR-1242-5	7.060	0.000	18622	0	18.910	N.D. #
24)	L5 AR-1248-4	7.023	0.000	17022	0	10.335	N.D. #
25)	L5 AR-1248-5	7.060	0.000	18622	0	11.654	N.D. #
26)	L6 AR-1254-1	7.023f	0.000	17022	0	9.398	N.D. #
28)	L6 AR-1254-3	7.628f	6.862f	16878	44240	5.743	21.801 #
29)	L6 AR-1254-4	7.906	0.000	21735	0	10.537	N.D. #
32)	L7 AR-1260-2	0.000	7.203f	0	11327	N.D.	6.746 #
45)	L9 AR-1268-5	0.000	9.216	0	141843	N.D.	18.406 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035490.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 9:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:28:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

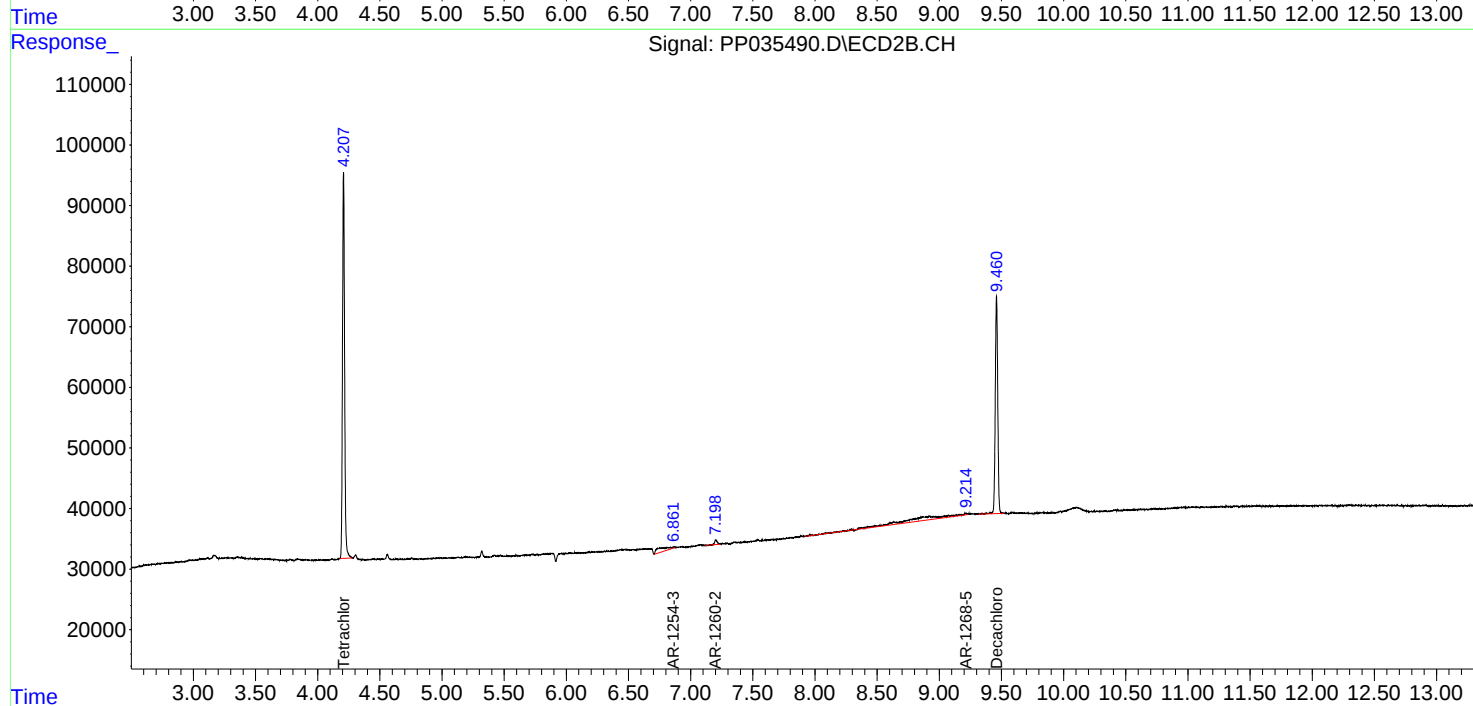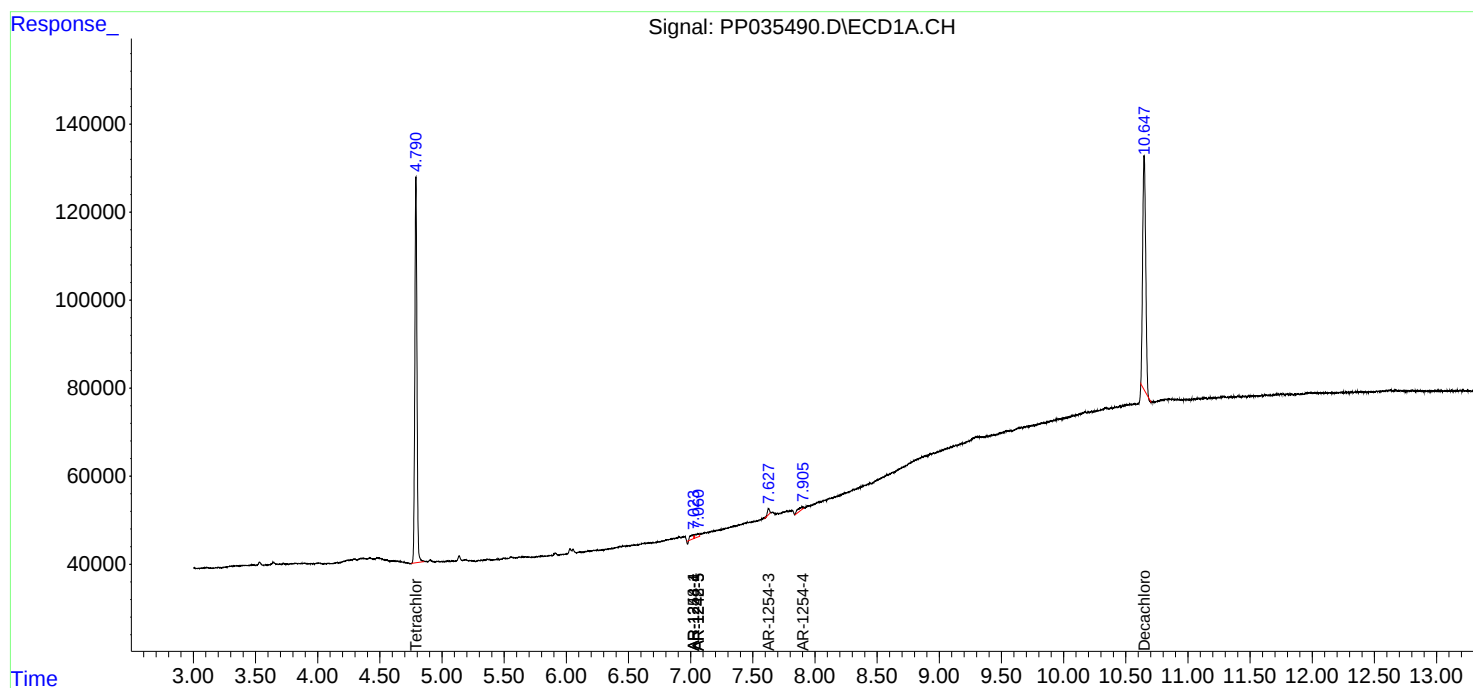


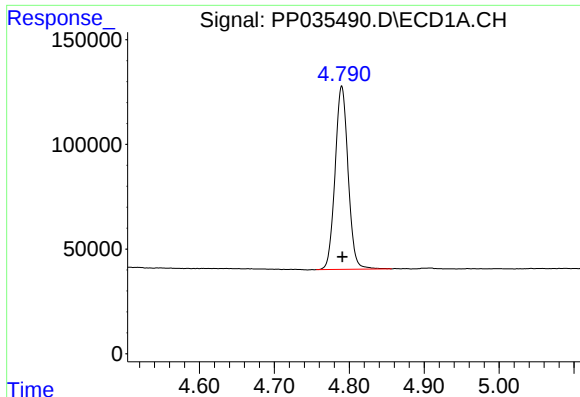

#1 Tetrachloro-m-xylene


R.T.: 4.790 min
Delta R.T.: -0.001 min
Response: 1056728
Conc: 20.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

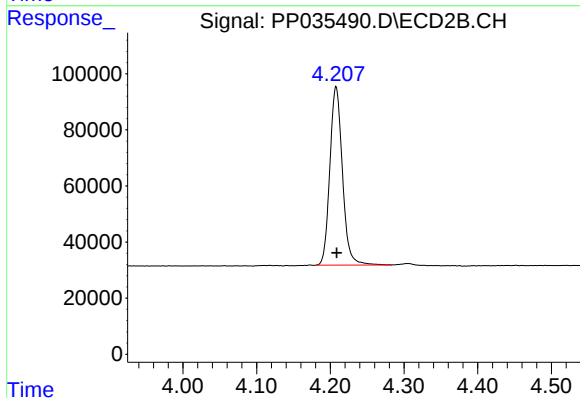


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 754127
Conc: 22.15 ng/ml

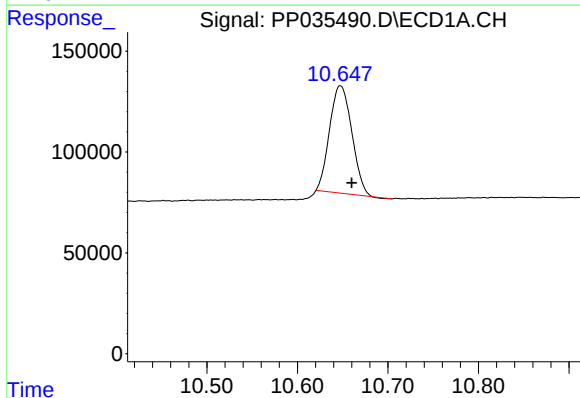


#2 Decachlorobiphenyl

R.T.: 10.647 min
Delta R.T.: -0.013 min
Response: 909098
Conc: 22.39 ng/ml

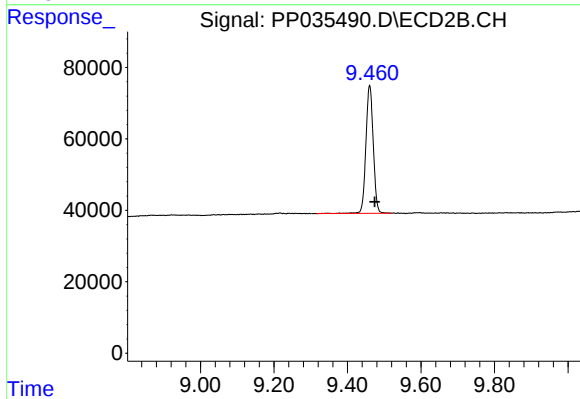

#2 Decachlorobiphenyl


R.T.: 9.460 min
Delta R.T.: -0.014 min
Response: 497999
Conc: 25.70 ng/ml

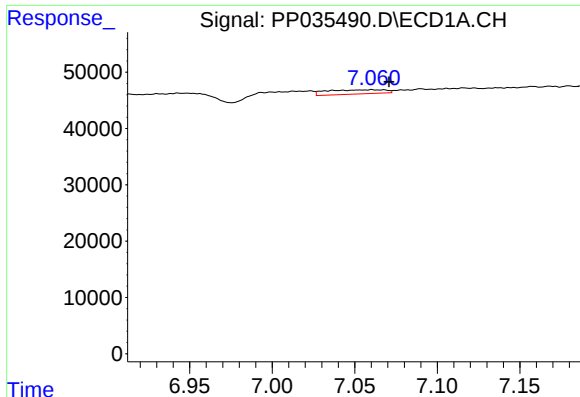

#20 AR-1242-5


R.T.: 7.060 min
Delta R.T.: -0.011 min
Response: 18622
Conc: 18.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

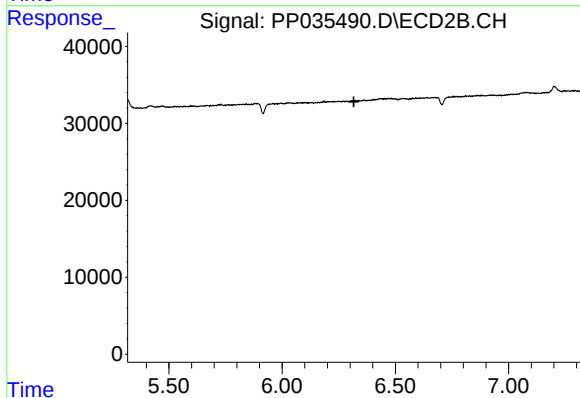


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.317 min
Response: 0
Conc: N.D.

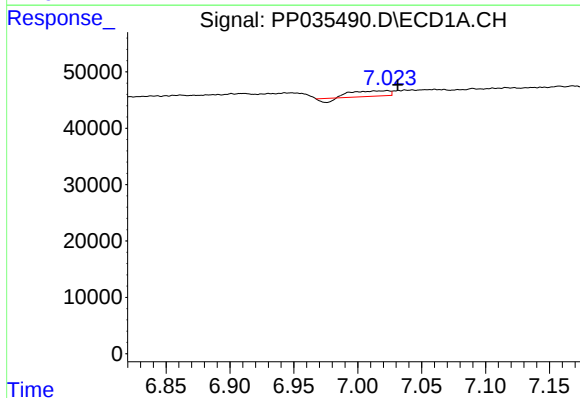


#24 AR-1248-4

R.T.: 7.023 min
Delta R.T.: -0.008 min
Response: 17022
Conc: 10.34 ng/ml

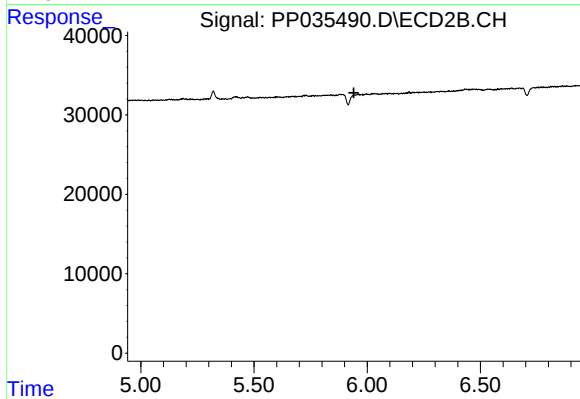

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

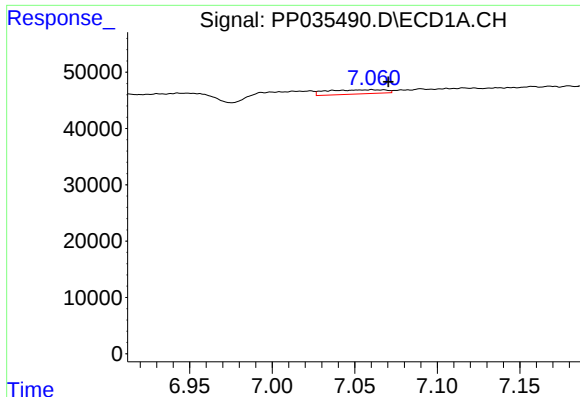

#25 AR-1248-5


R.T.: 7.060 min
Delta R.T.: -0.010 min
Response: 18622
Conc: 11.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

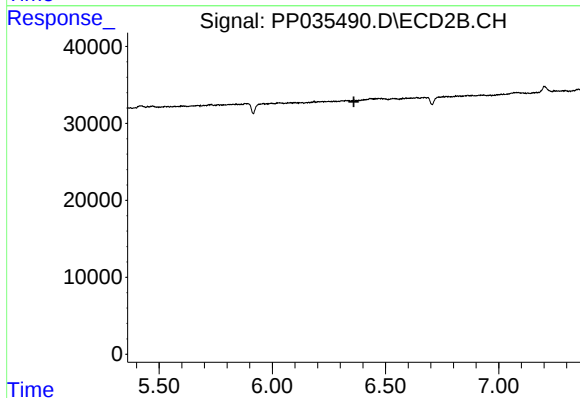


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.360 min
Response: 0
Conc: N.D.

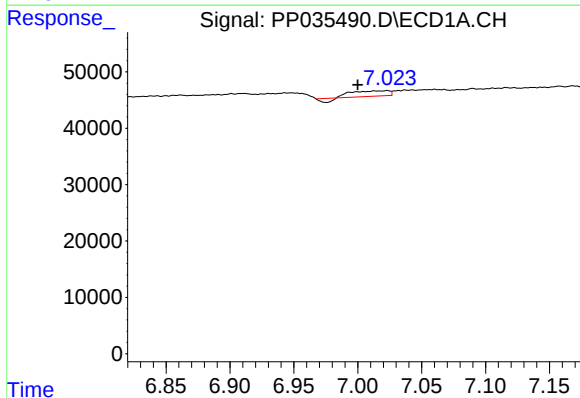


#26 AR-1254-1

R.T.: 7.023 min
Delta R.T.: 0.023 min
Response: 17022
Conc: 9.40 ng/ml

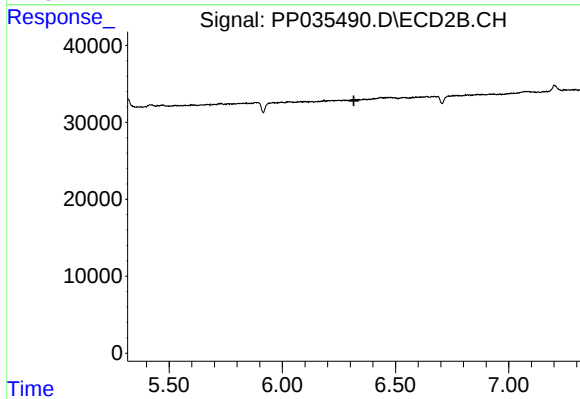

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

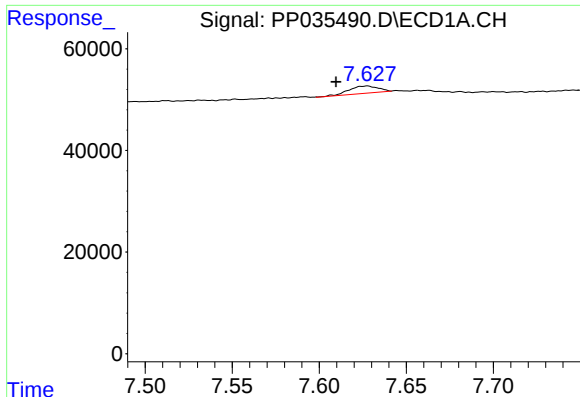

#28 AR-1254-3


R.T.: 7.628 min
Delta R.T.: 0.018 min
Response: 16878
Conc: 5.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

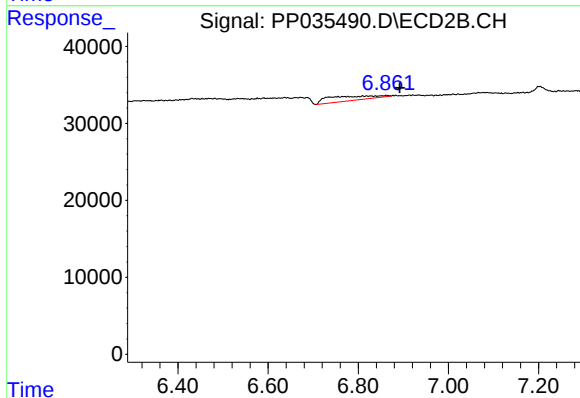


#28 AR-1254-3

R.T.: 6.862 min
Delta R.T.: -0.030 min
Response: 44240
Conc: 21.80 ng/ml

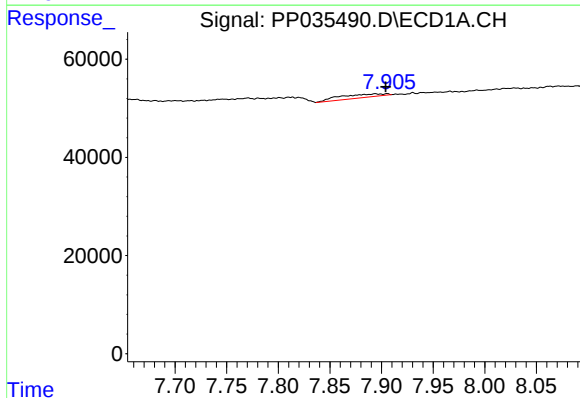


#29 AR-1254-4

R.T.: 7.906 min
Delta R.T.: 0.002 min
Response: 21735
Conc: 10.54 ng/ml

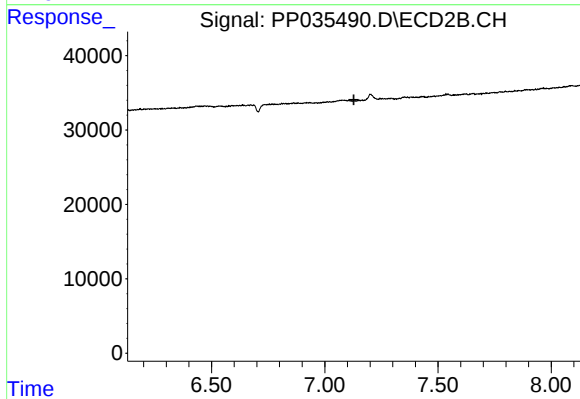

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.128 min
Response: 0
Conc: N.D.

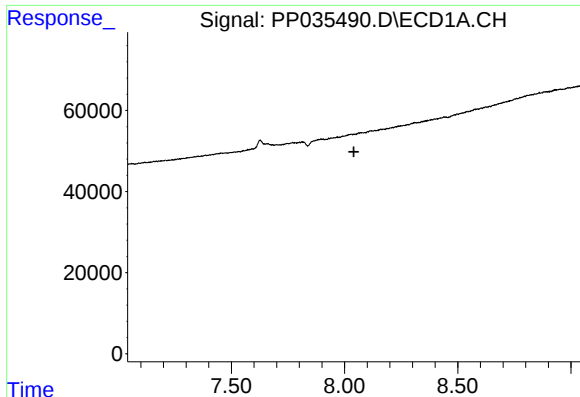

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

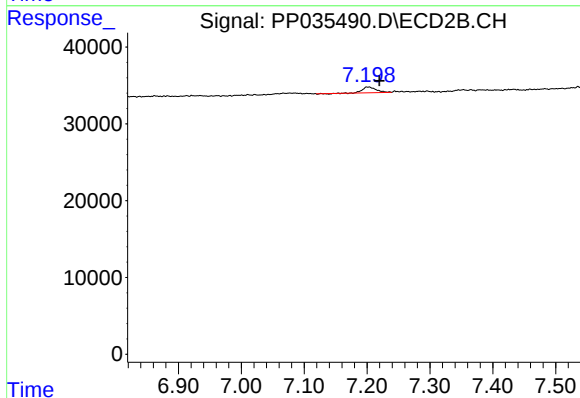


#32 AR-1260-2

R.T.: 7.203 min
Delta R.T.: -0.016 min
Response: 11327
Conc: 6.75 ng/ml

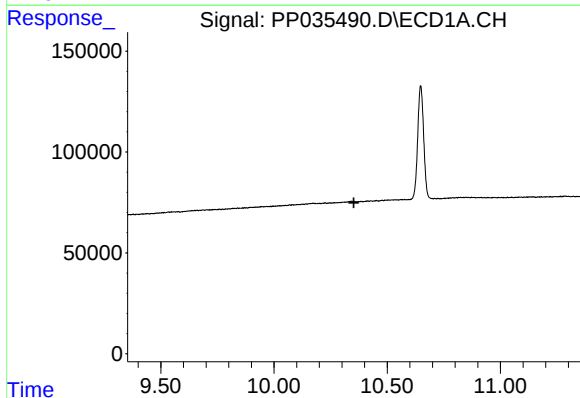

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.353 min
Response: 0
Conc: N.D.

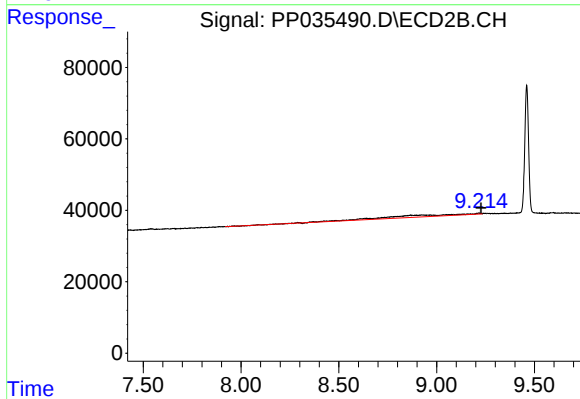

#45 AR-1268-5

R.T.: 9.216 min
Delta R.T.: -0.011 min
Response: 141843
Conc: 18.41 ng/ml