

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035525.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 00:24
 Operator : DD\AJ
 Sample : M2273-12 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 04:49:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.789	4.207	102619	84570	2.021	2.484
2) SA Decachlor...	10.644f	9.461	107612	55195	2.650	2.848
Target Compounds						
34) L7 AR-1260-4	8.632	0.000	5510	0	2.602	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035525.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 00:24
Operator : DD\AJ
Sample : M2273-12 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 04:49:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

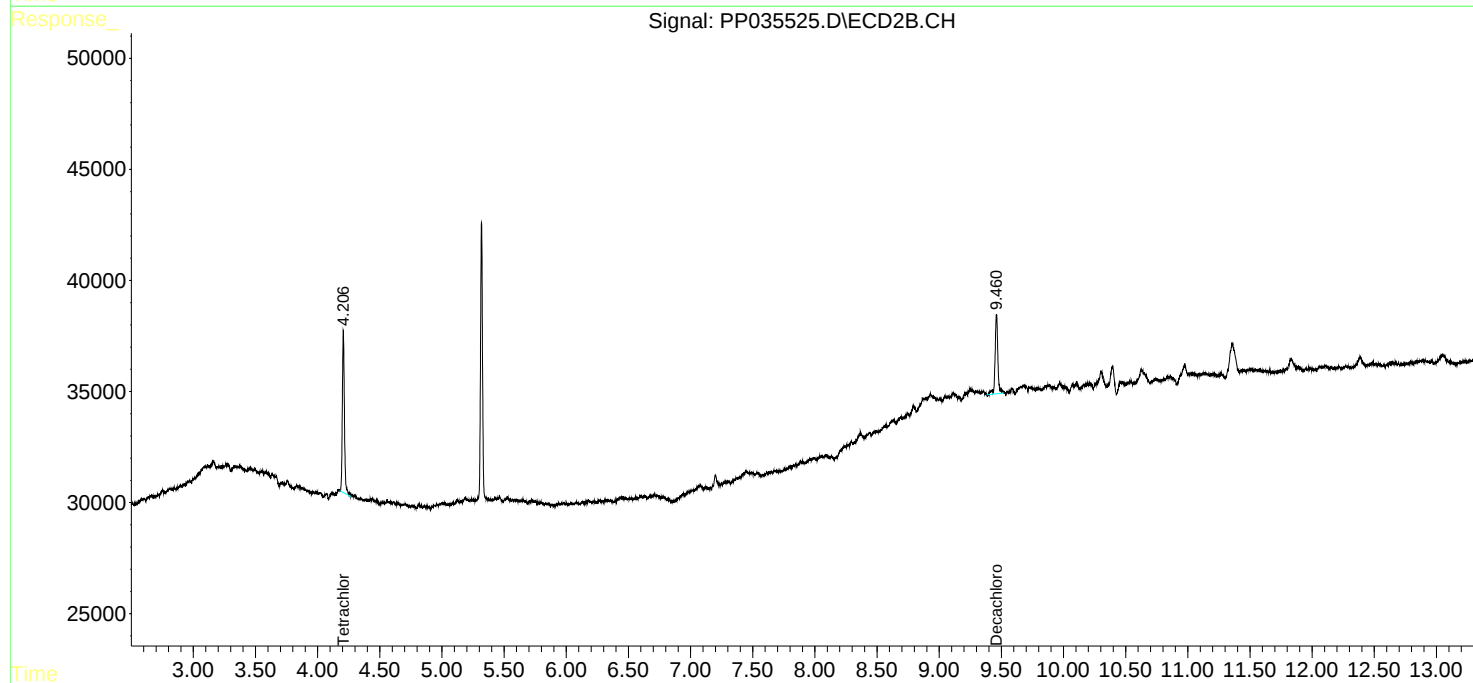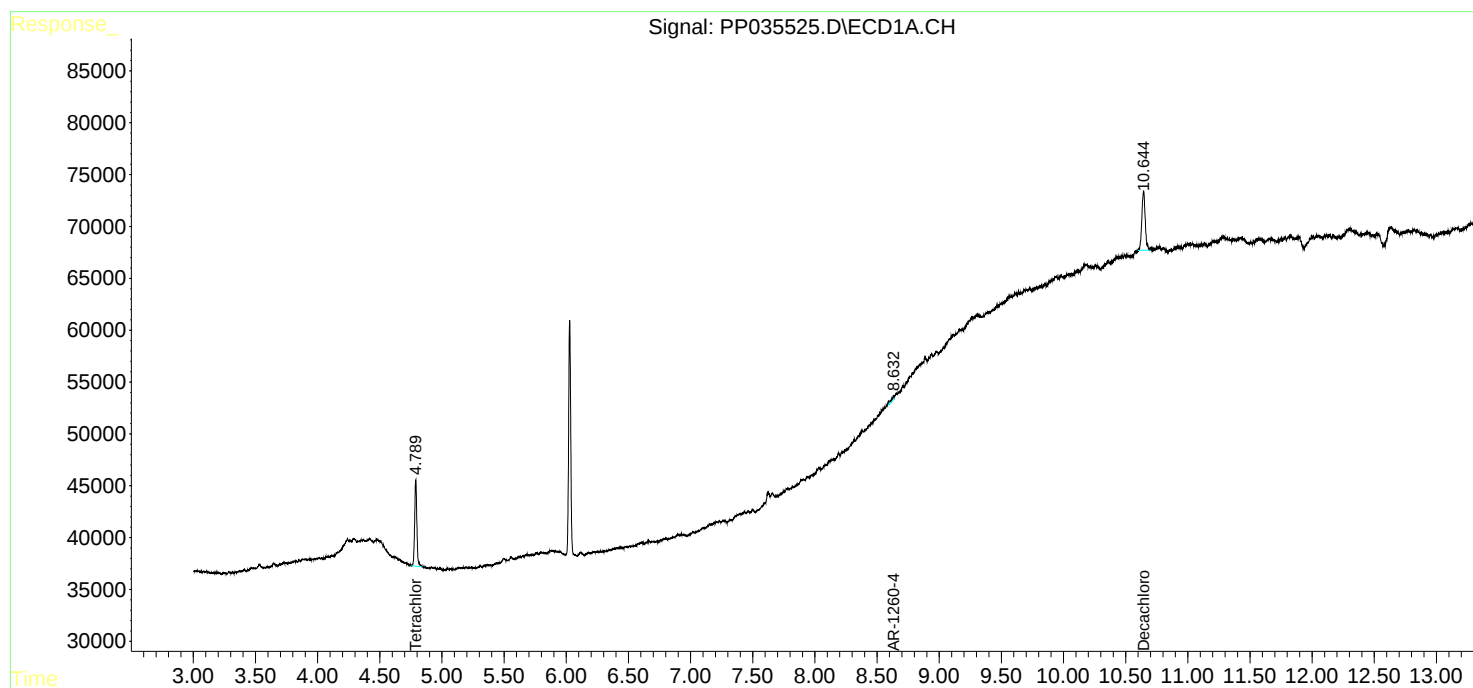


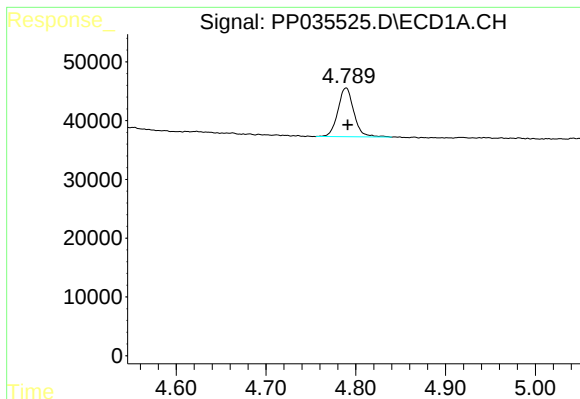

#1 Tetrachloro-m-xylene


R.T.: 4.789 min
Delta R.T.: -0.002 min
Response: 102619
Conc: 2.02 ng/ml

Instrument :
ECD_P
ClientSampleId :

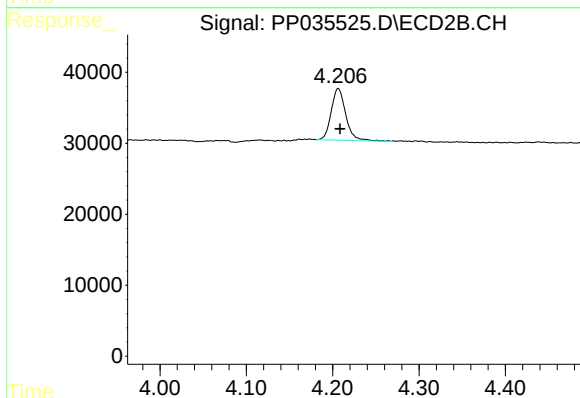


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: -0.002 min
Response: 84570
Conc: 2.48 ng/ml

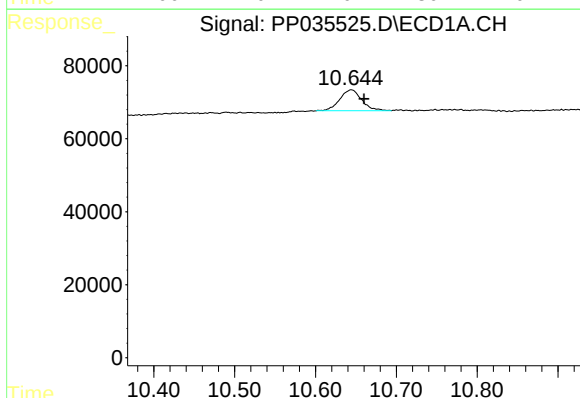


#2 Decachlorobiphenyl

R.T.: 10.644 min
Delta R.T.: -0.016 min
Response: 107612
Conc: 2.65 ng/ml

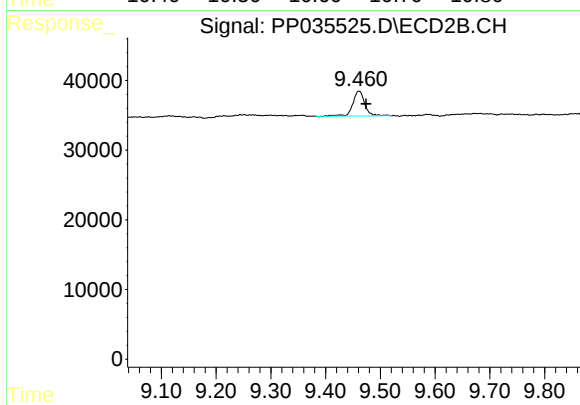

#2 Decachlorobiphenyl


R.T.: 9.461 min
Delta R.T.: -0.013 min
Response: 55195
Conc: 2.85 ng/ml

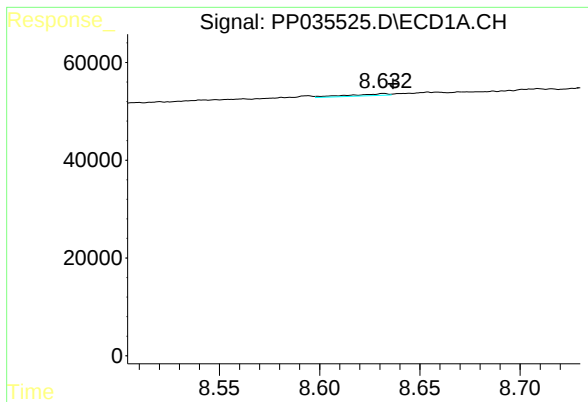

#34 AR-1260-4

R.T.: 8.632 min
Delta R.T.: -0.005 min
Response: 5510
Conc: 2.60 ng/ml

Instrument :
ECD_P
ClientSampleId :

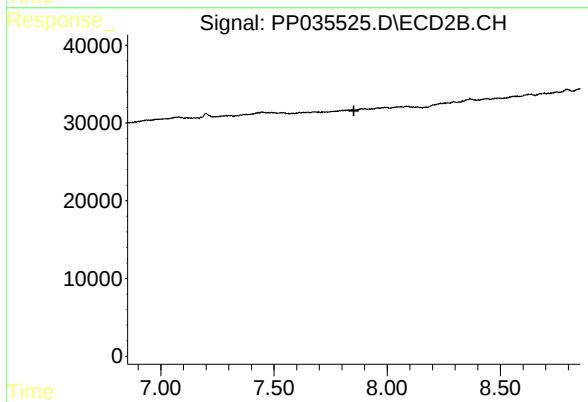

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.853 min
Response: 0
Conc: N.D.