

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035492.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 10:33
 Operator : DD\AJ
 Sample : M2245-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HA-21

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:29:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.789	4.208	1226756	870589	24.162	25.572
2) SA Decachlor...	10.646	9.459f	1183302	573860	29.138m	29.614m
Target Compounds						
26) L6 AR-1254-1	6.997	6.311	22315	20868	12.320	14.158
27) L6 AR-1254-2	7.223	6.466	64475	23325	23.043	17.618
28) L6 AR-1254-3	7.602	6.885	67666	48910	23.024	24.102
29) L6 AR-1254-4	7.896	7.121	44545	24383	21.595m	19.821
30) L6 AR-1254-5	8.323	7.543	68983	38157	29.158m	20.382 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035492.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 10:33
Operator : DD\AJ
Sample : M2245-02
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
HA-21


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:29:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

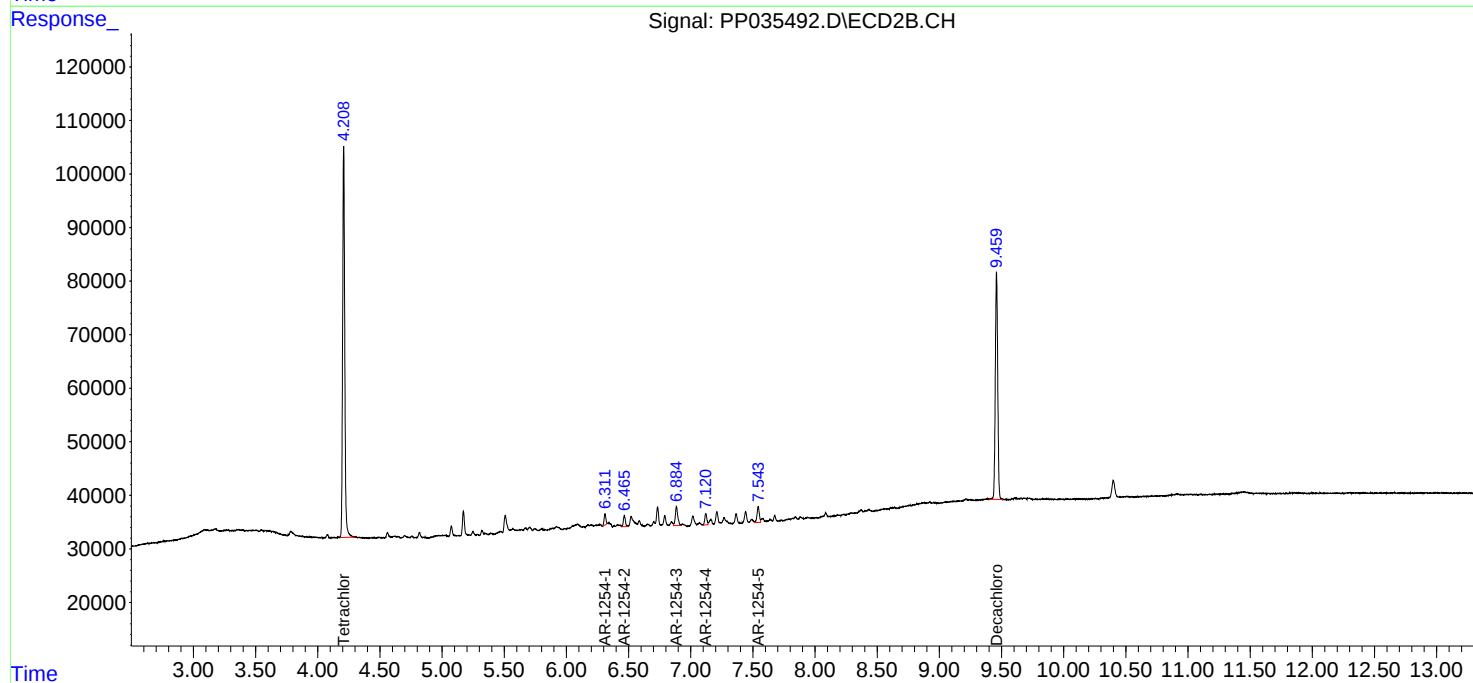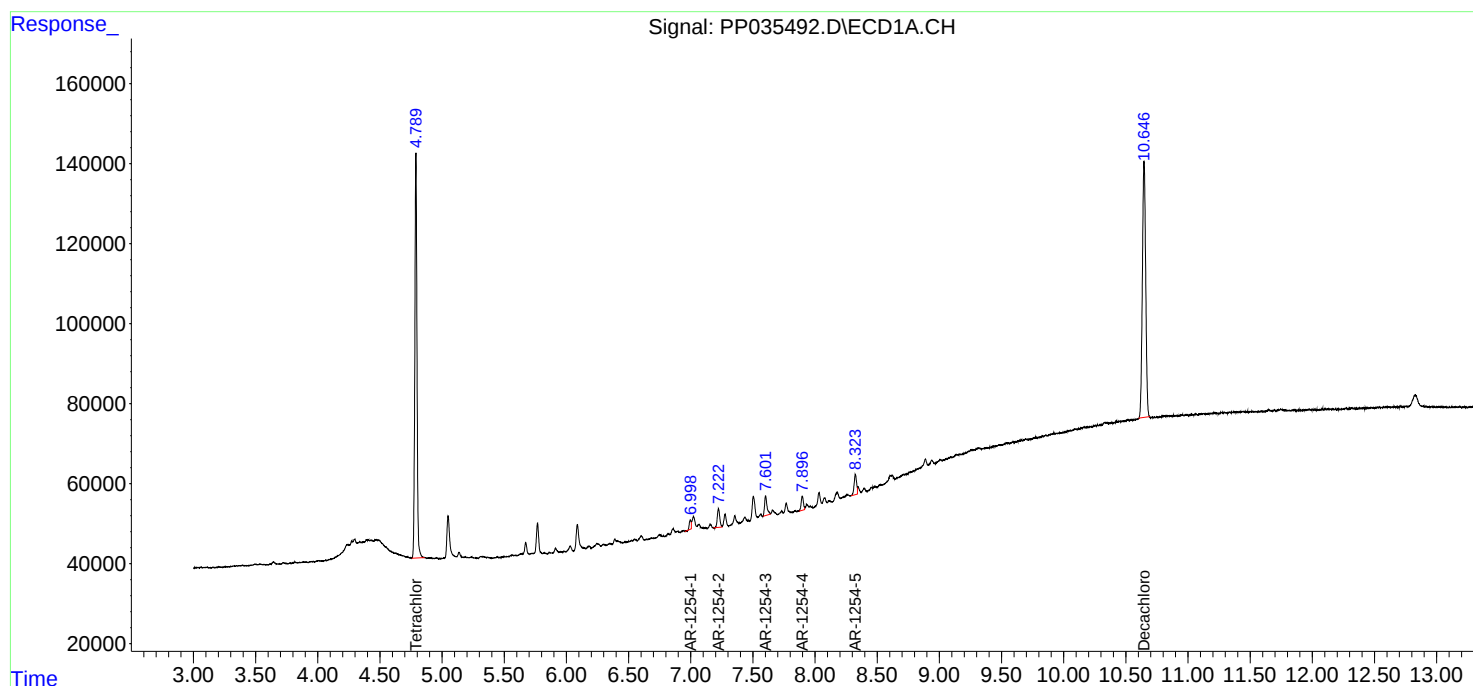

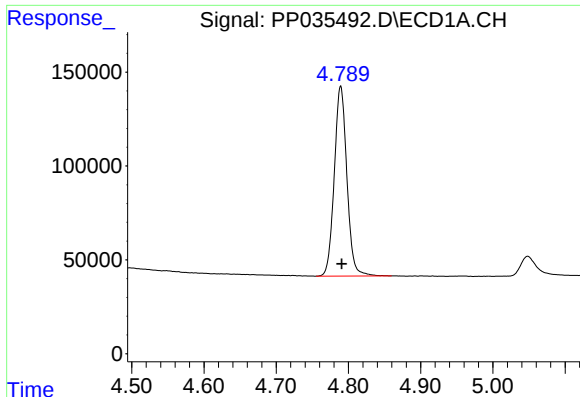


#1 Tetrachloro-m-xylene

R.T.: 4.789 min
Delta R.T.: -0.002 min
Response: 1226756
Conc: 24.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-21


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:26 AM

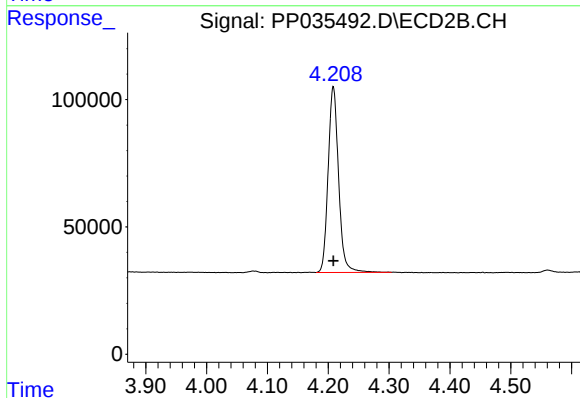


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 870589
Conc: 25.57 ng/ml

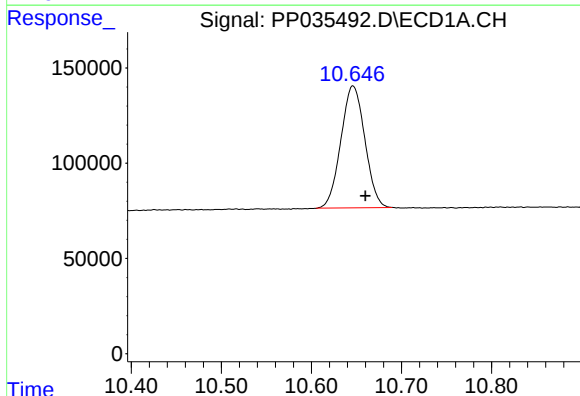


#2 Decachlorobiphenyl

R.T.: 10.646 min
Delta R.T.: -0.014 min
Response: 1183302
Conc: 29.14 ng/ml m

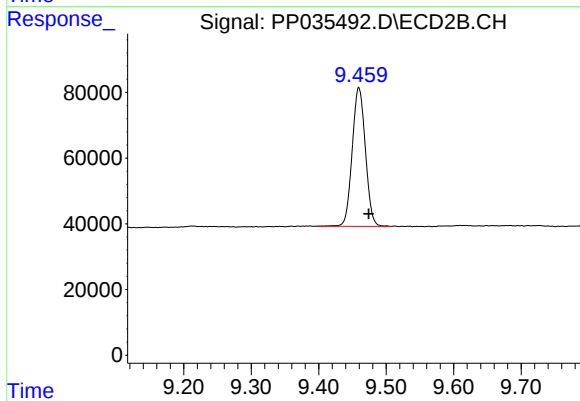

#2 Decachlorobiphenyl

R.T.: 9.459 min
Delta R.T.: -0.015 min
Response: 573860
Conc: 29.61 ng/ml m

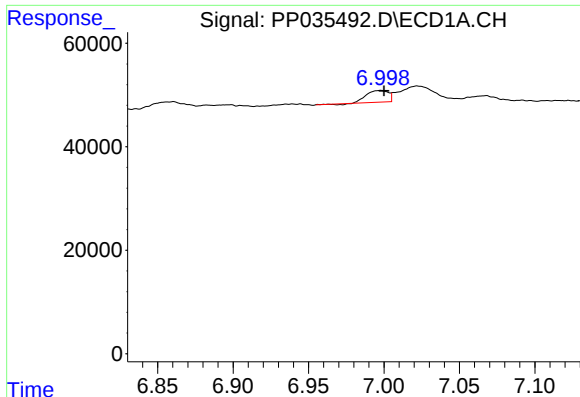


#26 AR-1254-1

R.T.: 6.997 min
Delta R.T.: -0.003 min
Response: 22315
Conc: 12.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-21


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:26 AM

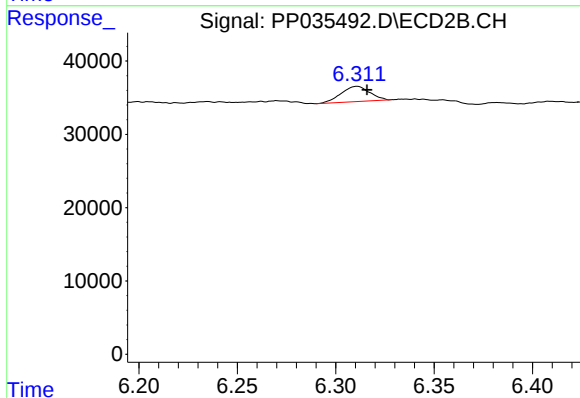


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 20868
Conc: 14.16 ng/ml

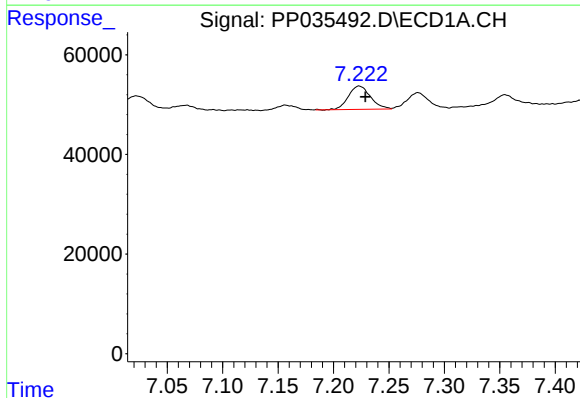


#27 AR-1254-2

R.T.: 7.223 min
Delta R.T.: -0.006 min
Response: 64475
Conc: 23.04 ng/ml

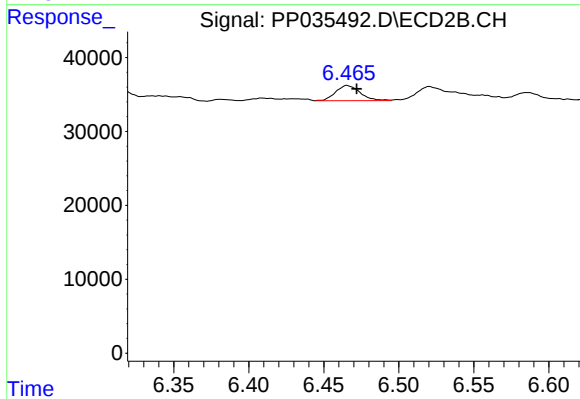

#27 AR-1254-2

R.T.: 6.466 min
Delta R.T.: -0.006 min
Response: 23325
Conc: 17.62 ng/ml

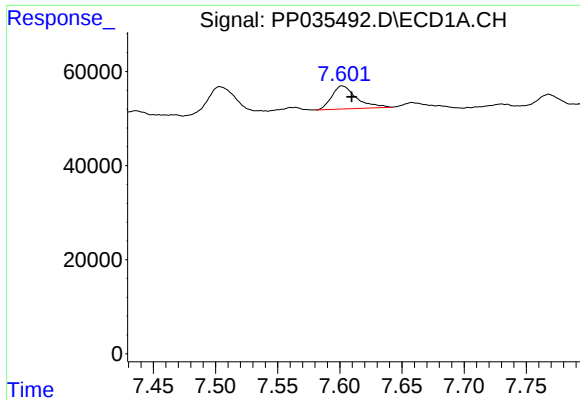


#28 AR-1254-3

R.T.: 7.602 min
Delta R.T.: -0.008 min
Response: 67666
Conc: 23.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-21


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:26 AM

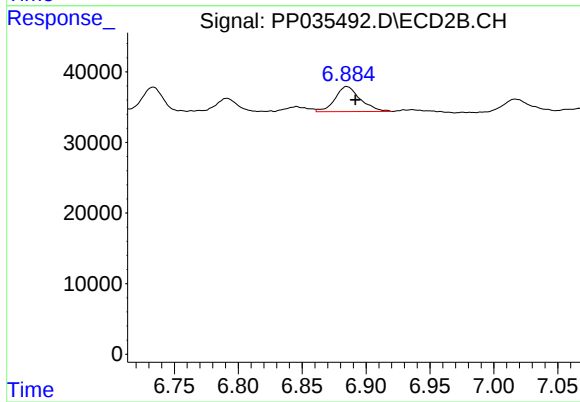


#28 AR-1254-3

R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 48910
Conc: 24.10 ng/ml

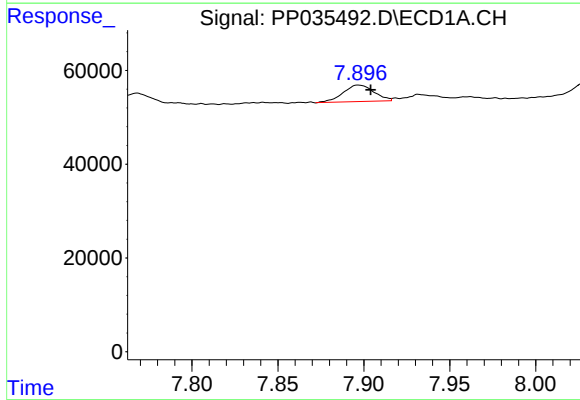


#29 AR-1254-4

R.T.: 7.896 min
Delta R.T.: -0.008 min
Response: 44545
Conc: 21.60 ng/ml m

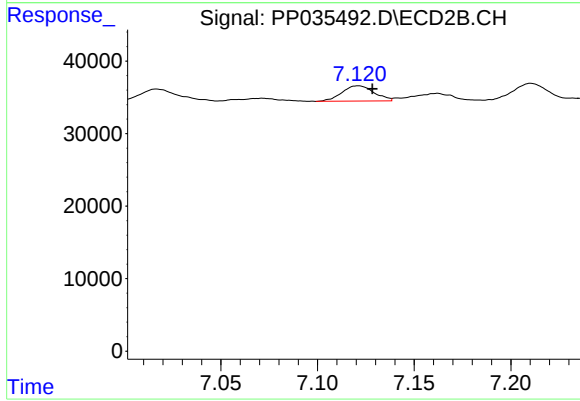

#29 AR-1254-4

R.T.: 7.121 min
Delta R.T.: -0.007 min
Response: 24383
Conc: 19.82 ng/ml

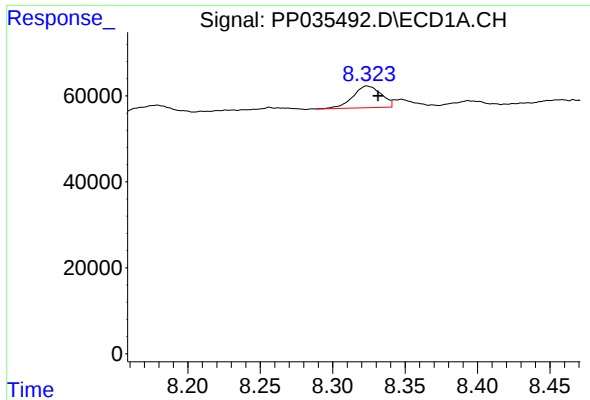


#30 AR-1254-5

R.T.: 8.323 min
Delta R.T.: -0.008 min
Response: 68983
Conc: 29.16 ng/ml m

Instrument :
ECD_P
ClientSampleId :
HA-21

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:26 AM

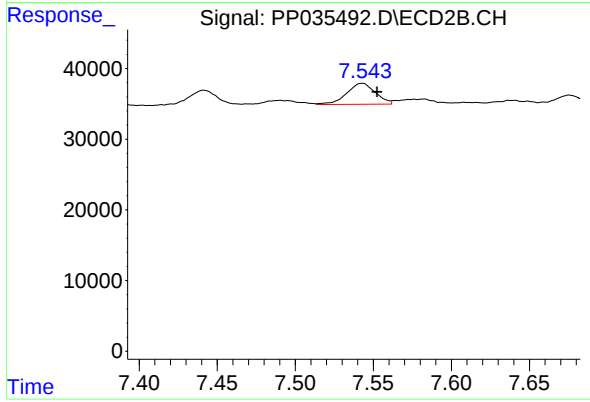

#30 AR-1254-5

R.T.: 7.543 min
Delta R.T.: -0.009 min
Response: 38157
Conc: 20.38 ng/ml