

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035493.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 10:50
 Operator : DD\AJ
 Sample : M2245-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HA-33

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:29:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	1119533	796913	22.050	23.408
2) SA Decachlor...	10.648	9.460	1101074	538977	27.113m	27.814
Target Compounds						
26) L6 AR-1254-1	6.996	6.310	99310	65819	54.831	44.653m
27) L6 AR-1254-2	7.224	6.466	150280	56439	53.710	42.628m
28) L6 AR-1254-3	7.603	6.885	198396	127875	67.507	63.015
29) L6 AR-1254-4	7.897	7.122	106077	62368	51.426	50.699
30) L6 AR-1254-5	8.323	7.543	150987	96205	63.821	51.387

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035493.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 10:50
Operator : DD\AJ
Sample : M2245-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
HA-33


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:29:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

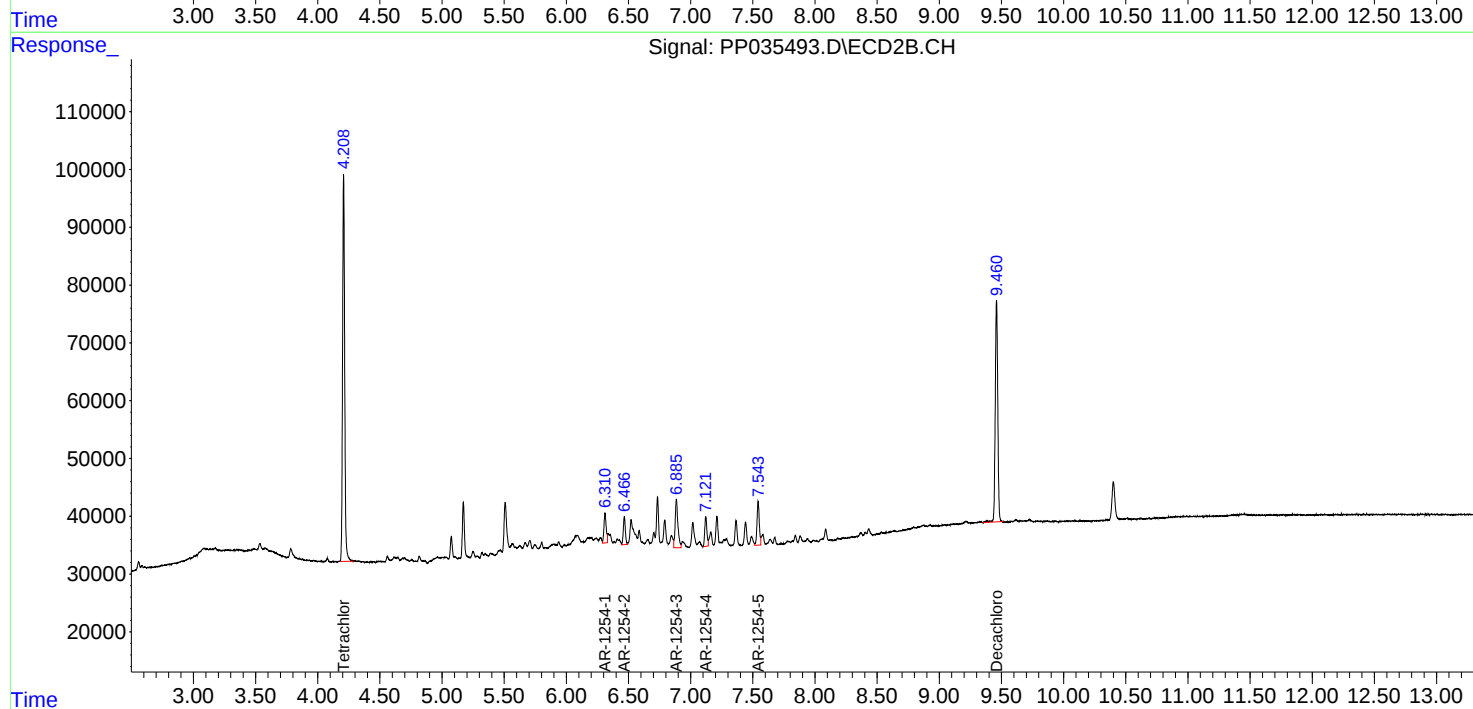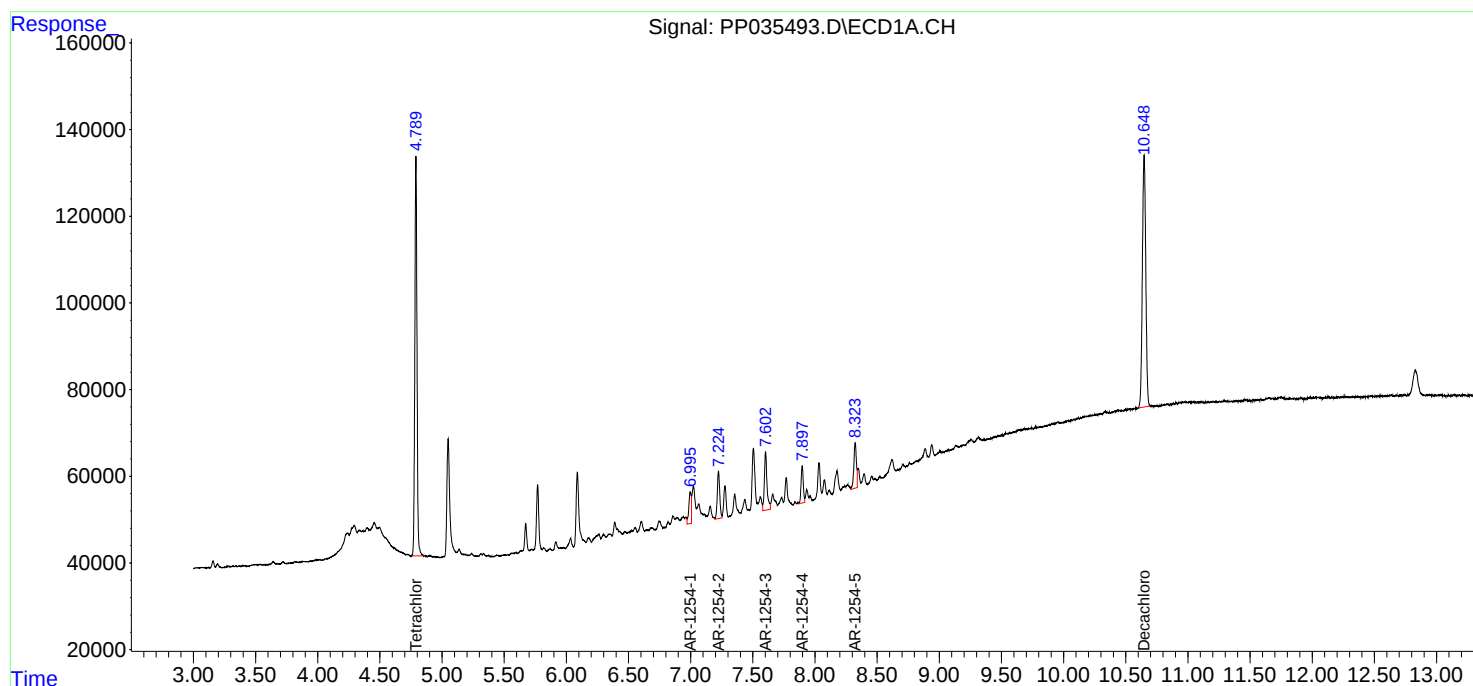

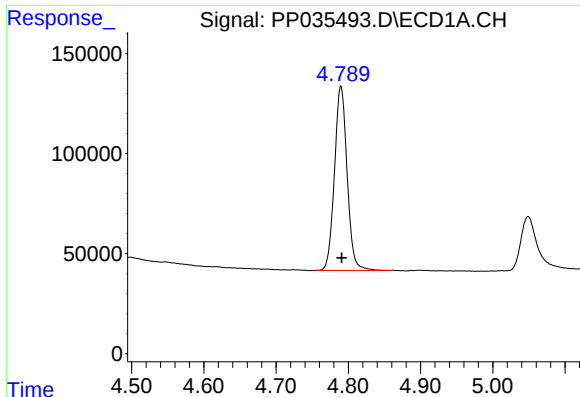


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: -0.001 min
Response: 1119533
Conc: 22.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-33


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:29 AM

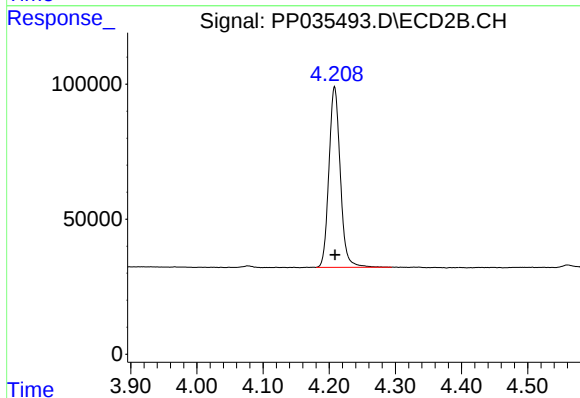


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 796913
Conc: 23.41 ng/ml

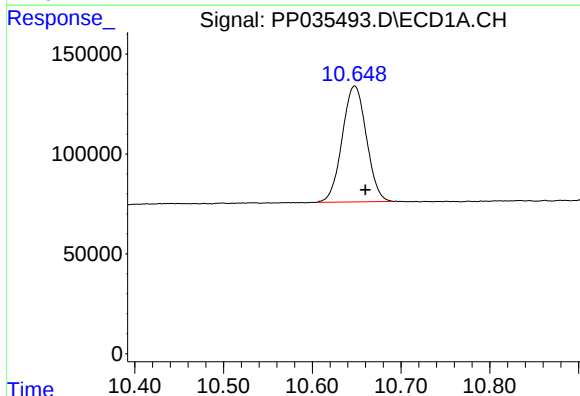


#2 Decachlorobiphenyl

R.T.: 10.648 min
Delta R.T.: -0.012 min
Response: 1101074
Conc: 27.11 ng/ml m

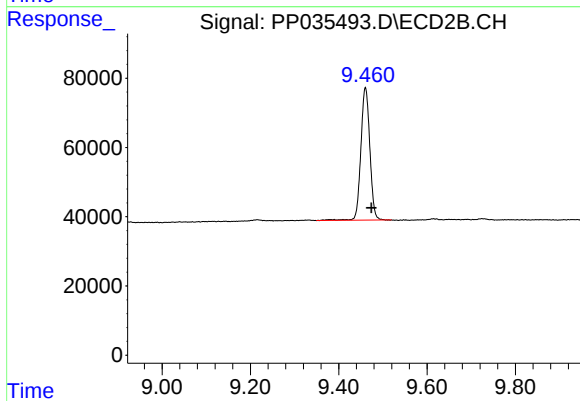

#2 Decachlorobiphenyl

R.T.: 9.460 min
Delta R.T.: -0.014 min
Response: 538977
Conc: 27.81 ng/ml

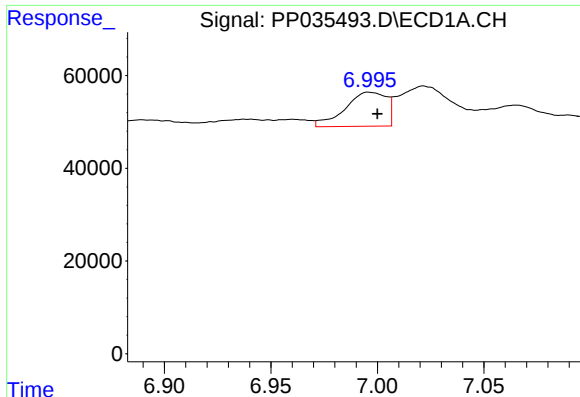


#26 AR-1254-1

R.T.: 6.996 min
Delta R.T.: -0.004 min
Response: 99310
Conc: 54.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-33


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:29 AM

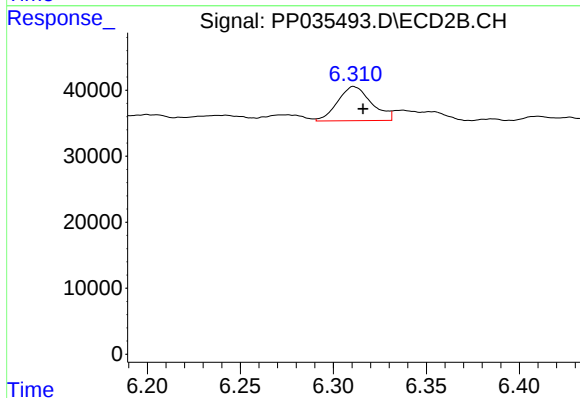


#26 AR-1254-1

R.T.: 6.310 min
Delta R.T.: -0.005 min
Response: 65819
Conc: 44.65 ng/ml m

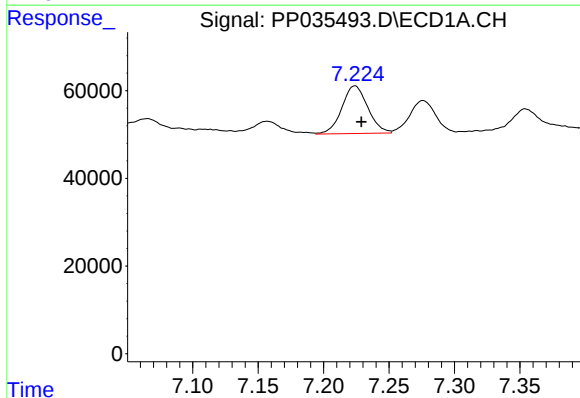


#27 AR-1254-2

R.T.: 7.224 min
Delta R.T.: -0.005 min
Response: 150280
Conc: 53.71 ng/ml

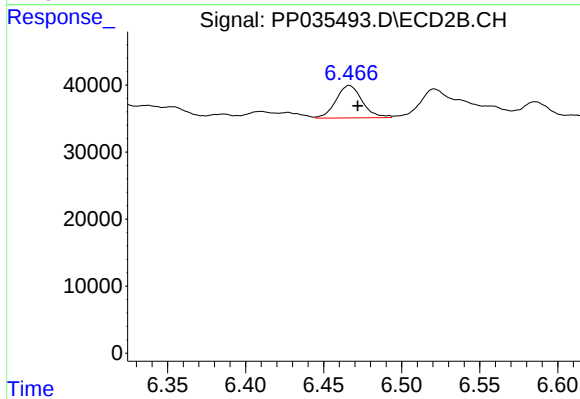

#27 AR-1254-2

R.T.: 6.466 min
Delta R.T.: -0.006 min
Response: 56439
Conc: 42.63 ng/ml m

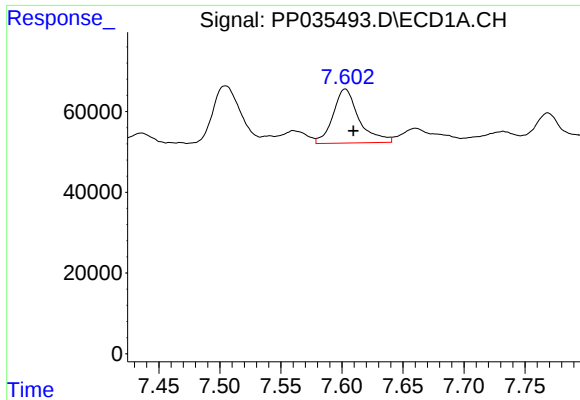


#28 AR-1254-3

R.T.: 7.603 min
Delta R.T.: -0.007 min
Response: 198396
Conc: 67.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-33


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:29 AM

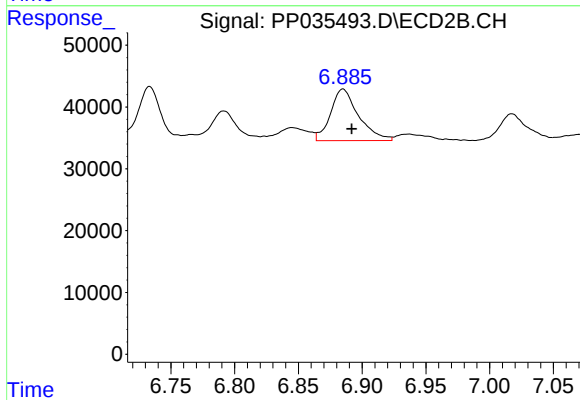


#28 AR-1254-3

R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 127875
Conc: 63.02 ng/ml

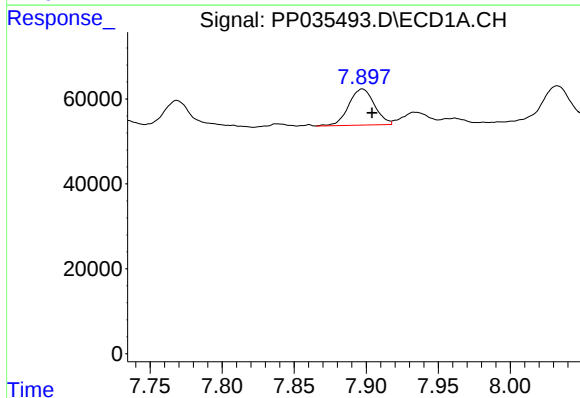


#29 AR-1254-4

R.T.: 7.897 min
Delta R.T.: -0.007 min
Response: 106077
Conc: 51.43 ng/ml

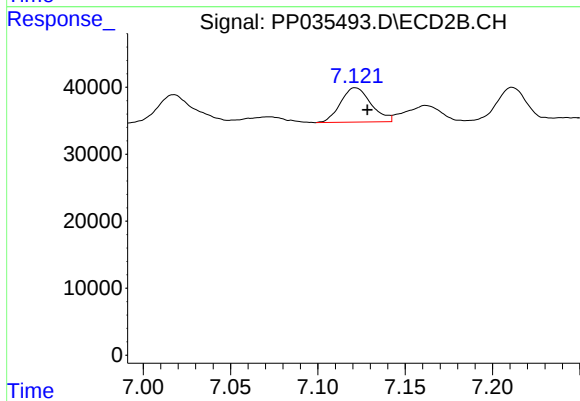

#29 AR-1254-4

R.T.: 7.122 min
Delta R.T.: -0.007 min
Response: 62368
Conc: 50.70 ng/ml

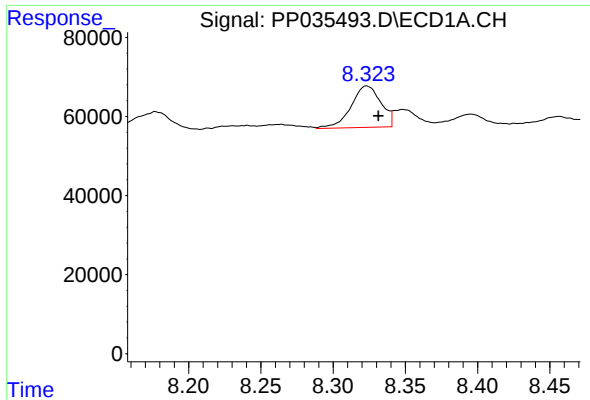


#30 AR-1254-5

R.T.: 8.323 min
Delta R.T.: -0.008 min
Response: 150987
Conc: 63.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-33

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:29 AM

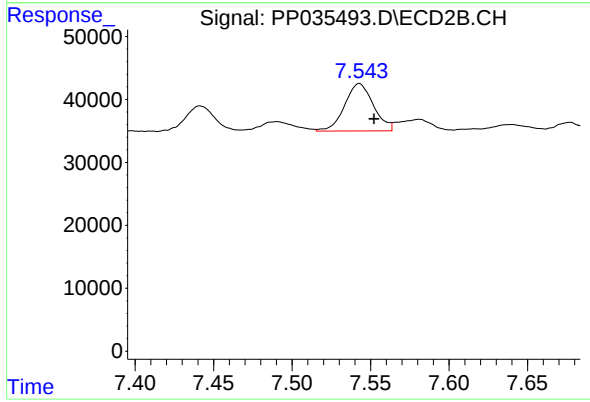

#30 AR-1254-5

R.T.: 7.543 min
Delta R.T.: -0.010 min
Response: 96205
Conc: 51.39 ng/ml