

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 11:06
 Operator : DD\AJ
 Sample : M2245-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HA-61

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:30:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.789	4.208	1022820	798192	20.145	23.446
2) SA Decachlor...	10.644f	9.460	1039492	600300	25.597m	30.978
Target Compounds						
26) L6 AR-1254-1	6.998	6.309	55880	37301	30.852m	25.306m
27) L6 AR-1254-2	7.224	6.469	76375	39529	27.296	29.856
28) L6 AR-1254-3	7.602	6.886	64162	54754	21.832	26.982
29) L6 AR-1254-4	7.894	7.118	65370	37904	31.691	30.812
30) L6 AR-1254-5	8.323	7.541	90955	91271	38.446	48.752 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 11:06
Operator : DD\AJ
Sample : M2245-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:30:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

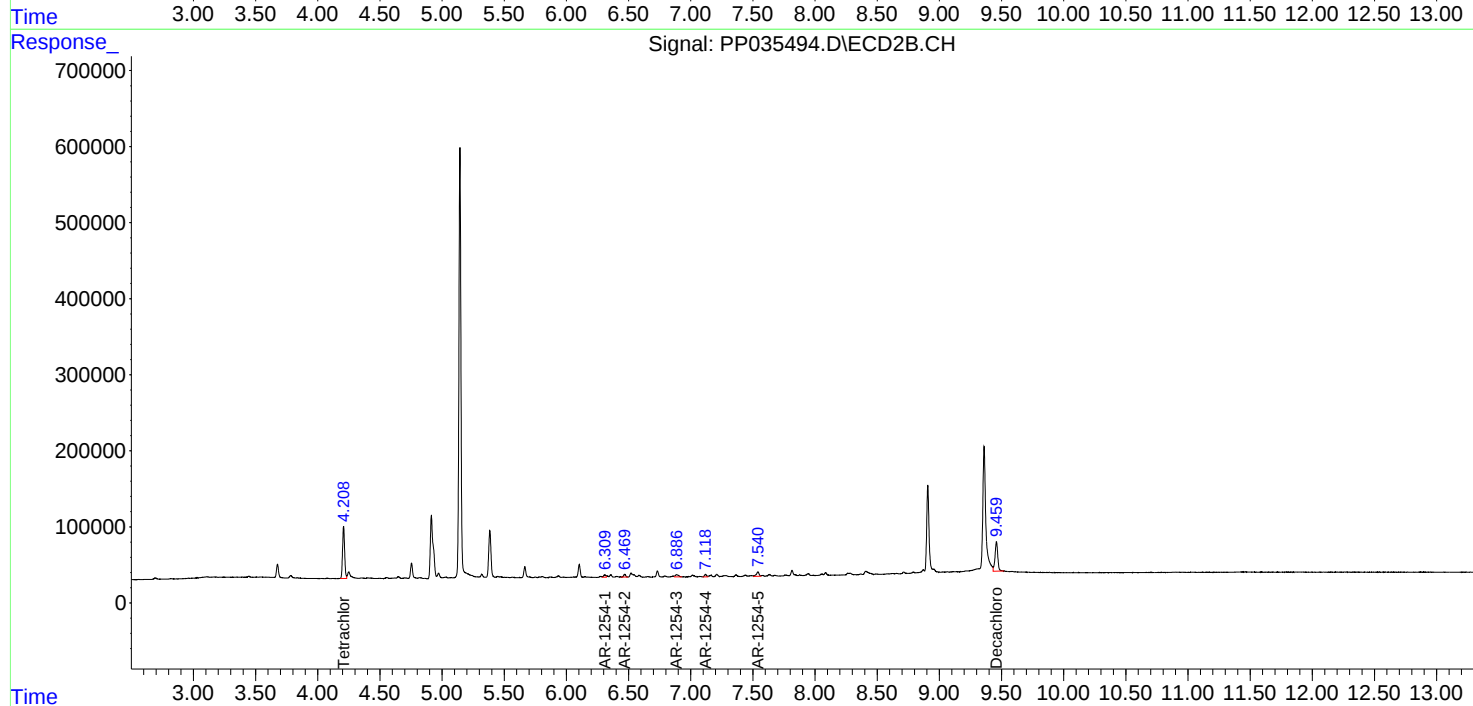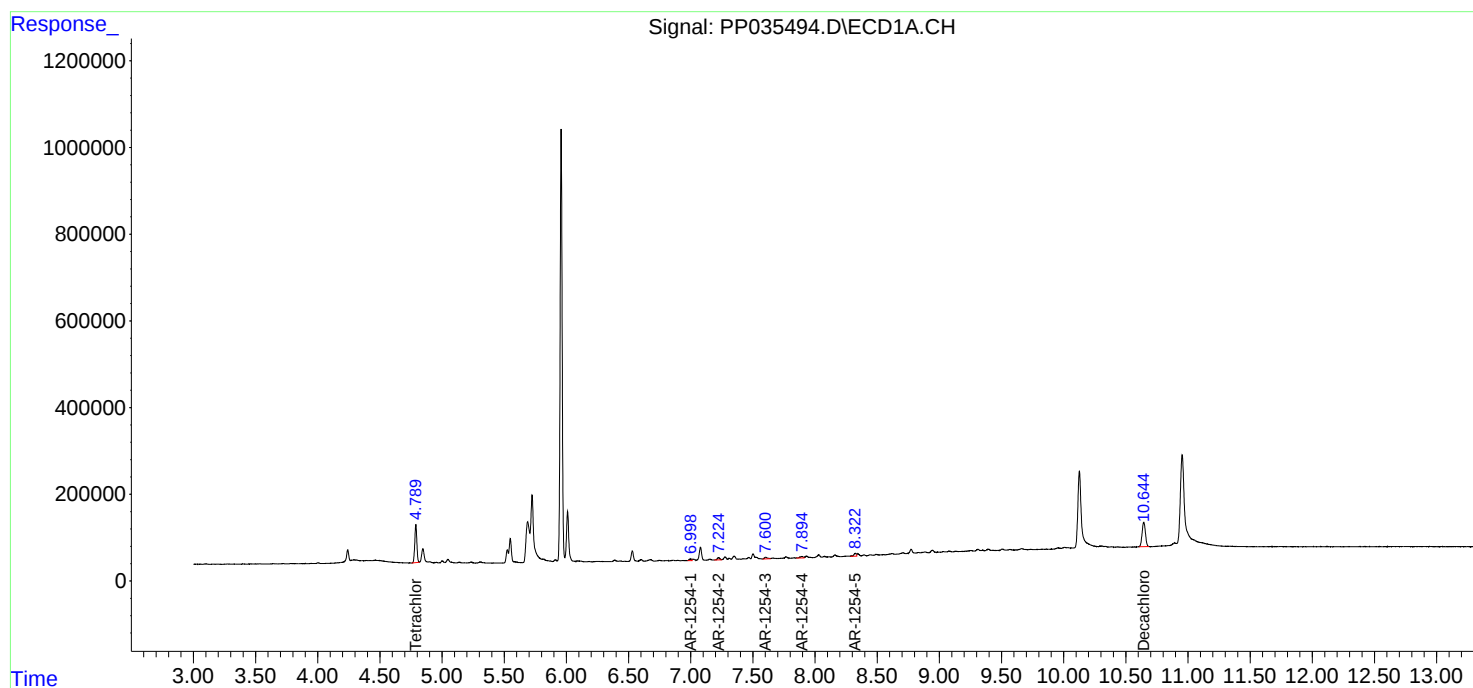

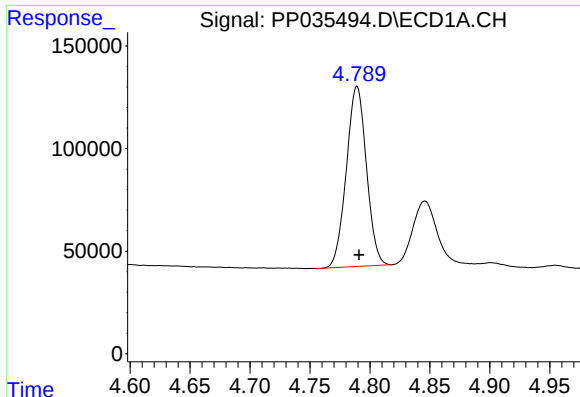


#1 Tetrachloro-m-xylene

R.T.: 4.789 min
Delta R.T.: -0.002 min
Response: 1022820
Conc: 20.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:30 AM

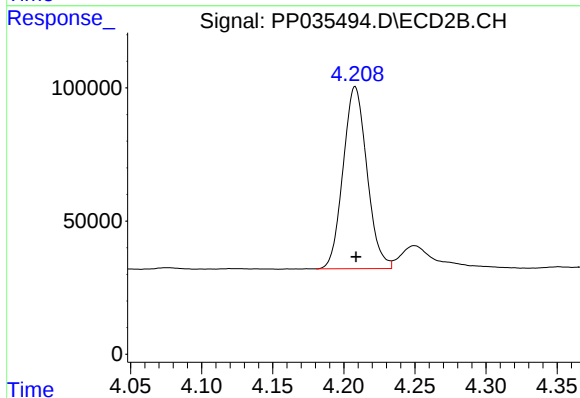


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 798192
Conc: 23.45 ng/ml

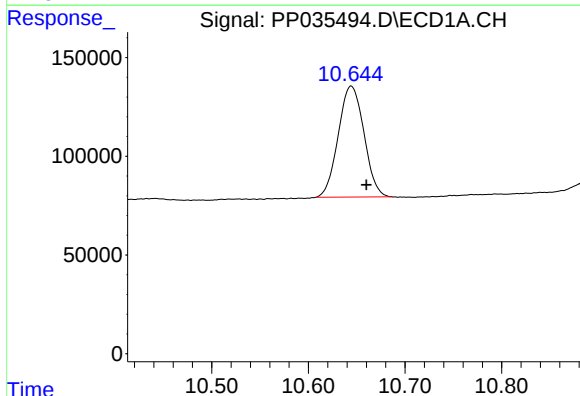


#2 Decachlorobiphenyl

R.T.: 10.644 min
Delta R.T.: -0.016 min
Response: 1039492
Conc: 25.60 ng/ml m

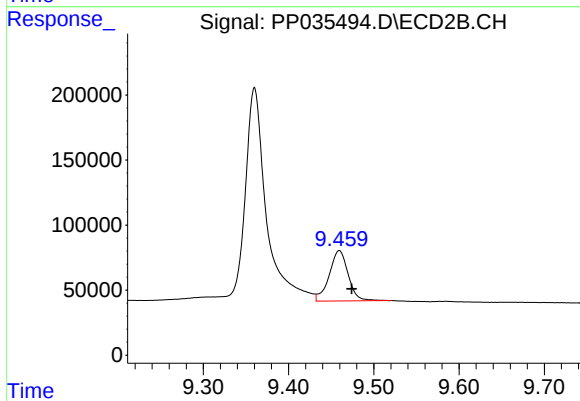

#2 Decachlorobiphenyl

R.T.: 9.460 min
Delta R.T.: -0.014 min
Response: 600300
Conc: 30.98 ng/ml

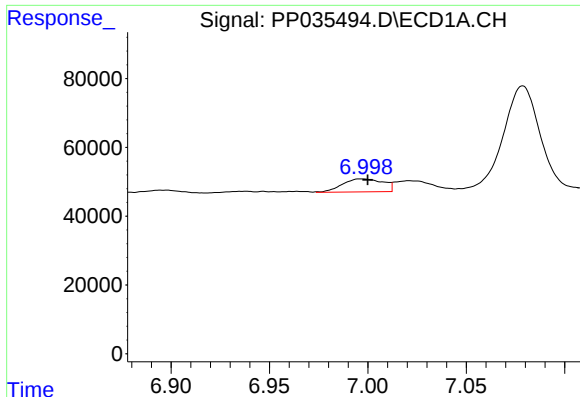


#26 AR-1254-1

R.T.: 6.998 min
Delta R.T.: -0.002 min
Response: 55880
Conc: 30.85 ng/ml m

Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:30 AM

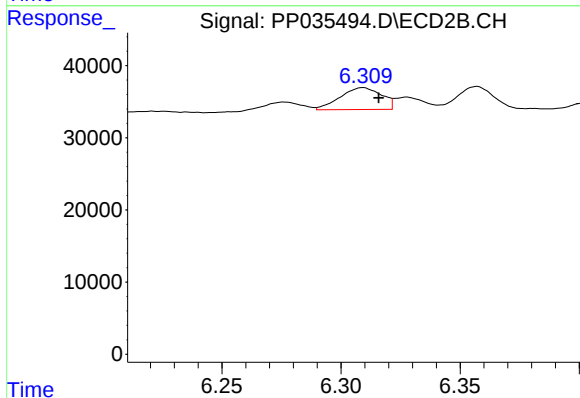


#26 AR-1254-1

R.T.: 6.309 min
Delta R.T.: -0.007 min
Response: 37301
Conc: 25.31 ng/ml m

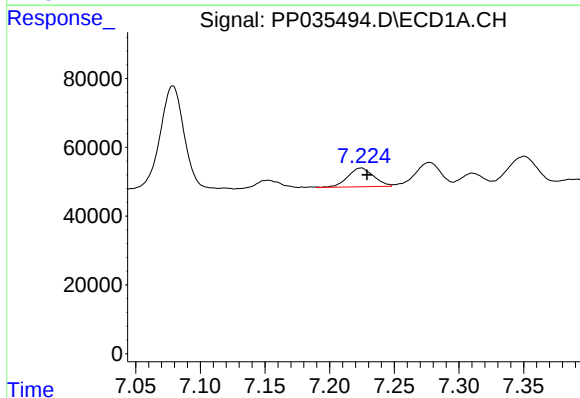


#27 AR-1254-2

R.T.: 7.224 min
Delta R.T.: -0.005 min
Response: 76375
Conc: 27.30 ng/ml

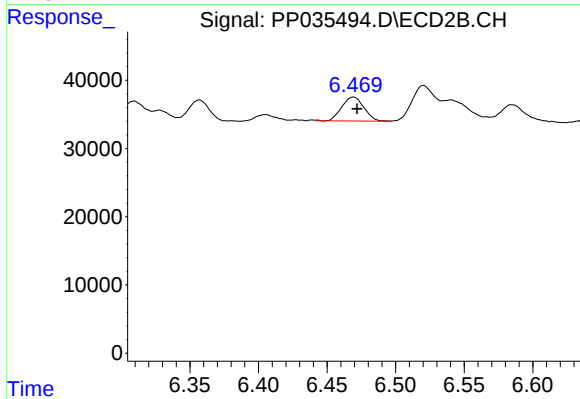

#27 AR-1254-2

R.T.: 6.469 min
Delta R.T.: -0.003 min
Response: 39529
Conc: 29.86 ng/ml

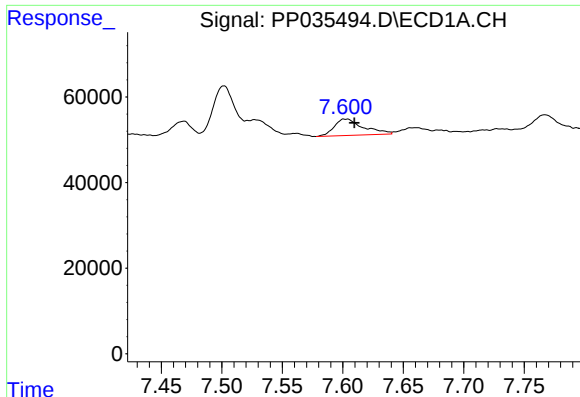


#28 AR-1254-3

R.T.: 7.602 min
Delta R.T.: -0.007 min
Response: 64162
Conc: 21.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-61


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:30 AM

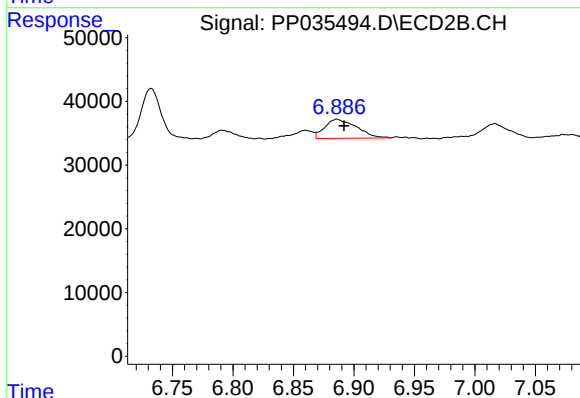


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 54754
Conc: 26.98 ng/ml

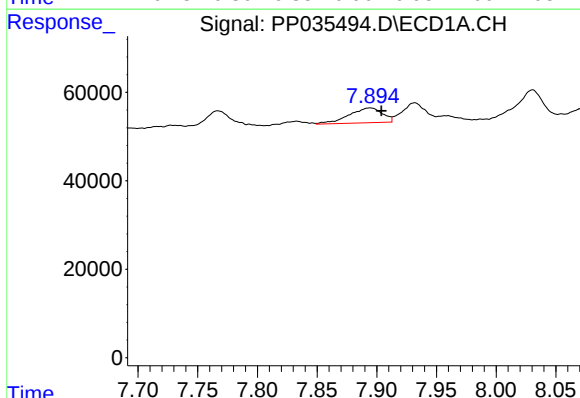


#29 AR-1254-4

R.T.: 7.894 min
Delta R.T.: -0.010 min
Response: 65370
Conc: 31.69 ng/ml

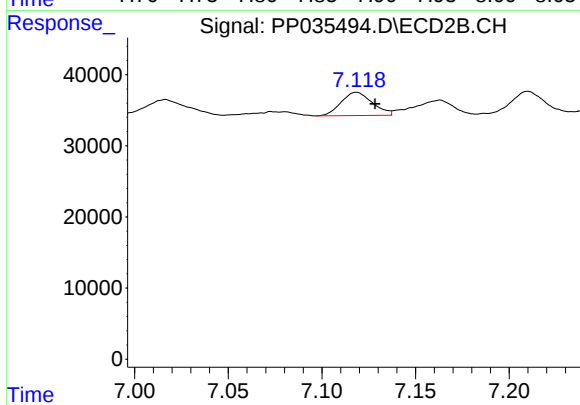

#29 AR-1254-4

R.T.: 7.118 min
Delta R.T.: -0.010 min
Response: 37904
Conc: 30.81 ng/ml

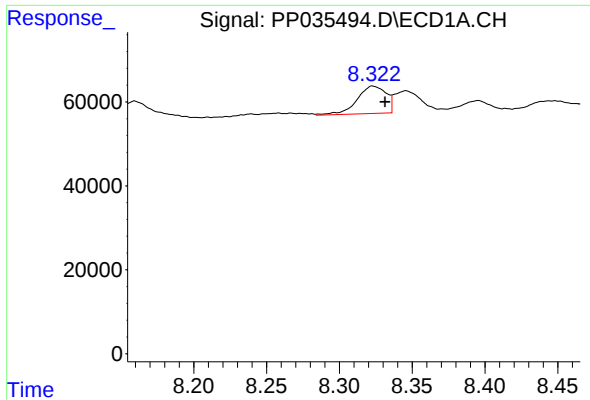


#30 AR-1254-5

R.T.: 8.323 min
Delta R.T.: -0.008 min
Response: 90955
Conc: 38.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
HA-61

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:30 AM

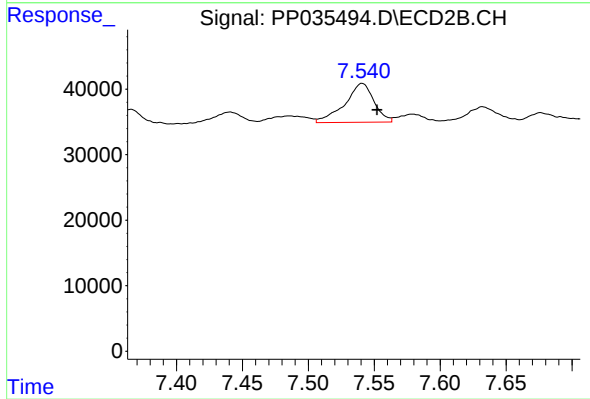

#30 AR-1254-5

R.T.: 7.541 min
Delta R.T.: -0.011 min
Response: 91271
Conc: 48.75 ng/ml