

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035497.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 12:48
 Operator : DD\AJ
 Sample : M2259-07 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC258873-1-1

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:31:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.209	67542	60259	1.330	1.770 #
2) SA Decachlor...	10.653	9.463	91279	35306	2.248	1.822m
Target Compounds						
26) L6 AR-1254-1	6.998	6.311	815704	691807	450.363	469.341
27) L6 AR-1254-2	7.226	6.468	1221364	516559	436.516	390.153
28) L6 AR-1254-3	7.606	6.886	1135393	729114	386.332	359.299
29) L6 AR-1254-4	7.900	7.121	937740	503182	454.615	409.037
30) L6 AR-1254-5	8.326	7.545	867289	592288	366.595	316.367

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035497.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 12:48
Operator : DD\AJ
Sample : M2259-07 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
BC258873-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:31:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

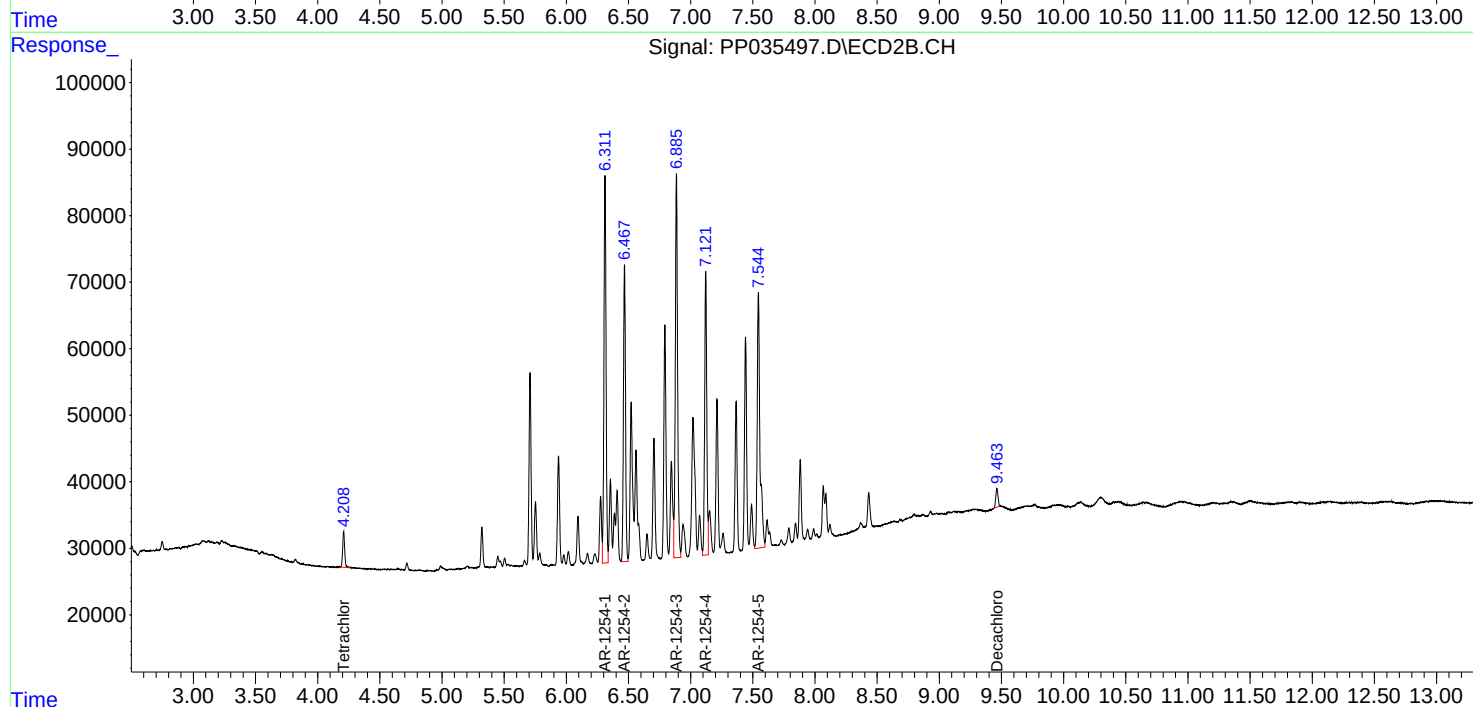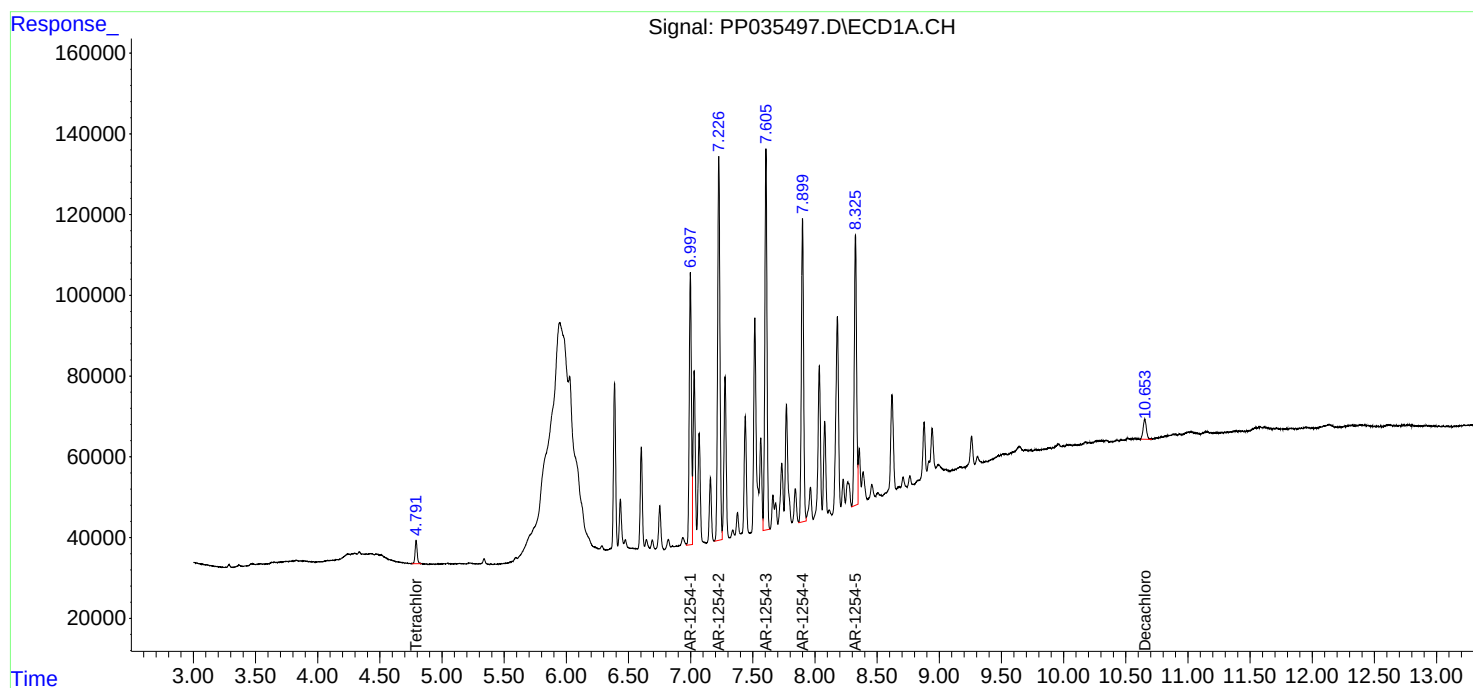

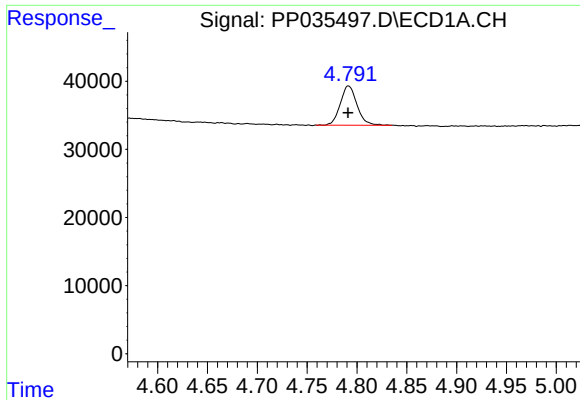


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 67542
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258873-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:47 AM

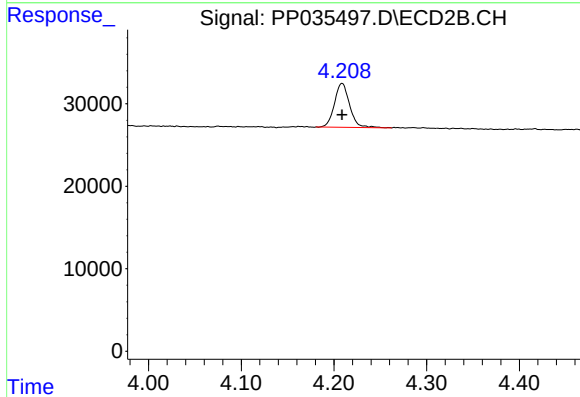


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 60259
Conc: 1.77 ng/ml

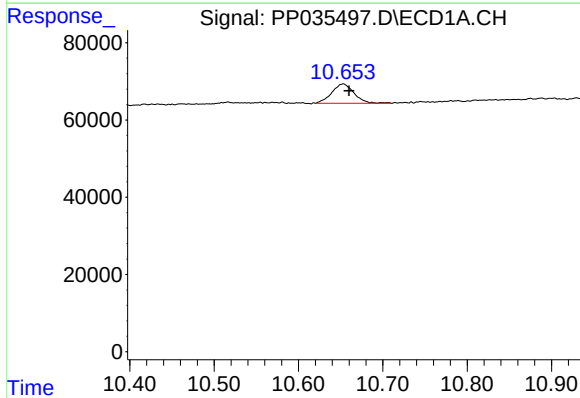


#2 Decachlorobiphenyl

R.T.: 10.653 min
Delta R.T.: -0.007 min
Response: 91279
Conc: 2.25 ng/ml

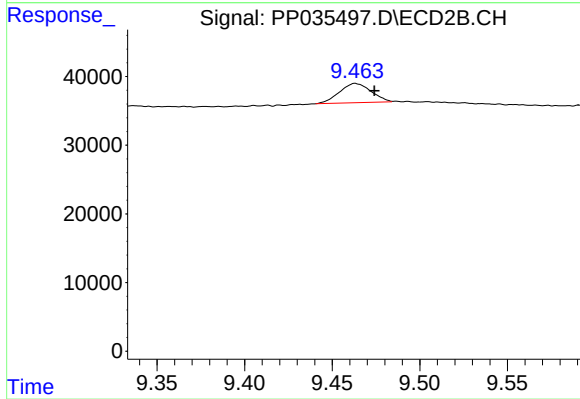

#2 Decachlorobiphenyl

R.T.: 9.463 min
Delta R.T.: -0.011 min
Response: 35306
Conc: 1.82 ng/ml m

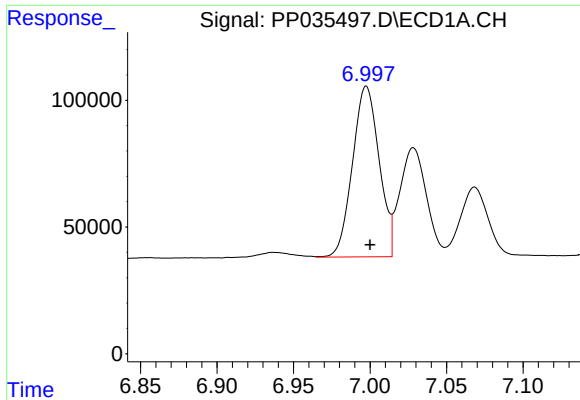


#26 AR-1254-1

R.T.: 6.998 min
Delta R.T.: -0.002 min
Response: 815704
Conc: 450.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258873-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:47 AM

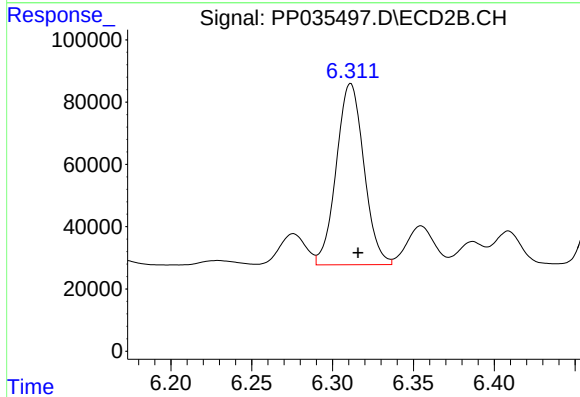


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 691807
Conc: 469.34 ng/ml

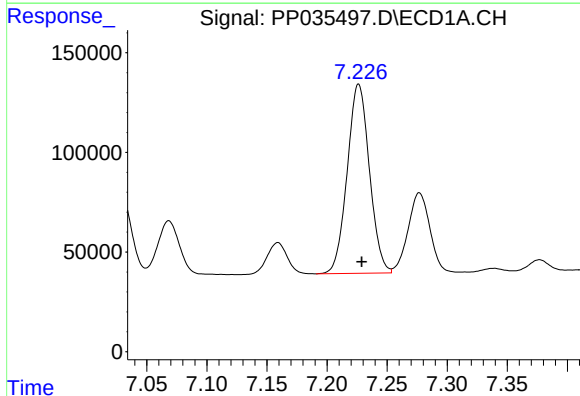


#27 AR-1254-2

R.T.: 7.226 min
Delta R.T.: -0.003 min
Response: 1221364
Conc: 436.52 ng/ml

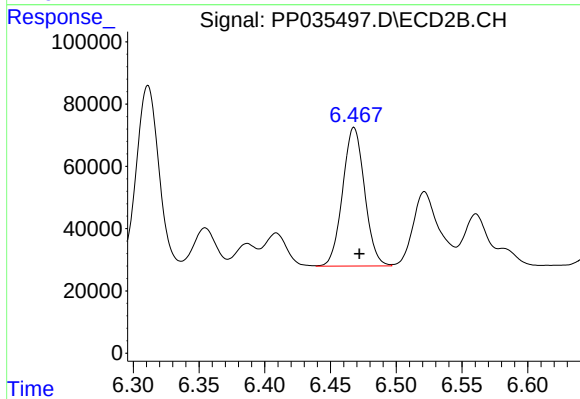

#27 AR-1254-2

R.T.: 6.468 min
Delta R.T.: -0.004 min
Response: 516559
Conc: 390.15 ng/ml

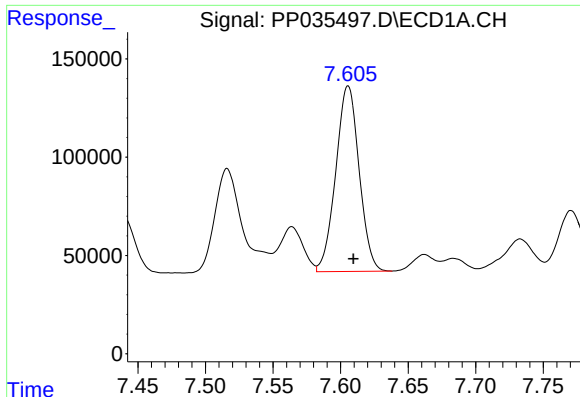


#28 AR-1254-3

R.T.: 7.606 min
Delta R.T.: -0.004 min
Response: 1135393
Conc: 386.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258873-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:47 AM

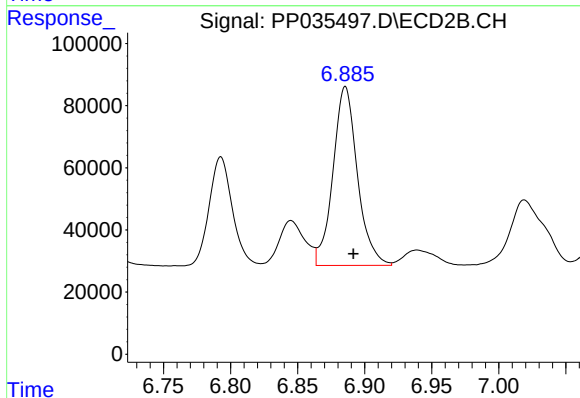


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 729114
Conc: 359.30 ng/ml

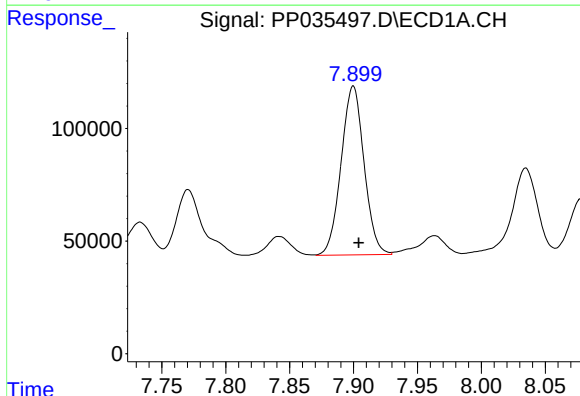


#29 AR-1254-4

R.T.: 7.900 min
Delta R.T.: -0.004 min
Response: 937740
Conc: 454.61 ng/ml

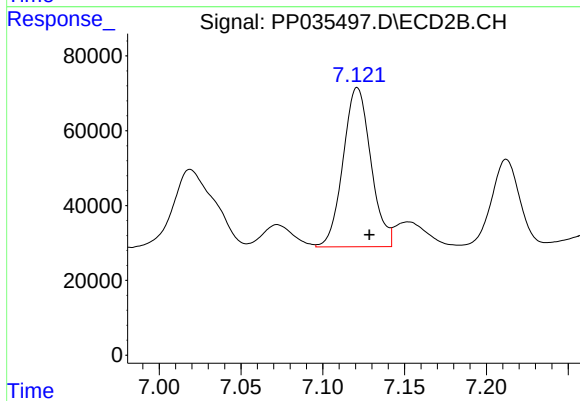

#29 AR-1254-4

R.T.: 7.121 min
Delta R.T.: -0.007 min
Response: 503182
Conc: 409.04 ng/ml

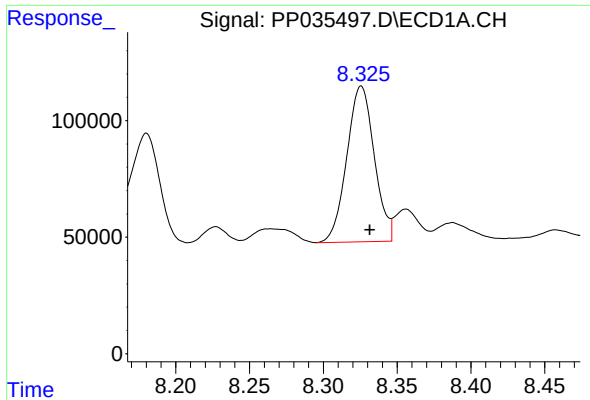


#30 AR-1254-5

R.T.: 8.326 min
Delta R.T.: -0.006 min
Response: 867289
Conc: 366.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258873-1-1

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:47 AM

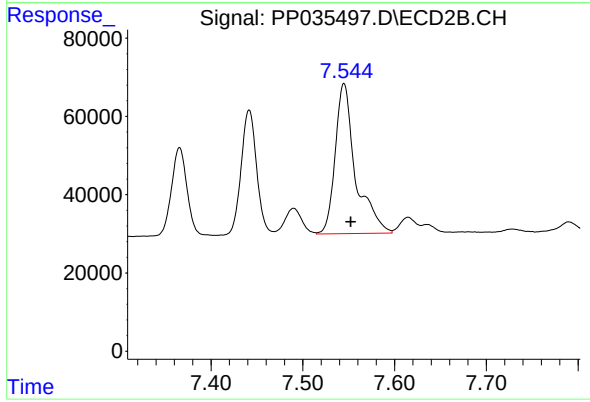

#30 AR-1254-5

R.T.: 7.545 min
Delta R.T.: -0.007 min
Response: 592288
Conc: 316.37 ng/ml