

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035499.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 13:22
 Operator : DD\AJ
 Sample : M2259-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BCZ58713-1-1

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:32:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	77170	72447	1.520	2.128 #
2) SA Decachlor...	10.651	9.460	75683	43361	1.864	2.238m
Target Compounds						
26) L6 AR-1254-1	6.997	6.310	16758	25281	9.253	17.151 #
27) L6 AR-1254-2	7.225	6.466	36928	21646	13.198	16.349
28) L6 AR-1254-3	7.605	6.884	41962	29927	14.278	14.748
29) L6 AR-1254-4	7.899	7.120	31819	20760	15.426	16.876
30) L6 AR-1254-5	8.325	7.544	32532	25656	13.751	13.704

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035499.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 13:22
Operator : DD\AJ
Sample : M2259-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:32:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

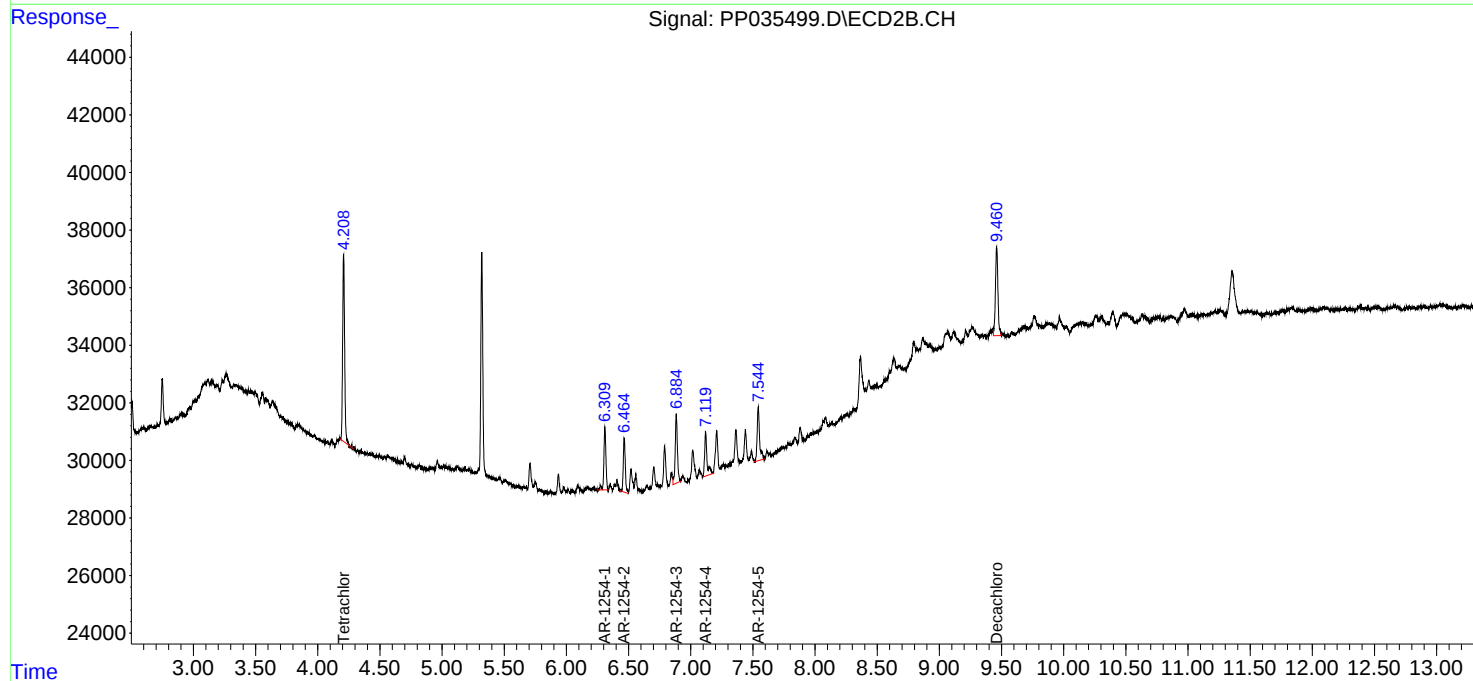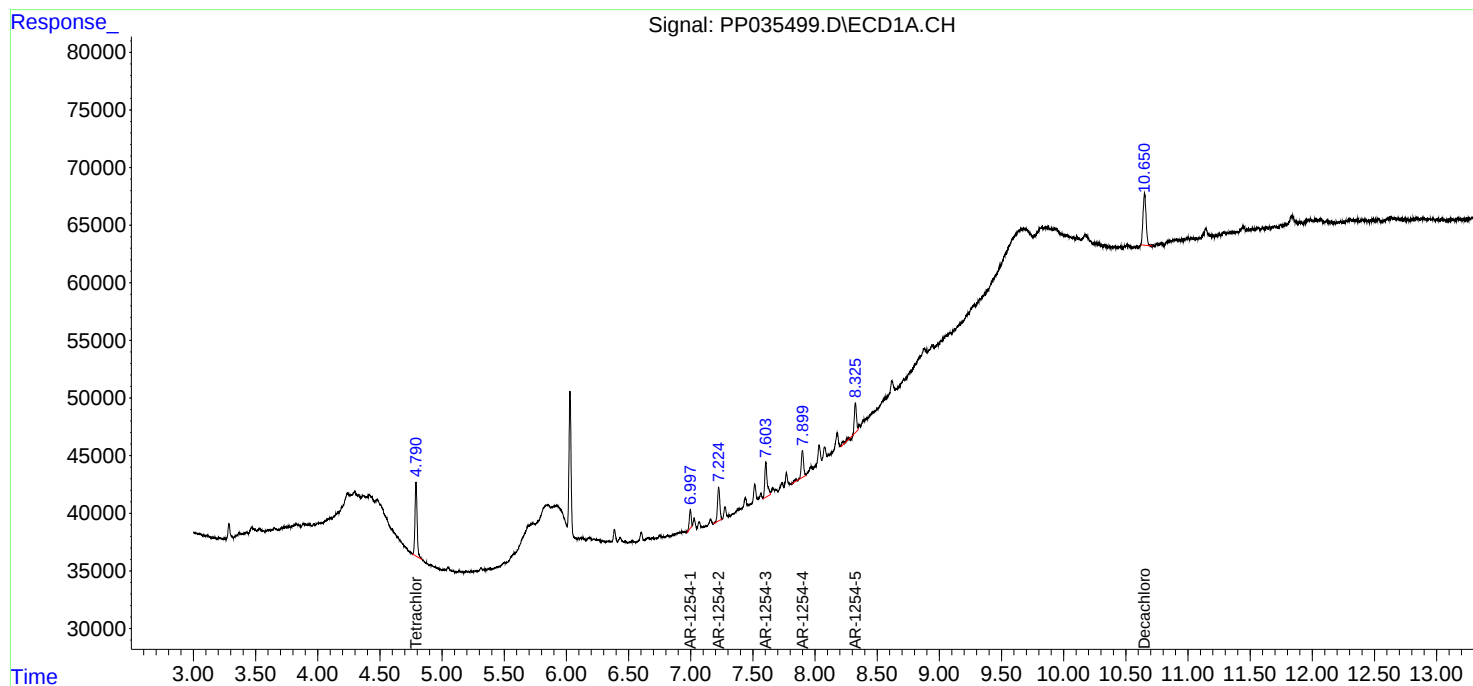

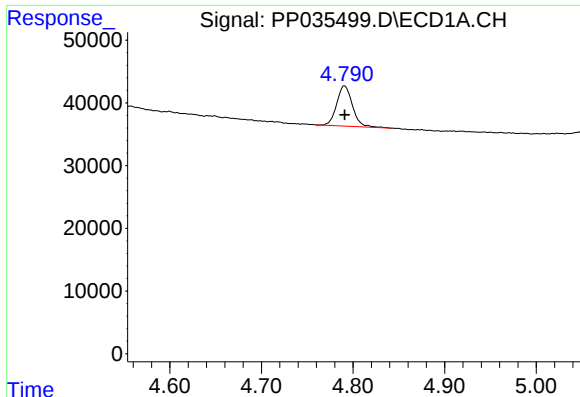


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 77170
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:51 AM

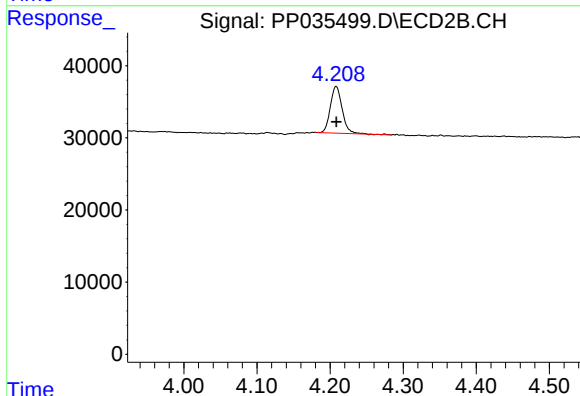


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 72447
Conc: 2.13 ng/ml

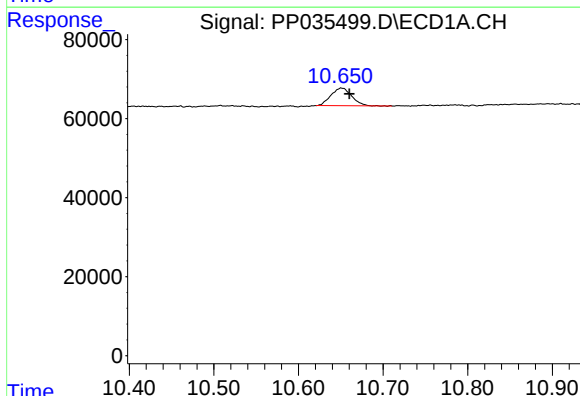


#2 Decachlorobiphenyl

R.T.: 10.651 min
Delta R.T.: -0.009 min
Response: 75683
Conc: 1.86 ng/ml

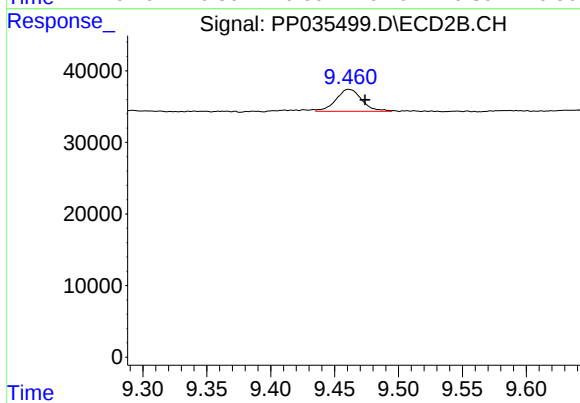

#2 Decachlorobiphenyl

R.T.: 9.460 min
Delta R.T.: -0.014 min
Response: 43361
Conc: 2.24 ng/ml m

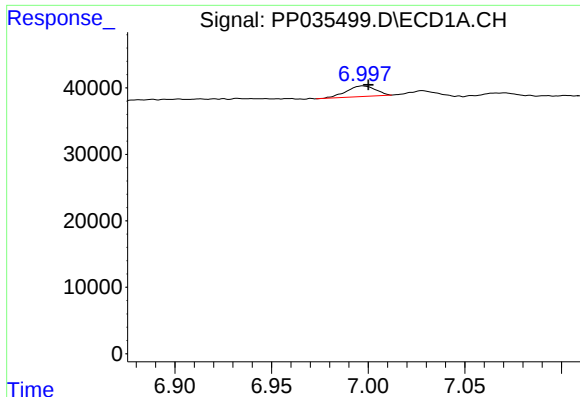


#26 AR-1254-1

R.T.: 6.997 min
Delta R.T.: -0.003 min
Response: 16758
Conc: 9.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:51 AM

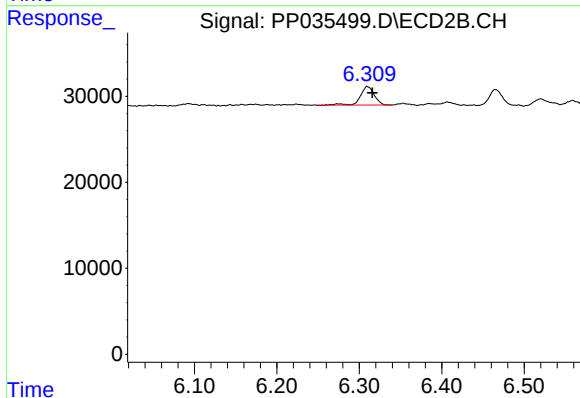


#26 AR-1254-1

R.T.: 6.310 min
Delta R.T.: -0.006 min
Response: 25281
Conc: 17.15 ng/ml

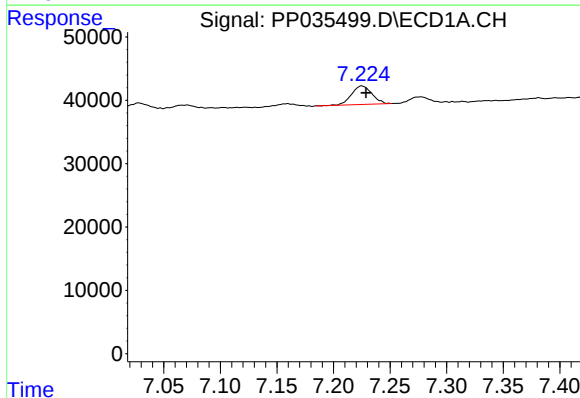


#27 AR-1254-2

R.T.: 7.225 min
Delta R.T.: -0.004 min
Response: 36928
Conc: 13.20 ng/ml

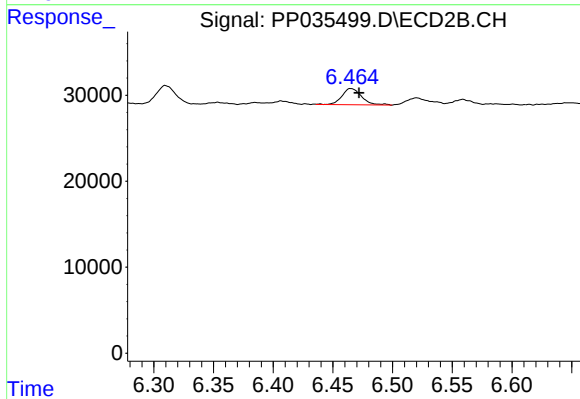

#27 AR-1254-2

R.T.: 6.466 min
Delta R.T.: -0.006 min
Response: 21646
Conc: 16.35 ng/ml

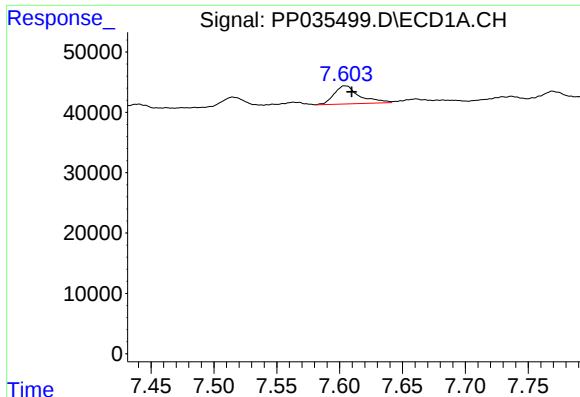


#28 AR-1254-3

R.T.: 7.605 min
Delta R.T.: -0.005 min
Response: 41962
Conc: 14.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:51 AM

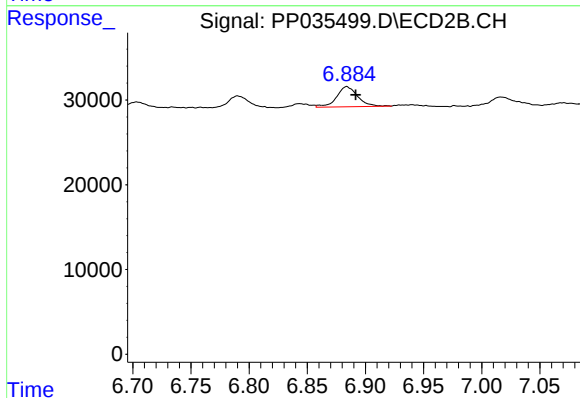


#28 AR-1254-3

R.T.: 6.884 min
Delta R.T.: -0.007 min
Response: 29927
Conc: 14.75 ng/ml

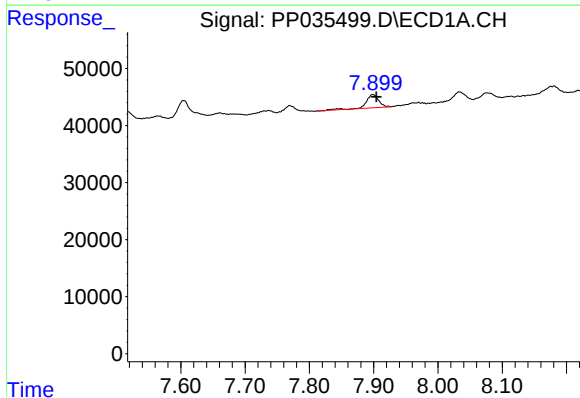


#29 AR-1254-4

R.T.: 7.899 min
Delta R.T.: -0.005 min
Response: 31819
Conc: 15.43 ng/ml

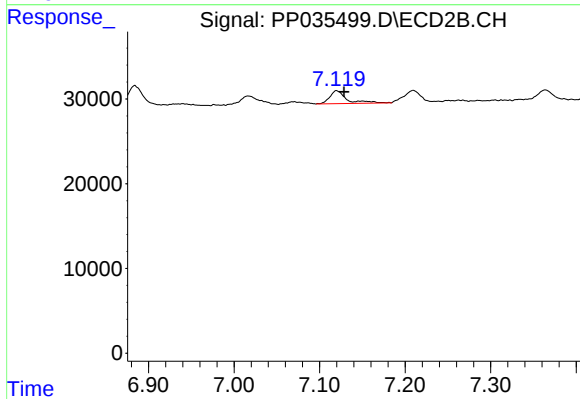

#29 AR-1254-4

R.T.: 7.120 min
Delta R.T.: -0.008 min
Response: 20760
Conc: 16.88 ng/ml

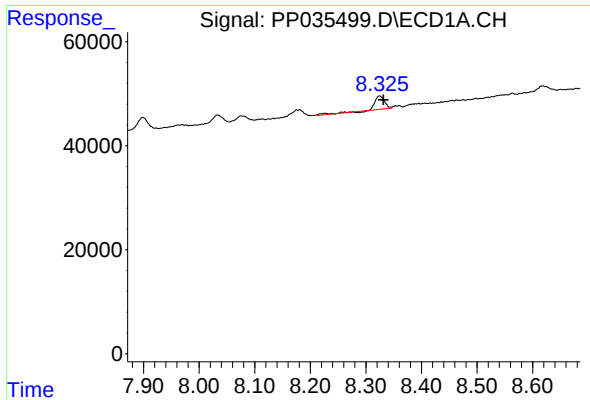


#30 AR-1254-5

R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 32532
Conc: 13.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:51 AM

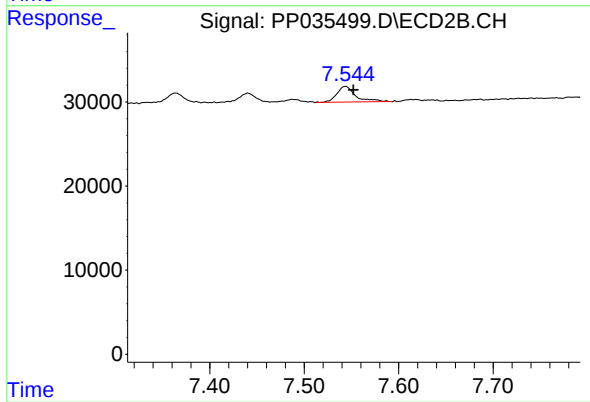

#30 AR-1254-5

R.T.: 7.544 min
Delta R.T.: -0.009 min
Response: 25656
Conc: 13.70 ng/ml