

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035500.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 13:56
 Operator : DD\AJ
 Sample : M2259-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BCZ58713-1-2

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 15:02:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.208	902867	650801	17.782	19.116
2) SA Decachlor...	10.654	9.469	849102	388445	20.909m	20.046
Target Compounds						
26) L6 AR-1254-1	6.996	6.311	278134	244229	153.562	165.692
27) L6 AR-1254-2	7.226	6.467	454042	200020	162.275	151.073
28) L6 AR-1254-3	7.604	6.885	451709	304448	153.700	150.029
29) L6 AR-1254-4	7.899	7.120	336762	187851	163.262	152.704
30) L6 AR-1254-5	8.325	7.545	363900	247121	153.817	131.998

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035500.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 13:56
Operator : DD\AJ
Sample : M2259-04
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
BCZ58713-1-2


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 15:02:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

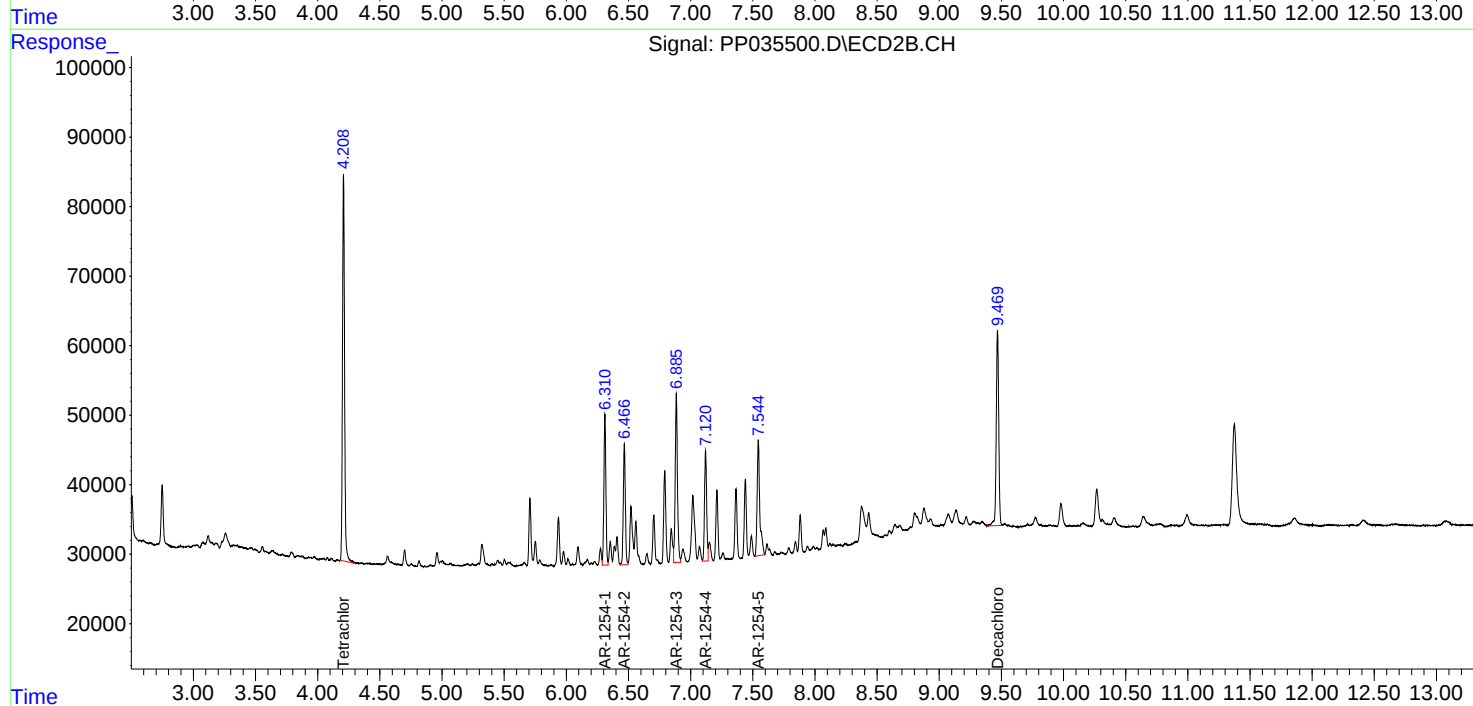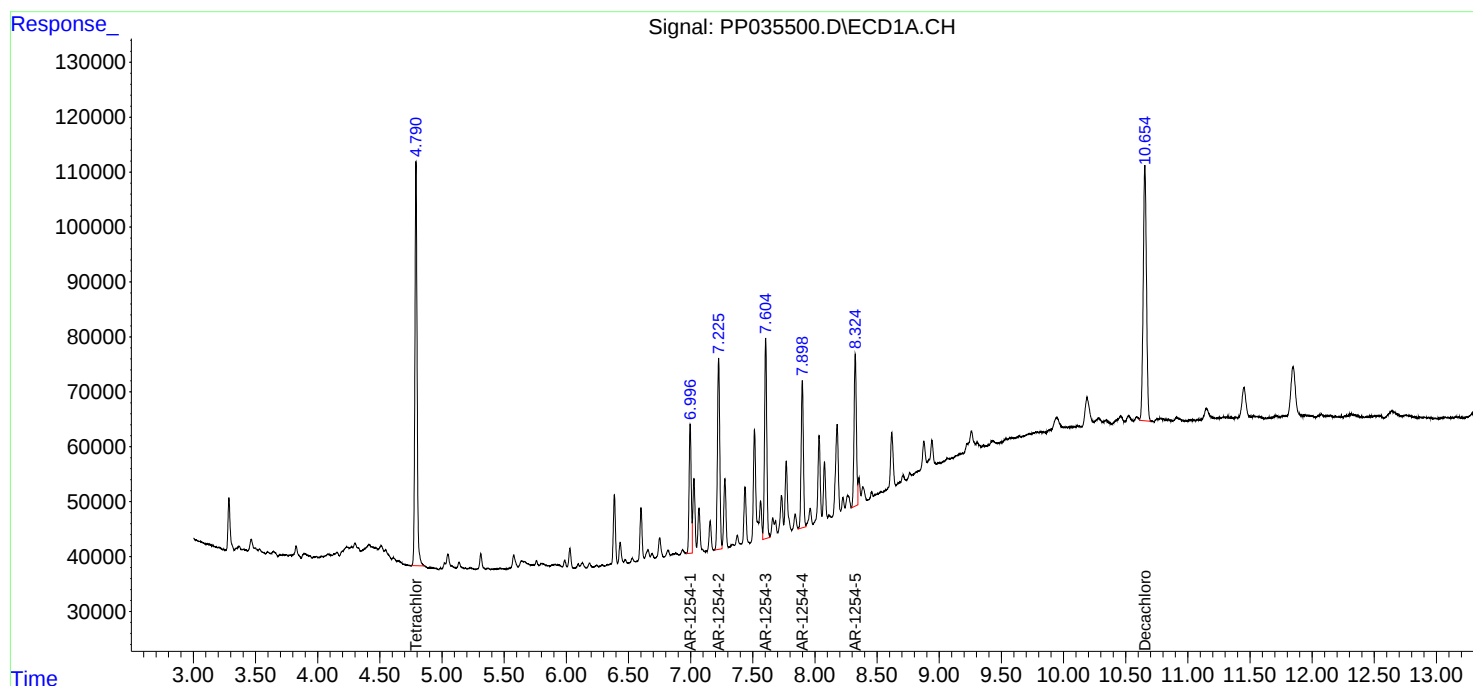

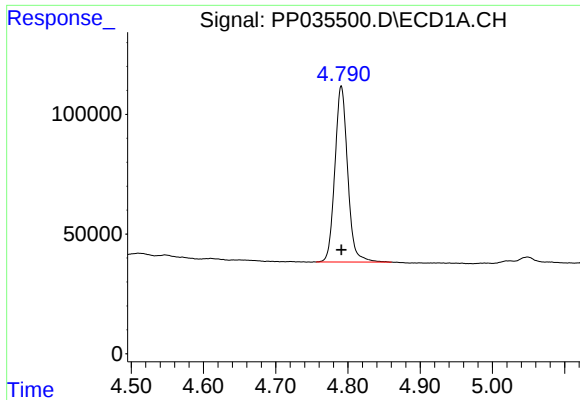


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 902867
Conc: 17.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-2


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:53 AM

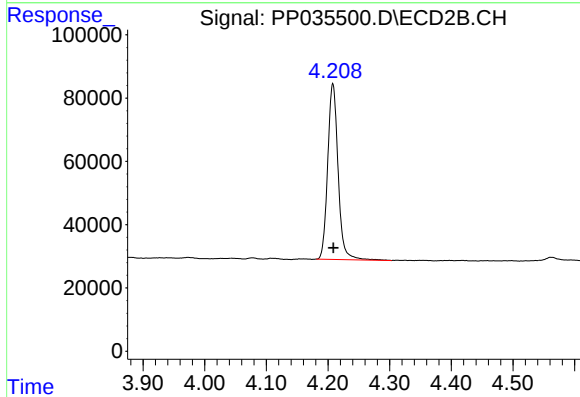


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 650801
Conc: 19.12 ng/ml

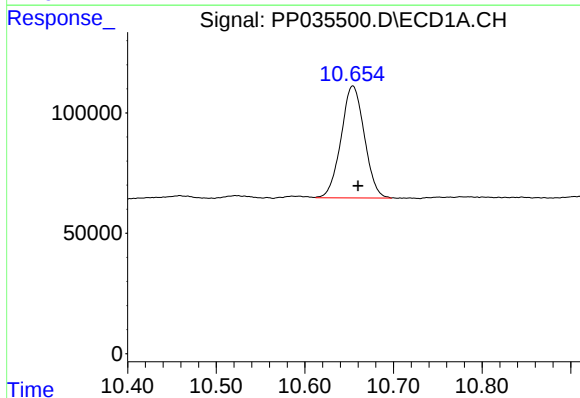


#2 Decachlorobiphenyl

R.T.: 10.654 min
Delta R.T.: -0.006 min
Response: 849102
Conc: 20.91 ng/ml m

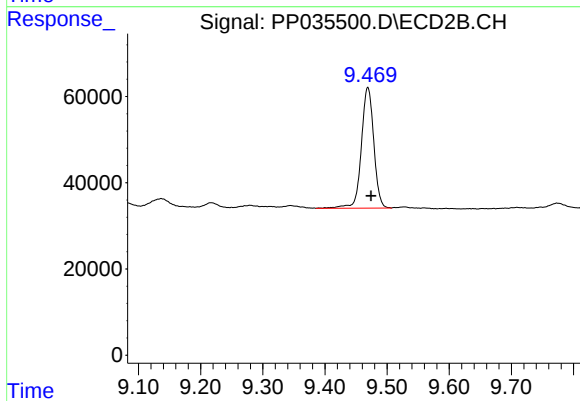

#2 Decachlorobiphenyl

R.T.: 9.469 min
Delta R.T.: -0.005 min
Response: 388445
Conc: 20.05 ng/ml

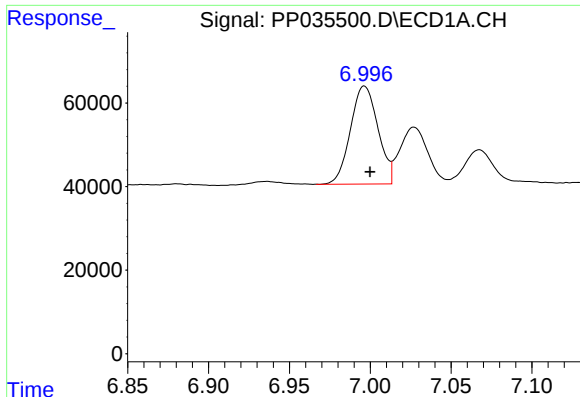


#26 AR-1254-1

R.T.: 6.996 min
Delta R.T.: -0.004 min
Response: 278134
Conc: 153.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-2


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:53 AM

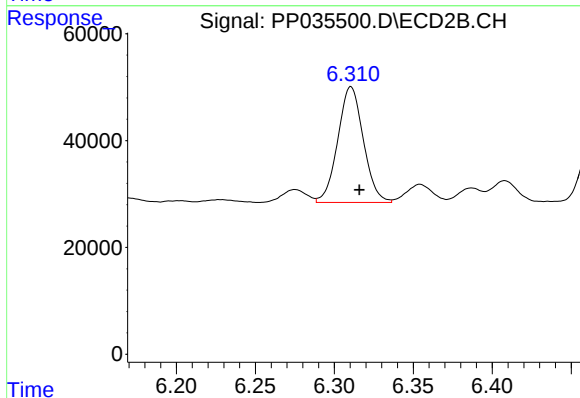


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 244229
Conc: 165.69 ng/ml

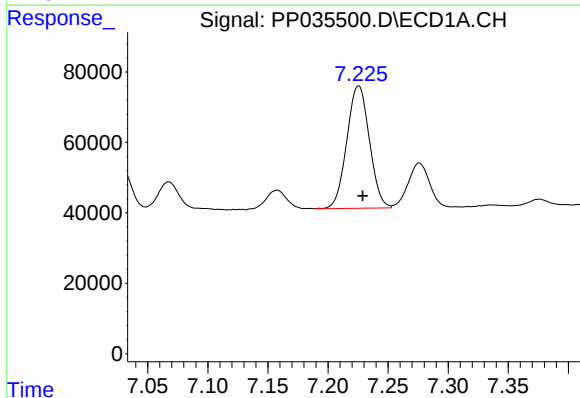


#27 AR-1254-2

R.T.: 7.226 min
Delta R.T.: -0.003 min
Response: 454042
Conc: 162.27 ng/ml

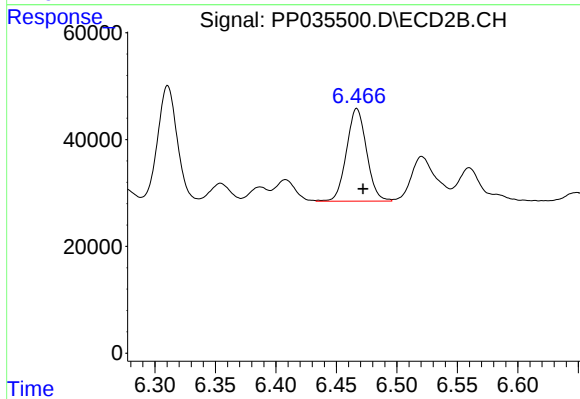

#27 AR-1254-2

R.T.: 6.467 min
Delta R.T.: -0.005 min
Response: 200020
Conc: 151.07 ng/ml

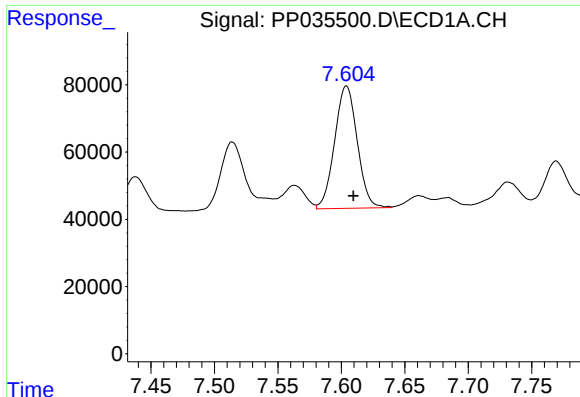


#28 AR-1254-3

R.T.: 7.604 min
Delta R.T.: -0.006 min
Response: 451709
Conc: 153.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-2


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:53 AM

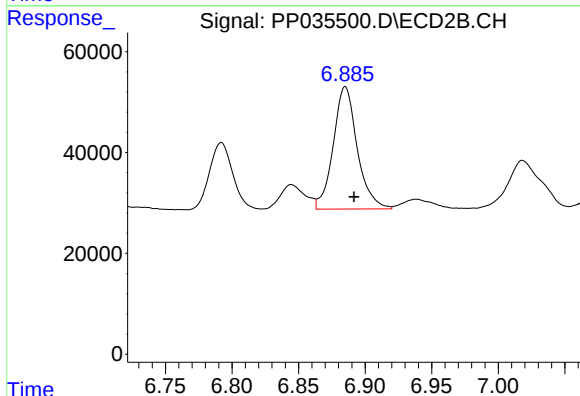


#28 AR-1254-3

R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 304448
Conc: 150.03 ng/ml

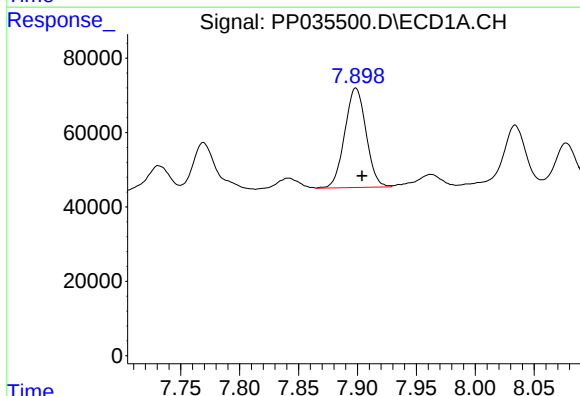


#29 AR-1254-4

R.T.: 7.899 min
Delta R.T.: -0.005 min
Response: 336762
Conc: 163.26 ng/ml

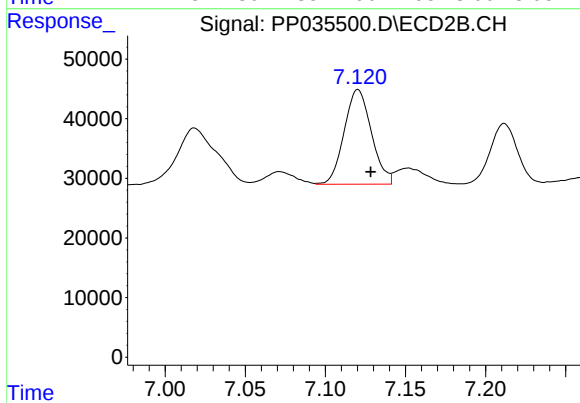

#29 AR-1254-4

R.T.: 7.120 min
Delta R.T.: -0.008 min
Response: 187851
Conc: 152.70 ng/ml

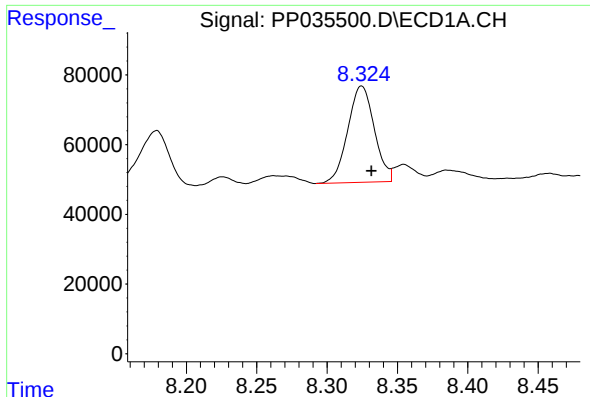


#30 AR-1254-5

R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 363900
Conc: 153.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-2

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:53 AM

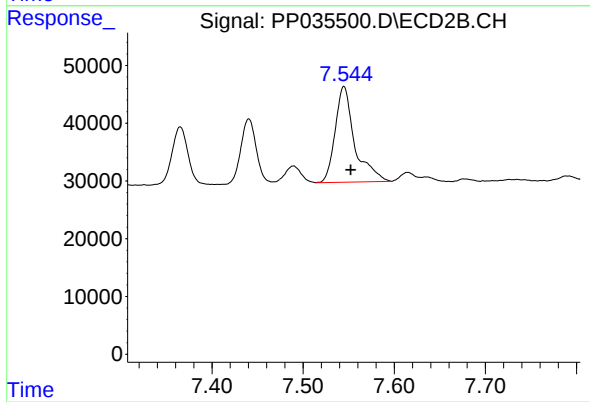

#30 AR-1254-5

R.T.: 7.545 min
Delta R.T.: -0.007 min
Response: 247121
Conc: 132.00 ng/ml