

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035502.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2021 14:29
 Operator : DD\AJ
 Sample : M2259-03 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BCZ58713-1-1

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:40:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 15:03:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.791	4.208	361950	299230	7.129	8.789
2) SA Decachlor...	10.653	9.465	404369	179479	9.957m	9.262m
Target Compounds						
26) L6 AR-1254-1	6.997	6.311	99205	99057	54.772	67.203
27) L6 AR-1254-2	7.225	6.466	181345	84963	64.813	64.172
28) L6 AR-1254-3	7.605	6.885	188744	123396	64.223	60.808
29) L6 AR-1254-4	7.898	7.121	155590	76266	75.430m	61.997
30) L6 AR-1254-5	8.325	7.544	162856	122028	68.838	65.180

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2021 14:29
Operator : DD\AJ
Sample : M2259-03 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 15:03:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

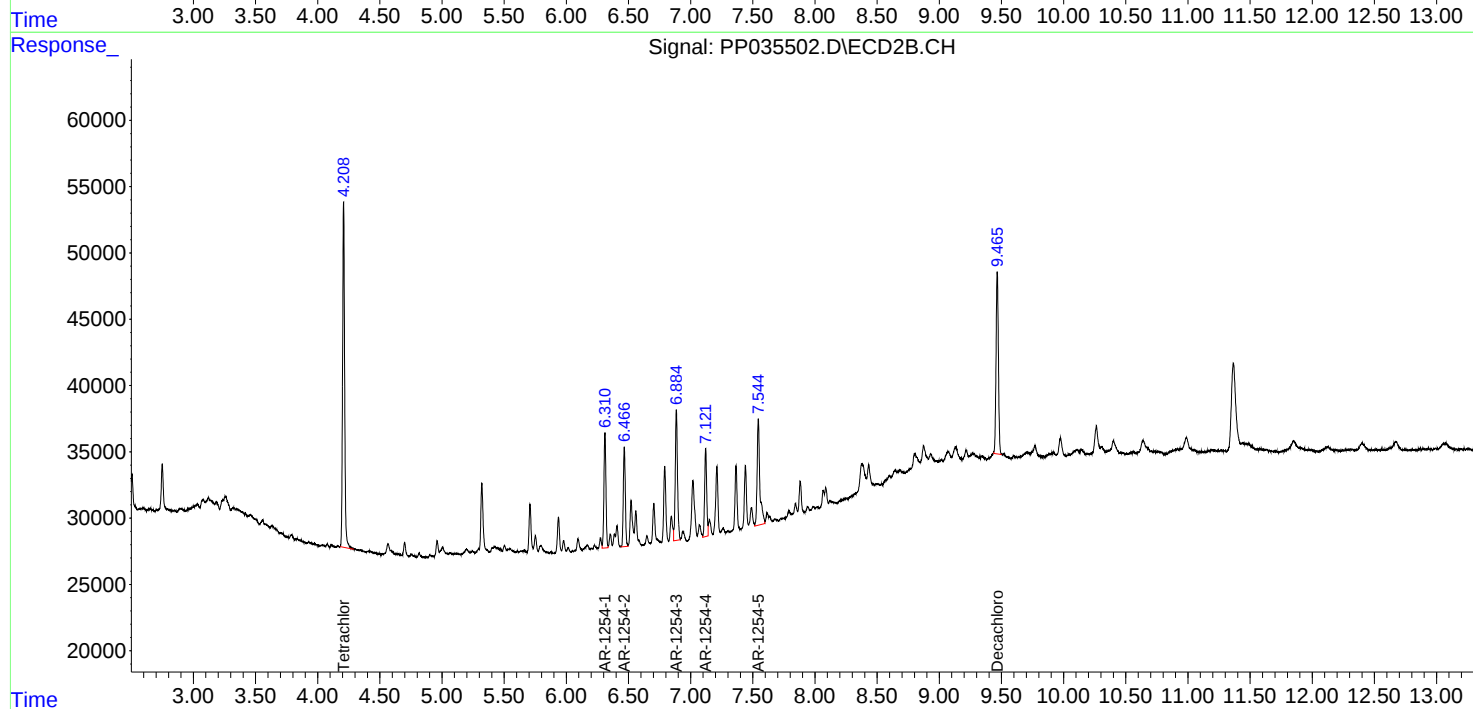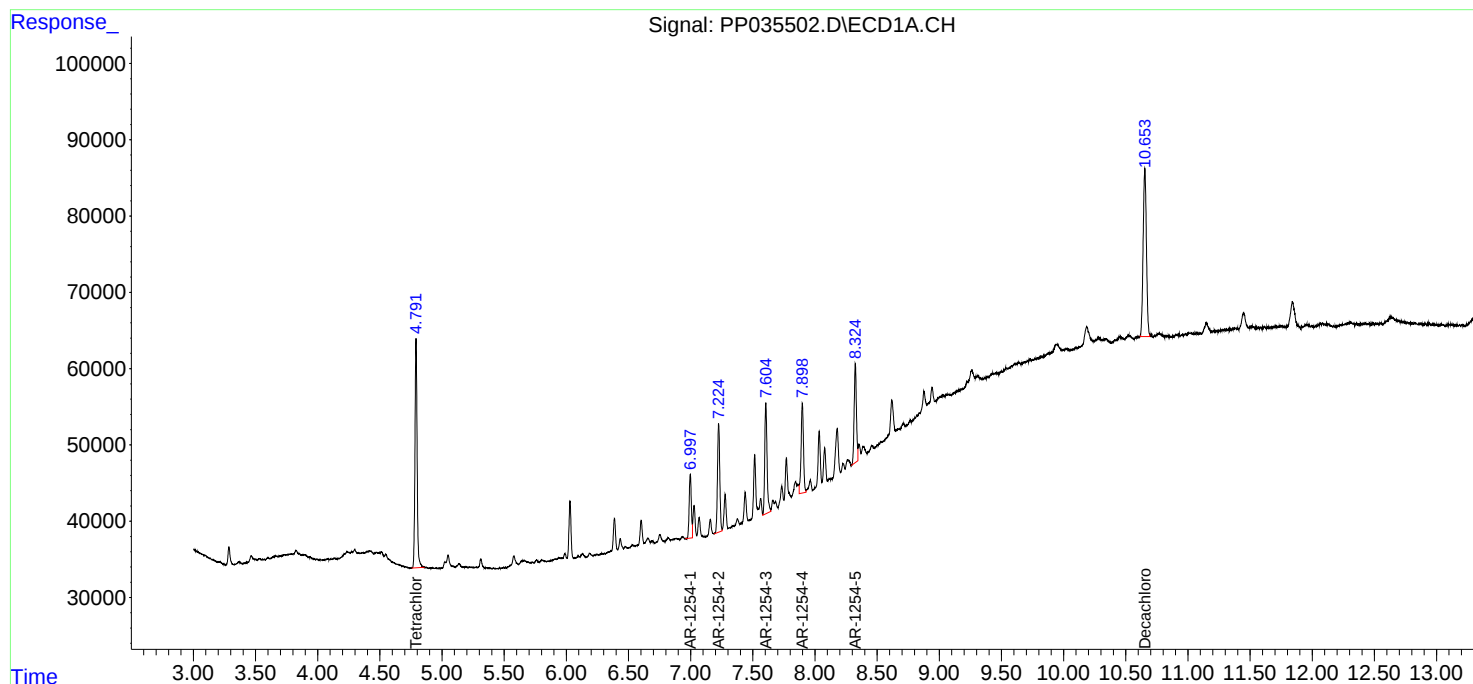

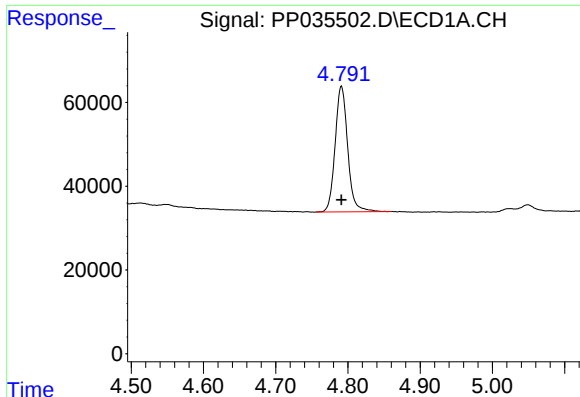


#1 Tetrachloro-m-xylene

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 361950
Conc: 7.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:55 AM

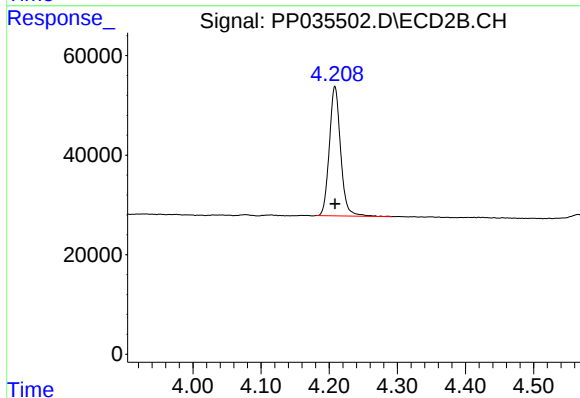


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 299230
Conc: 8.79 ng/ml

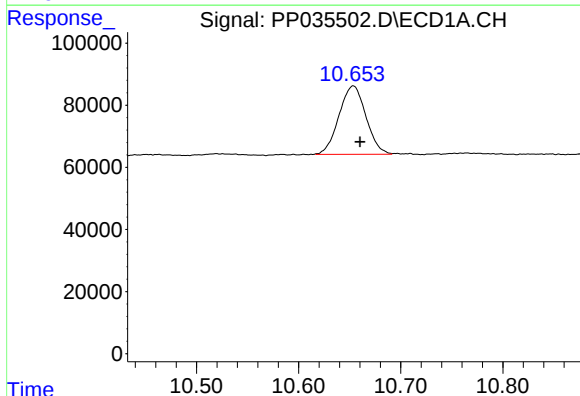


#2 Decachlorobiphenyl

R.T.: 10.653 min
Delta R.T.: -0.007 min
Response: 404369
Conc: 9.96 ng/ml m

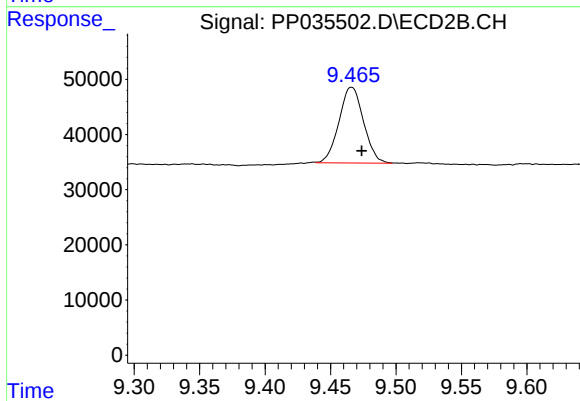

#2 Decachlorobiphenyl

R.T.: 9.465 min
Delta R.T.: -0.009 min
Response: 179479
Conc: 9.26 ng/ml m

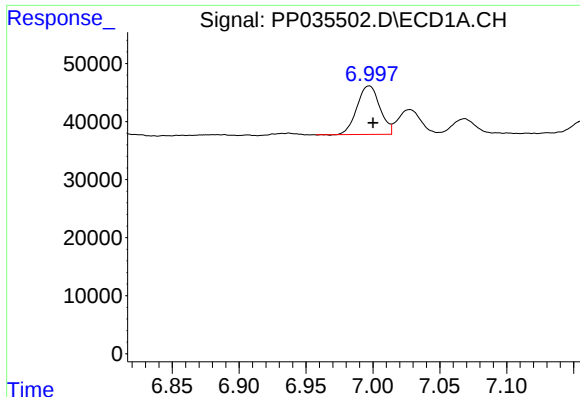


#26 AR-1254-1

R.T.: 6.997 min
Delta R.T.: -0.003 min
Response: 99205
Conc: 54.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:55 AM

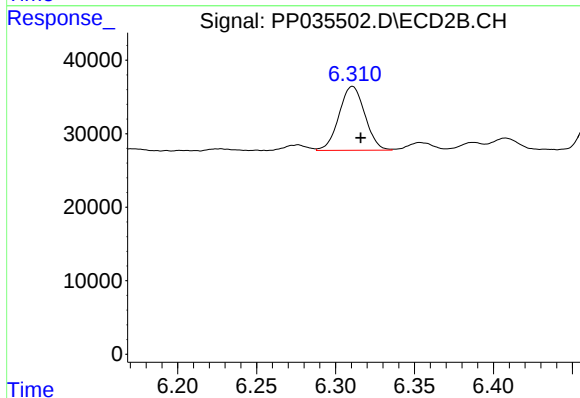


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 99057
Conc: 67.20 ng/ml

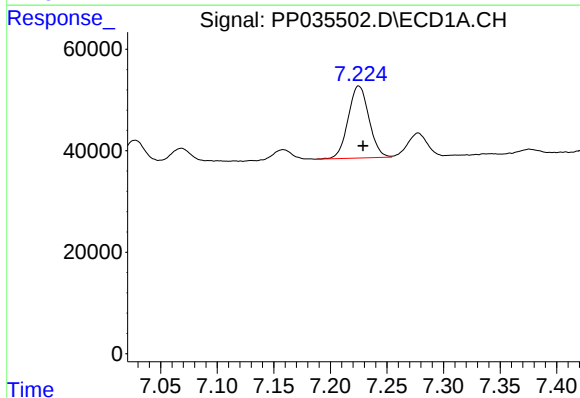


#27 AR-1254-2

R.T.: 7.225 min
Delta R.T.: -0.004 min
Response: 181345
Conc: 64.81 ng/ml

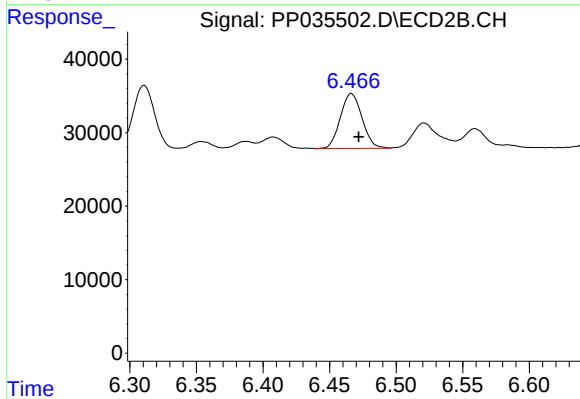

#27 AR-1254-2

R.T.: 6.466 min
Delta R.T.: -0.006 min
Response: 84963
Conc: 64.17 ng/ml

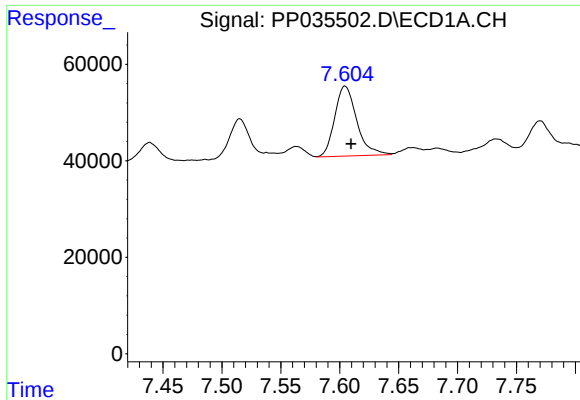


#28 AR-1254-3

R.T.: 7.605 min
Delta R.T.: -0.005 min
Response: 188744
Conc: 64.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1


Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:55 AM

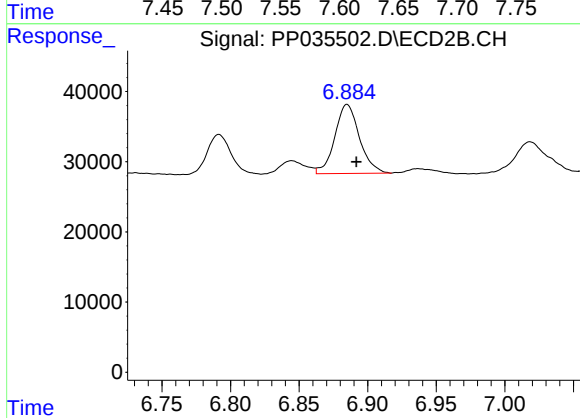


#28 AR-1254-3

R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 123396
Conc: 60.81 ng/ml

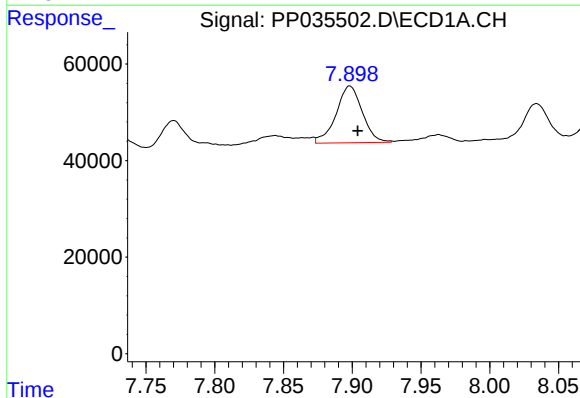


#29 AR-1254-4

R.T.: 7.898 min
Delta R.T.: -0.006 min
Response: 155590
Conc: 75.43 ng/ml m

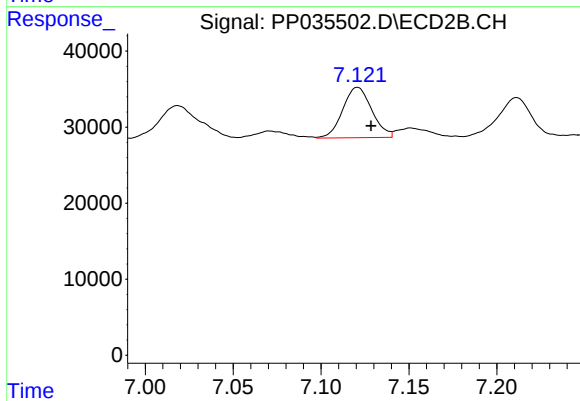

#29 AR-1254-4

R.T.: 7.121 min
Delta R.T.: -0.008 min
Response: 76266
Conc: 62.00 ng/ml

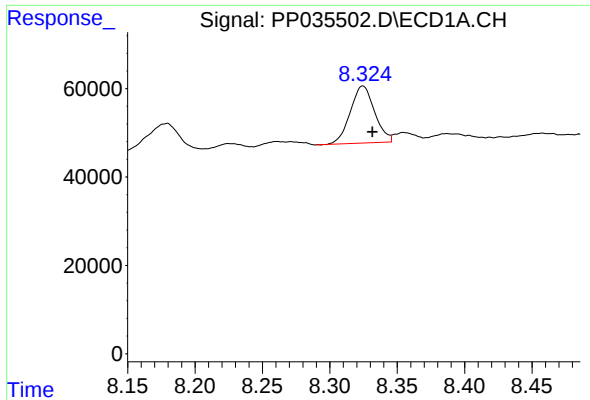


#30 AR-1254-5

R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 162856
Conc: 68.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
BCZ58713-1-1

Manual Integrations
APPROVED

Ankita
5/5/2021 10:40:55 AM

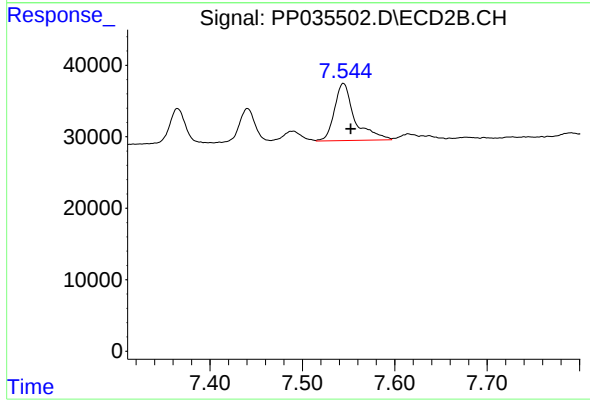

#30 AR-1254-5

R.T.: 7.544 min
Delta R.T.: -0.008 min
Response: 122028
Conc: 65.18 ng/ml