

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
 Data File : PP035529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 1:31
 Operator : DD\AJ
 Sample : M2273-16 20X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HED160B-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 05:17:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.788	4.206	45483	41637	0.896	1.223 #
2) SA Decachlor...	10.643f	9.460	64924	21573	1.599	1.113 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050421\
Data File : PP035529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 1:31
Operator : DD\AJ
Sample : M2273-16 20X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HED160B-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 05:17:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

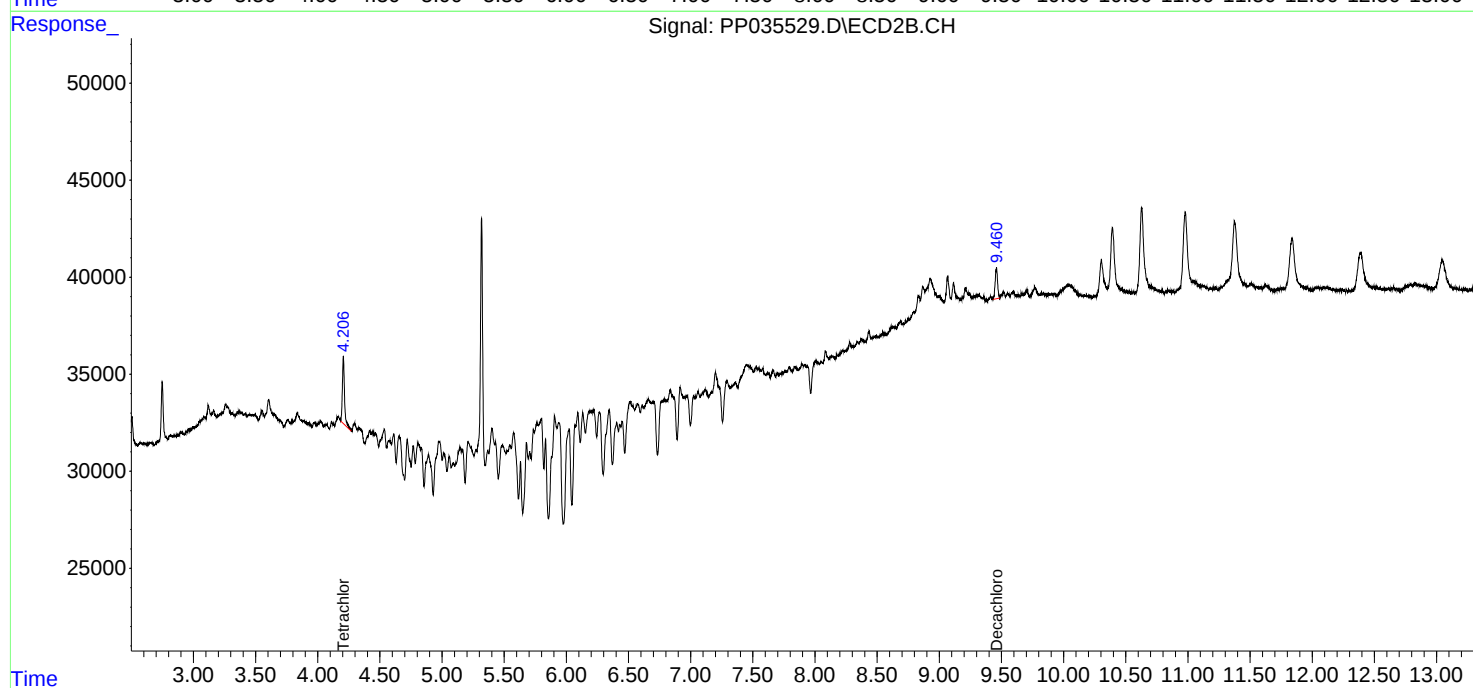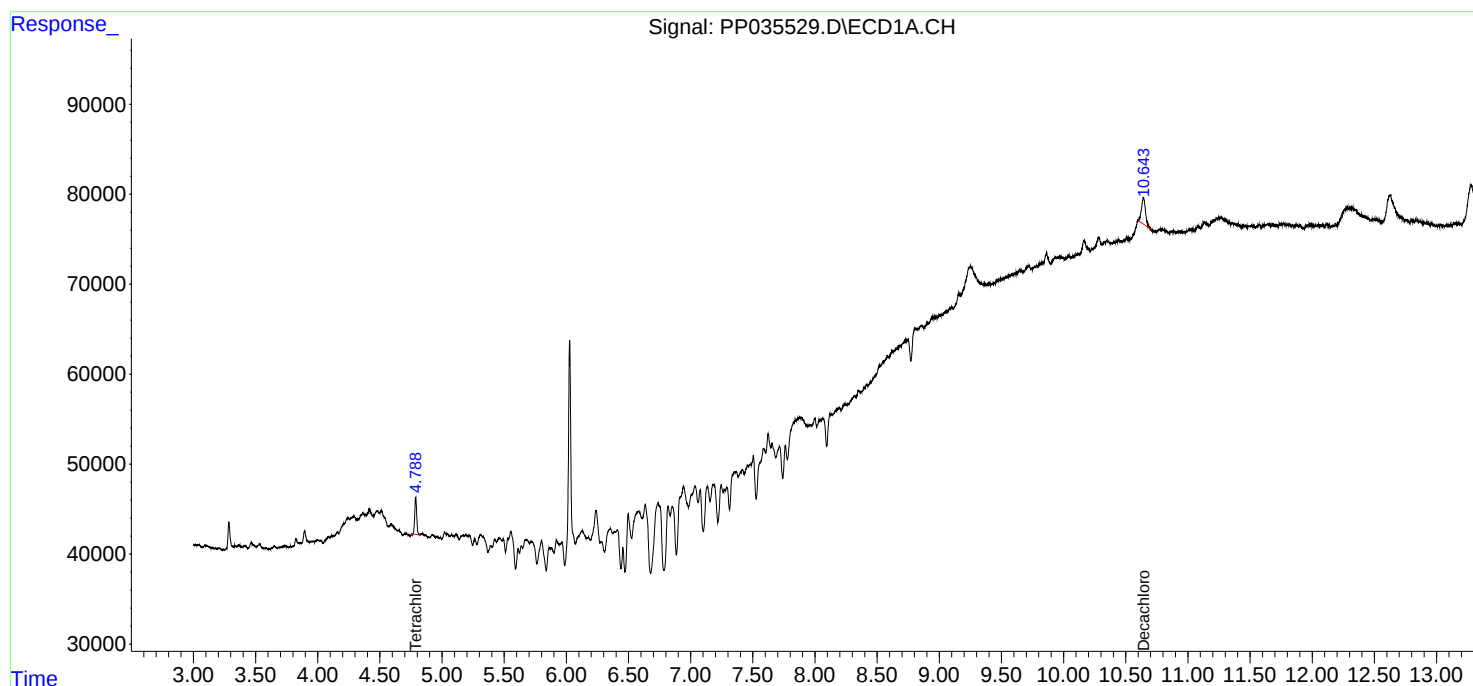


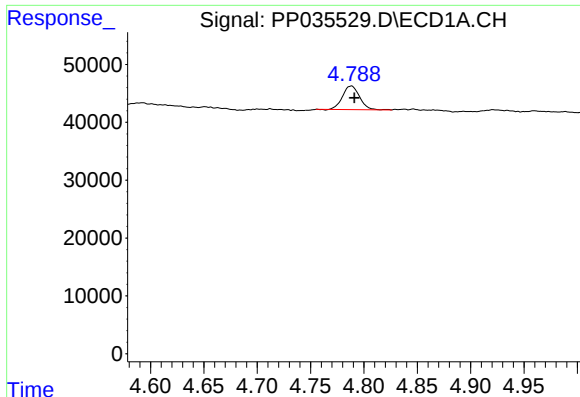

#1 Tetrachloro-m-xylene


R.T.: 4.788 min
Delta R.T.: -0.003 min
Response: 45483
Conc: 0.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
HED160B-1-2

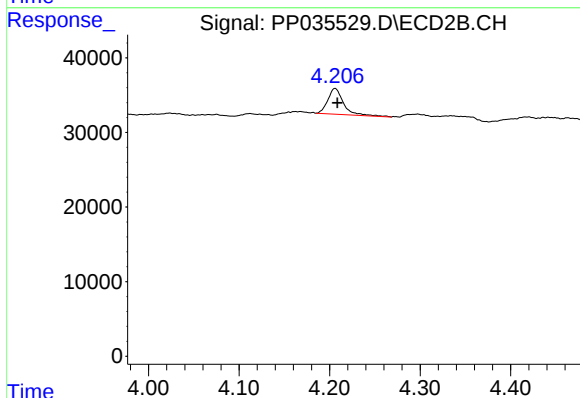


#1 Tetrachloro-m-xylene

R.T.: 4.206 min
Delta R.T.: -0.003 min
Response: 41637
Conc: 1.22 ng/ml

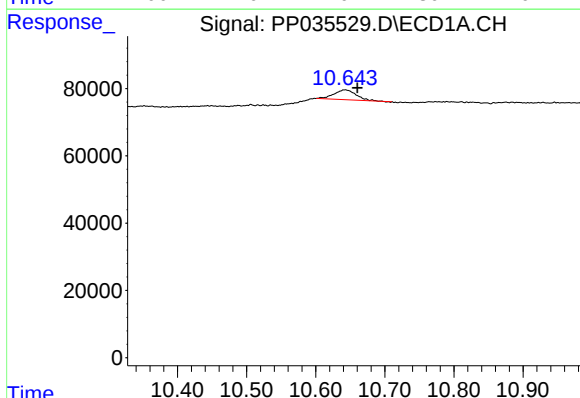

#2 Decachlorobiphenyl

R.T.: 10.643 min
Delta R.T.: -0.017 min
Response: 64924
Conc: 1.60 ng/ml

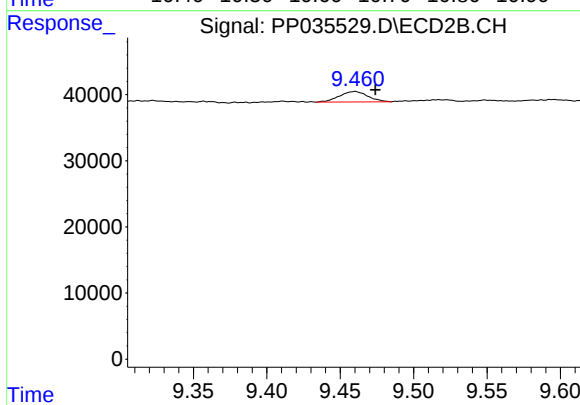

#2 Decachlorobiphenyl

R.T.: 9.460 min
Delta R.T.: -0.014 min
Response: 21573
Conc: 1.11 ng/ml