

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050422\
 Data File : PP047000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 19:11
 Operator : YP\AJ
 Sample : N2651-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-55-05-02-22-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2022
 Supervised By :mohammad ahmed 05/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 06:11:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 03 11:45:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.857	3.123	4055609	6707144	1.680	2.045
2) SA Decachlor...	9.928	8.434	3465625	5197059	2.355	2.179m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050422\
Data File : PP047000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 19:11
Operator : YP\AJ
Sample : N2651-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CL-55-05-02-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2022
Supervised By :mohammad ahmed 05/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 06:11:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 03 11:45:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

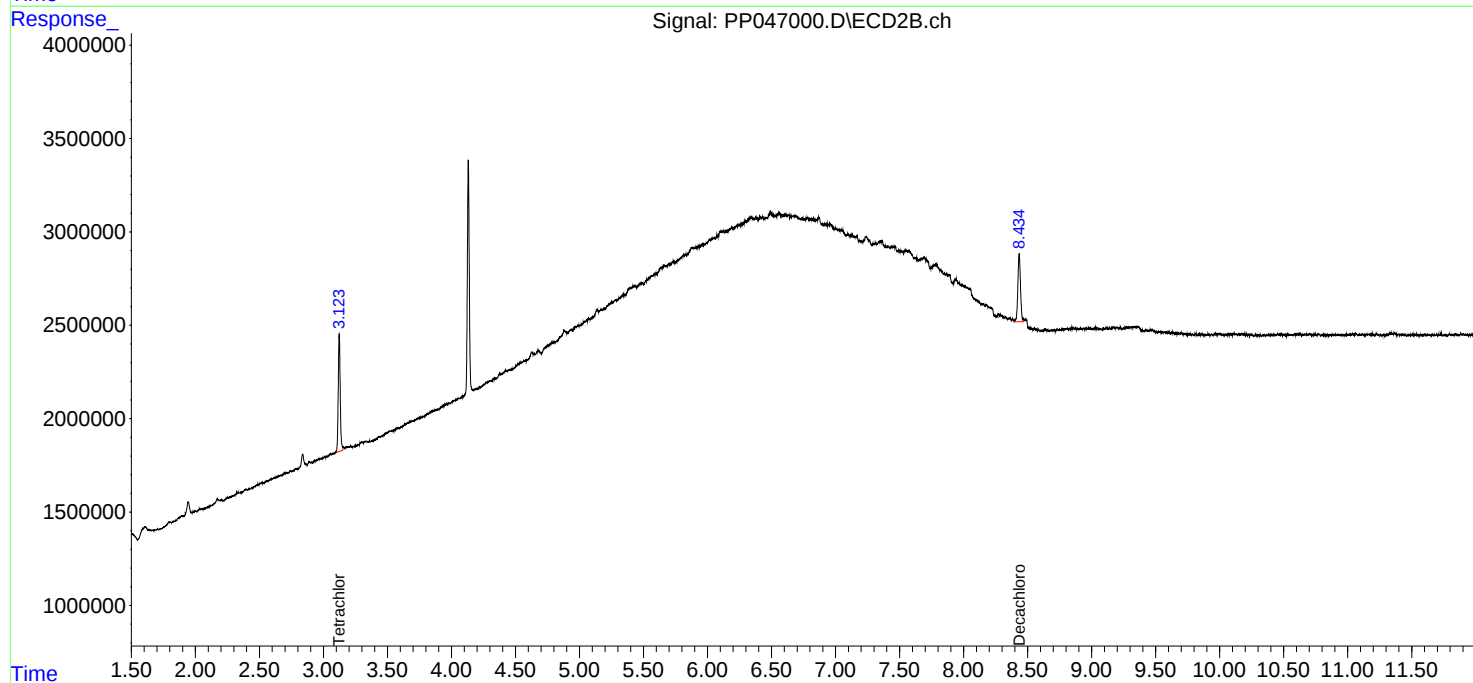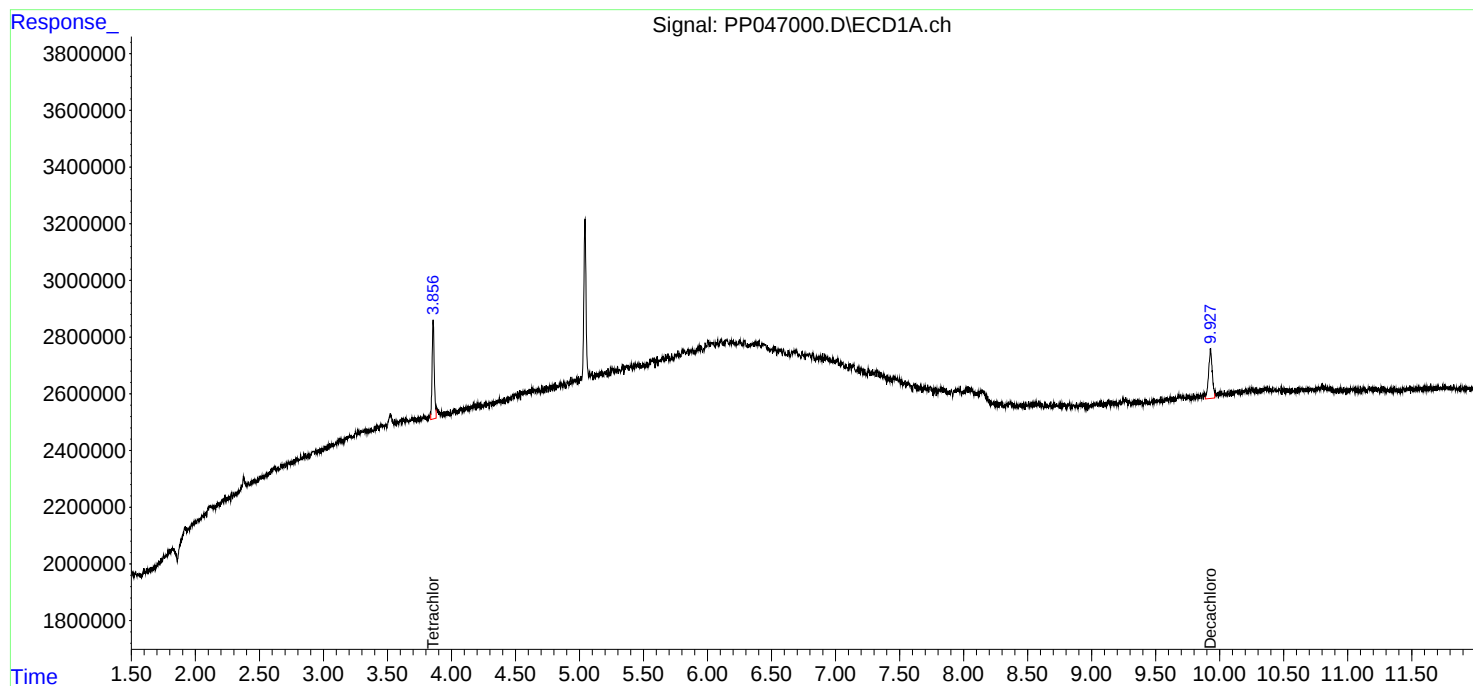

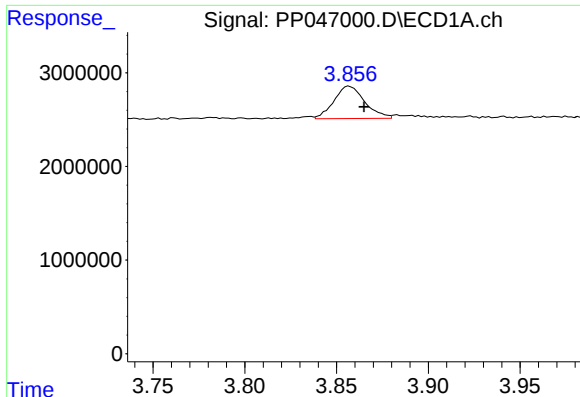


#1 Tetrachloro-m-xylene

R.T.: 3.857 min
Delta R.T.: -0.008 min
Response: 4055609
Conc: 1.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-55-05-02-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2022
Supervised By :mohammad ahmed 05/05/2022

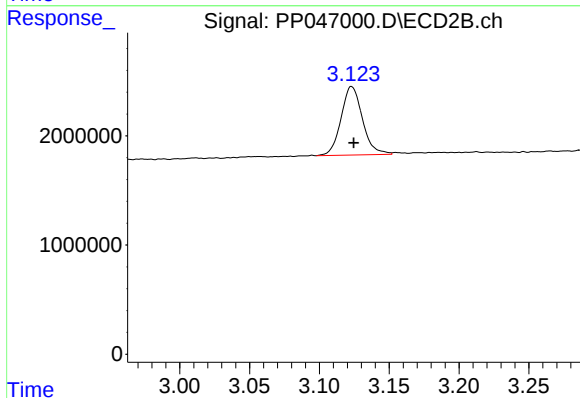


#1 Tetrachloro-m-xylene

R.T.: 3.123 min
Delta R.T.: -0.002 min
Response: 6707144
Conc: 2.04 ng/ml

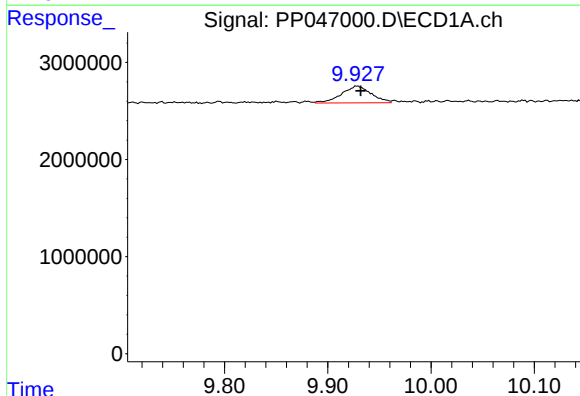

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.004 min
Response: 3465625
Conc: 2.36 ng/ml

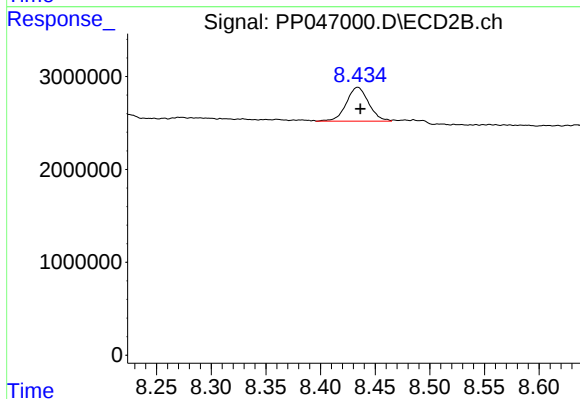

#2 Decachlorobiphenyl

R.T.: 8.434 min
Delta R.T.: -0.003 min
Response: 5197059
Conc: 2.18 ng/ml m