

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050423\
 Data File : PP057505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 14:10
 Operator : YP\AJ
 Sample : 02566-05DL 100X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-1989DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 21:09:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 04 07:27:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
16)	L4	AR-1242-1	5.571	4.723	52821610	1156.035
17)	L4	AR-1242-2	5.594	4.743	75055663	1133.990
18)	L4	AR-1242-3	5.657	4.921	46998780	1050.852
19)	L4	AR-1242-4	5.756	5.005	36580941	754.585 #
20)	L4	AR-1242-5	6.500	5.534	17730336	616.392
26)	L6	AR-1254-1	6.433	5.534	17684453	301.469
27)	L6	AR-1254-2	6.657	5.683	20973925	154.546 #
28)	L6	AR-1254-3	7.025	6.091	13325284	141.076
29)	L6	AR-1254-4	7.312	6.321	7990583	131.594
30)	L6	AR-1254-5	7.736	6.742	5284869	74.108



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050423\
Data File : PP057505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 14:10
Operator : YP\AJ
Sample : 02566-05DL 100X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 21:09:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 04 07:27:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

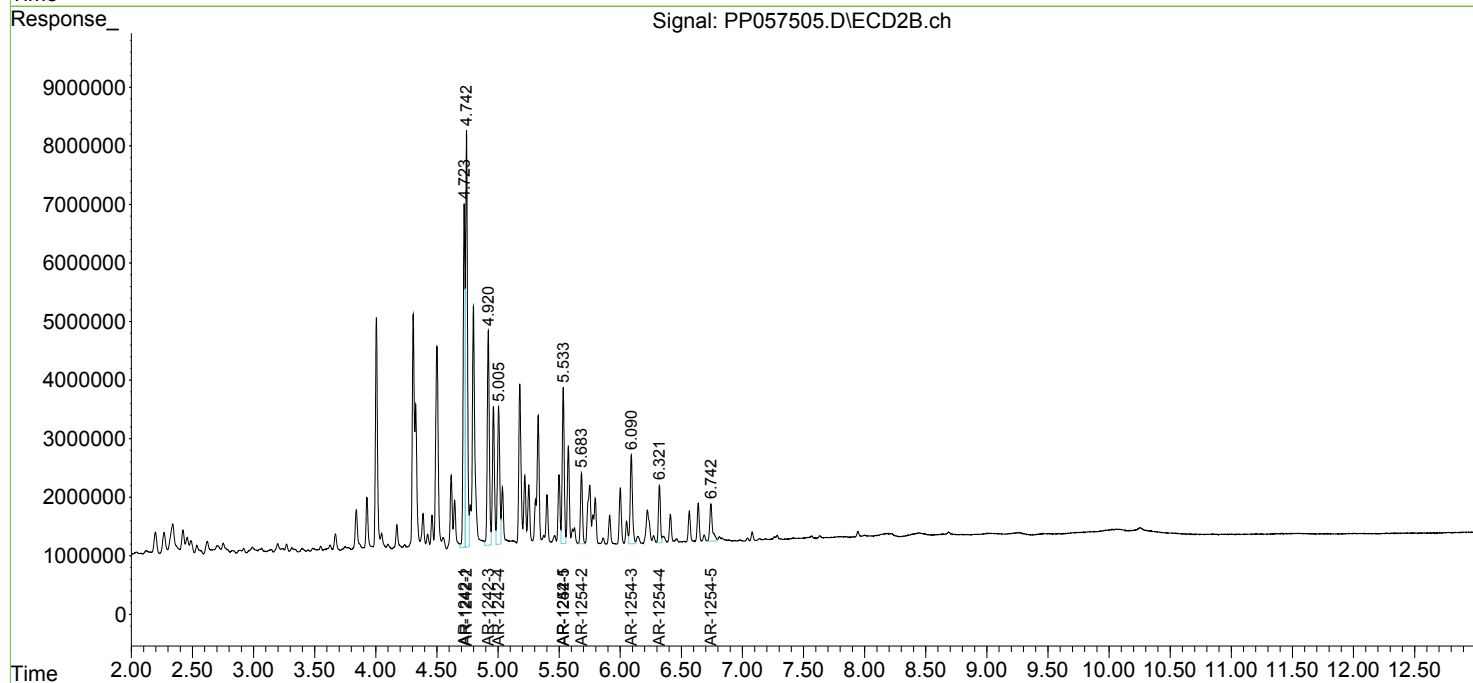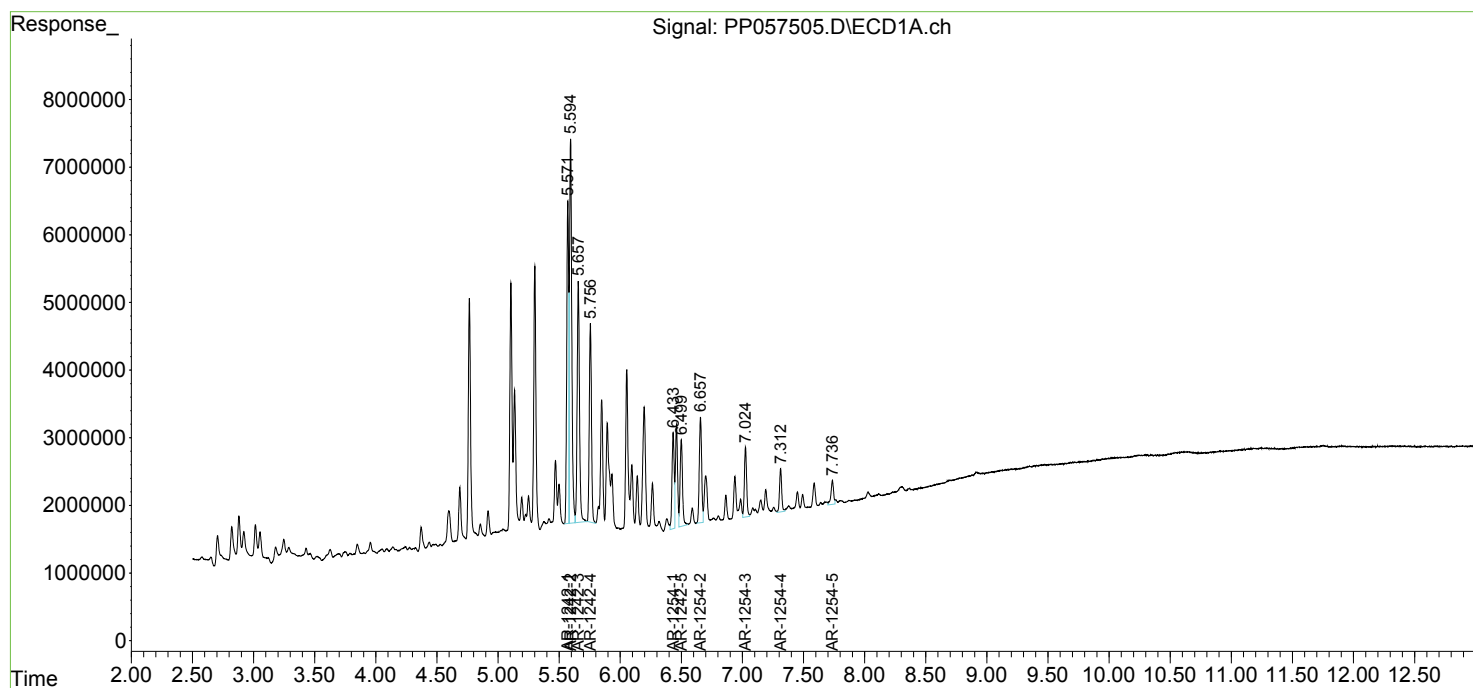


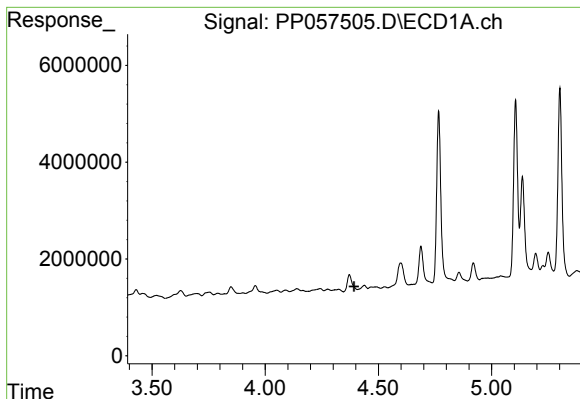

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

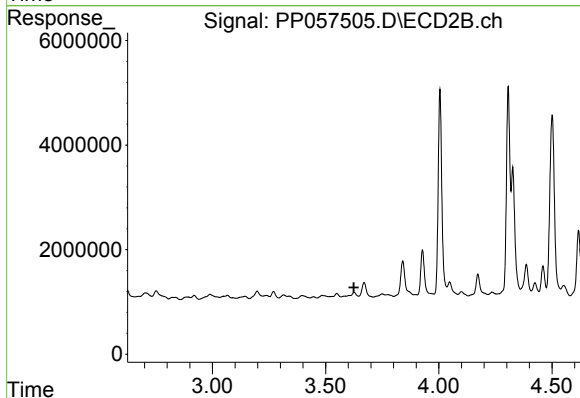


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.625 min
Response: 0
Conc: N.D.

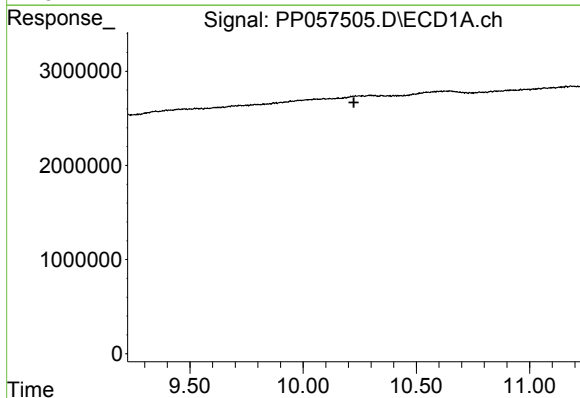


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.224 min
Response: 0
Conc: N.D.

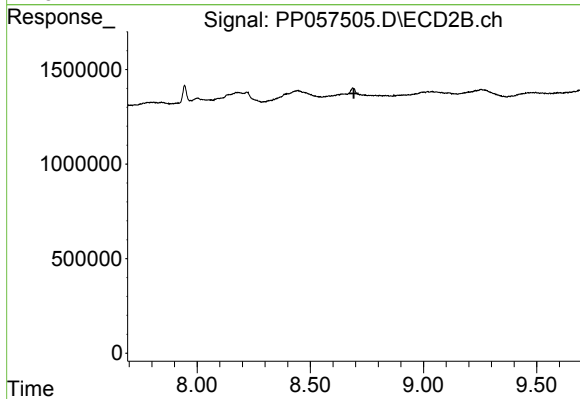

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.693 min
Response: 0
Conc: N.D.

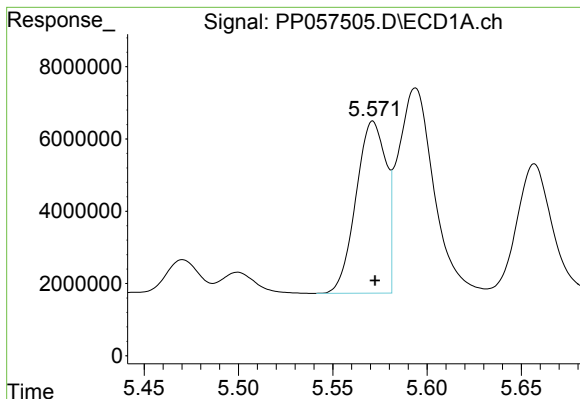

#16 AR-1242-1


R.T.: 5.571 min
Delta R.T.: -0.001 min
Response: 52821610
Conc: 1223.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

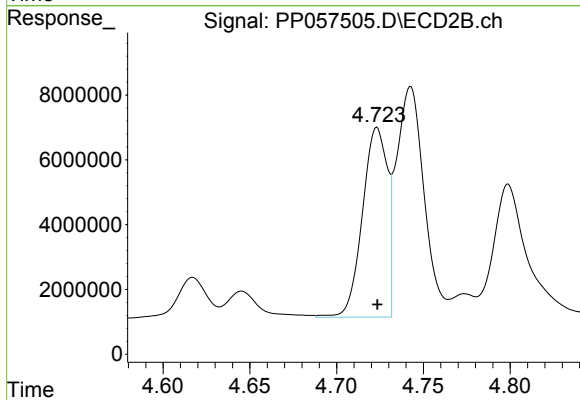


#16 AR-1242-1

R.T.: 4.723 min
Delta R.T.: 0.000 min
Response: 58626216
Conc: 1156.03 ng/ml

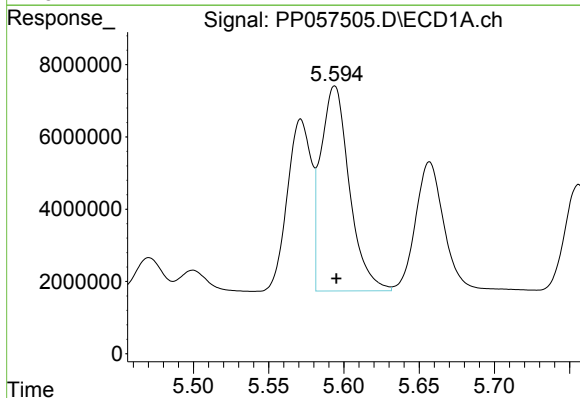


#17 AR-1242-2

R.T.: 5.594 min
Delta R.T.: -0.001 min
Response: 75055663
Conc: 1197.22 ng/ml

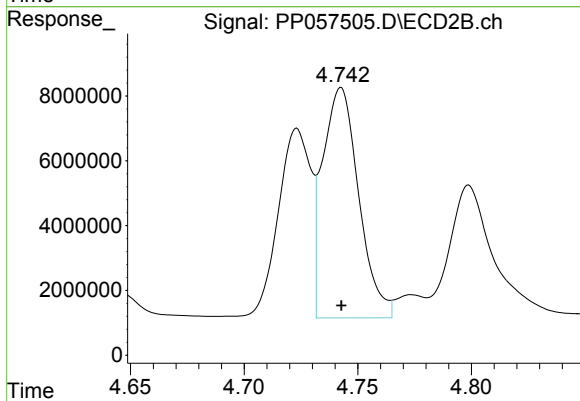

#17 AR-1242-2


R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 78717380
Conc: 1133.99 ng/ml

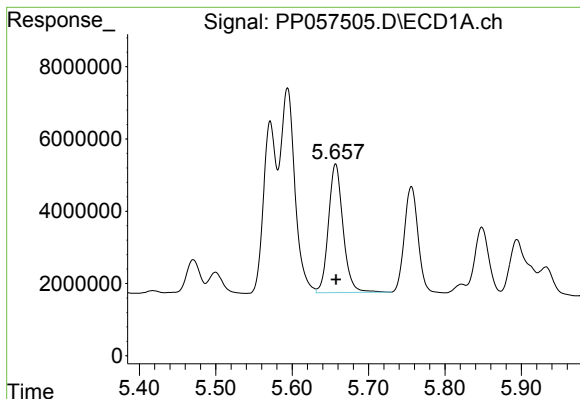

#18 AR-1242-3


R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 46998780
Conc: 1196.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

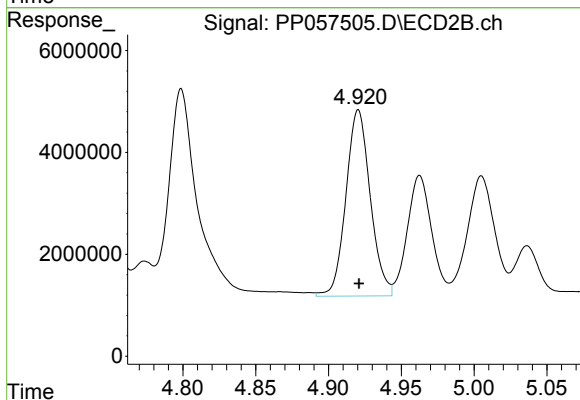


#18 AR-1242-3

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 42572644
Conc: 1050.85 ng/ml

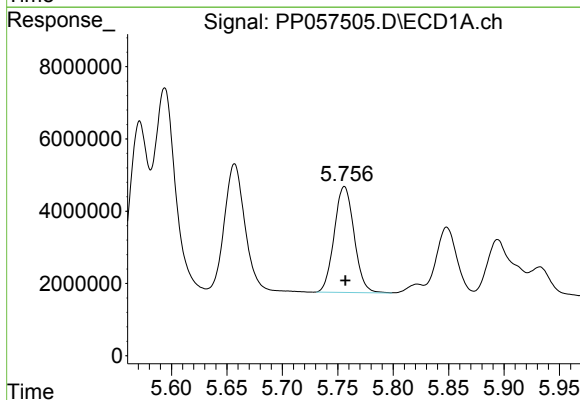


#19 AR-1242-4

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 36580941
Conc: 1149.15 ng/ml

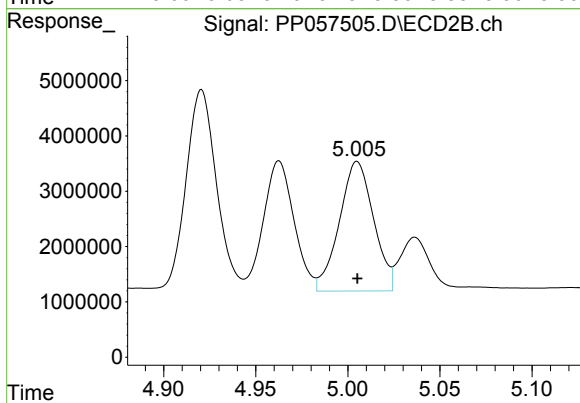

#19 AR-1242-4


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 30341402
Conc: 754.59 ng/ml

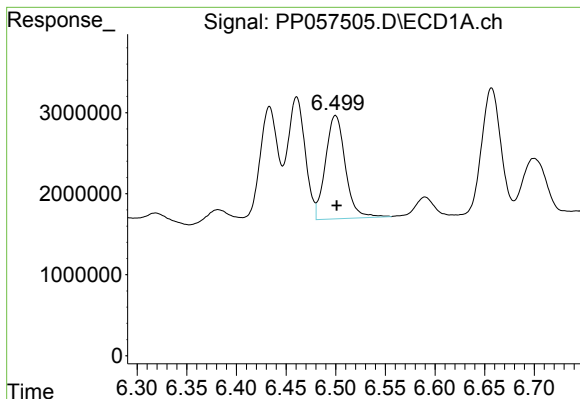

#20 AR-1242-5


R.T.: 6.500 min
Delta R.T.: -0.001 min
Response: 17730336
Conc: 637.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

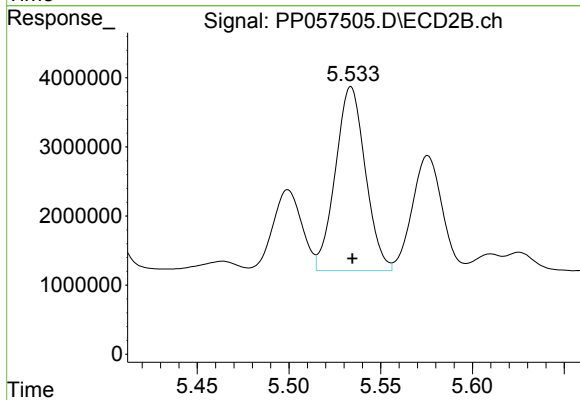


#20 AR-1242-5

R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 30252816
Conc: 616.39 ng/ml

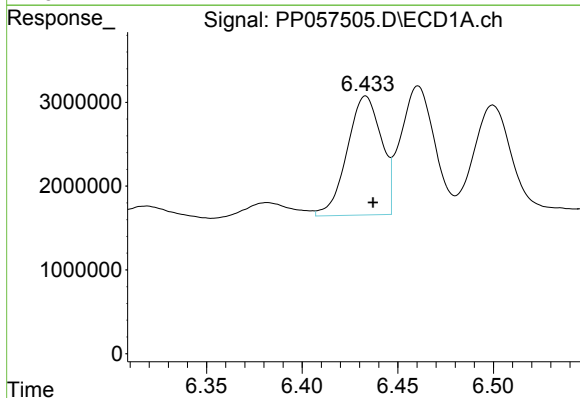


#26 AR-1254-1

R.T.: 6.433 min
Delta R.T.: -0.004 min
Response: 17684453
Conc: 288.56 ng/ml

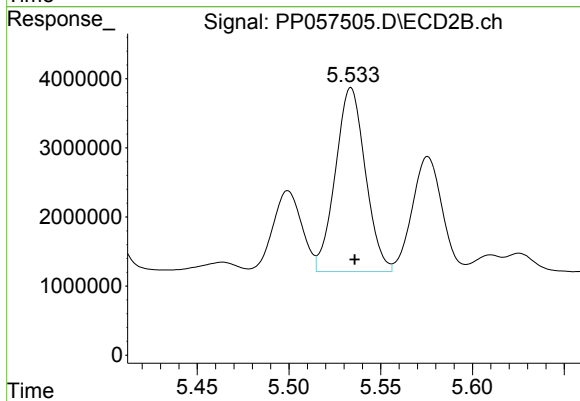

#26 AR-1254-1


R.T.: 5.534 min
Delta R.T.: -0.002 min
Response: 30252816
Conc: 301.47 ng/ml

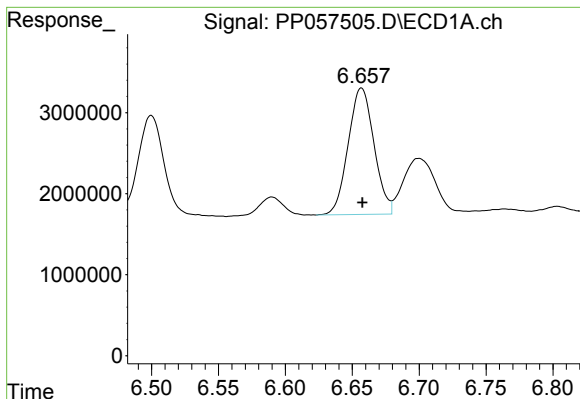

#27 AR-1254-2


R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 20973925
Conc: 246.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

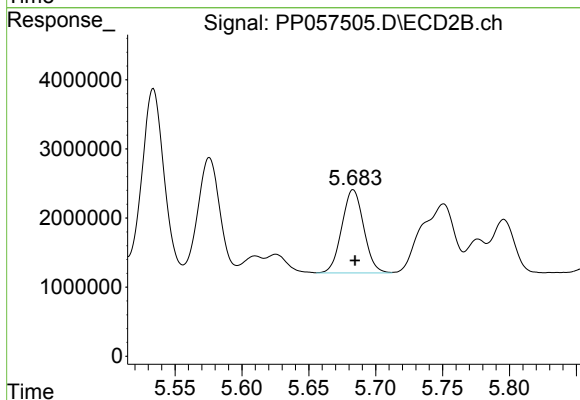


#27 AR-1254-2

R.T.: 5.683 min
Delta R.T.: -0.001 min
Response: 13741749
Conc: 154.55 ng/ml

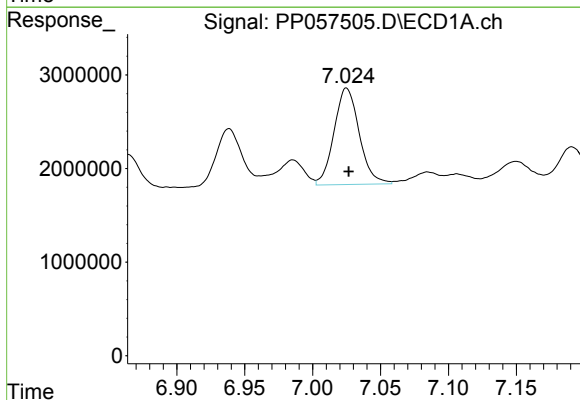


#28 AR-1254-3

R.T.: 7.025 min
Delta R.T.: -0.002 min
Response: 13325284
Conc: 166.80 ng/ml

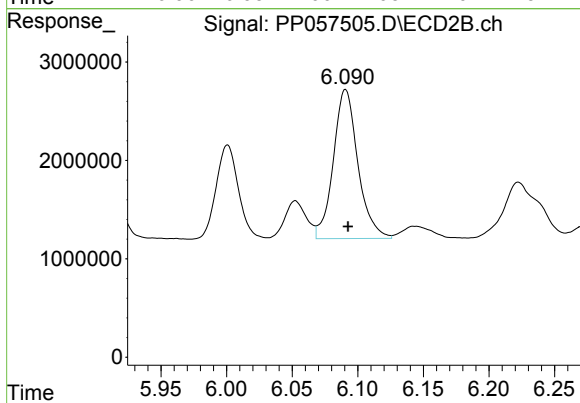

#28 AR-1254-3


R.T.: 6.091 min
Delta R.T.: -0.002 min
Response: 19757086
Conc: 141.08 ng/ml

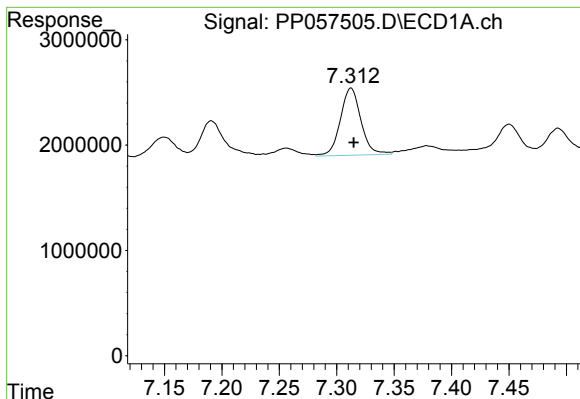

#29 AR-1254-4


R.T.: 7.312 min
Delta R.T.: -0.003 min
Response: 7990583
Conc: 143.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1989DL

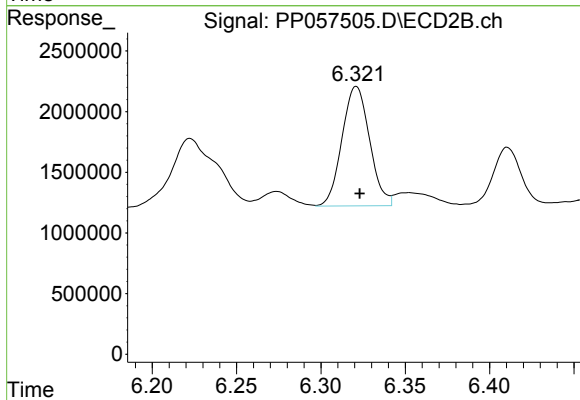


#29 AR-1254-4

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 11222751
Conc: 131.59 ng/ml

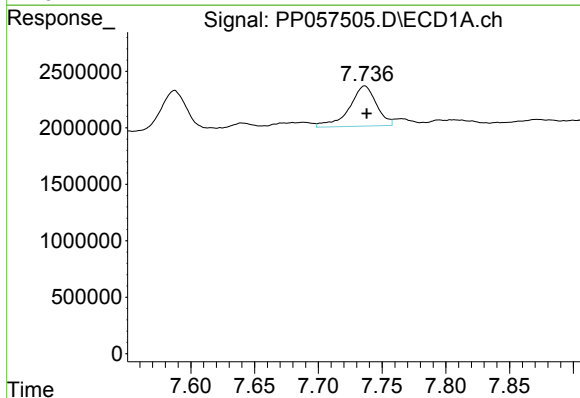

#30 AR-1254-5

R.T.: 7.736 min
Delta R.T.: -0.002 min
Response: 5284869
Conc: 86.89 ng/ml

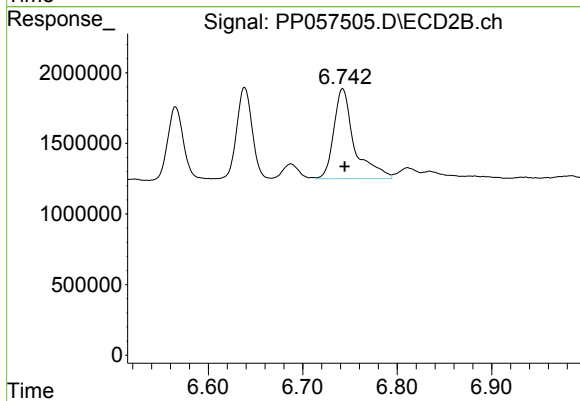

#30 AR-1254-5

R.T.: 6.742 min
Delta R.T.: -0.002 min
Response: 9691968
Conc: 74.11 ng/ml