

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050521\
 Data File : PP035591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2021 4:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 09:20:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 08:33:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.785	4.203	941653	702401	21.523	23.155
2) SA Decachlor...	10.638	9.455	882746	465193	22.380	24.111
Target Compounds						
9) L2 AR-1221-2	0.000	4.557	0	8728	N.D.	31.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050521\
Data File : PP035591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 4:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 09:20:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 08:33:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

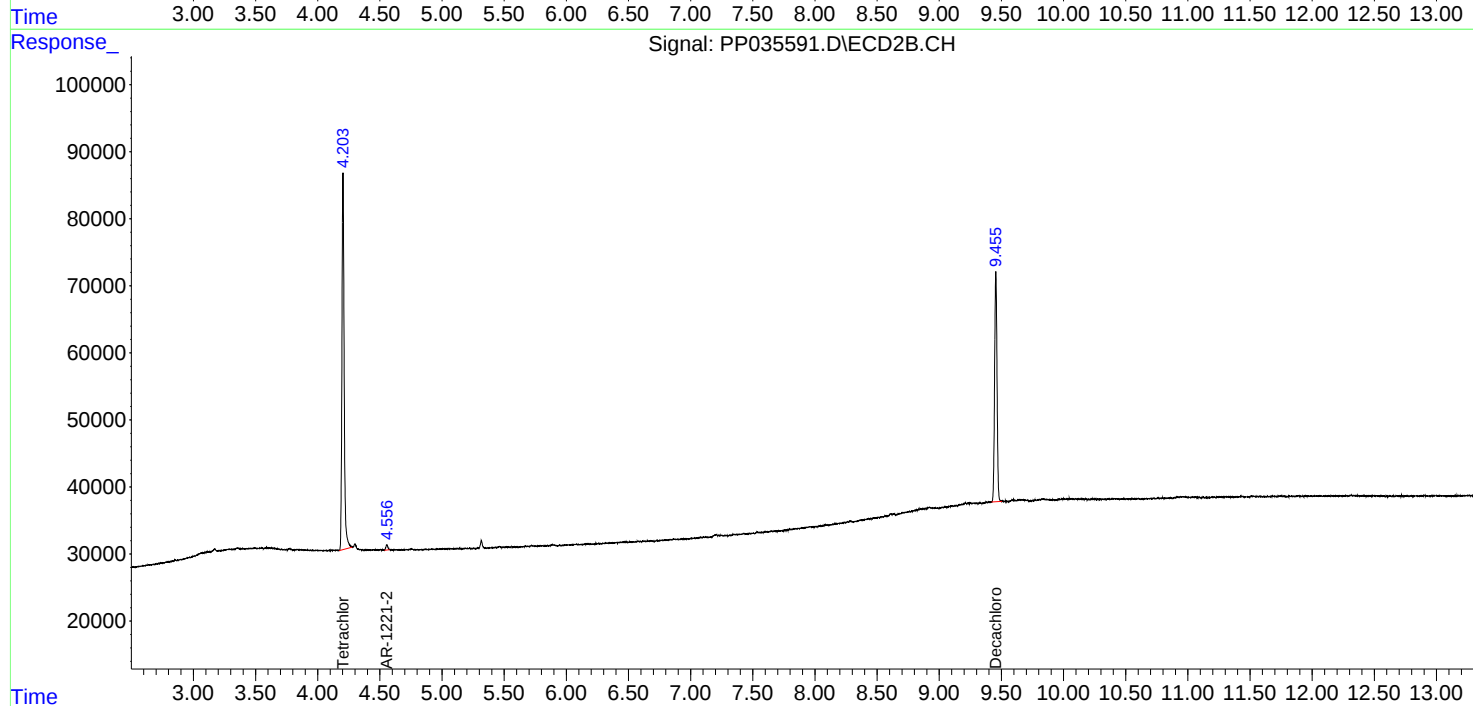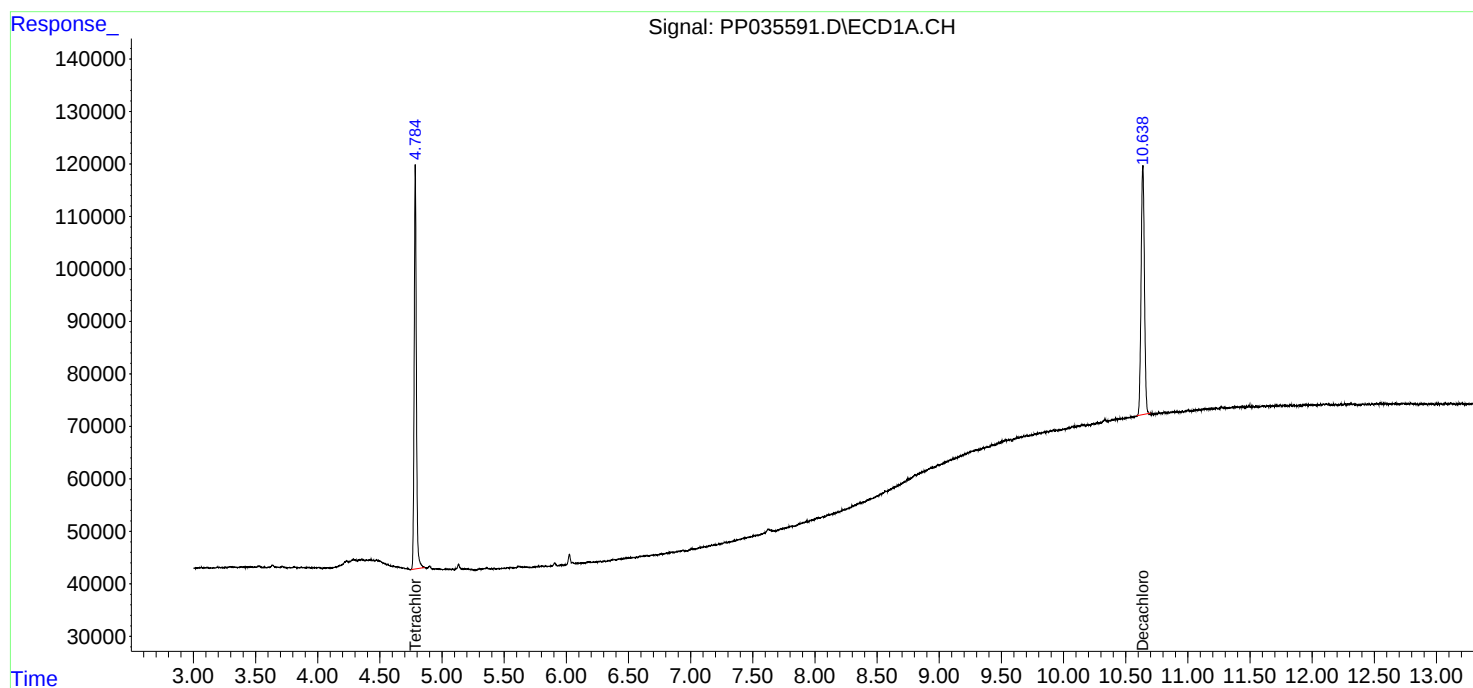


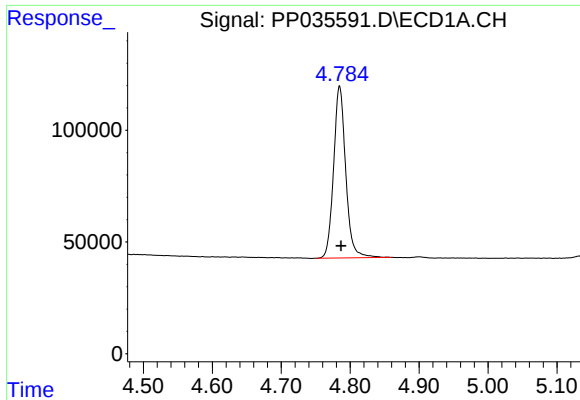

#1 Tetrachloro-m-xylene


R.T.: 4.785 min
Delta R.T.: -0.002 min
Response: 941653
Conc: 21.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

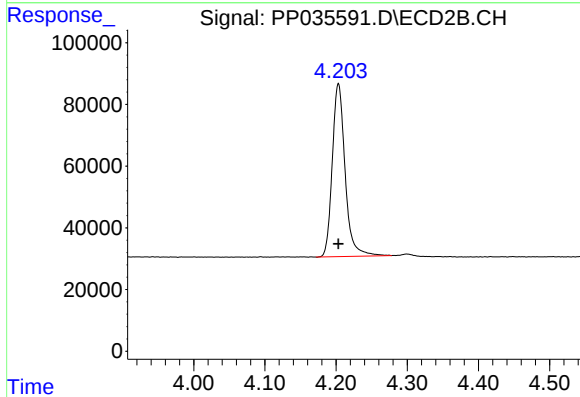


#1 Tetrachloro-m-xylene

R.T.: 4.203 min
Delta R.T.: 0.000 min
Response: 702401
Conc: 23.16 ng/ml

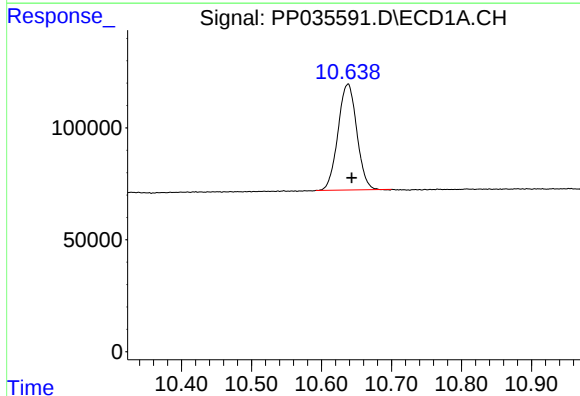


#2 Decachlorobiphenyl

R.T.: 10.638 min
Delta R.T.: -0.005 min
Response: 882746
Conc: 22.38 ng/ml

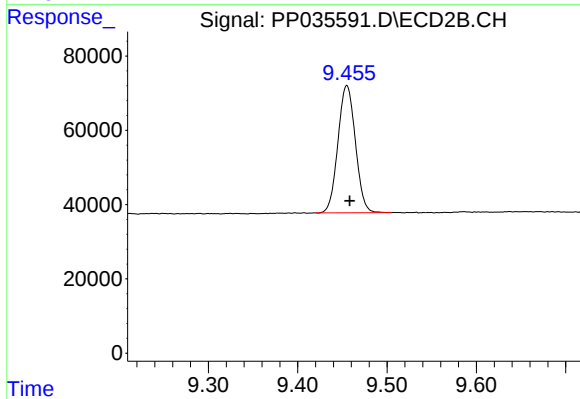

#2 Decachlorobiphenyl


R.T.: 9.455 min
Delta R.T.: -0.003 min
Response: 465193
Conc: 24.11 ng/ml

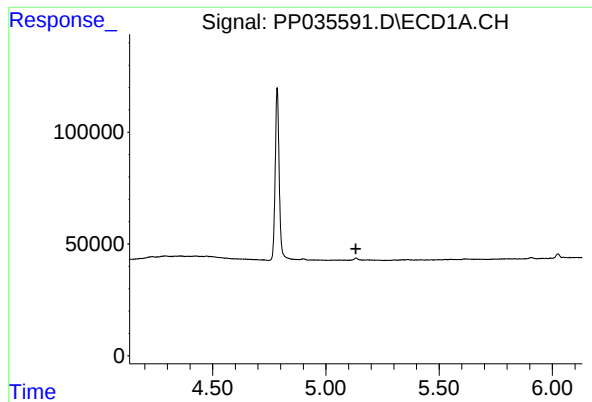

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

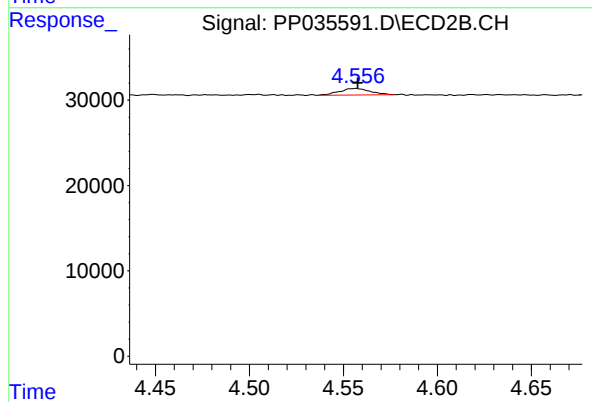

#9 AR-1221-2

R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 8728
Conc: 31.15 ng/ml