

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050521\
 Data File : PP035555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2021 17:47
 Operator : DD\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:14:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 06:59:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 06:58:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.786	4.204	232545	176699	5.169	5.461
2)	SA Decachlor...	10.642	9.457	207251	110827	5.067	5.583
Target Compounds							
21)	L5 AR-1248-1	6.093	5.448	42886	29207	49.952	54.330
22)	L5 AR-1248-2	6.383	5.705	70211	46213	56.437m	57.019
23)	L5 AR-1248-3	6.598	5.750	90417	48720	60.562m	56.743
24)	L5 AR-1248-4	7.024	5.935	80625	53165	53.365	53.394
25)	L5 AR-1248-5	7.064	6.353	77598	48546	51.936	52.025m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050521\
Data File : PP035555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2021 17:47
Operator : DD\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 06:59:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 06:58:09 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

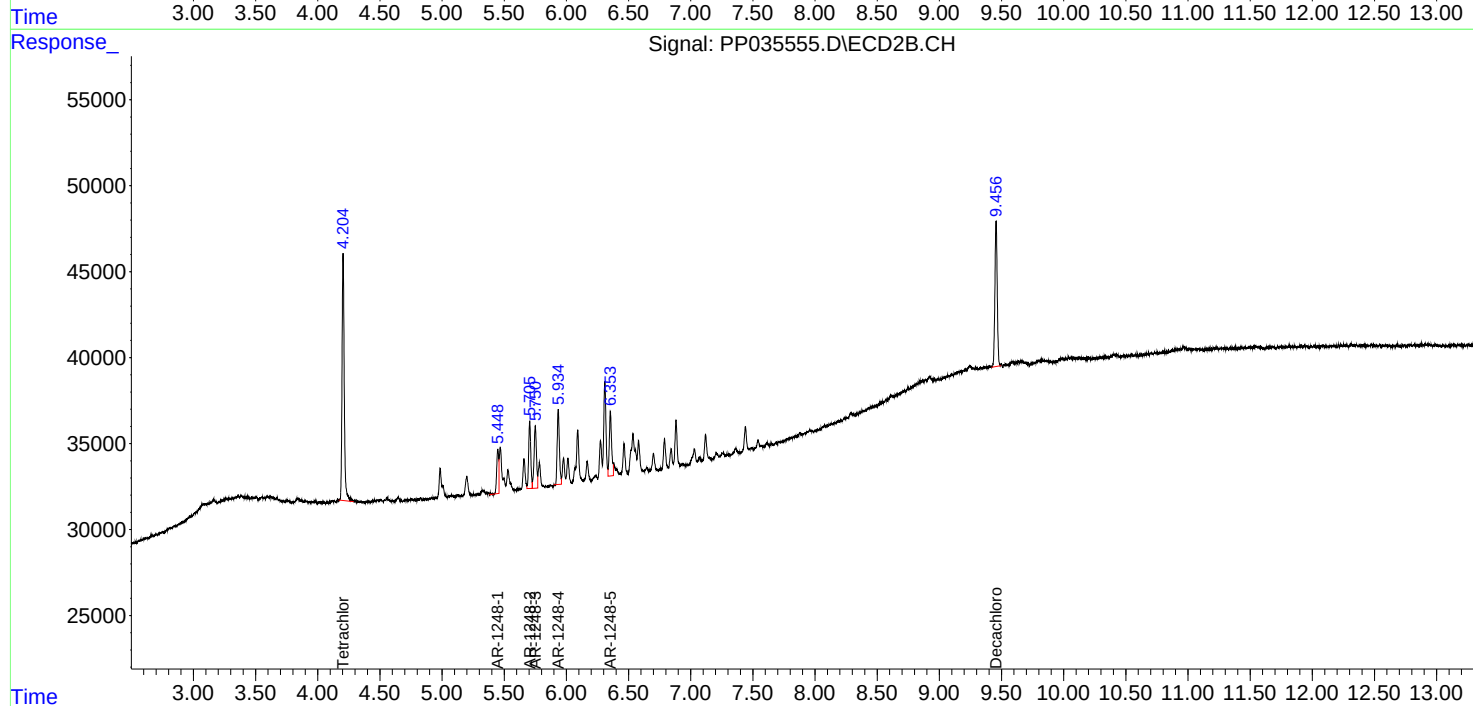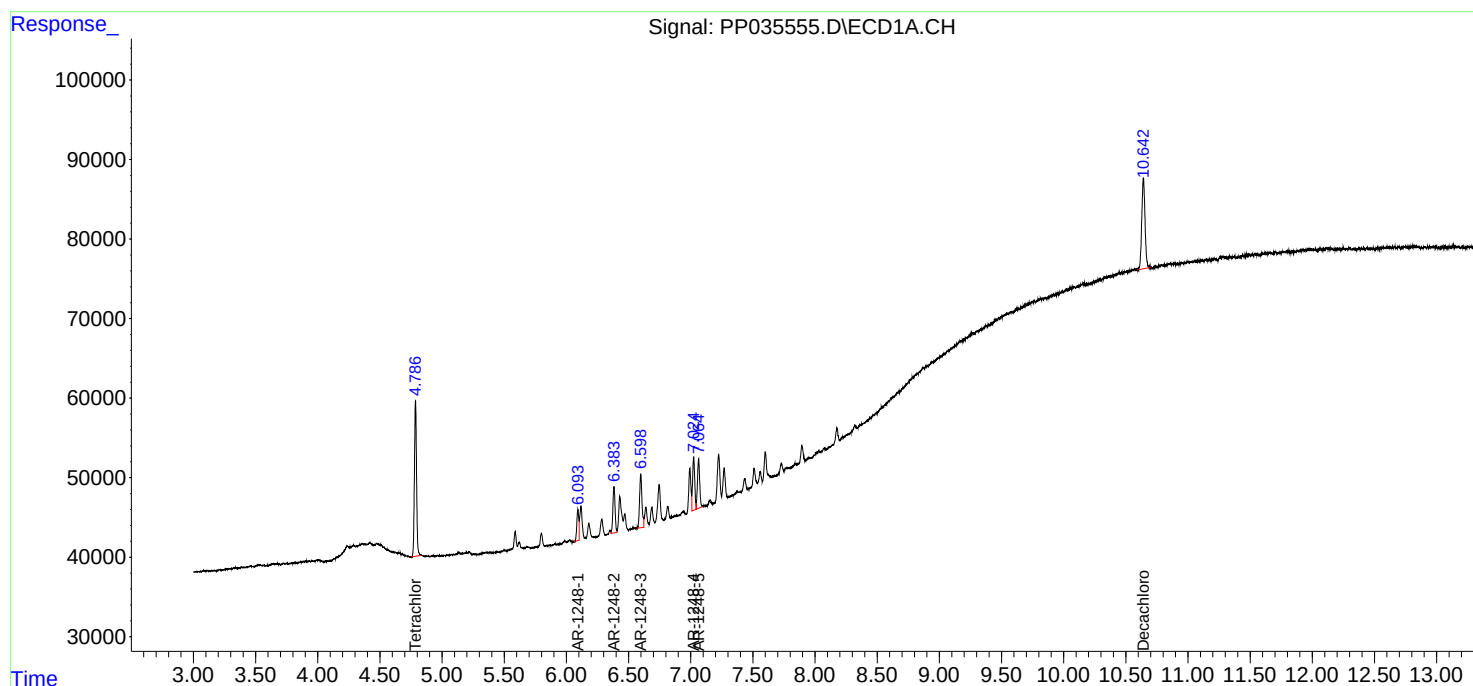

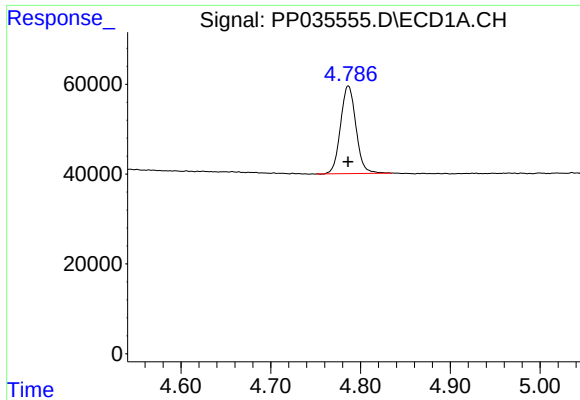


#1 Tetrachloro-m-xylene

R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 232545
Conc: 5.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:22 PM

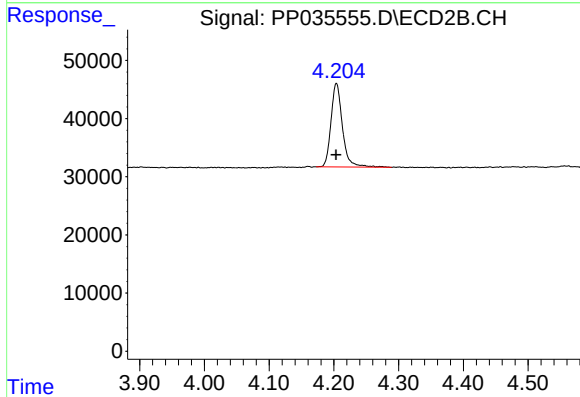


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: 0.000 min
Response: 176699
Conc: 5.46 ng/ml

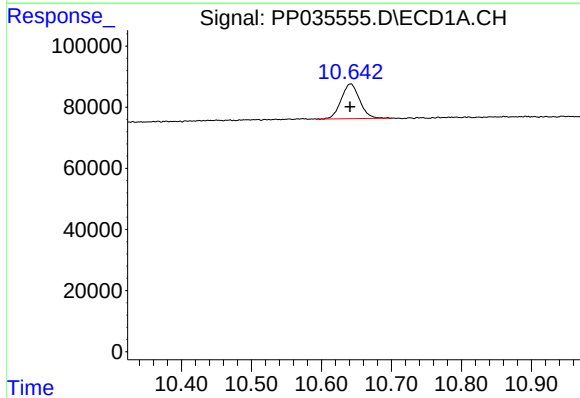


#2 Decachlorobiphenyl

R.T.: 10.642 min
Delta R.T.: 0.000 min
Response: 207251
Conc: 5.07 ng/ml

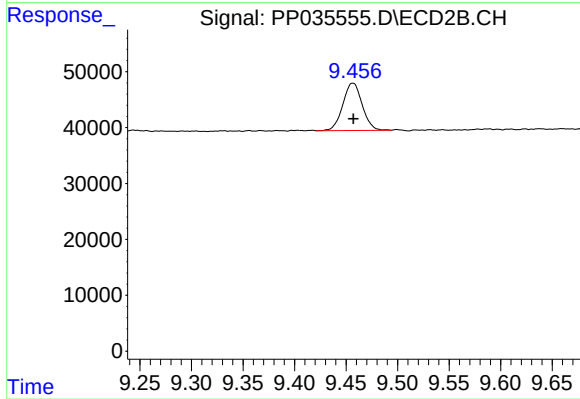

#2 Decachlorobiphenyl

R.T.: 9.457 min
Delta R.T.: 0.000 min
Response: 110827
Conc: 5.58 ng/ml

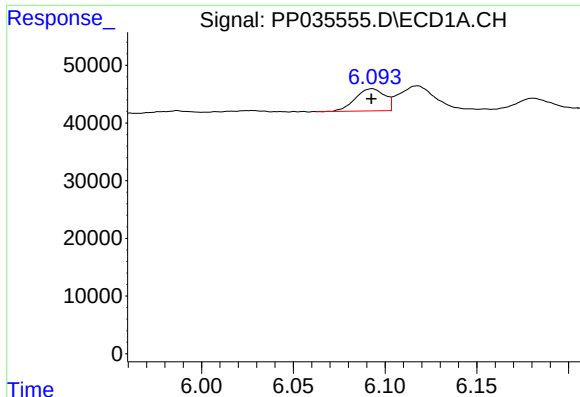


#21 AR-1248-1

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 42886
Conc: 49.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:22 PM

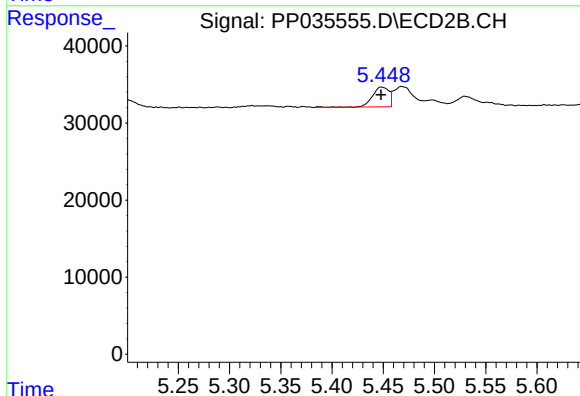


#21 AR-1248-1

R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 29207
Conc: 54.33 ng/ml

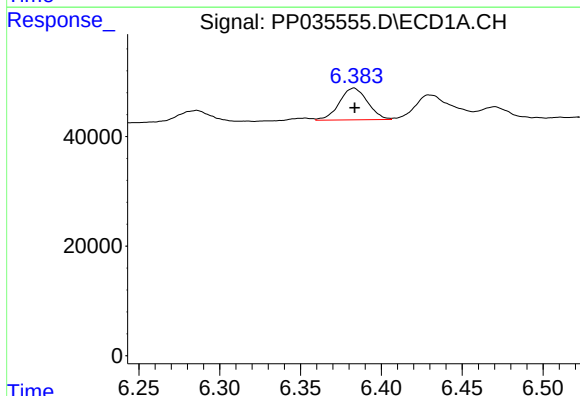


#22 AR-1248-2

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 70211
Conc: 56.44 ng/ml m

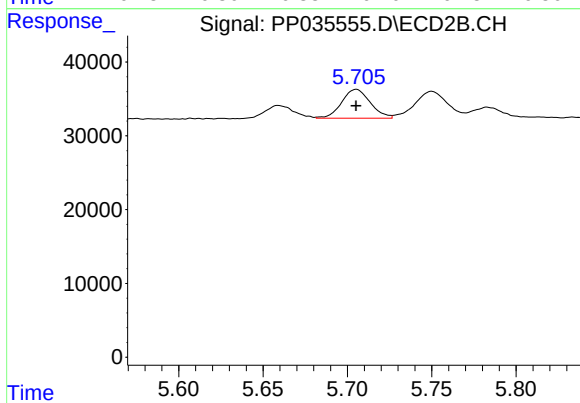

#22 AR-1248-2

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 46213
Conc: 57.02 ng/ml

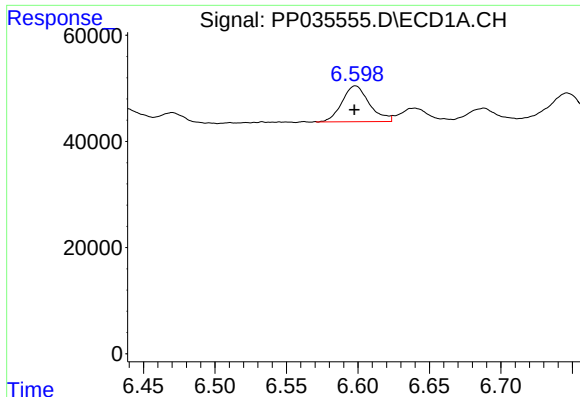


#23 AR-1248-3

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 90417
Conc: 60.56 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:22 PM

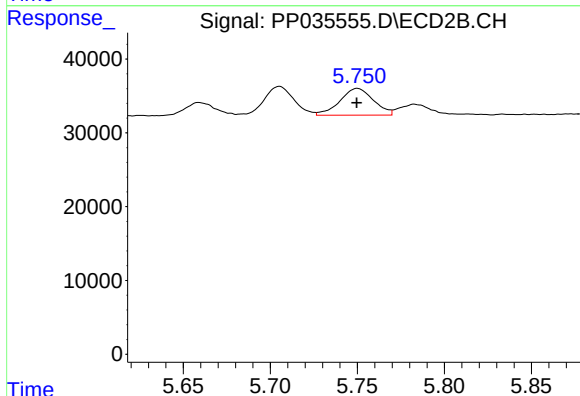


#23 AR-1248-3

R.T.: 5.750 min
Delta R.T.: 0.000 min
Response: 48720
Conc: 56.74 ng/ml

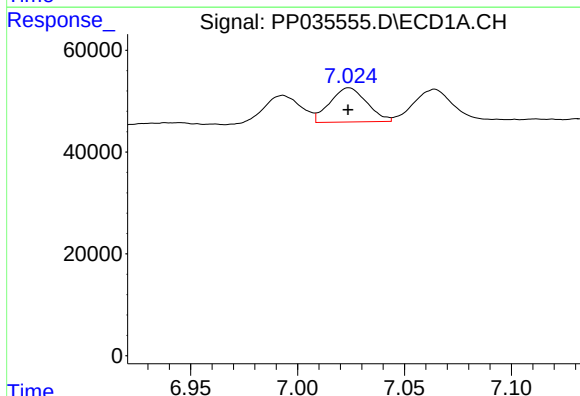


#24 AR-1248-4

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 80625
Conc: 53.37 ng/ml

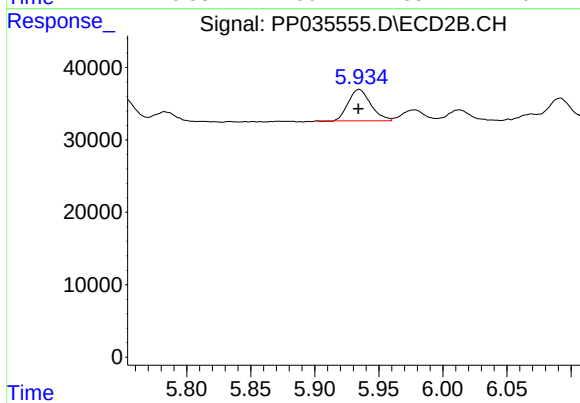

#24 AR-1248-4

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 53165
Conc: 53.39 ng/ml

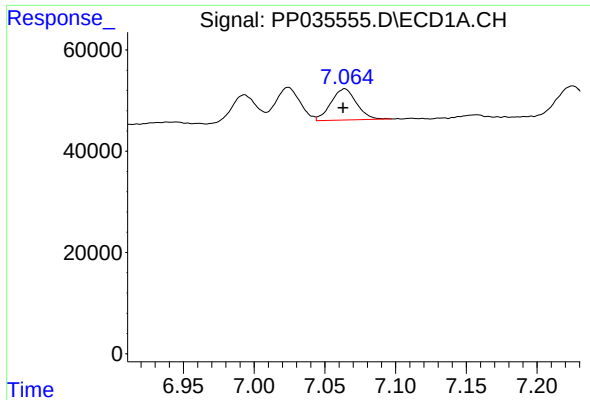


#25 AR-1248-5

R.T.: 7.064 min
Delta R.T.: 0.001 min
Response: 77598
Conc: 51.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Ankita
5/6/2021 4:14:22 PM

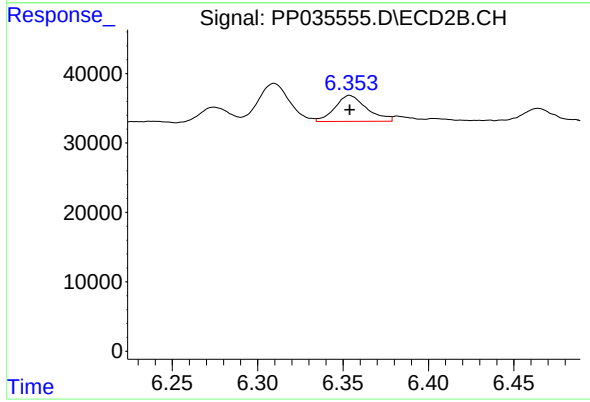

#25 AR-1248-5

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 48546
Conc: 52.03 ng/ml m