

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050523\
 Data File : PP057575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 18:08
 Operator : YP\AJ
 Sample : 02626-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 D2978

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/08/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 21:29:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 05 08:53:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.389	3.625	35772802	35450213	17.199m	17.502
2) SA Decachlor...	10.213	8.684	26842438	36176945	36.724	27.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050523\
Data File : PP057575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 18:08
Operator : YP\AJ
Sample : 02626-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
D2978


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/08/2023
Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 21:29:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 05 08:53:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

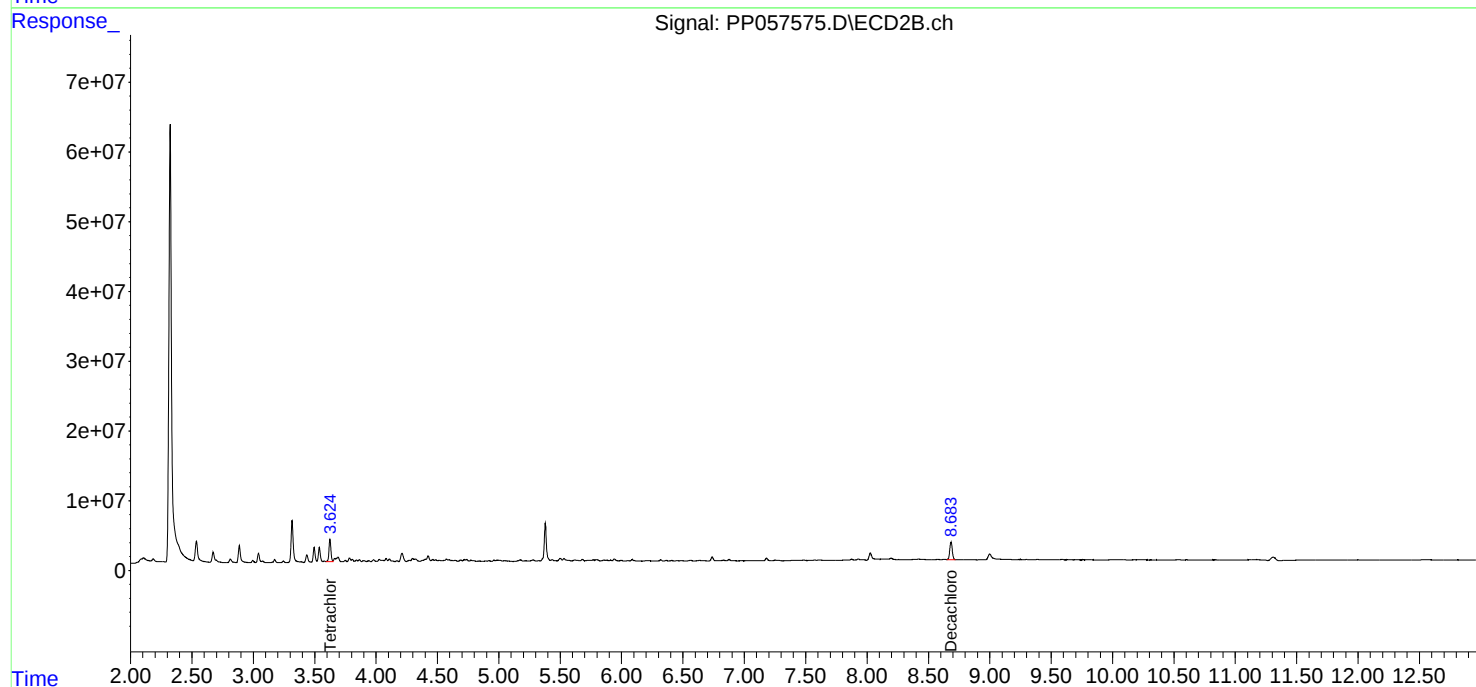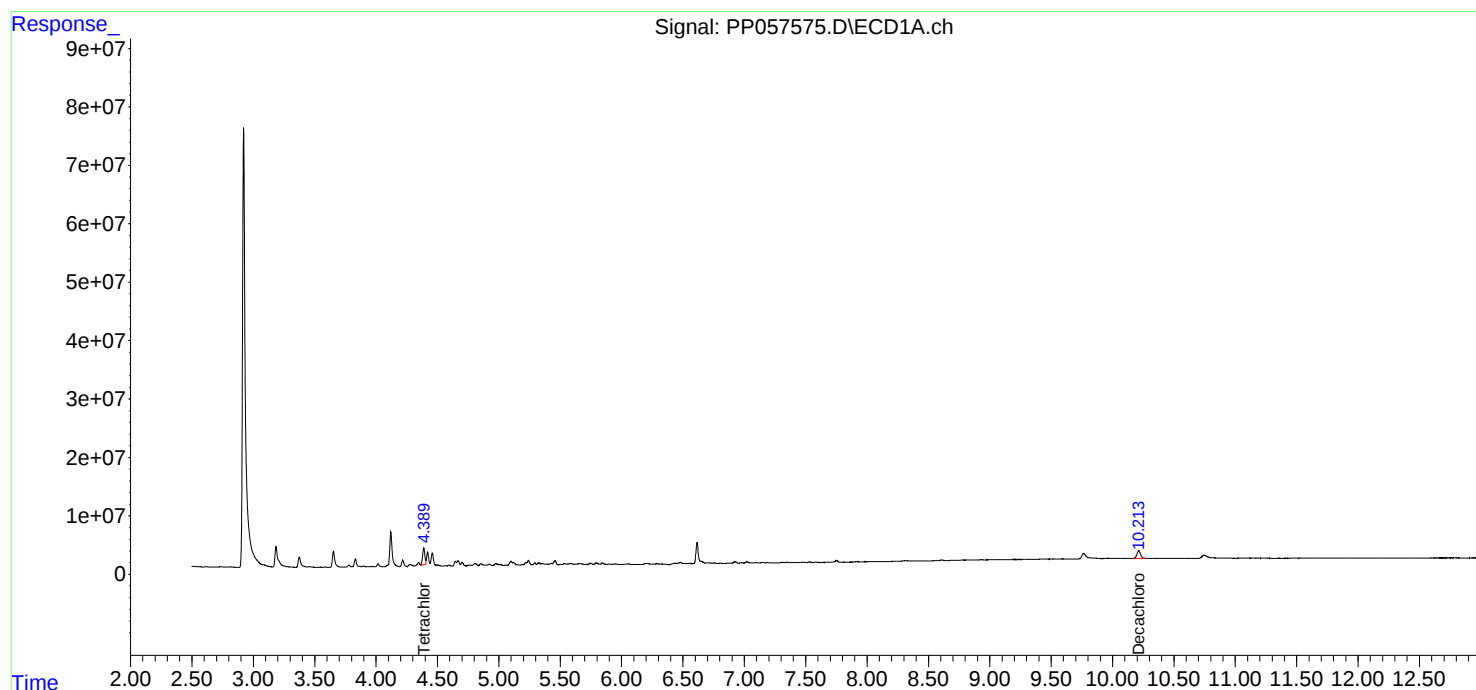

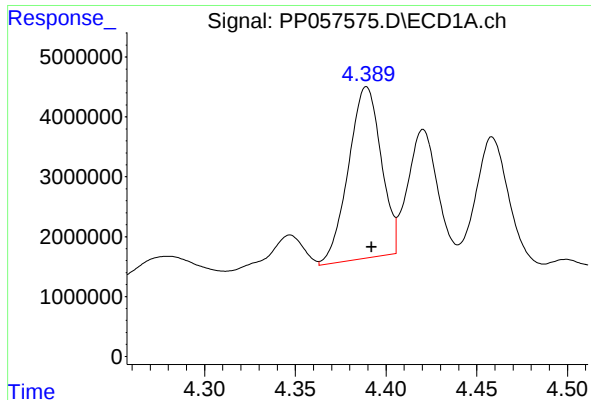


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: -0.003 min
Response: 35772802
Conc: 17.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
D2978


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/08/2023
Supervised By :Ankita Jodhani 05/08/2023

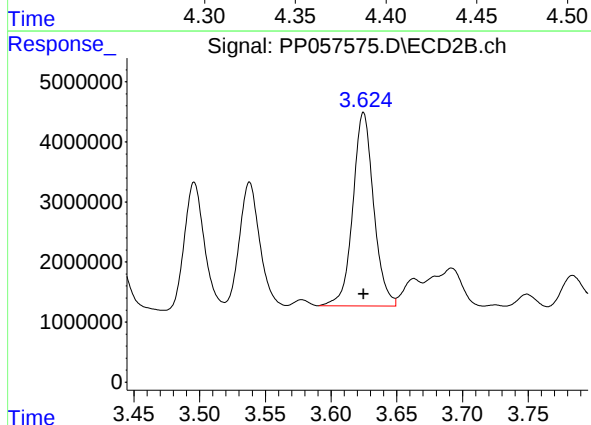


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 35450213
Conc: 17.50 ng/ml

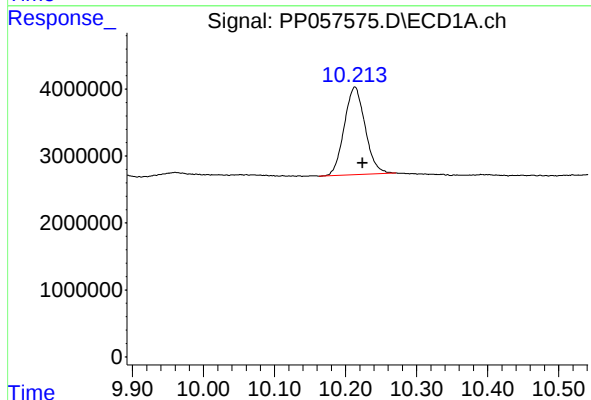

#2 Decachlorobiphenyl

R.T.: 10.213 min
Delta R.T.: -0.011 min
Response: 26842438
Conc: 36.72 ng/ml

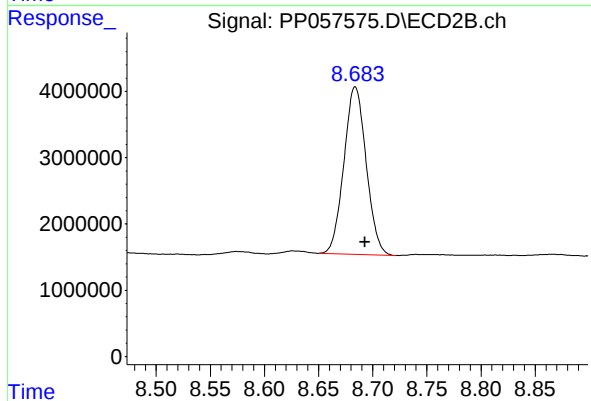

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.009 min
Response: 36176945
Conc: 27.81 ng/ml