

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050523\
 Data File : PP057595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2023 00:20
 Operator : YP\AJ
 Sample : 02629-02 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HED720F-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 07:30:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 05 08:53:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.624	3841776	4153871	1.847	2.051
2) SA Decachlor...	10.214	8.684	2043008	3164828	2.795	2.433

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050523\
Data File : PP057595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2023 00:20
Operator : YP\AJ
Sample : 02629-02 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HED720F-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 07:30:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050323.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 05 08:53:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

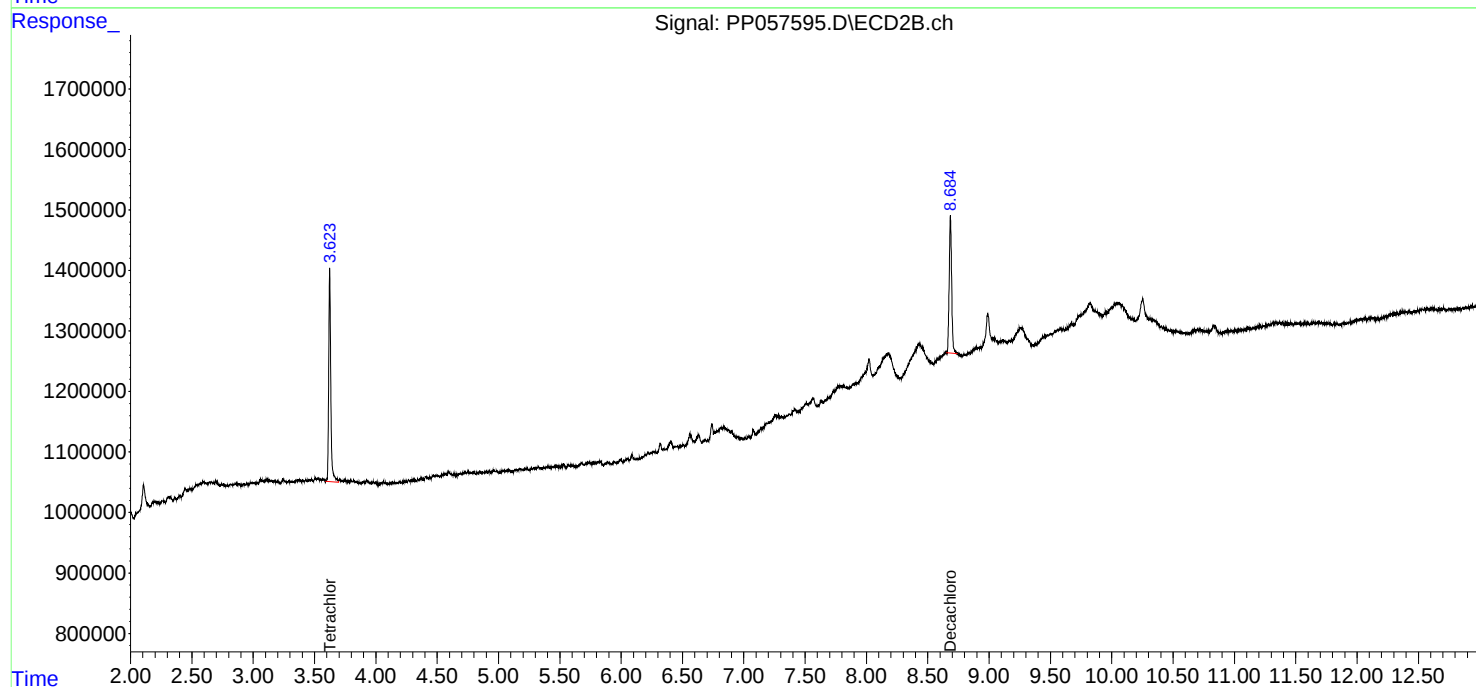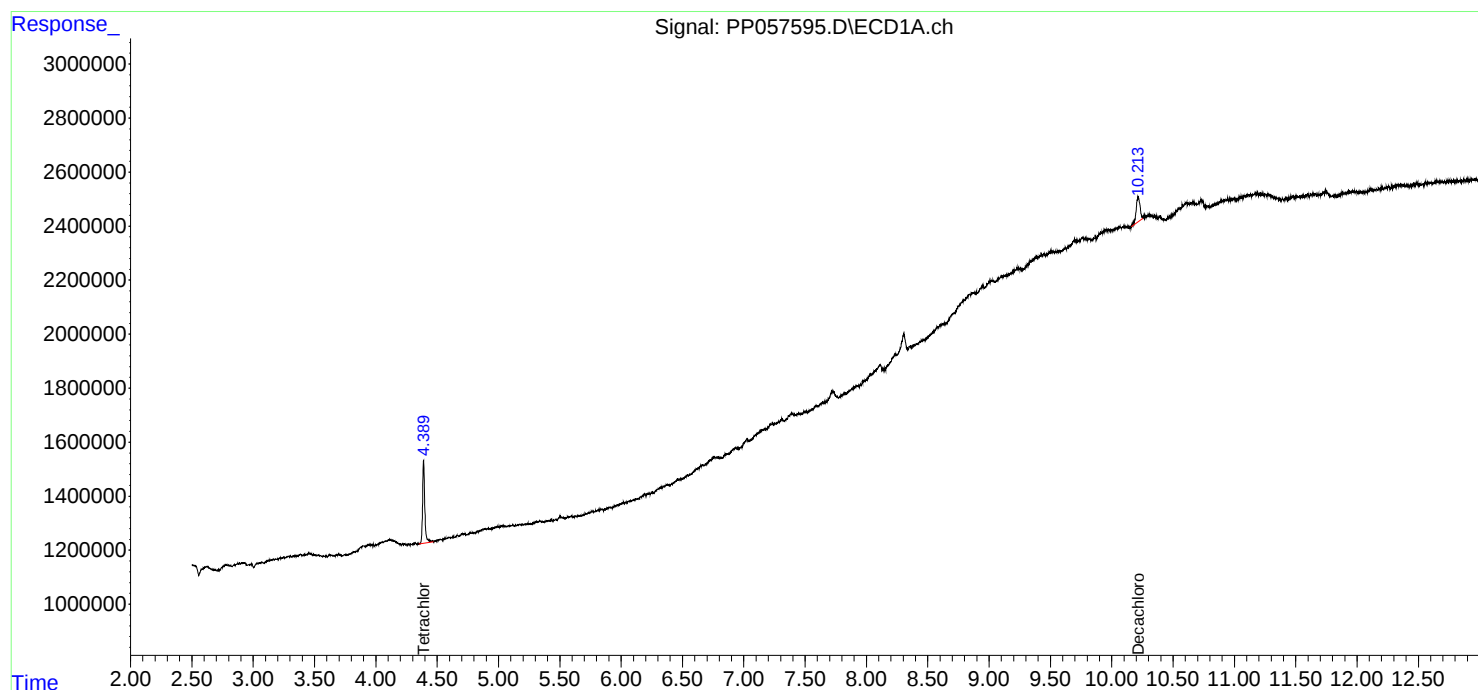


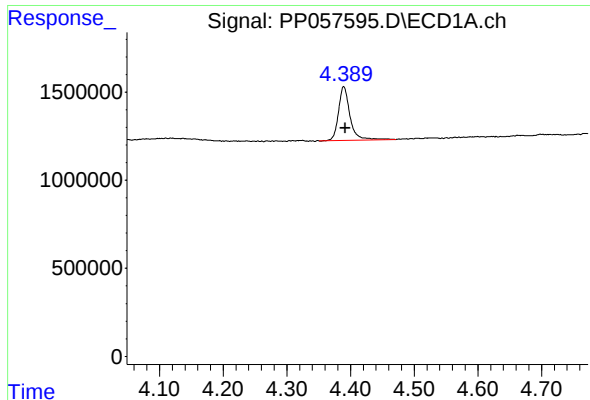

#1 Tetrachloro-m-xylene


R.T.: 4.389 min
Delta R.T.: -0.003 min
Response: 3841776
Conc: 1.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
HED720F-1-2

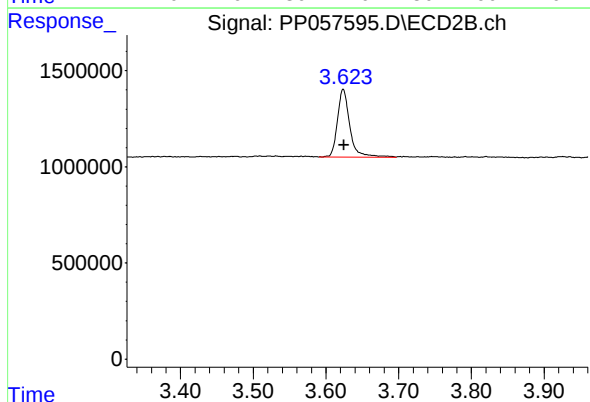


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.001 min
Response: 4153871
Conc: 2.05 ng/ml

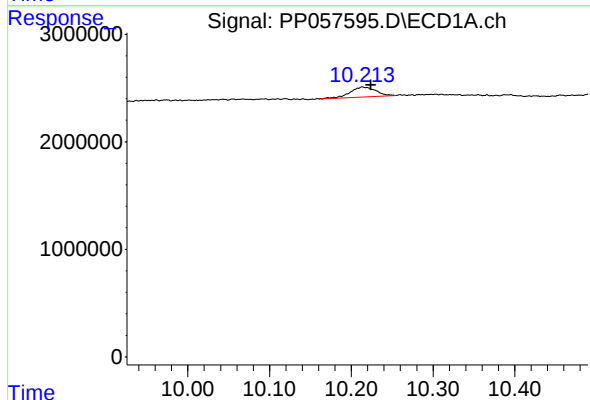

#2 Decachlorobiphenyl

R.T.: 10.214 min
Delta R.T.: -0.010 min
Response: 2043008
Conc: 2.80 ng/ml

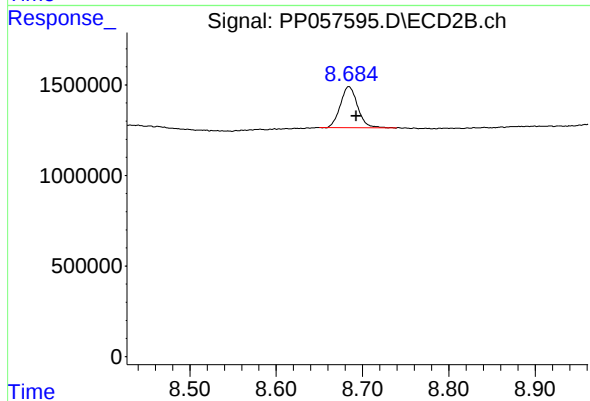

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.009 min
Response: 3164828
Conc: 2.43 ng/ml