

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
 Data File : PP035615.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2021 17:27
 Operator : DD\AJ
 Sample : M2275-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 18:02:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.784	4.202	829829	584947	18.967	19.283
2)	SA Decachlor...	10.634	9.455	886583	435717	22.477	22.583
Target Compounds							
30)	L6 AR-1254-5	8.323	0.000	98610	0	47.674	N.D. #
31)	L7 AR-1260-1	0.000	7.004	0	11212	N.D.	8.277 #
32)	L7 AR-1260-2	0.000	7.205	0	11274	N.D.	7.147 #
34)	L7 AR-1260-4	8.595f	7.812f	17931	4453	9.058	4.134 #
40)	L8 AR-1262-5	0.000	8.919	0	24262	N.D.	23.697 #
43)	L9 AR-1268-3	0.000	8.608f	0	18508	N.D.	7.600 #
44)	L9 AR-1268-4	0.000	8.919	0	24262	N.D.	24.301 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035615.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 17:27
Operator : DD\AJ
Sample : M2275-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 18:02:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

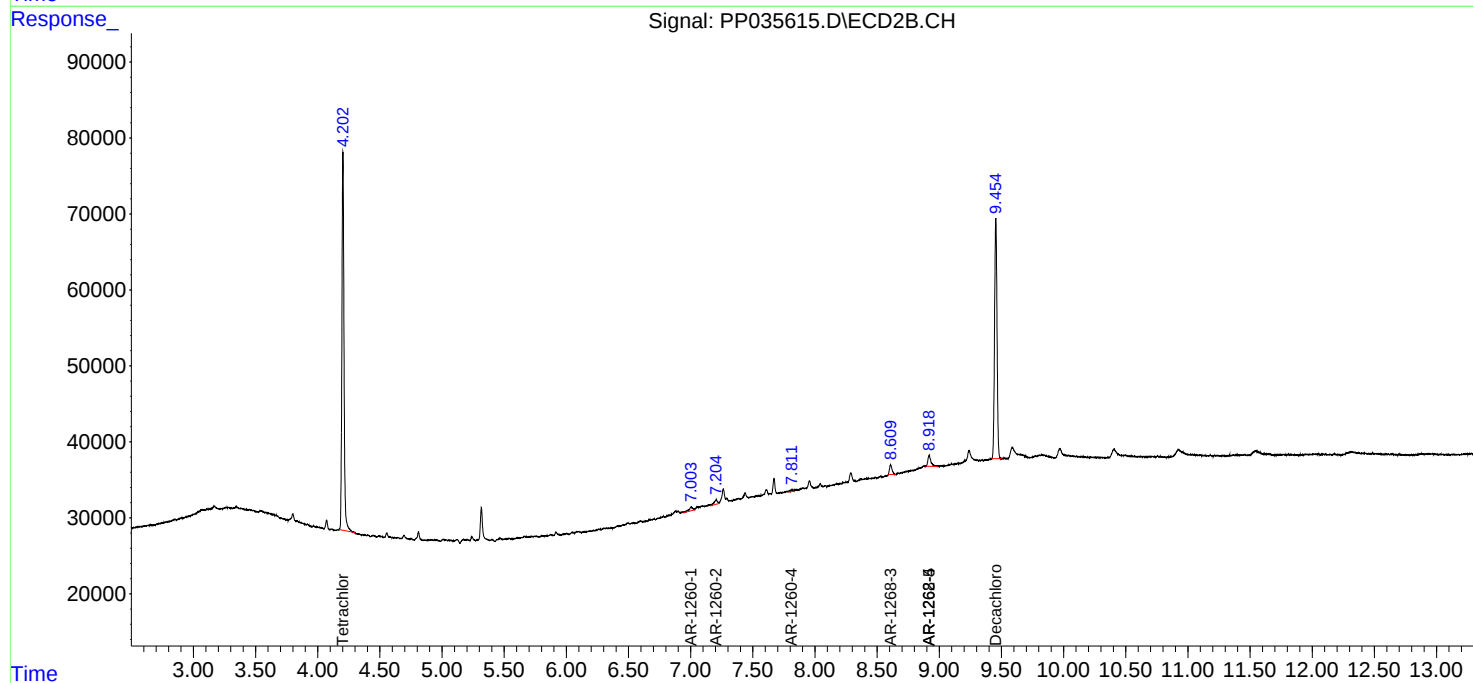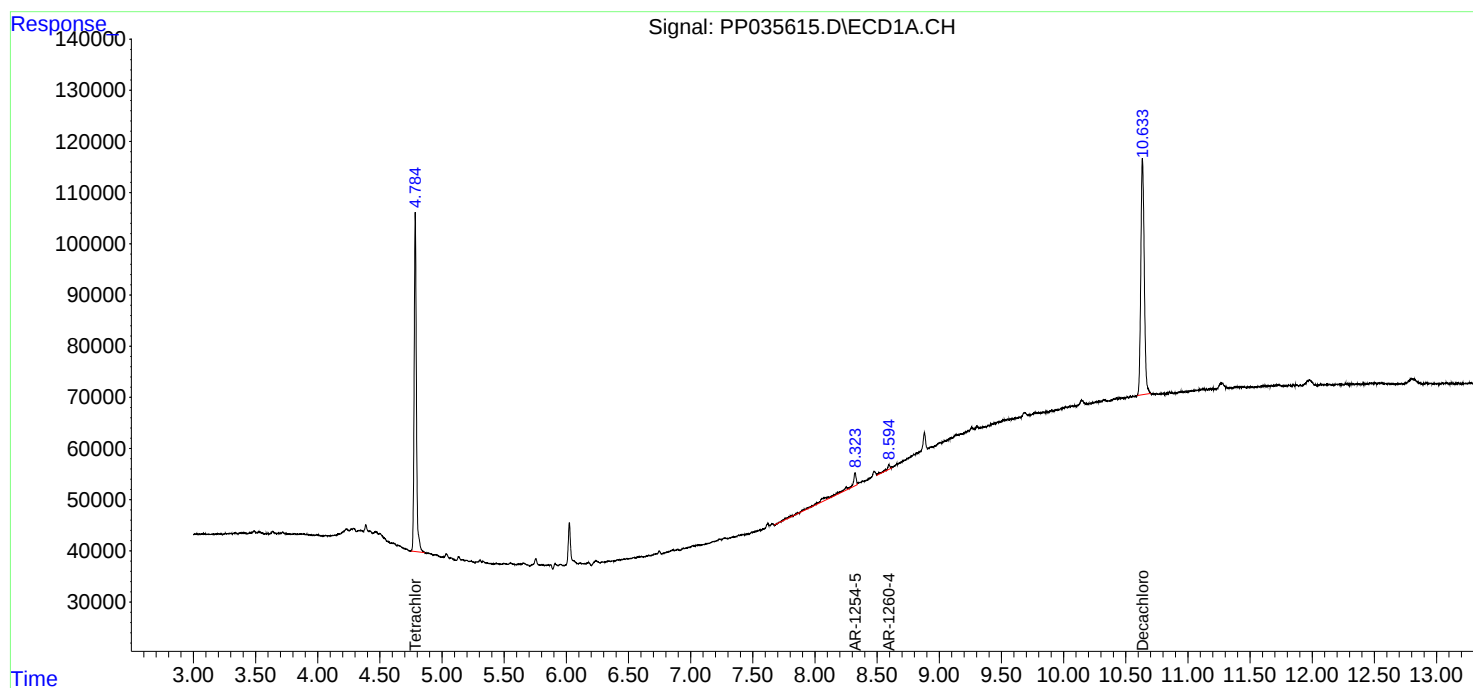


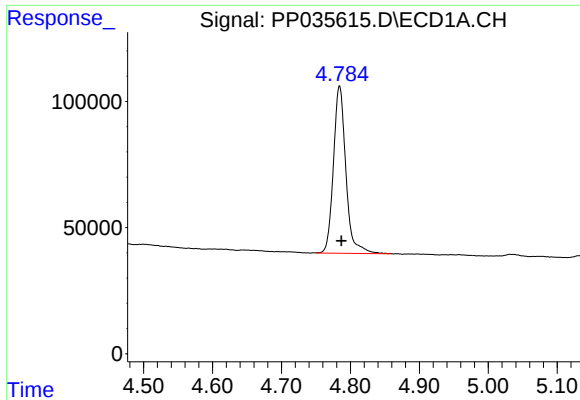

#1 Tetrachloro-m-xylene


R.T.: 4.784 min
Delta R.T.: -0.003 min
Response: 829829
Conc: 18.97 ng/ml

Instrument :
ECD_P
ClientSampleId :

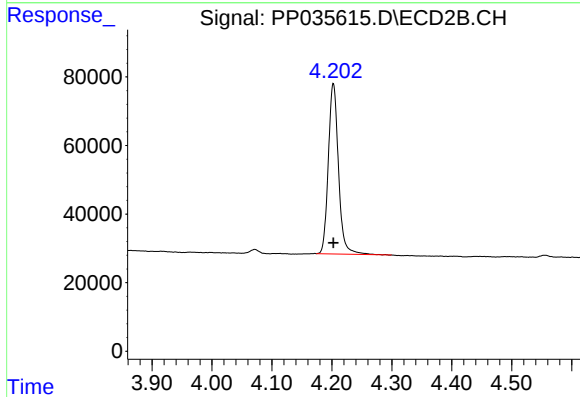


#1 Tetrachloro-m-xylene

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 584947
Conc: 19.28 ng/ml

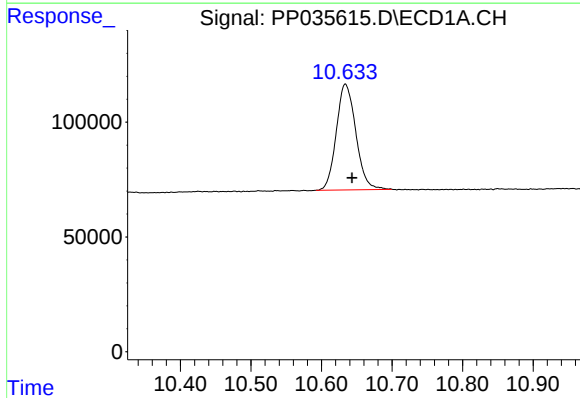


#2 Decachlorobiphenyl

R.T.: 10.634 min
Delta R.T.: -0.009 min
Response: 886583
Conc: 22.48 ng/ml

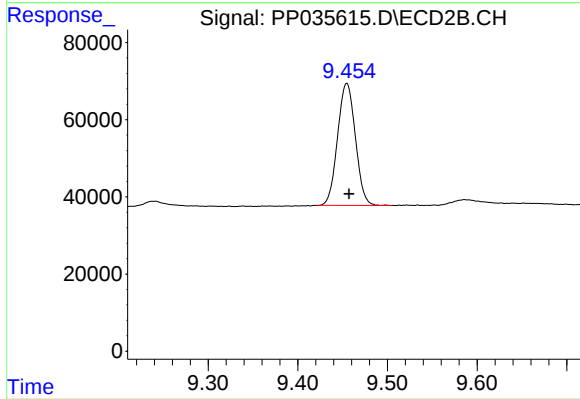

#2 Decachlorobiphenyl


R.T.: 9.455 min
Delta R.T.: -0.003 min
Response: 435717
Conc: 22.58 ng/ml

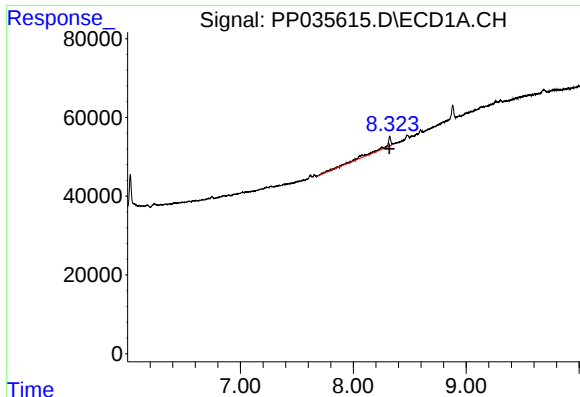

#30 AR-1254-5


R.T.: 8.323 min
Delta R.T.: 0.003 min
Response: 98610
Conc: 47.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

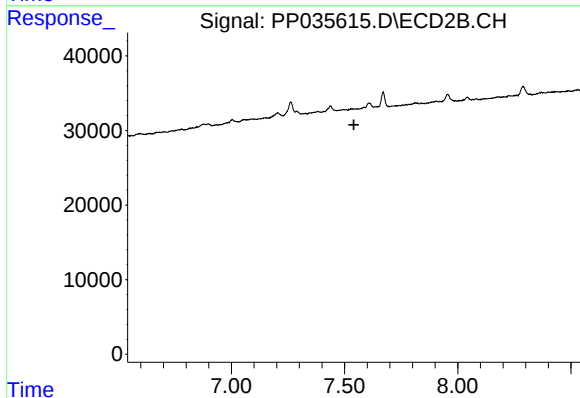


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.541 min
Response: 0
Conc: N.D.

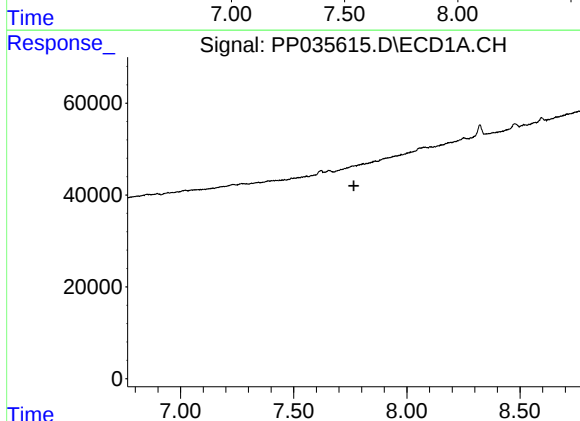


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.766 min
Response: 0
Conc: N.D.

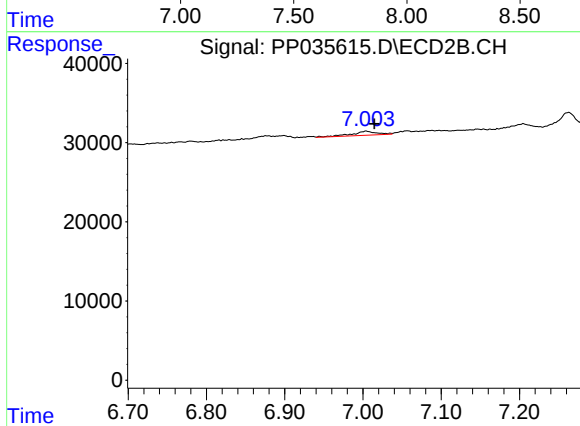

#31 AR-1260-1


R.T.: 7.004 min
Delta R.T.: -0.011 min
Response: 11212
Conc: 8.28 ng/ml

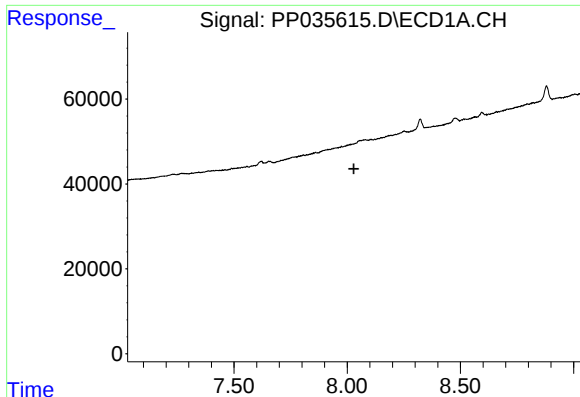

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

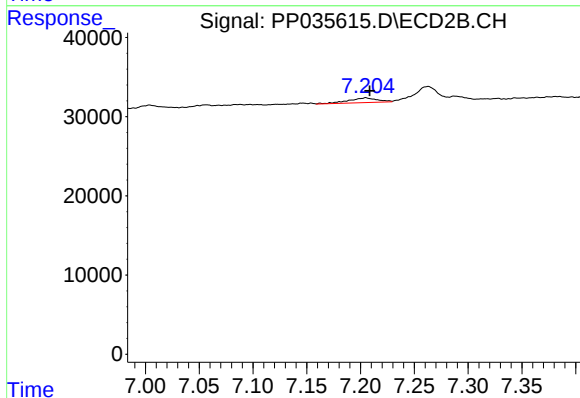


#32 AR-1260-2

R.T.: 7.205 min
Delta R.T.: -0.004 min
Response: 11274
Conc: 7.15 ng/ml

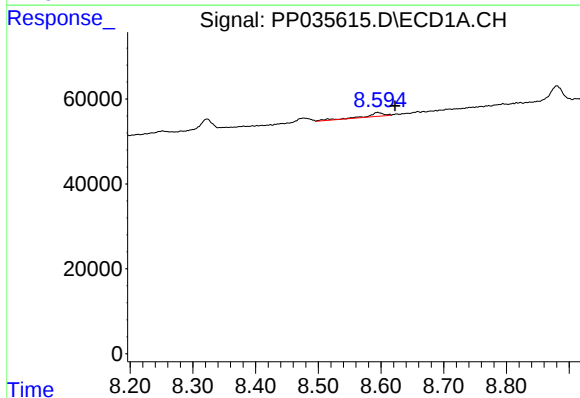


#34 AR-1260-4

R.T.: 8.595 min
Delta R.T.: -0.028 min
Response: 17931
Conc: 9.06 ng/ml

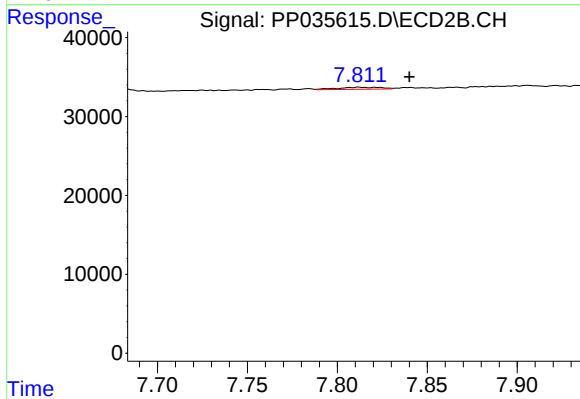

#34 AR-1260-4


R.T.: 7.812 min
Delta R.T.: -0.028 min
Response: 4453
Conc: 4.13 ng/ml

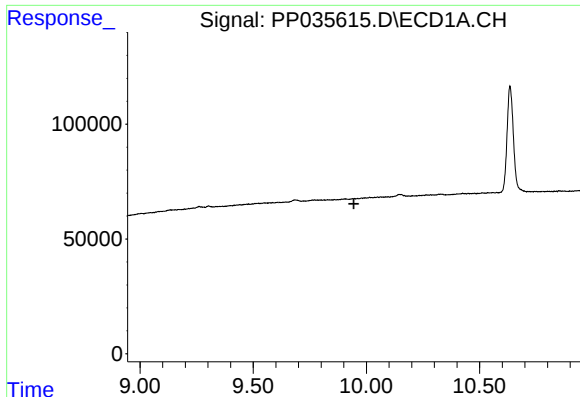

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

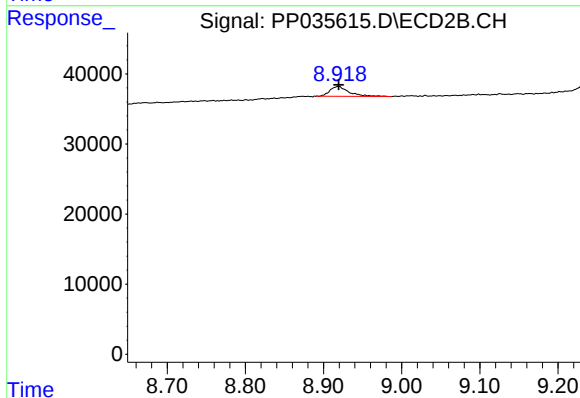


#40 AR-1262-5

R.T.: 8.919 min
Delta R.T.: 0.000 min
Response: 24262
Conc: 23.70 ng/ml

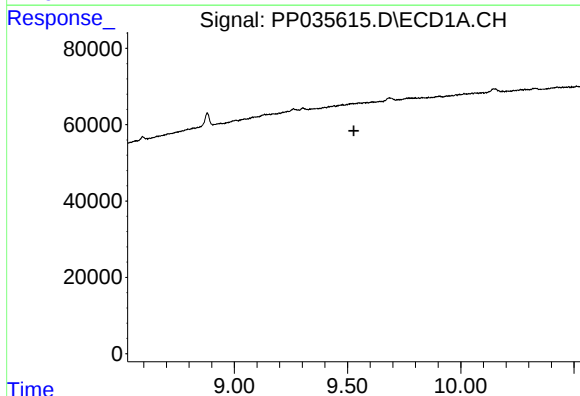


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.528 min
Response: 0
Conc: N.D.

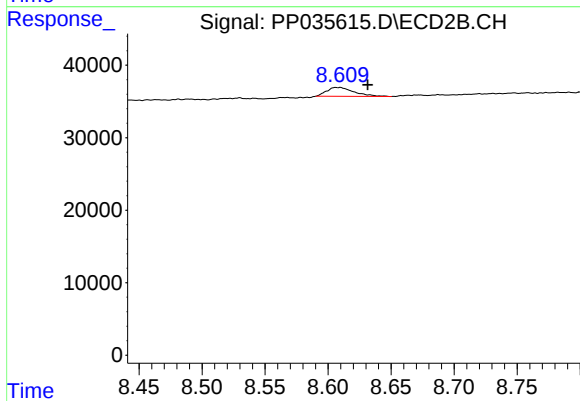

#43 AR-1268-3


R.T.: 8.608 min
Delta R.T.: -0.023 min
Response: 18508
Conc: 7.60 ng/ml

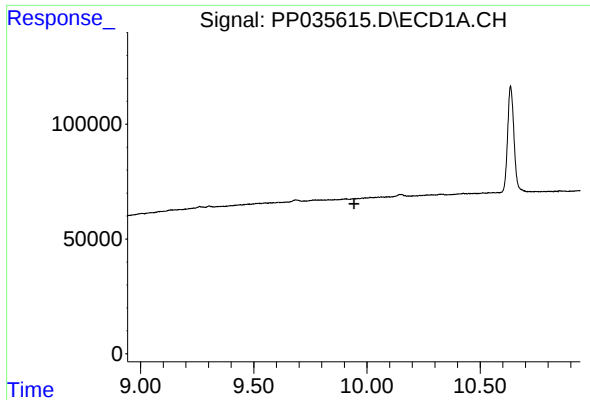

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

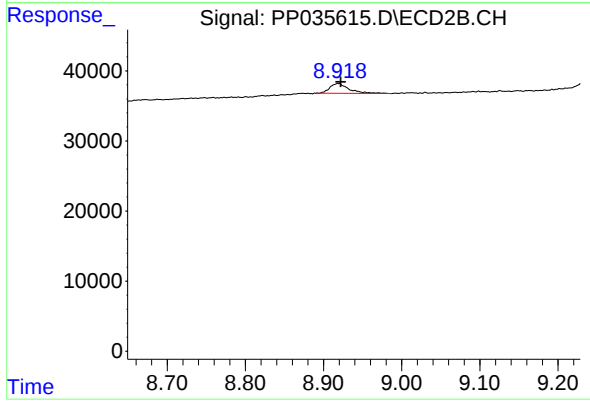

#44 AR-1268-4

R.T.: 8.919 min
Delta R.T.: -0.003 min
Response: 24262
Conc: 24.30 ng/ml