

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
 Data File : PP035621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2021 19:08
 Operator : DD\AJ
 Sample : M2295-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:57:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.784	4.202	870088	655124	19.887	21.597
2) SA Decachlor...	10.636	9.454	620575	321270	15.733	16.651
Target Compounds						
28) L6 AR-1254-3	7.619f	0.000	7353	0	2.840	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 19:08
Operator : DD\AJ
Sample : M2295-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:57:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

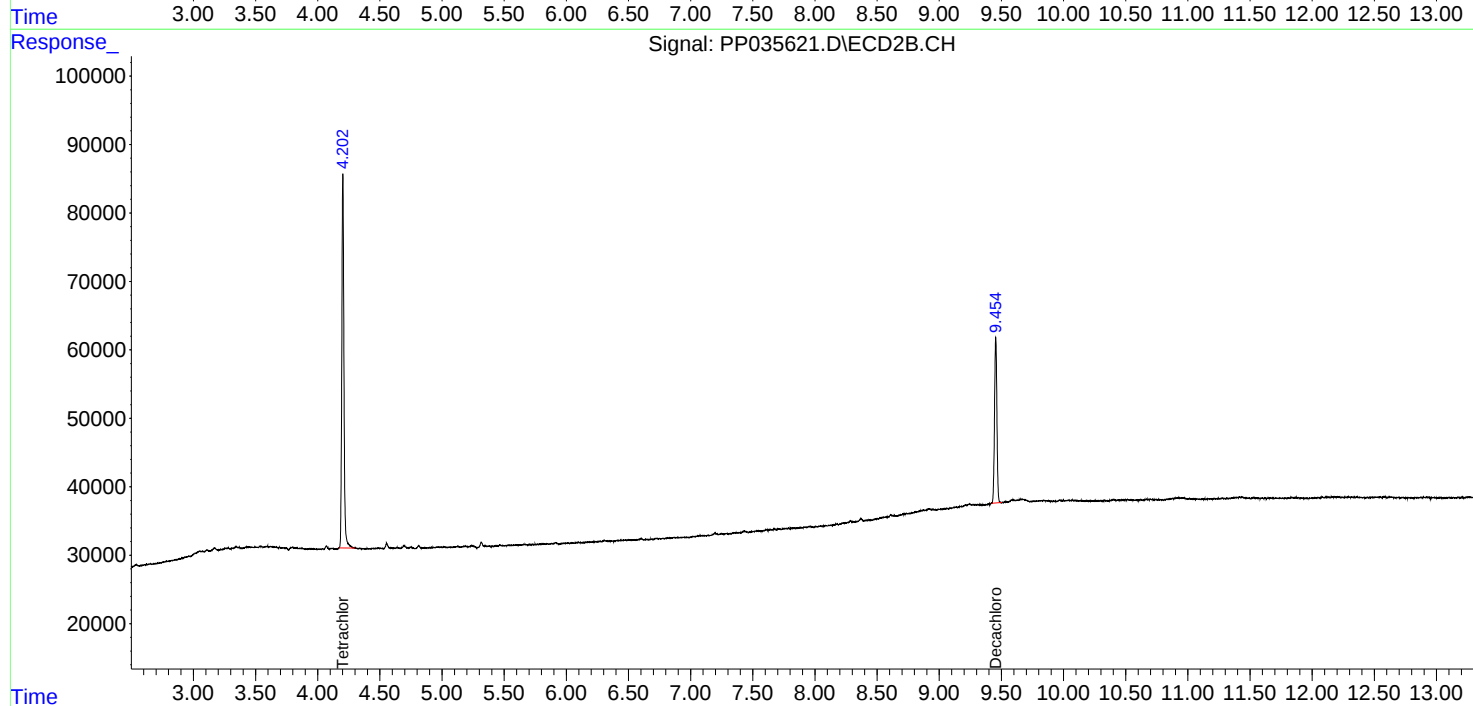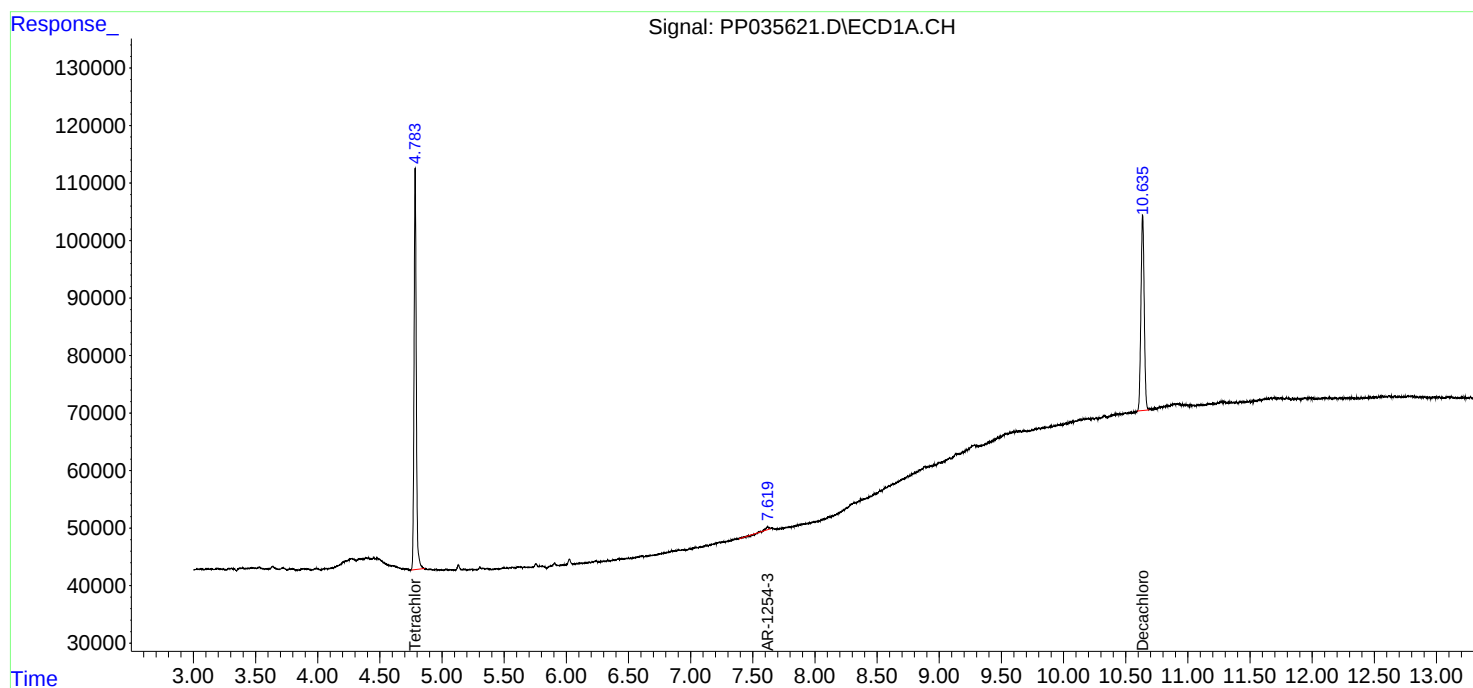


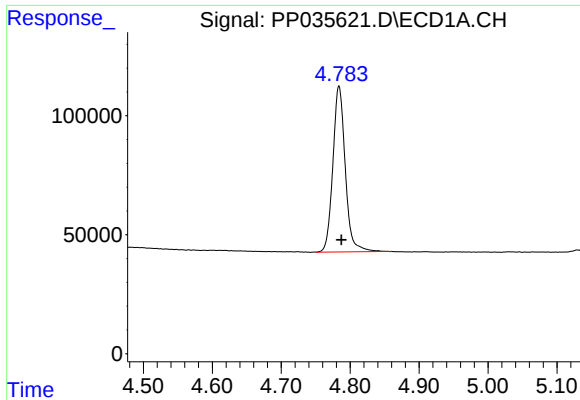

#1 Tetrachloro-m-xylene


R.T.: 4.784 min
Delta R.T.: -0.003 min
Response: 870088
Conc: 19.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

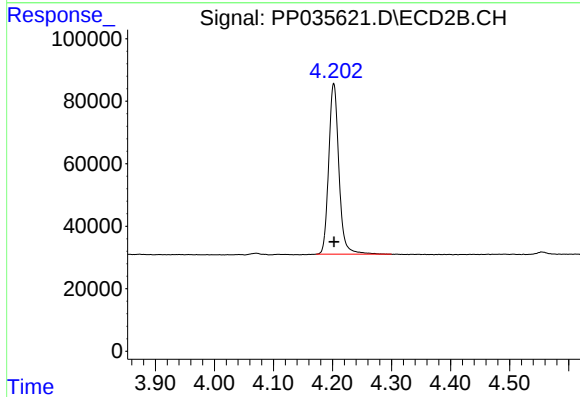


#1 Tetrachloro-m-xylene

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 655124
Conc: 21.60 ng/ml

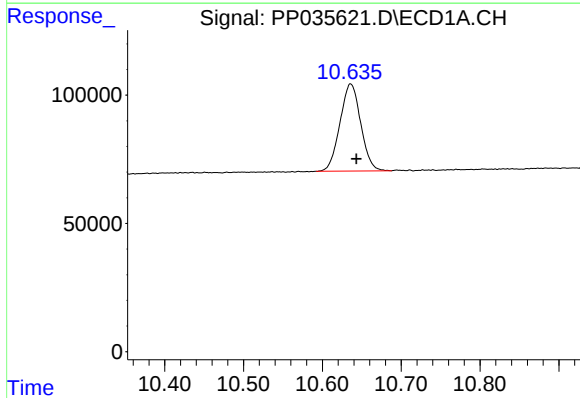


#2 Decachlorobiphenyl

R.T.: 10.636 min
Delta R.T.: -0.007 min
Response: 620575
Conc: 15.73 ng/ml

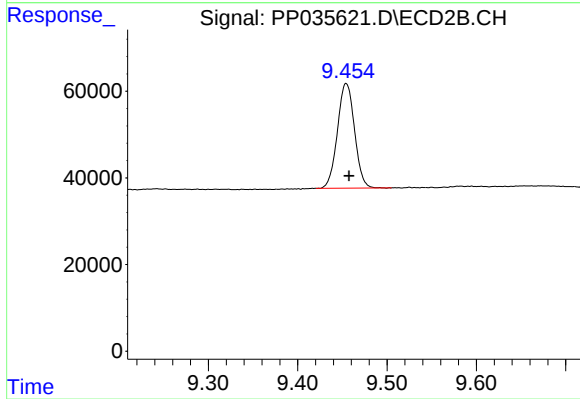

#2 Decachlorobiphenyl


R.T.: 9.454 min
Delta R.T.: -0.003 min
Response: 321270
Conc: 16.65 ng/ml

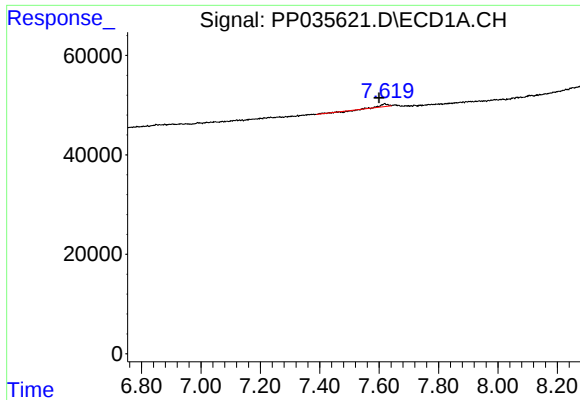

#28 AR-1254-3

R.T.: 7.619 min
Delta R.T.: 0.019 min
Response: 7353
Conc: 2.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

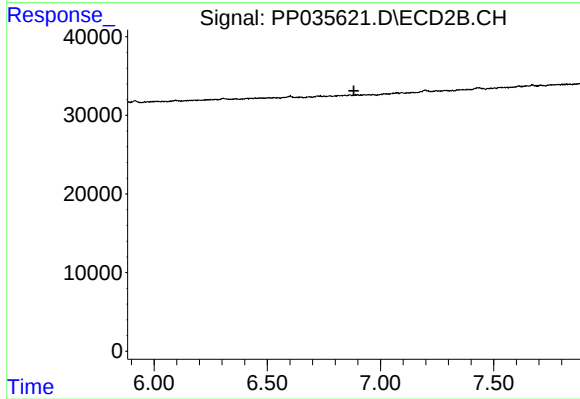

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.883 min
Response: 0
Conc: N.D.