

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
 Data File : PP035607.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2021 15:11
 Operator : DD\AJ
 Sample : M2266-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT-016

Manual Integrations
 APPROVED

Ankita
 5/7/2021 2:05:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 17:10:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.784	4.202	947718	716366	21.661	23.616
2) SA Decachlor...	10.636	9.454	886251	440748	22.469	22.844m
Target Compounds						
31) L7 AR-1260-1	7.761	7.012	407122	64033	187.893m	47.271 #
32) L7 AR-1260-2	8.025	7.206	155630	75684	63.274	47.981
33) L7 AR-1260-3	8.390	7.361	102821	60300	63.427	40.403 #
34) L7 AR-1260-4	8.618	7.837	155823	63620	78.716	59.054
35) L7 AR-1260-5	8.933	8.082	232312	137842	62.887	57.962

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 15:11
Operator : DD\AJ
Sample : M2266-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
CRT-016


Manual Integrations
APPROVED

Ankita
5/7/2021 2:05:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 17:10:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

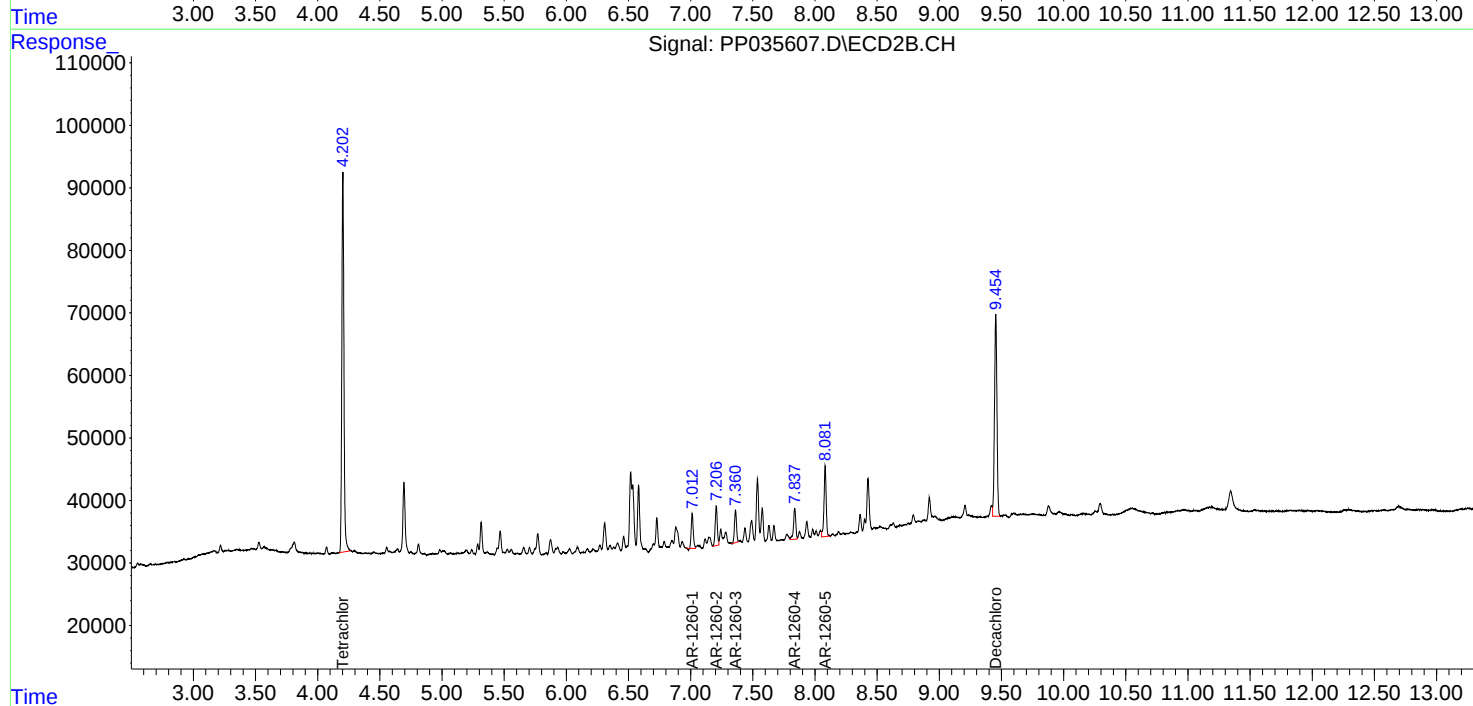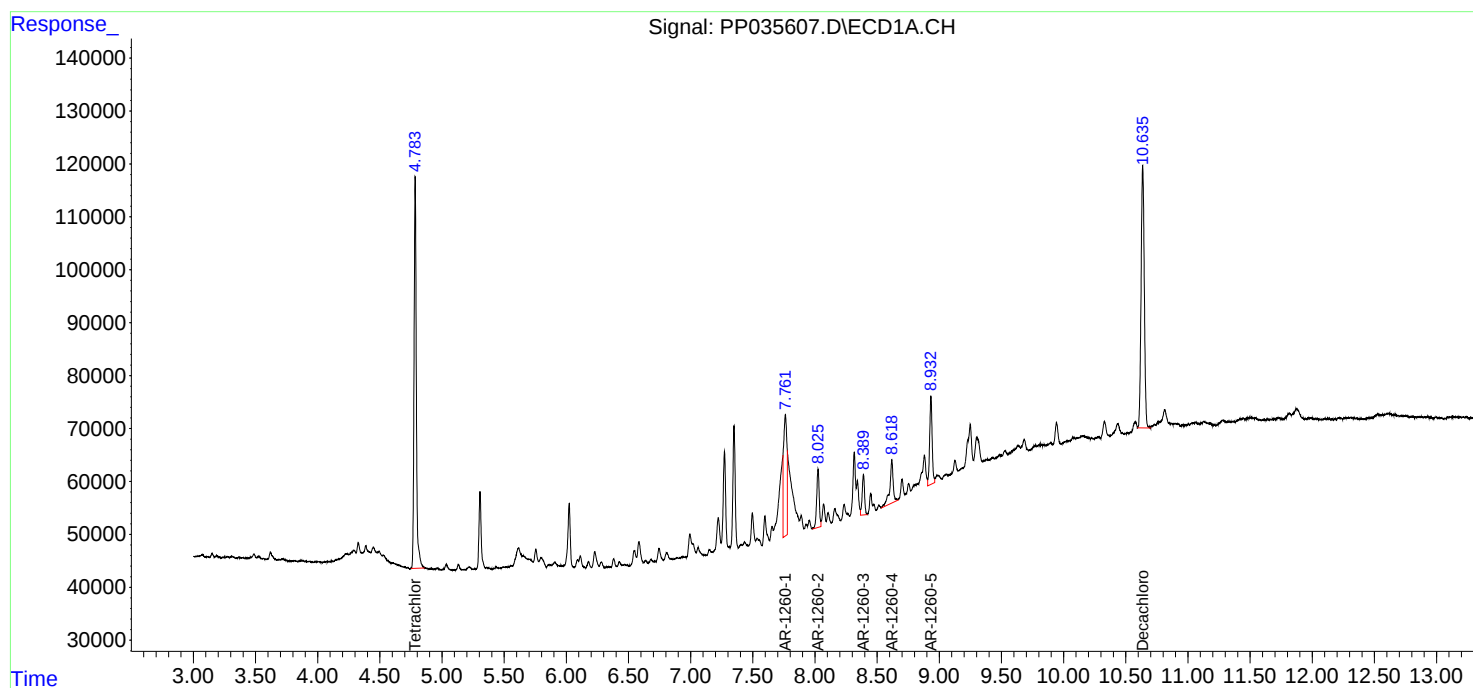

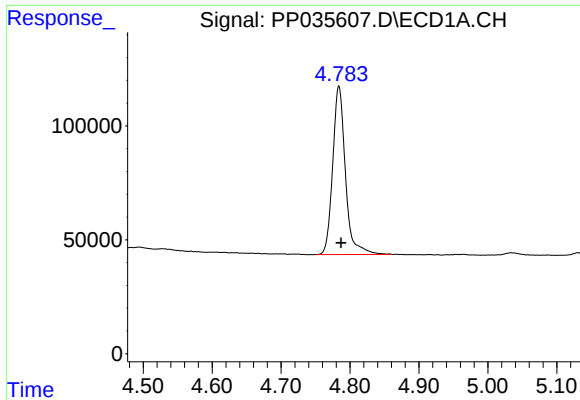


#1 Tetrachloro-m-xylene

R.T.: 4.784 min
Delta R.T.: -0.003 min
Response: 947718
Conc: 21.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/7/2021 2:05:20 PM

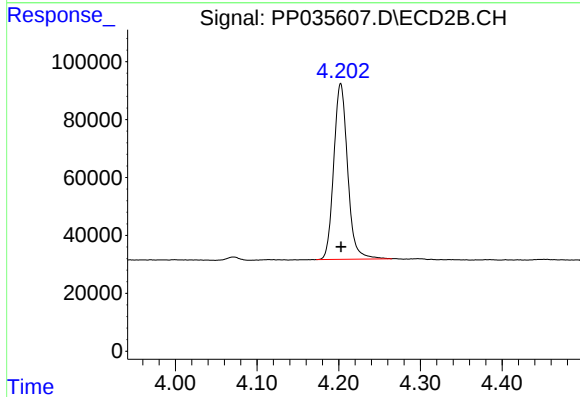


#1 Tetrachloro-m-xylene

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 716366
Conc: 23.62 ng/ml

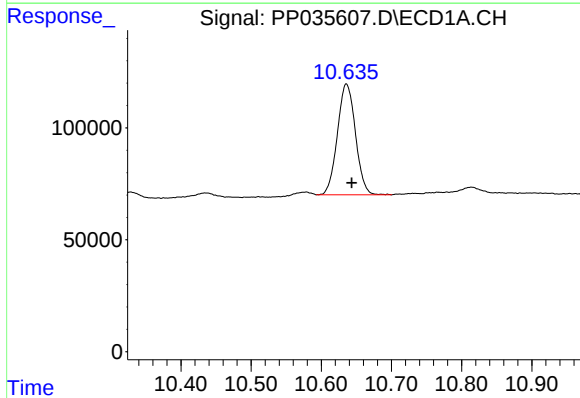


#2 Decachlorobiphenyl

R.T.: 10.636 min
Delta R.T.: -0.007 min
Response: 886251
Conc: 22.47 ng/ml

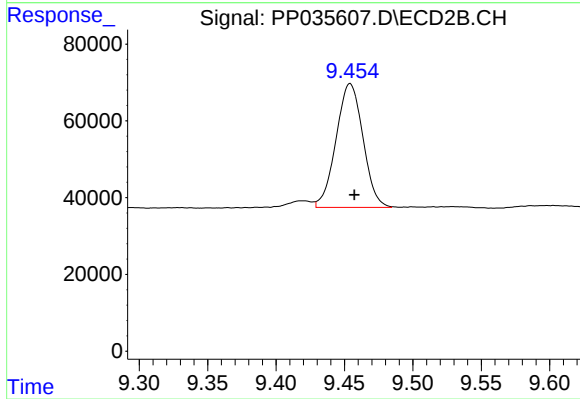

#2 Decachlorobiphenyl

R.T.: 9.454 min
Delta R.T.: -0.004 min
Response: 440748
Conc: 22.84 ng/ml m

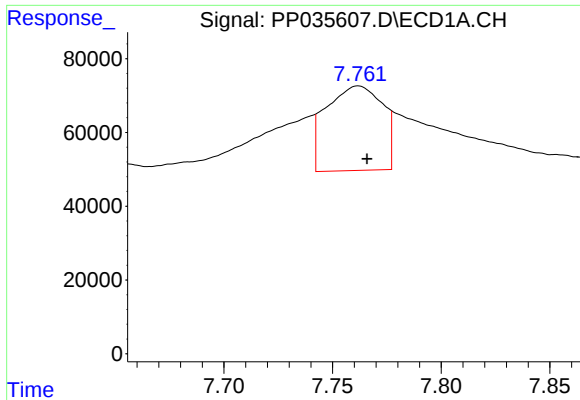


#31 AR-1260-1

R.T.: 7.761 min
Delta R.T.: -0.004 min
Response: 407122
Conc: 187.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/7/2021 2:05:20 PM

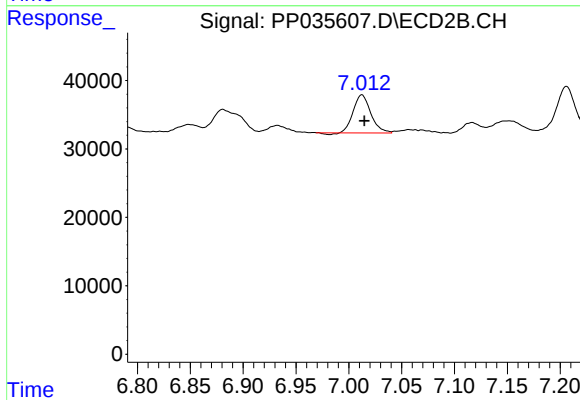


#31 AR-1260-1

R.T.: 7.012 min
Delta R.T.: -0.003 min
Response: 64033
Conc: 47.27 ng/ml

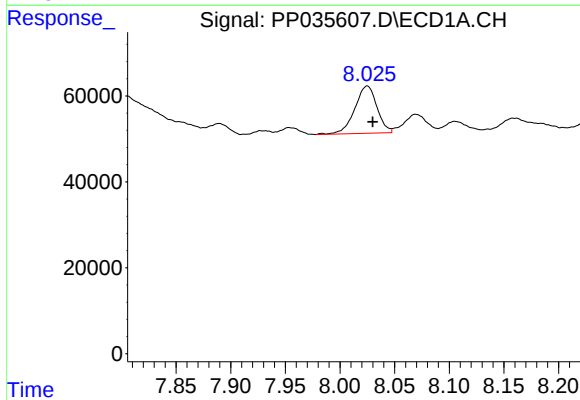


#32 AR-1260-2

R.T.: 8.025 min
Delta R.T.: -0.005 min
Response: 155630
Conc: 63.27 ng/ml

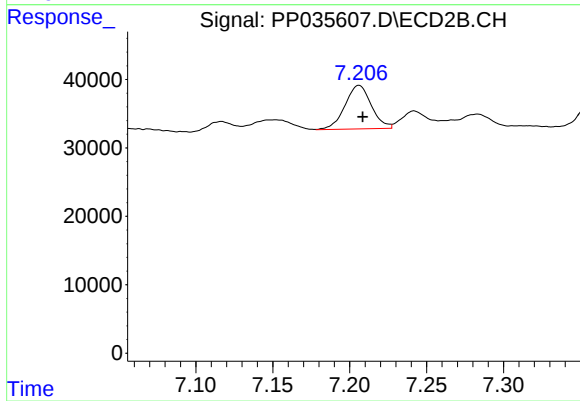

#32 AR-1260-2

R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 75684
Conc: 47.98 ng/ml

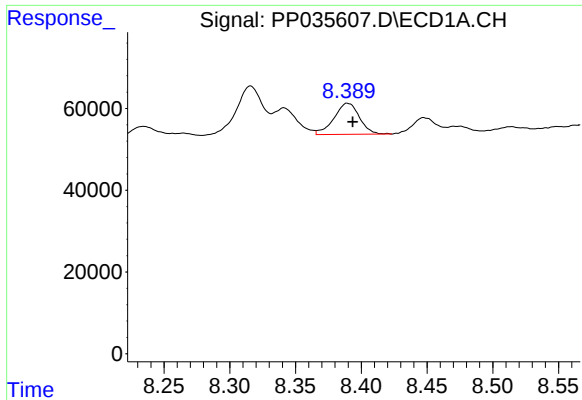


#33 AR-1260-3

R.T.: 8.390 min
Delta R.T.: -0.004 min
Response: 102821
Conc: 63.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/7/2021 2:05:20 PM

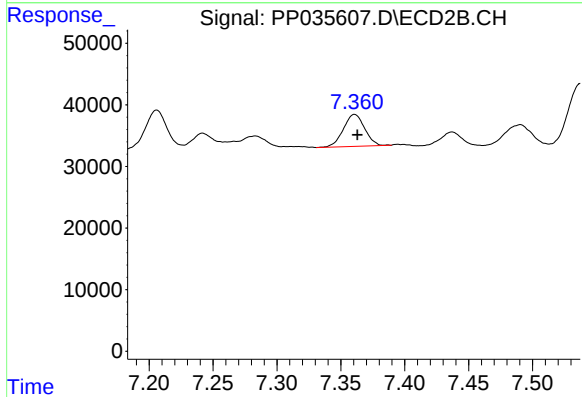


#33 AR-1260-3

R.T.: 7.361 min
Delta R.T.: -0.002 min
Response: 60300
Conc: 40.40 ng/ml

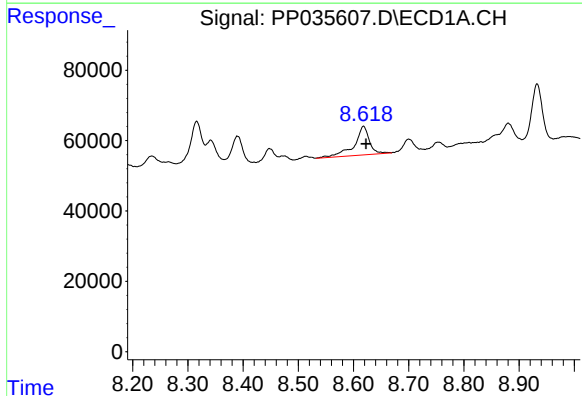


#34 AR-1260-4

R.T.: 8.618 min
Delta R.T.: -0.005 min
Response: 155823
Conc: 78.72 ng/ml

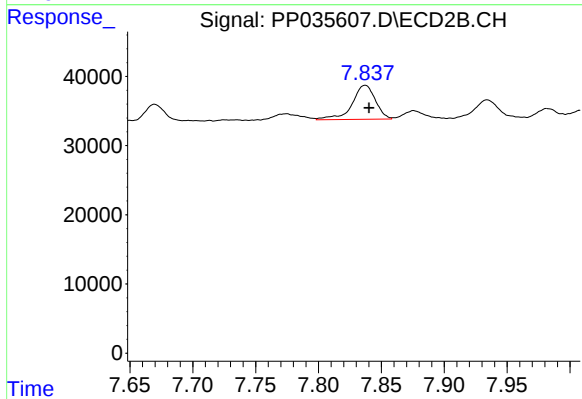

#34 AR-1260-4

R.T.: 7.837 min
Delta R.T.: -0.003 min
Response: 63620
Conc: 59.05 ng/ml

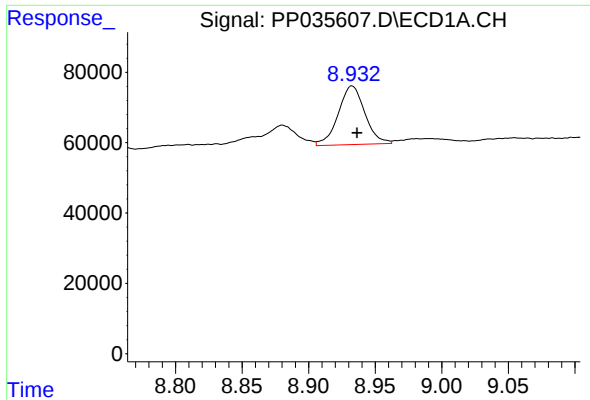


#35 AR-1260-5

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 232312
Conc: 62.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016

Manual Integrations
APPROVED

Ankita
5/7/2021 2:05:20 PM

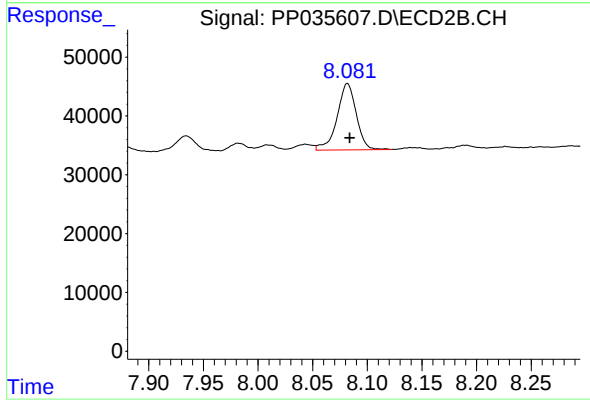

#35 AR-1260-5

R.T.: 8.082 min
Delta R.T.: -0.002 min
Response: 137842
Conc: 57.96 ng/ml