

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035630.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 21:56
Operator : DD\AJ
Sample : M2306-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
C-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:59:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.783	4.202	985627	750760	22.528	24.749
2) SA Decachlor...	10.635	9.453	901082	462878	22.845	23.991

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035630.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2021 21:56
Operator : DD\AJ
Sample : M2306-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
C-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:59:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

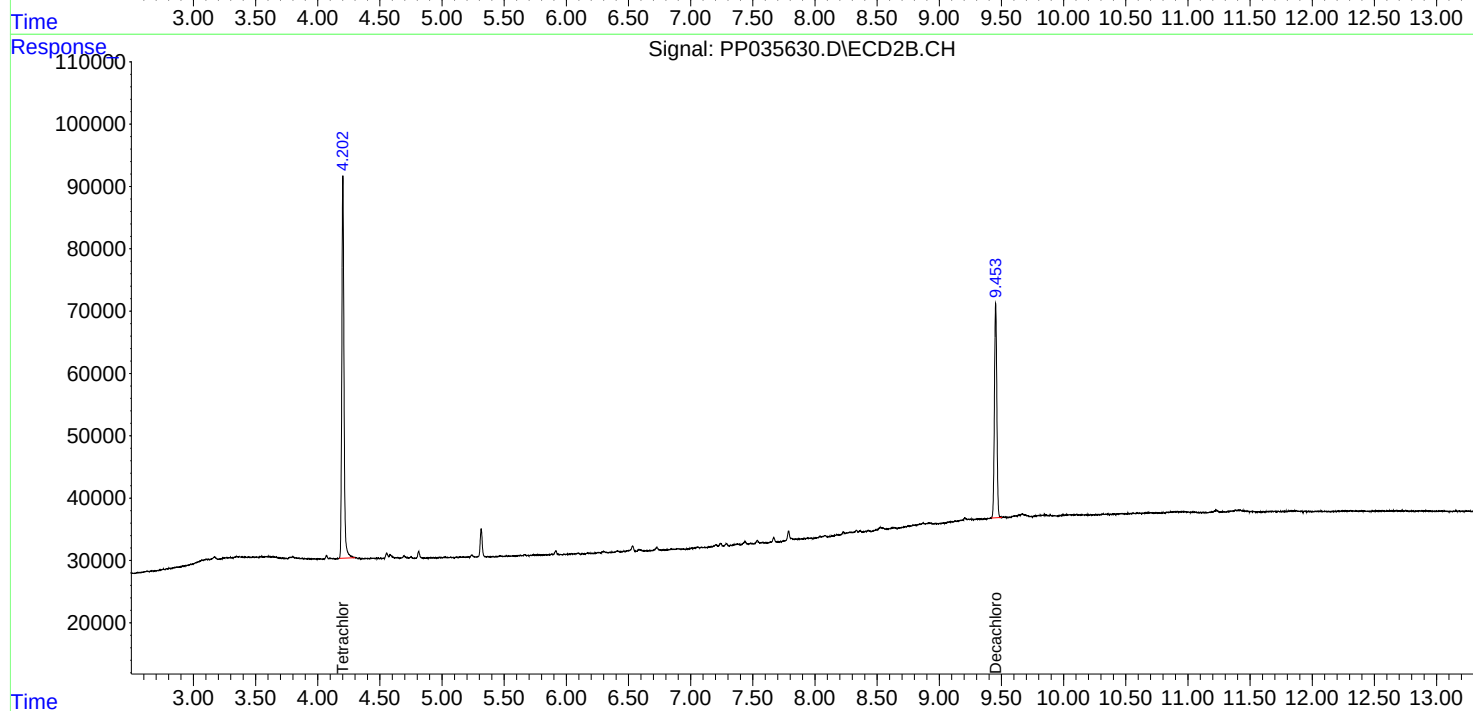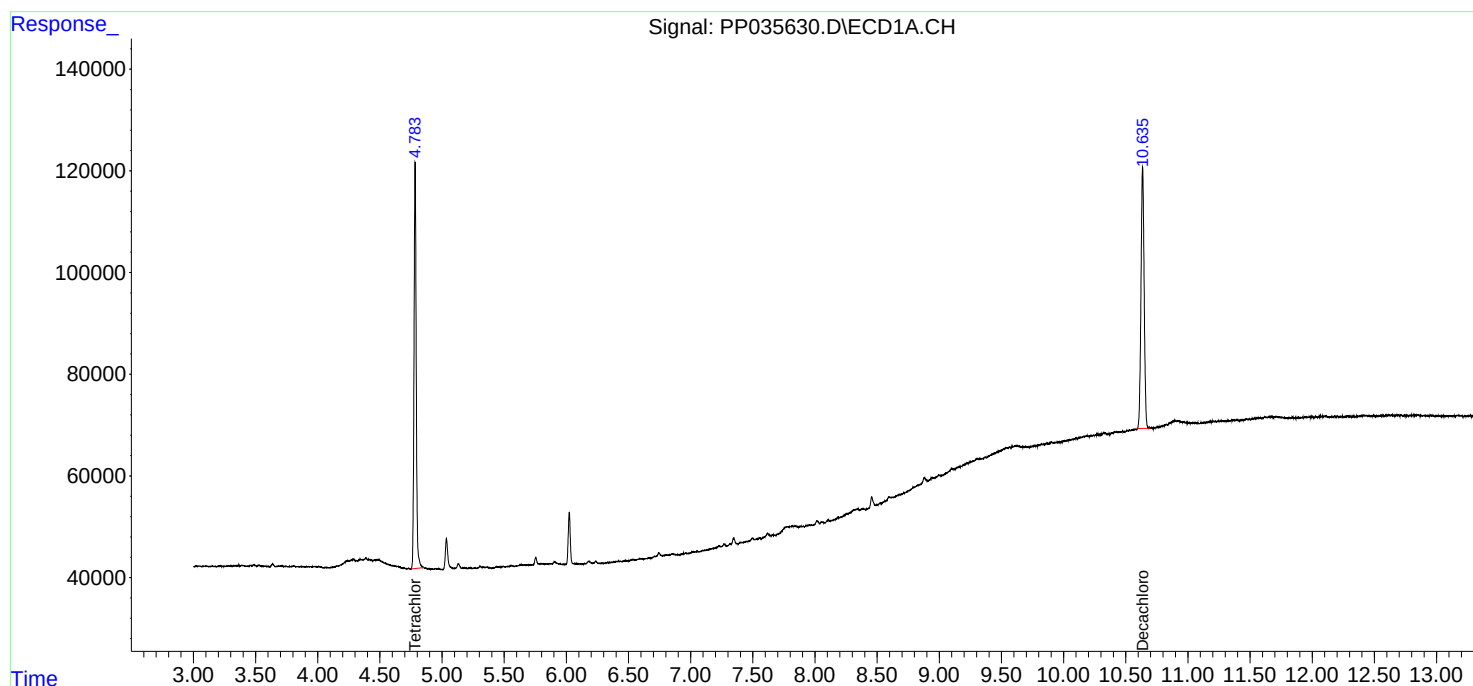


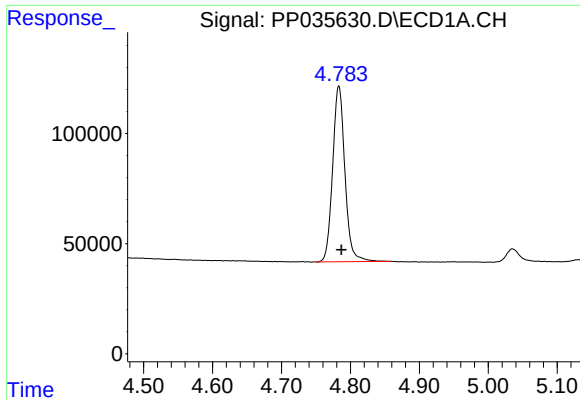

#1 Tetrachloro-m-xylene


R.T.: 4.783 min
Delta R.T.: -0.004 min
Response: 985627
Conc: 22.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
C-1

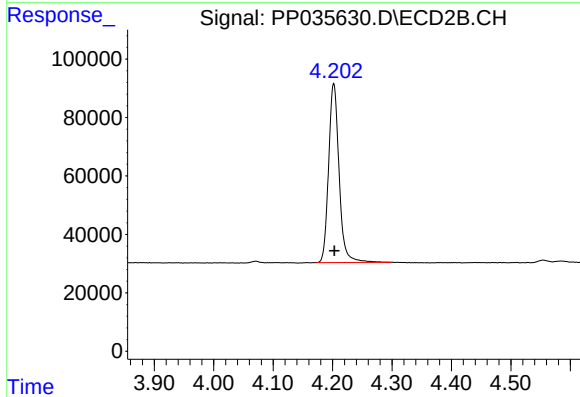


#1 Tetrachloro-m-xylene

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 750760
Conc: 24.75 ng/ml

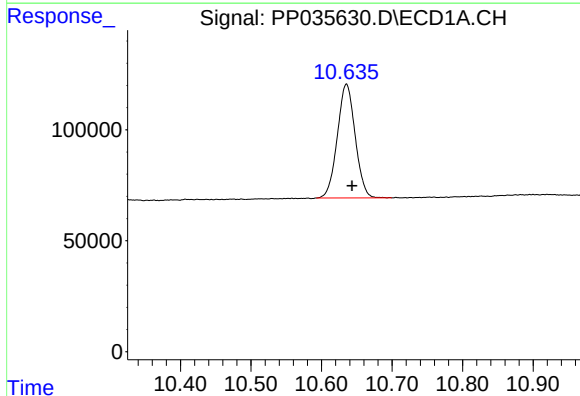

#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.008 min
Response: 901082
Conc: 22.85 ng/ml

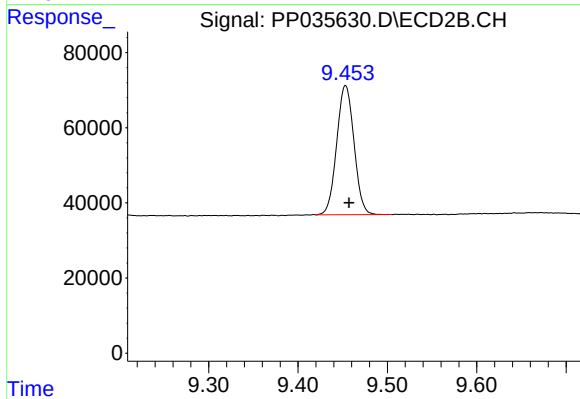

#2 Decachlorobiphenyl

R.T.: 9.453 min
Delta R.T.: -0.004 min
Response: 462878
Conc: 23.99 ng/ml