

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
 Data File : PP035660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2021 7:42
 Operator : DD\AJ
 Sample : M2273-15 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HED160B-1-1

Manual Integrations
 APPROVED

Ankita
 5/11/2021 1:39:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 09:08:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.783	4.201	77170	54937	1.764	1.811m
2) SA Decachlor...	10.631	9.453	88345	35830	2.240	1.857

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050621\
Data File : PP035660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2021 7:42
Operator : DD\AJ
Sample : M2273-15 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HED160B-1-1


Manual Integrations
APPROVED

Ankita
5/11/2021 1:39:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 09:08:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

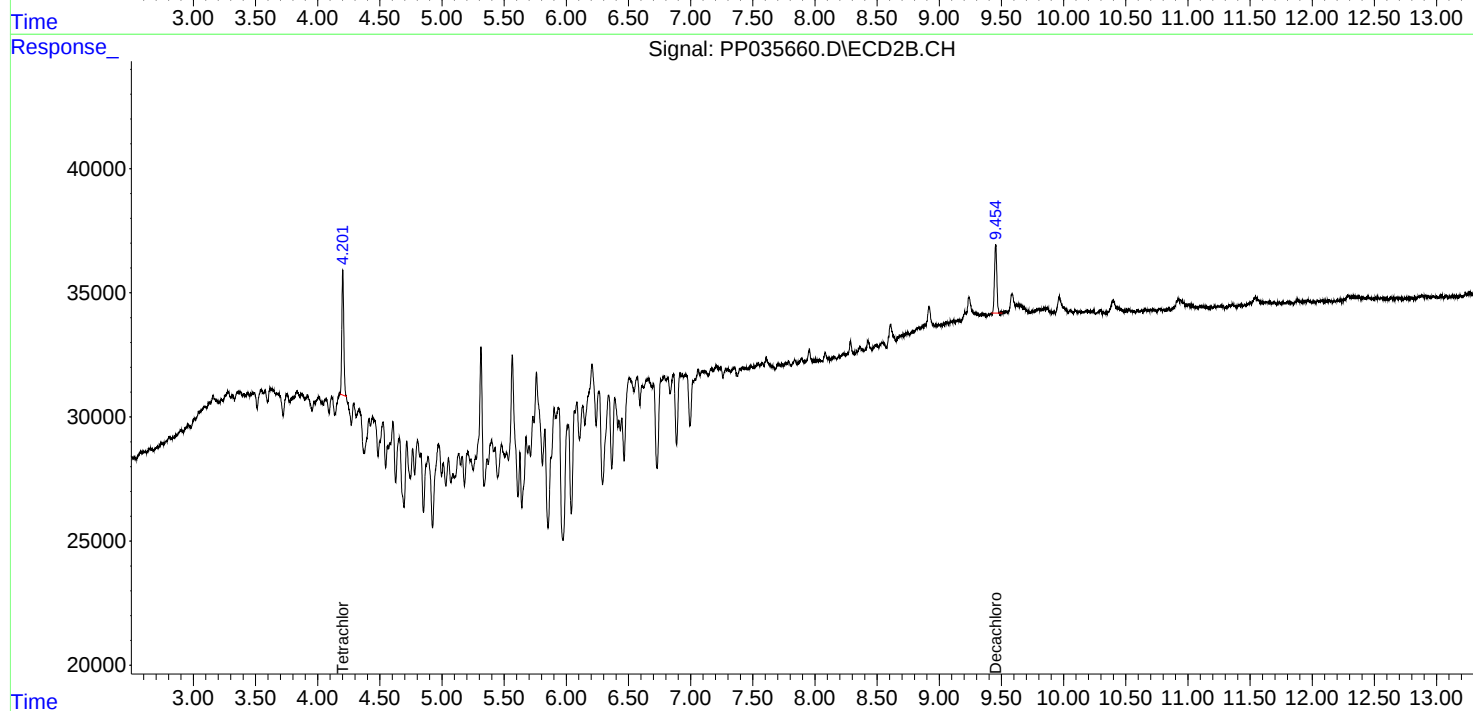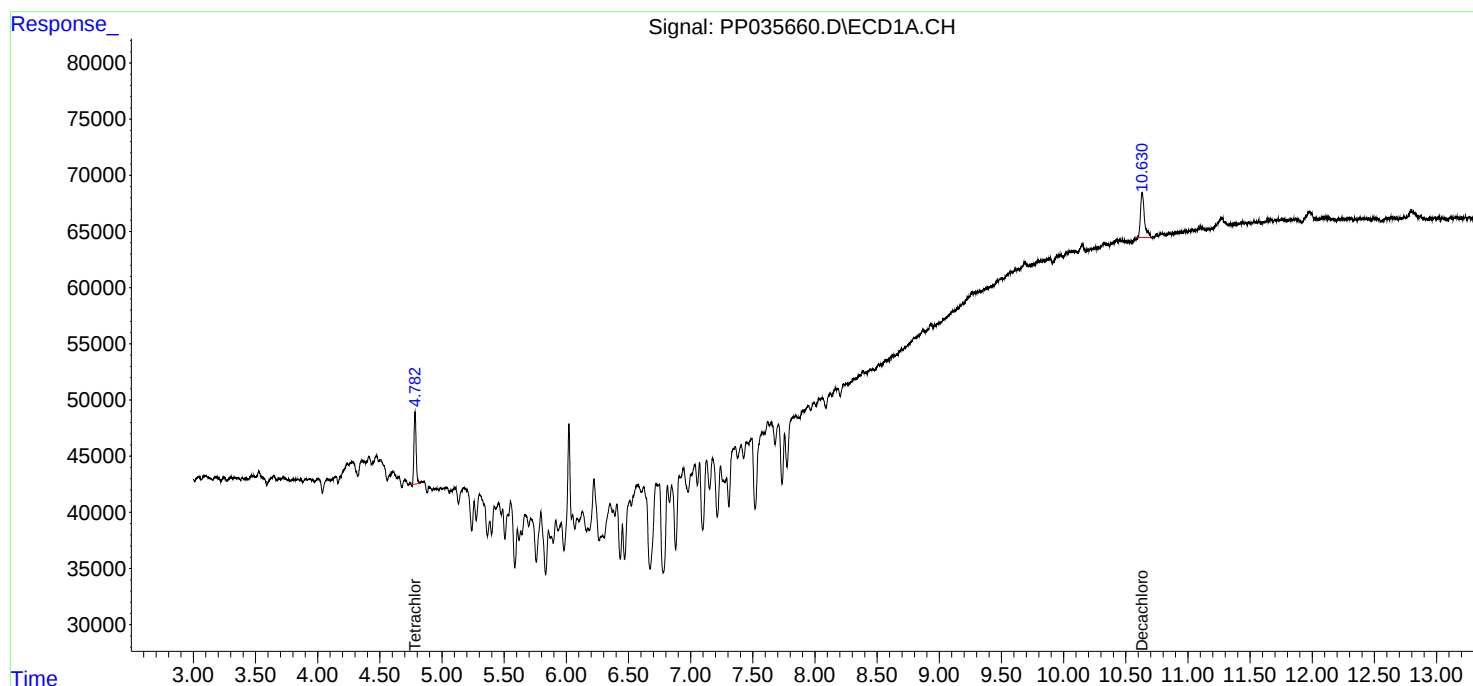

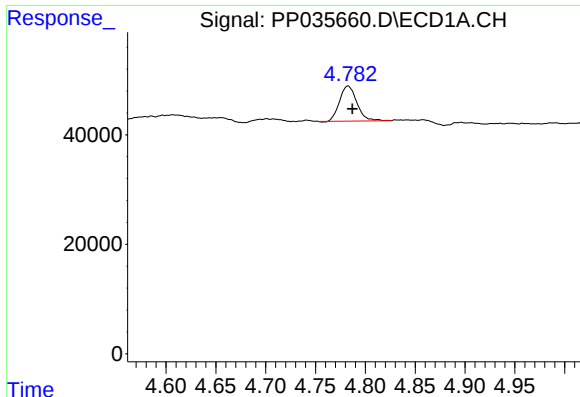


#1 Tetrachloro-m-xylene

R.T.: 4.783 min
Delta R.T.: -0.004 min
Response: 77170
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
HED160B-1-1


Manual Integrations
APPROVED

Ankita
5/11/2021 1:39:45 PM

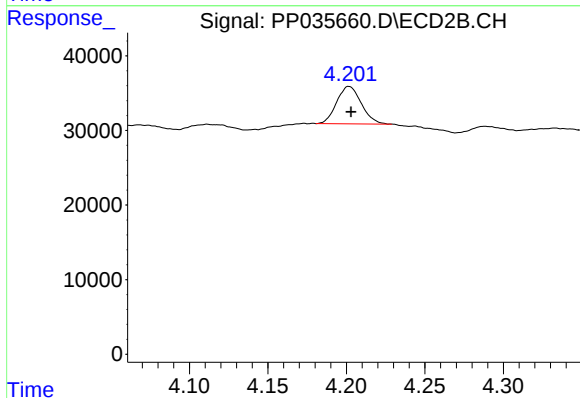


#1 Tetrachloro-m-xylene

R.T.: 4.201 min
Delta R.T.: -0.002 min
Response: 54937
Conc: 1.81 ng/ml m

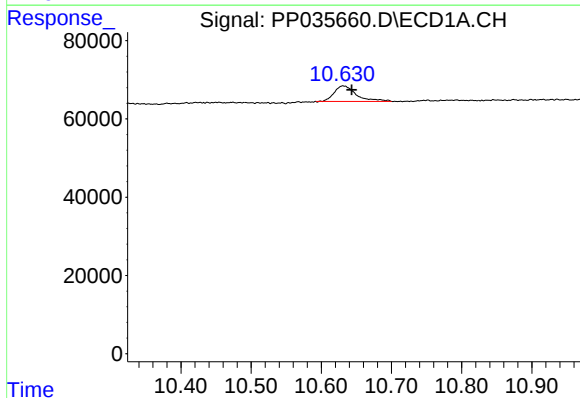

#2 Decachlorobiphenyl

R.T.: 10.631 min
Delta R.T.: -0.012 min
Response: 88345
Conc: 2.24 ng/ml

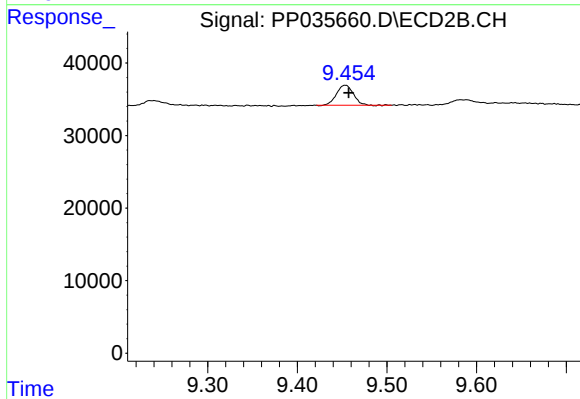

#2 Decachlorobiphenyl

R.T.: 9.453 min
Delta R.T.: -0.004 min
Response: 35830
Conc: 1.86 ng/ml