

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050622\
 Data File : PP047120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 16:30
 Operator : YP\AJ
 Sample : N2619-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB03-13-14-FT

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/09/2022
 Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 17:48:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.854	3.121	43458147	55383788	18.003m	16.883m
2) SA Decachlor...	9.922	8.429	22329606	37503302	15.175	15.723

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050622\
Data File : PP047120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 16:30
Operator : YP\AJ
Sample : N2619-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB03-13-14-FT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 17:48:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

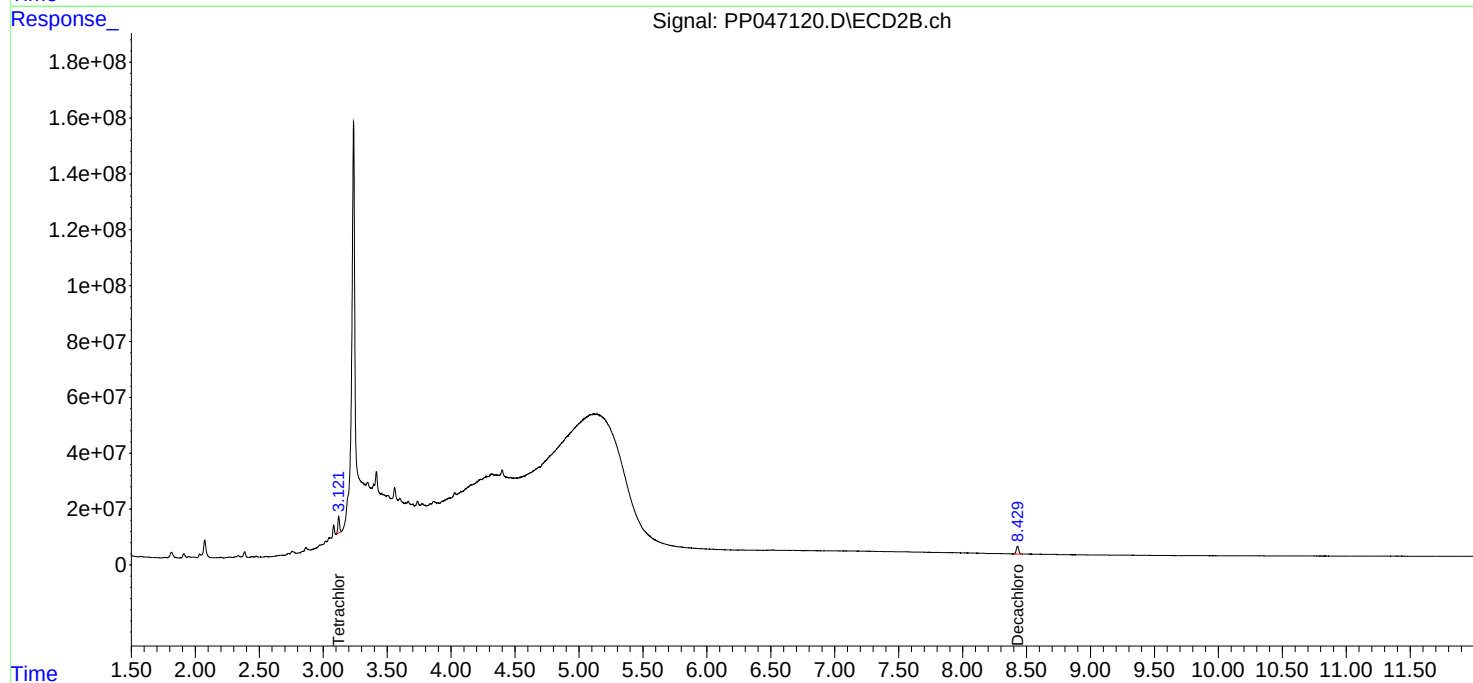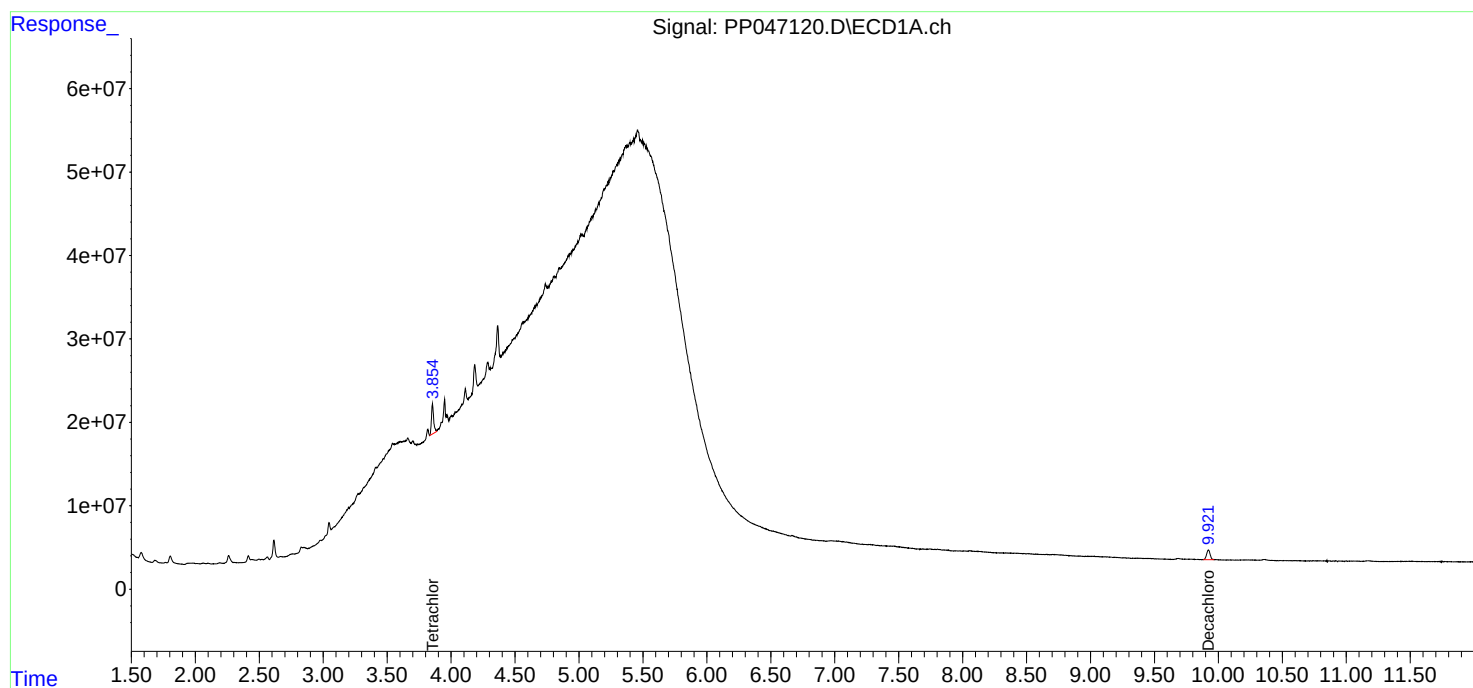

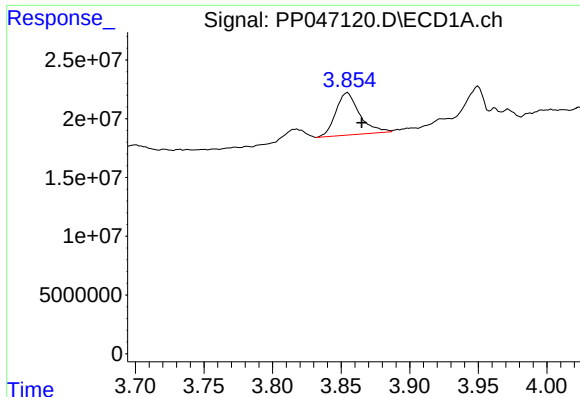


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.011 min
Response: 43458147
Conc: 18.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB03-13-14-FT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

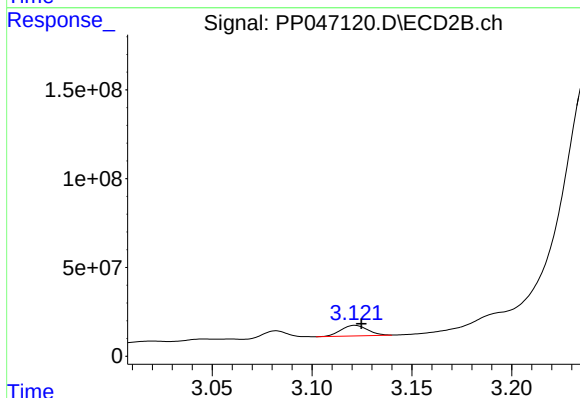


#1 Tetrachloro-m-xylene

R.T.: 3.121 min
Delta R.T.: -0.004 min
Response: 55383788
Conc: 16.88 ng/ml m

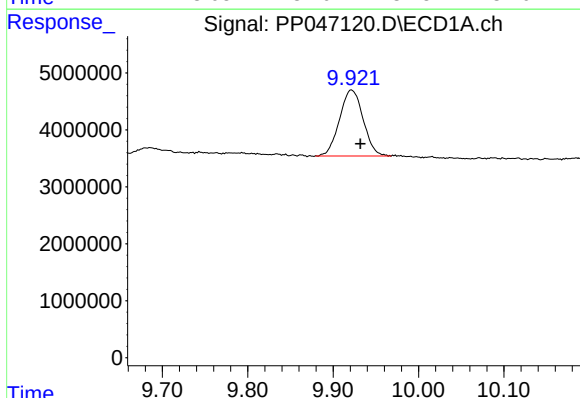

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.010 min
Response: 22329606
Conc: 15.17 ng/ml

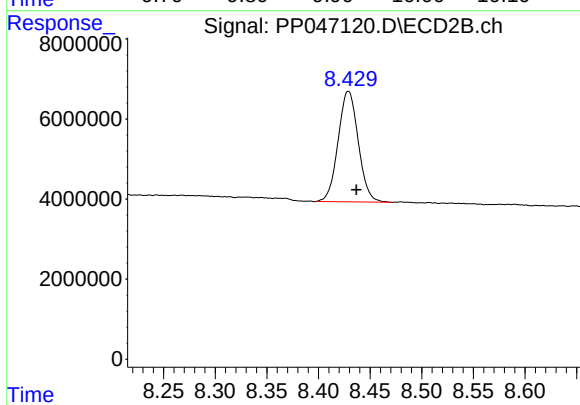

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: -0.008 min
Response: 37503302
Conc: 15.72 ng/ml