

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
 Data File : PP035669.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2021 10:32
 Operator : DD\AJ
 Sample : M2266-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT-016

Manual Integrations
 APPROVED

Ankita
 5/10/2021 2:04:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 16:50:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.784	4.203	971221	722434	22.198	23.816
2) SA Decachlor...	10.634	9.452	956836	494723	24.259	25.642m
Target Compounds						
31) L7 AR-1260-1	7.760	7.012	97102	87636	44.814m	64.696 #
32) L7 AR-1260-2	8.023	7.204	163563	124483	66.499	78.917
33) L7 AR-1260-3	8.389	7.360	107244	70140	66.156	46.997 #
34) L7 AR-1260-4	8.617	7.836	116903	79102	59.055m	73.426
35) L7 AR-1260-5	8.931	8.081	245636	163428	66.494	68.721

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
Data File : PP035669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2021 10:32
Operator : DD\AJ
Sample : M2266-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
CRT-016


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 16:50:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

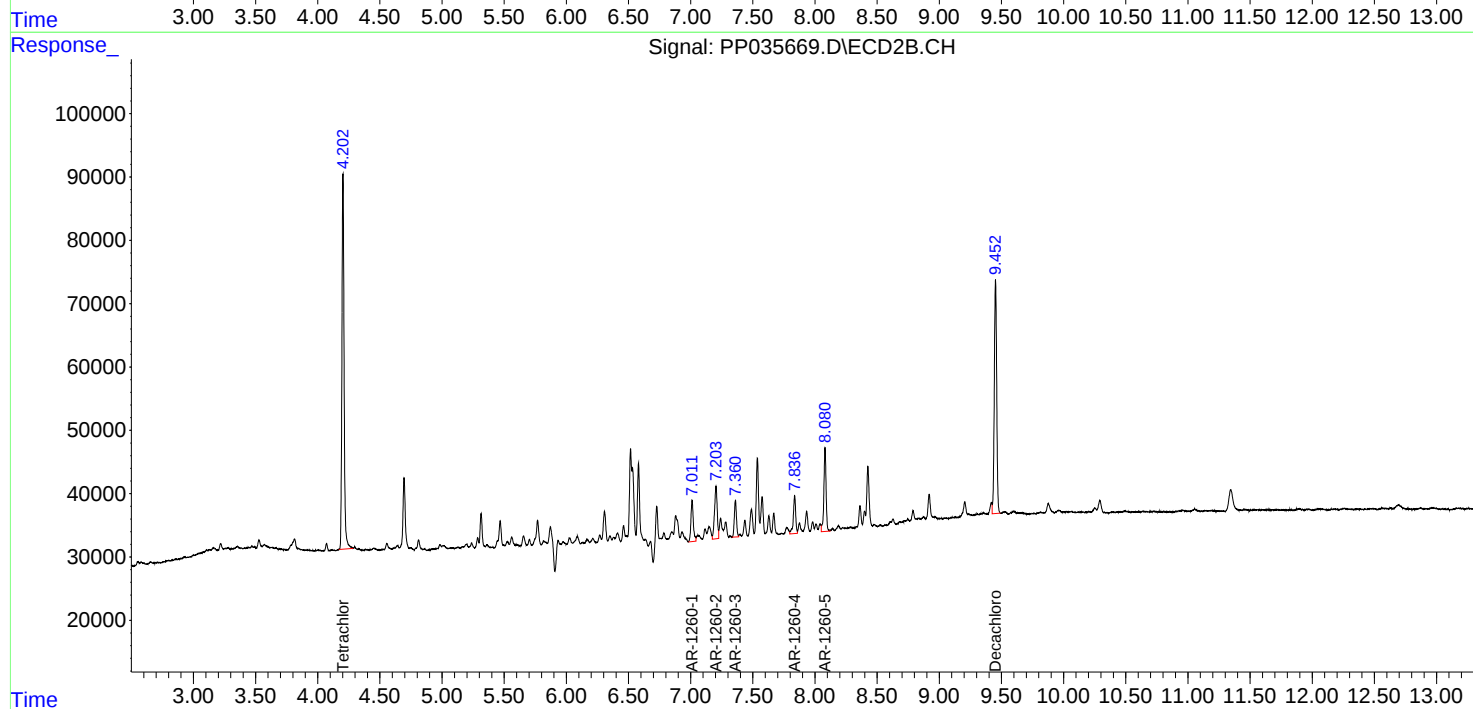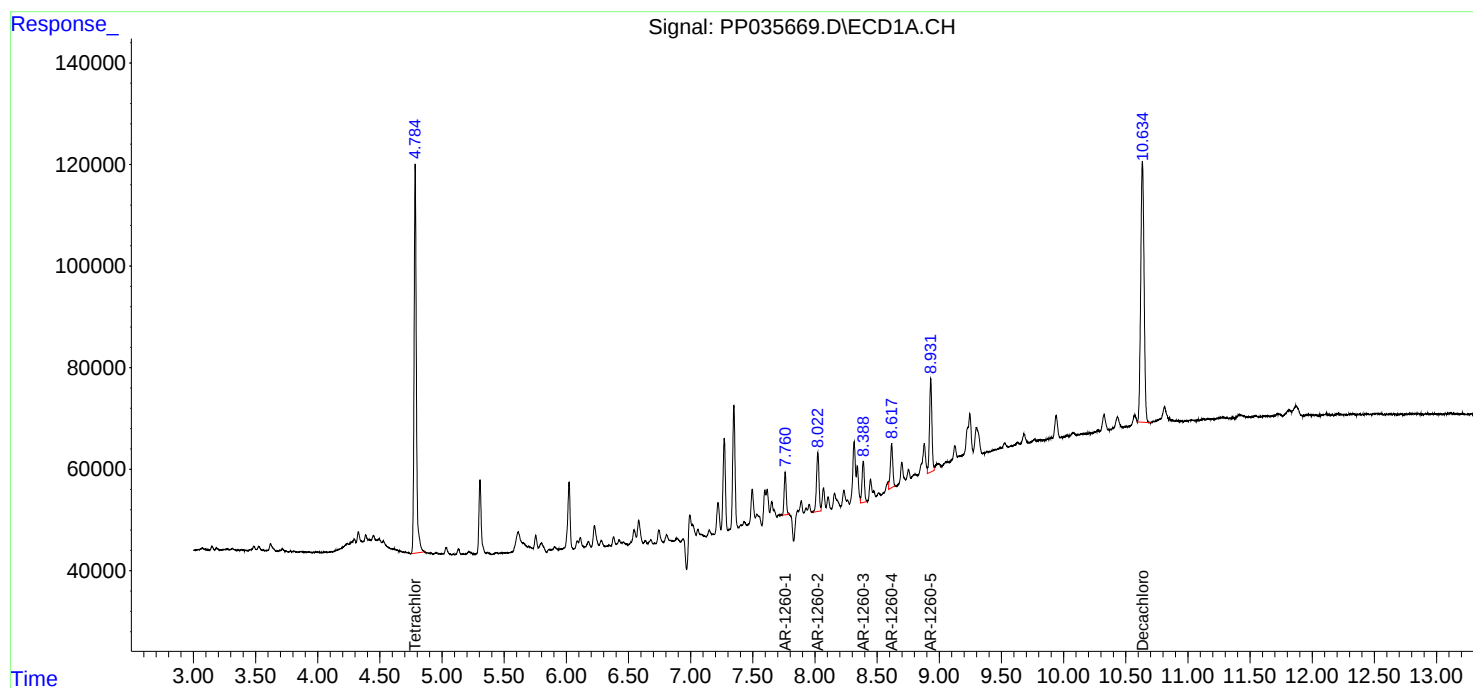

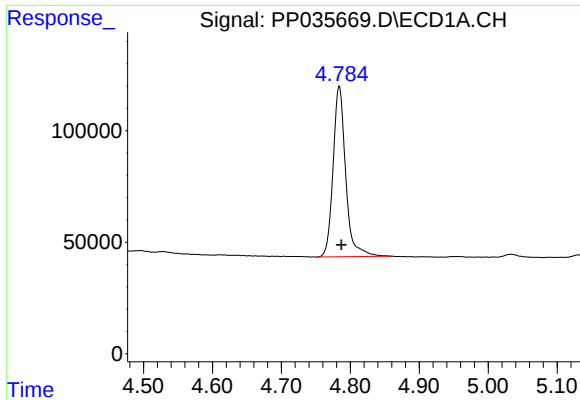


#1 Tetrachloro-m-xylene

R.T.: 4.784 min
Delta R.T.: -0.003 min
Response: 971221
Conc: 22.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:06 PM

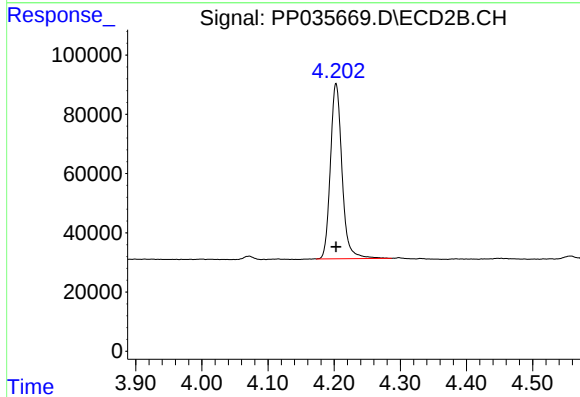


#1 Tetrachloro-m-xylene

R.T.: 4.203 min
Delta R.T.: 0.000 min
Response: 722434
Conc: 23.82 ng/ml

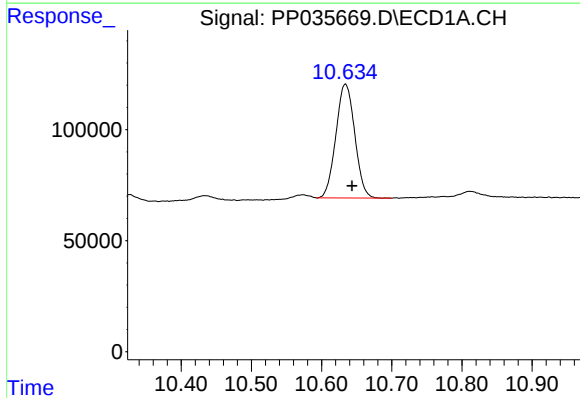


#2 Decachlorobiphenyl

R.T.: 10.634 min
Delta R.T.: -0.009 min
Response: 956836
Conc: 24.26 ng/ml

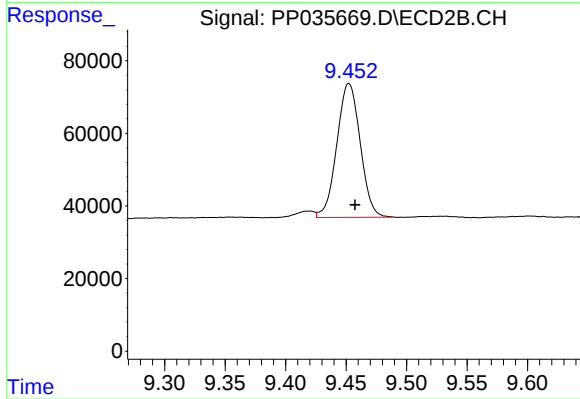

#2 Decachlorobiphenyl

R.T.: 9.452 min
Delta R.T.: -0.005 min
Response: 494723
Conc: 25.64 ng/ml m

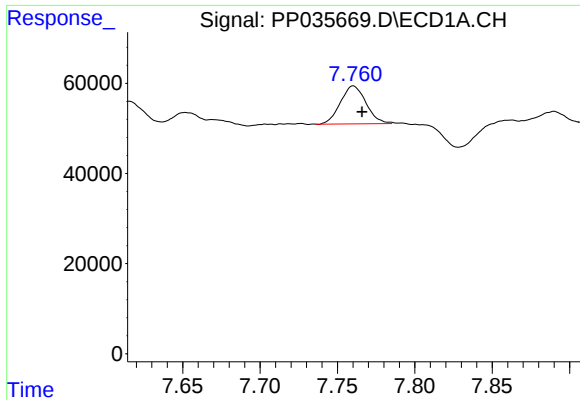


#31 AR-1260-1

R.T.: 7.760 min
Delta R.T.: -0.006 min
Response: 97102
Conc: 44.81 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:06 PM

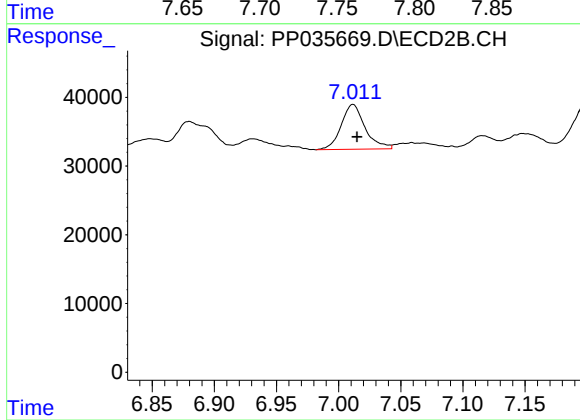


#31 AR-1260-1

R.T.: 7.012 min
Delta R.T.: -0.003 min
Response: 87636
Conc: 64.70 ng/ml

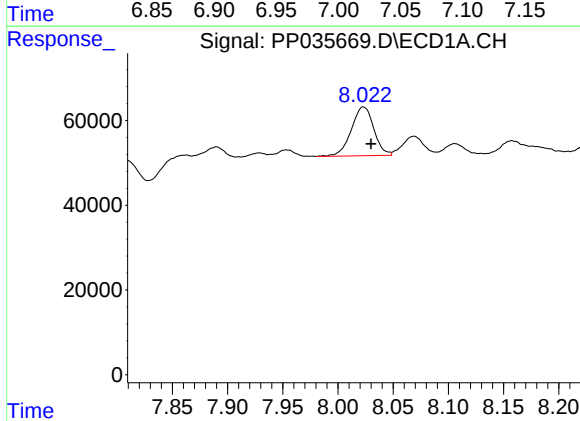


#32 AR-1260-2

R.T.: 8.023 min
Delta R.T.: -0.007 min
Response: 163563
Conc: 66.50 ng/ml

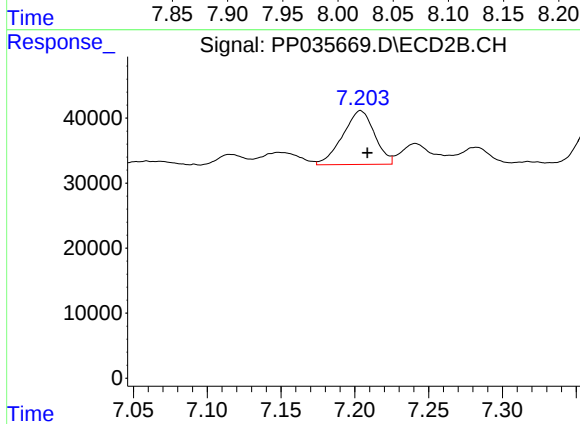

#32 AR-1260-2

R.T.: 7.204 min
Delta R.T.: -0.005 min
Response: 124483
Conc: 78.92 ng/ml

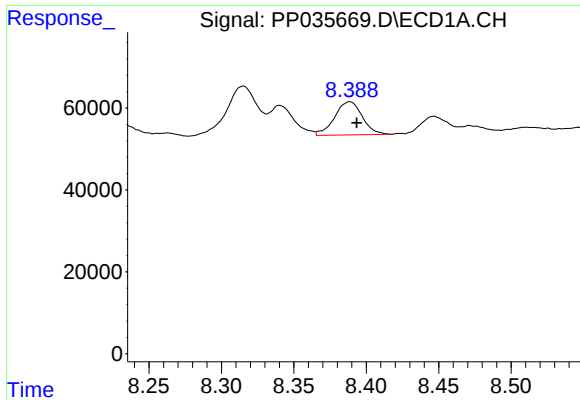


#33 AR-1260-3

R.T.: 8.389 min
Delta R.T.: -0.005 min
Response: 107244
Conc: 66.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:06 PM

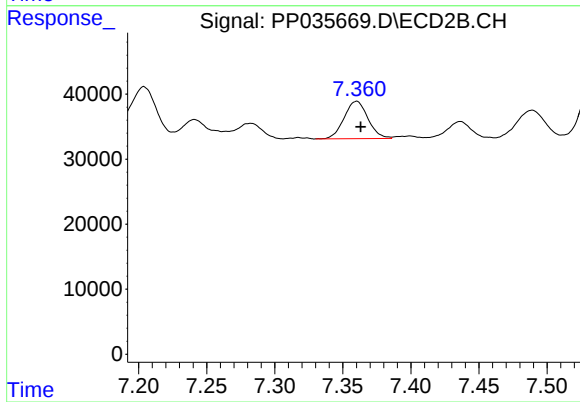


#33 AR-1260-3

R.T.: 7.360 min
Delta R.T.: -0.003 min
Response: 70140
Conc: 47.00 ng/ml

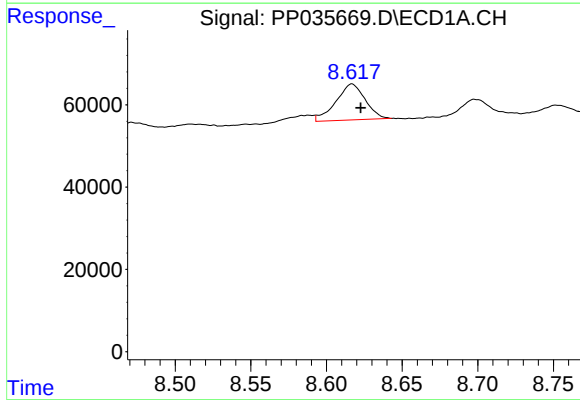


#34 AR-1260-4

R.T.: 8.617 min
Delta R.T.: -0.006 min
Response: 116903
Conc: 59.05 ng/ml m

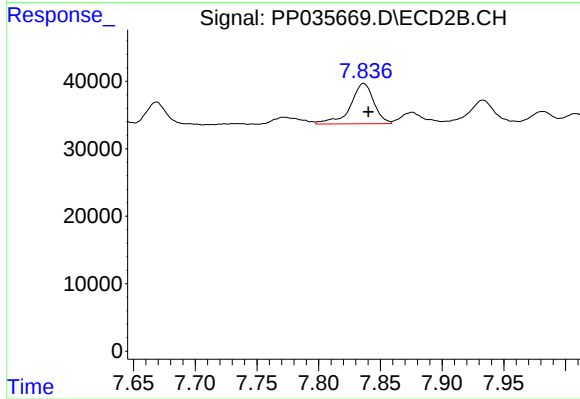

#34 AR-1260-4

R.T.: 7.836 min
Delta R.T.: -0.004 min
Response: 79102
Conc: 73.43 ng/ml

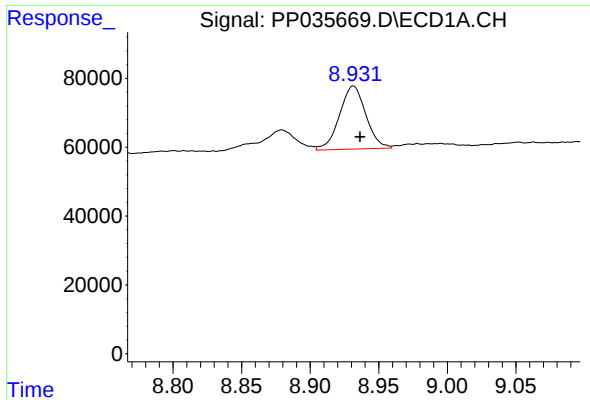


#35 AR-1260-5

R.T.: 8.931 min
Delta R.T.: -0.005 min
Response: 245636
Conc: 66.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-016

Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:06 PM

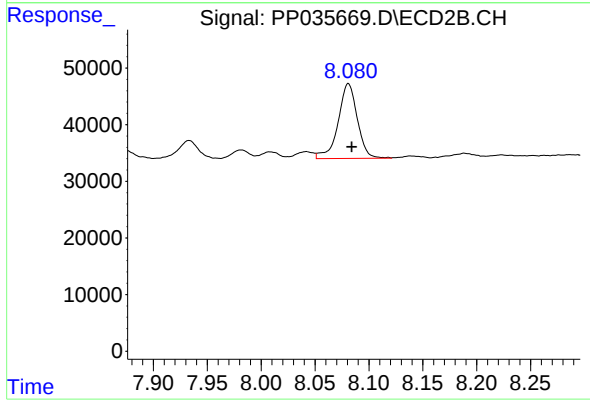

#35 AR-1260-5

R.T.: 8.081 min
Delta R.T.: -0.003 min
Response: 163428
Conc: 68.72 ng/ml