

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
 Data File : PP035680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2021 17:46
 Operator : DD\AJ
 Sample : M2323-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AST2-COPR2-1

Manual Integrations
 APPROVED

Ankita
 5/10/2021 2:04:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 00:43:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.197	685889	518493	15.677	17.093
2) SA Decachlor...	10.630	9.450	581702	294750	14.748	15.277
Target Compounds						
31) L7 AR-1260-1	7.758	7.009	1053472	670455	486.195m	494.948
32) L7 AR-1260-2	8.023	7.203	1358596	834030	552.361	528.742
33) L7 AR-1260-3	8.386	7.357	1095765	735615	675.947	492.891 #
34) L7 AR-1260-4	8.615	7.835	1281025	721079	647.125	669.331
35) L7 AR-1260-5	8.928	8.079	2777899	1587988	751.978	667.743

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
Data File : PP035680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2021 17:46
Operator : DD\AJ
Sample : M2323-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
AST2-COPR2-1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 00:43:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

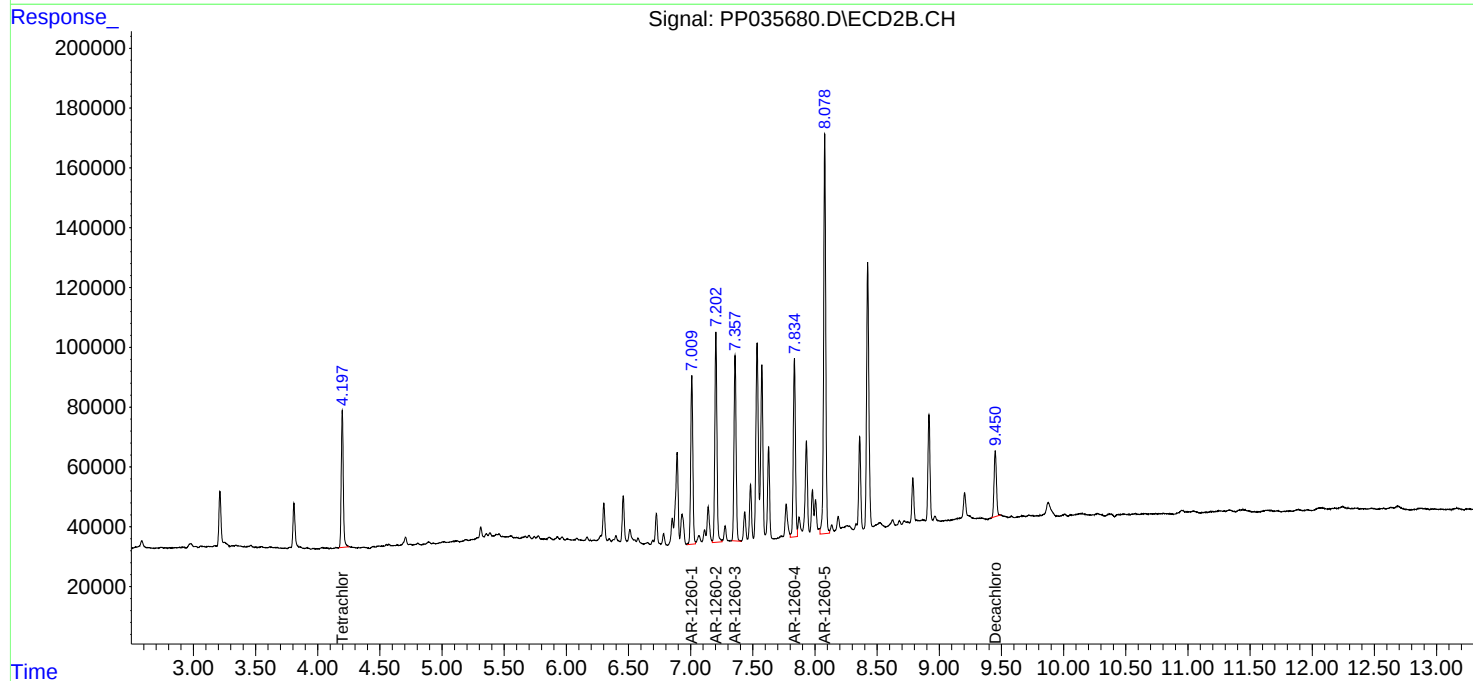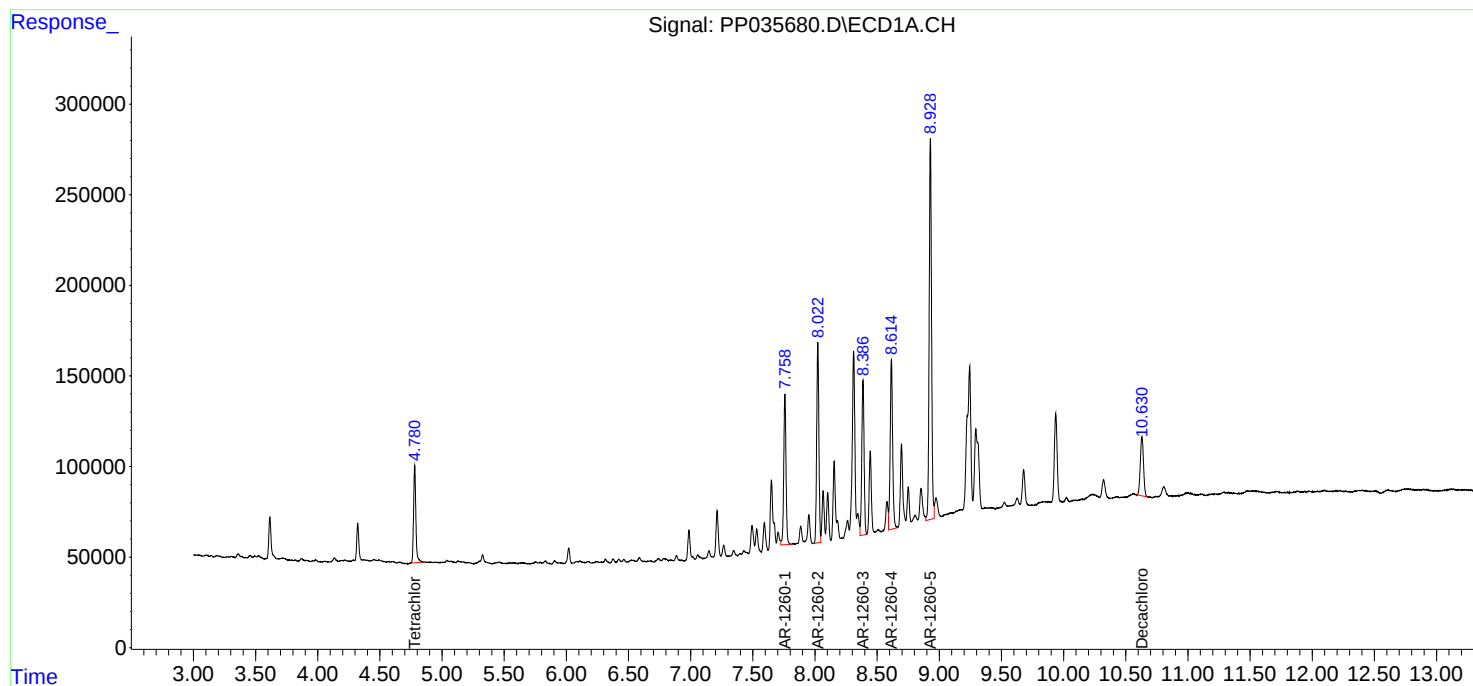

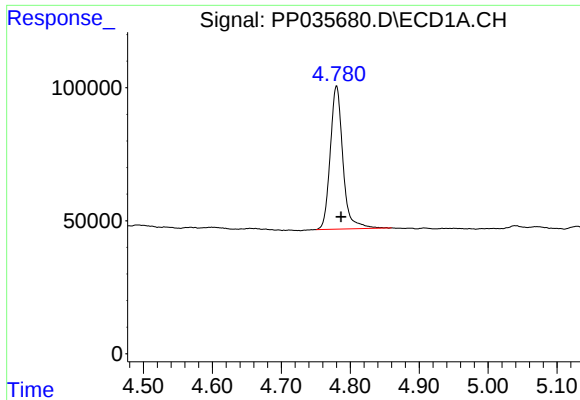


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.007 min
Response: 685889
Conc: 15.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AST2-COPR2-1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:12 PM

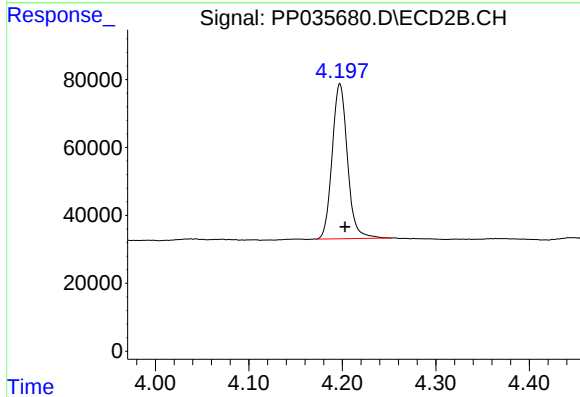


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.005 min
Response: 518493
Conc: 17.09 ng/ml

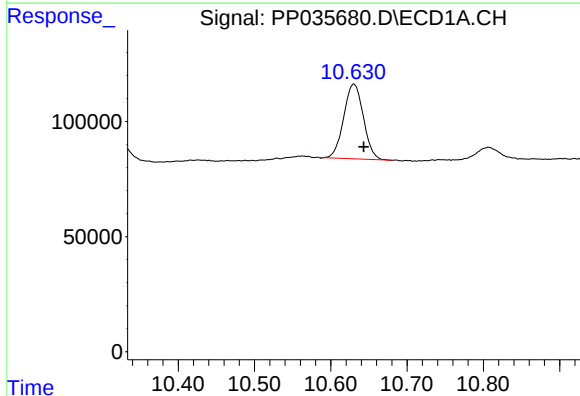


#2 Decachlorobiphenyl

R.T.: 10.630 min
Delta R.T.: -0.013 min
Response: 581702
Conc: 14.75 ng/ml

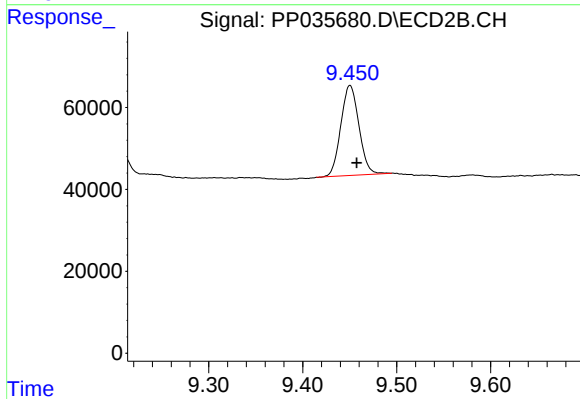

#2 Decachlorobiphenyl

R.T.: 9.450 min
Delta R.T.: -0.007 min
Response: 294750
Conc: 15.28 ng/ml

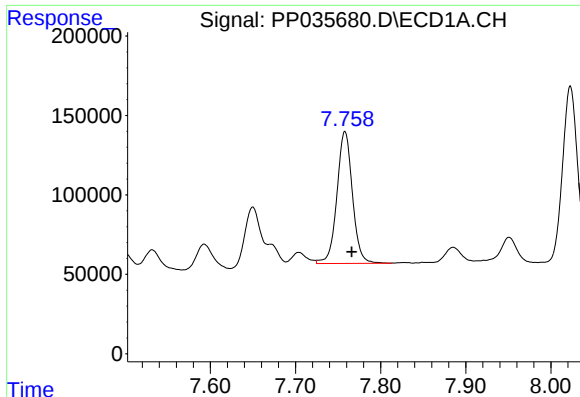


#31 AR-1260-1

R.T.: 7.758 min
Delta R.T.: -0.008 min
Response: 1053472
Conc: 486.19 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AST2-COPR2-1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:12 PM

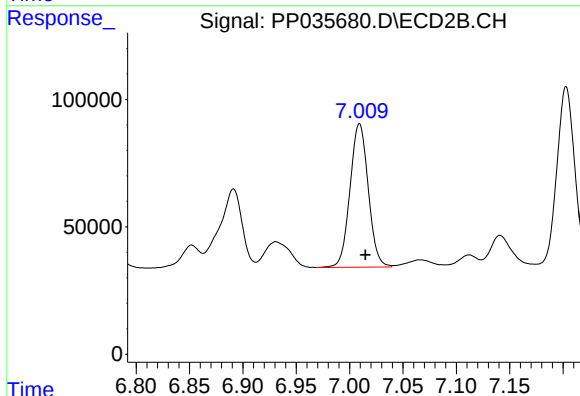


#31 AR-1260-1

R.T.: 7.009 min
Delta R.T.: -0.006 min
Response: 670455
Conc: 494.95 ng/ml

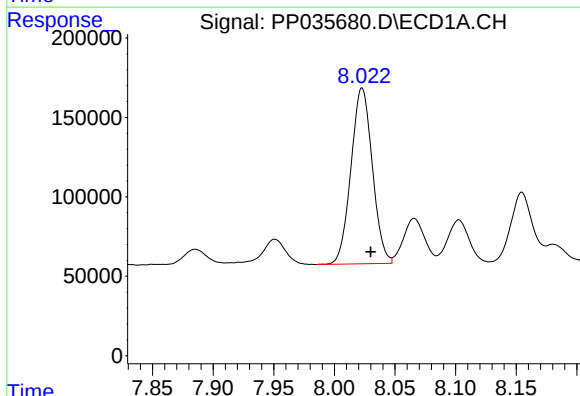


#32 AR-1260-2

R.T.: 8.023 min
Delta R.T.: -0.007 min
Response: 1358596
Conc: 552.36 ng/ml

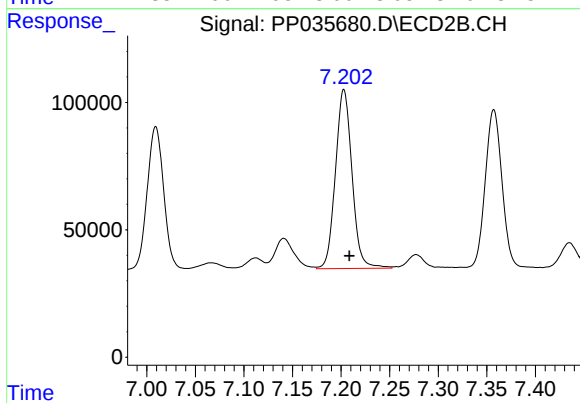

#32 AR-1260-2

R.T.: 7.203 min
Delta R.T.: -0.006 min
Response: 834030
Conc: 528.74 ng/ml

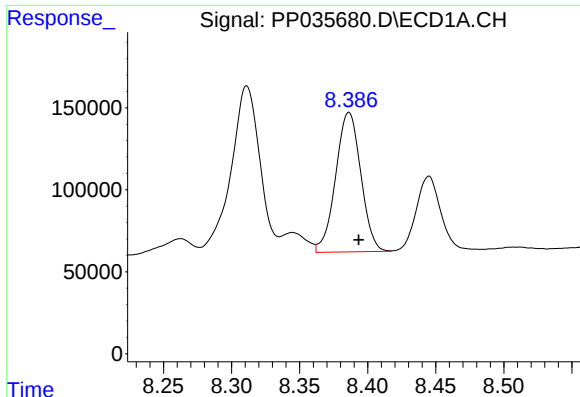


#33 AR-1260-3

R.T.: 8.386 min
Delta R.T.: -0.007 min
Response: 1095765
Conc: 675.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
AST2-COPR2-1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:12 PM

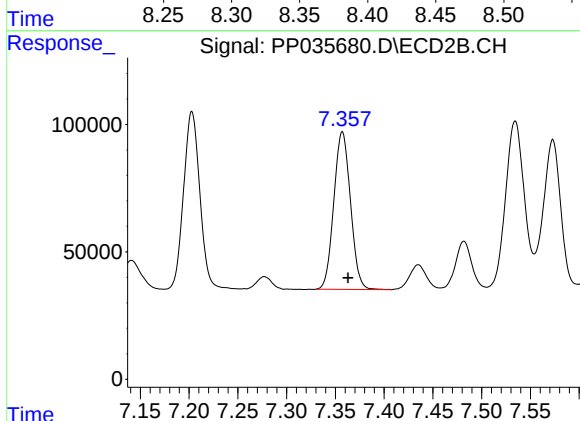


#33 AR-1260-3

R.T.: 7.357 min
Delta R.T.: -0.006 min
Response: 735615
Conc: 492.89 ng/ml

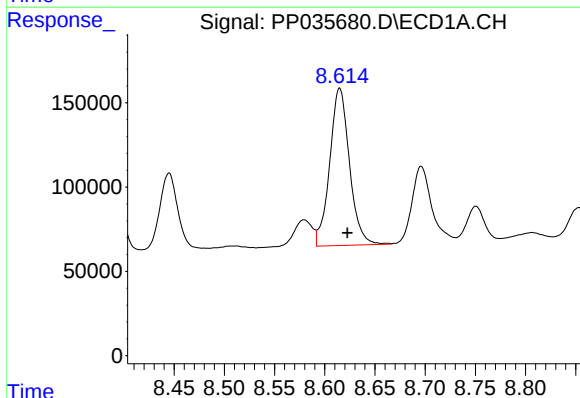


#34 AR-1260-4

R.T.: 8.615 min
Delta R.T.: -0.008 min
Response: 1281025
Conc: 647.13 ng/ml

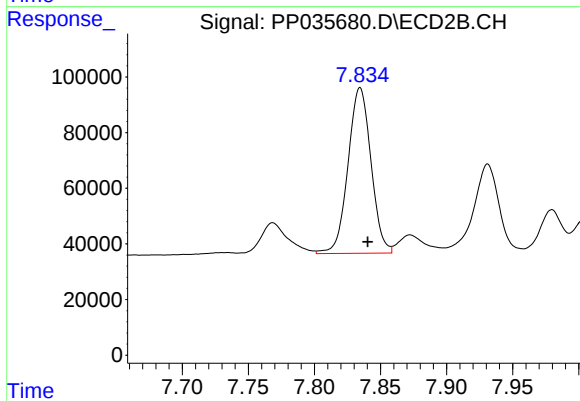

#34 AR-1260-4

R.T.: 7.835 min
Delta R.T.: -0.006 min
Response: 721079
Conc: 669.33 ng/ml

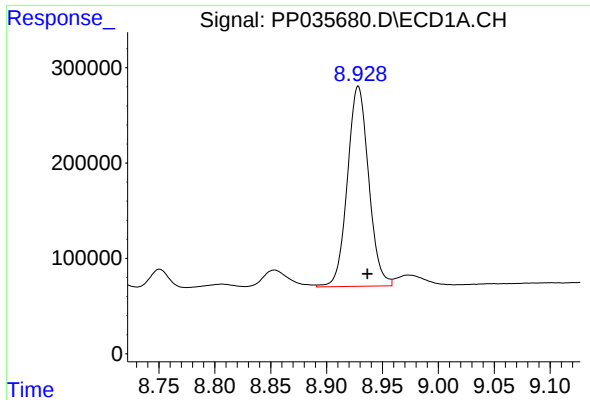


#35 AR-1260-5

R.T.: 8.928 min
Delta R.T.: -0.008 min
Response: 2777899
Conc: 751.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AST2-COPR2-1

Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:12 PM

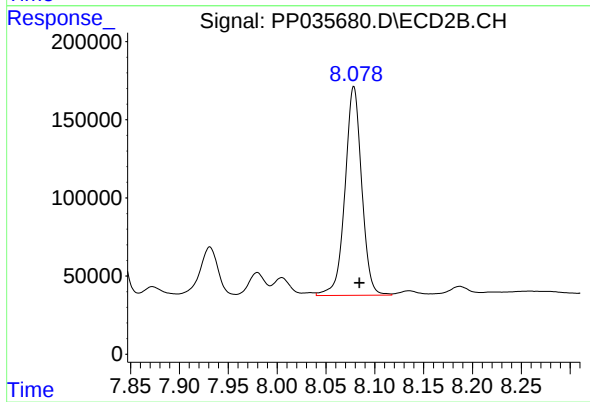

#35 AR-1260-5

R.T.: 8.079 min
Delta R.T.: -0.006 min
Response: 1587988
Conc: 667.74 ng/ml