

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
 Data File : PP035683.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2021 18:36
 Operator : DD\AJ
 Sample : M2309-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MH-TP2

Manual Integrations
 APPROVED

Ankita
 5/10/2021 2:04:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 00:45:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.198	828058	659721	18.926	21.748
2) SA Decachlor...	10.629	9.449	568300	313997	14.408	16.275
Target Compounds						
26) L6 AR-1254-1	6.988	6.303	41690	43321	24.851m	30.502m
27) L6 AR-1254-2	7.216	6.458	61676	27467	24.483	21.808
28) L6 AR-1254-3	7.593	6.876	71224	38350	27.508	20.207 #
29) L6 AR-1254-4	7.887	7.114	36232	27505	21.208m	25.002m
30) L6 AR-1254-5	8.312	7.536	44590	36611	21.557	21.838m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
Data File : PP035683.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2021 18:36
Operator : DD\AJ
Sample : M2309-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
MH-TP2


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 00:45:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

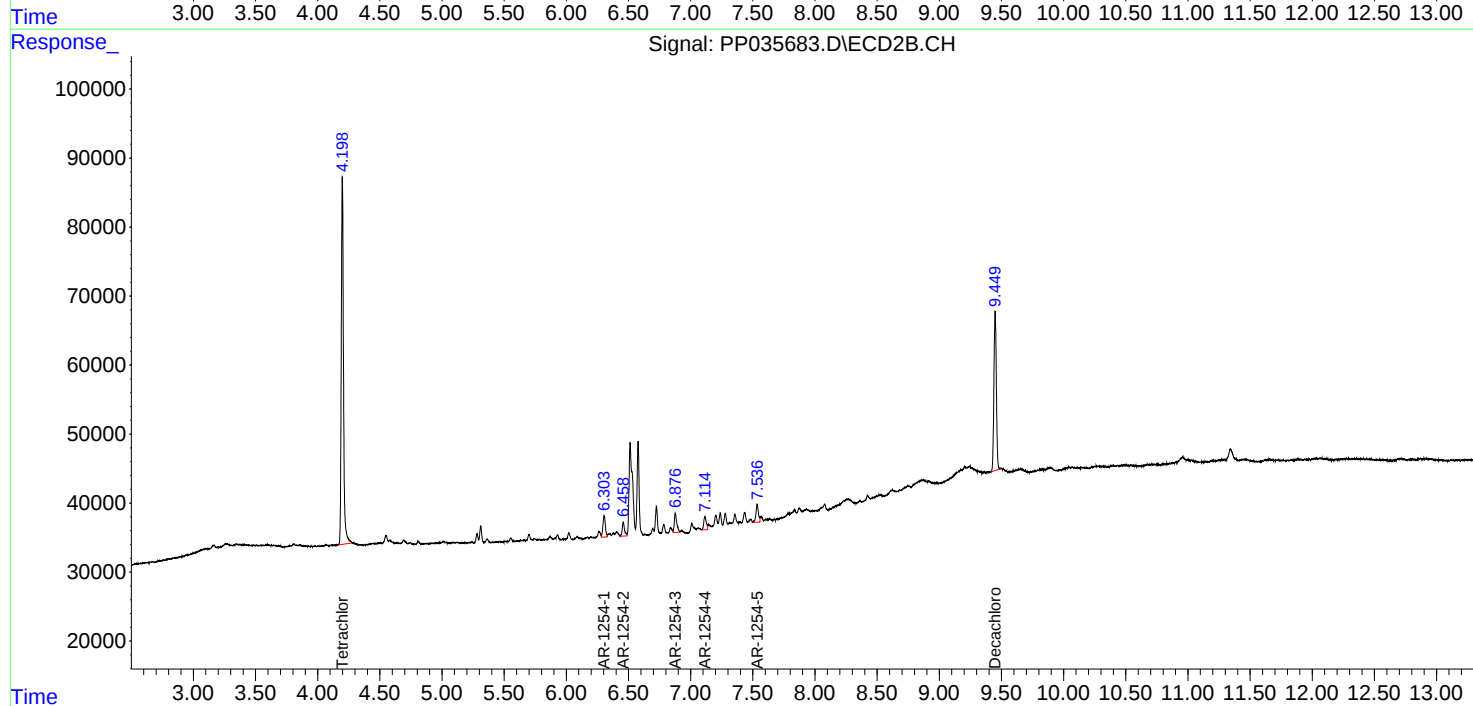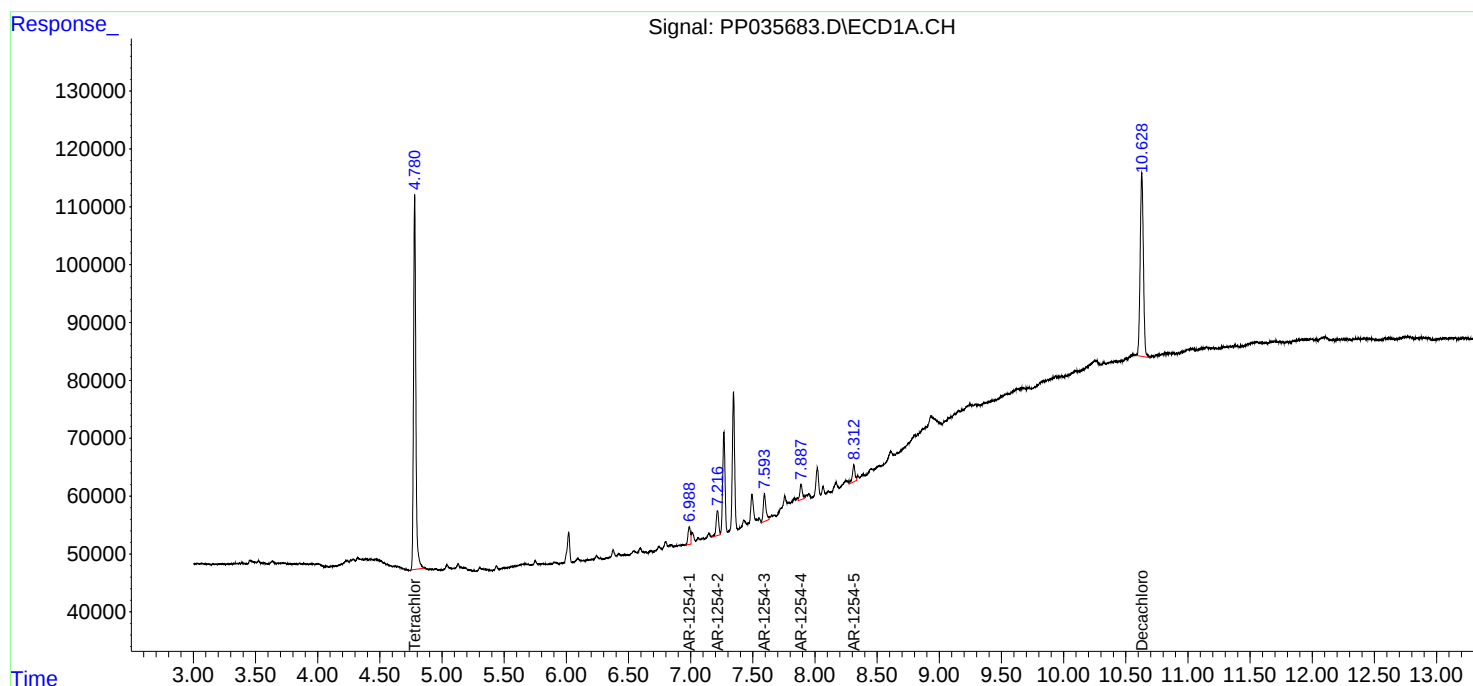

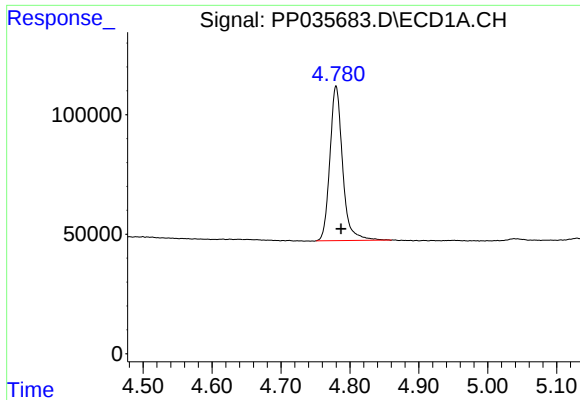


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.007 min
Response: 828058
Conc: 18.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-TP2


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:14 PM

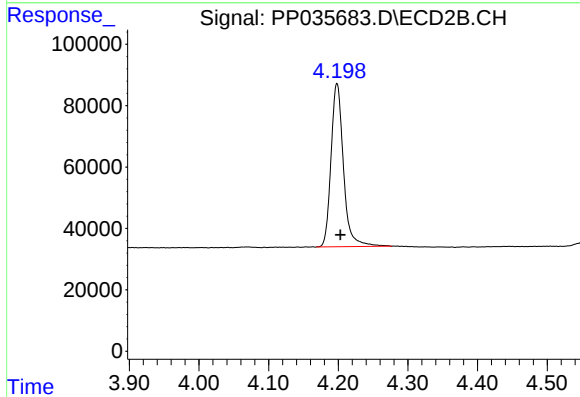


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: -0.005 min
Response: 659721
Conc: 21.75 ng/ml

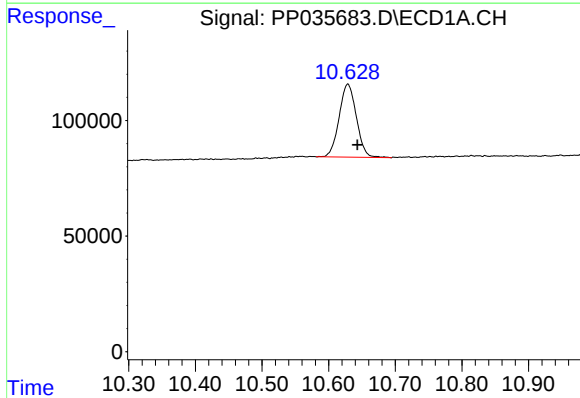


#2 Decachlorobiphenyl

R.T.: 10.629 min
Delta R.T.: -0.014 min
Response: 568300
Conc: 14.41 ng/ml

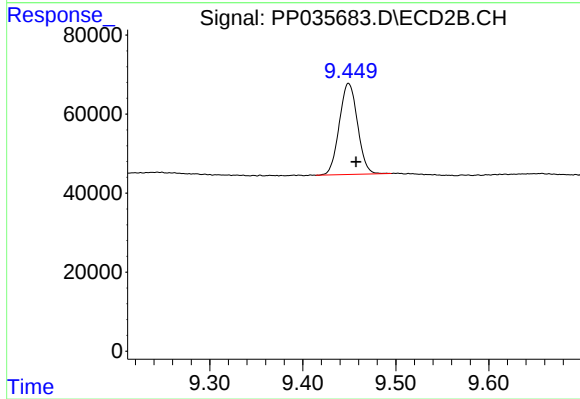

#2 Decachlorobiphenyl

R.T.: 9.449 min
Delta R.T.: -0.008 min
Response: 313997
Conc: 16.27 ng/ml

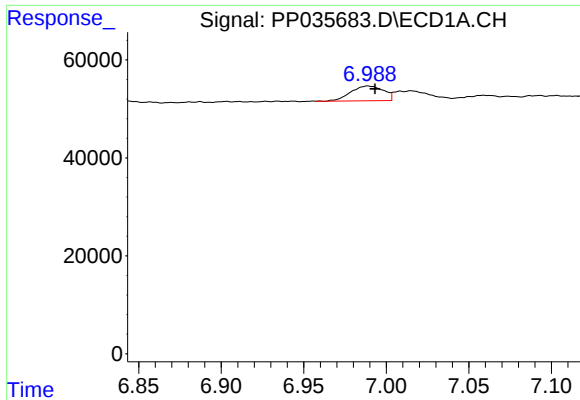


#26 AR-1254-1

R.T.: 6.988 min
Delta R.T.: -0.005 min
Response: 41690
Conc: 24.85 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MH-TP2


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:14 PM

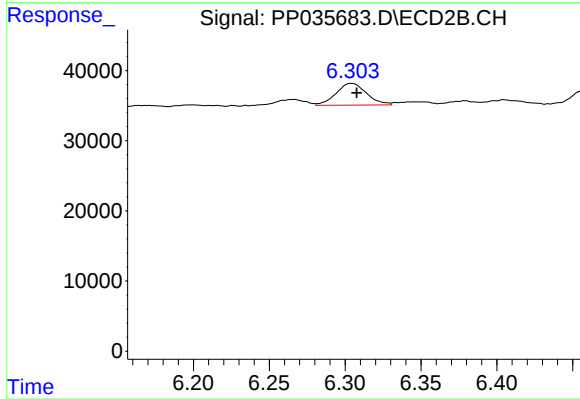


#26 AR-1254-1

R.T.: 6.303 min
Delta R.T.: -0.004 min
Response: 43321
Conc: 30.50 ng/ml m

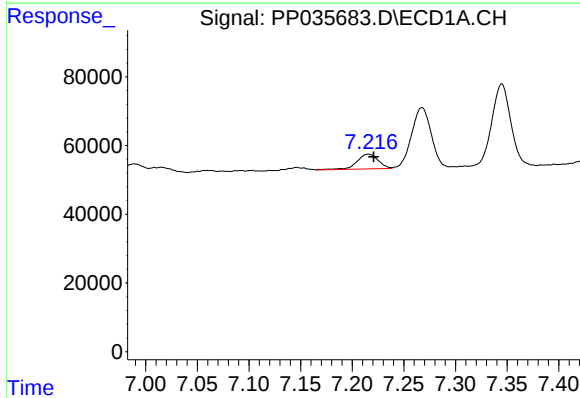


#27 AR-1254-2

R.T.: 7.216 min
Delta R.T.: -0.005 min
Response: 61676
Conc: 24.48 ng/ml

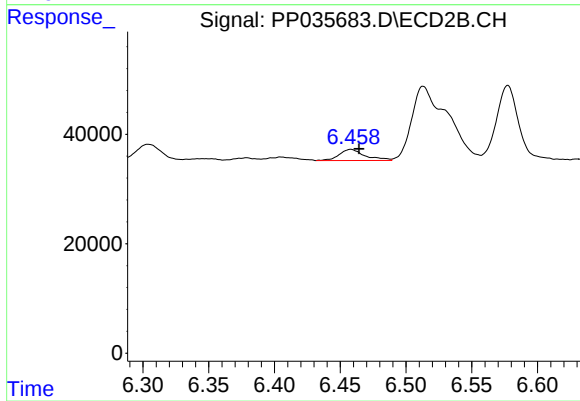

#27 AR-1254-2

R.T.: 6.458 min
Delta R.T.: -0.006 min
Response: 27467
Conc: 21.81 ng/ml

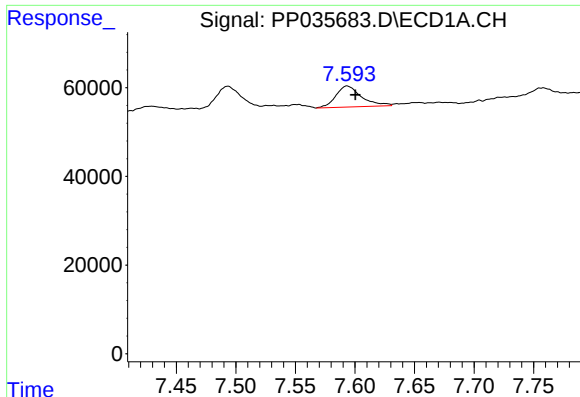


#28 AR-1254-3

R.T.: 7.593 min
Delta R.T.: -0.007 min
Response: 71224
Conc: 27.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-TP2


Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:14 PM

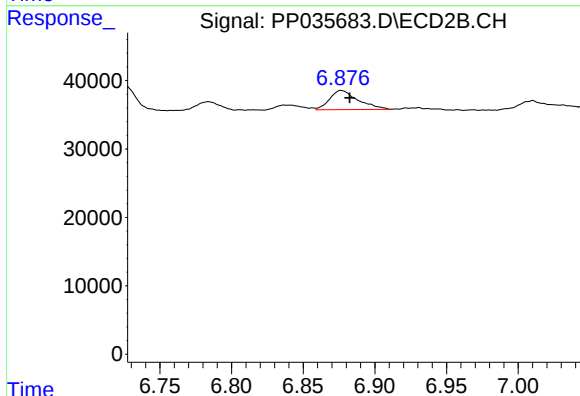


#28 AR-1254-3

R.T.: 6.876 min
Delta R.T.: -0.006 min
Response: 38350
Conc: 20.21 ng/ml

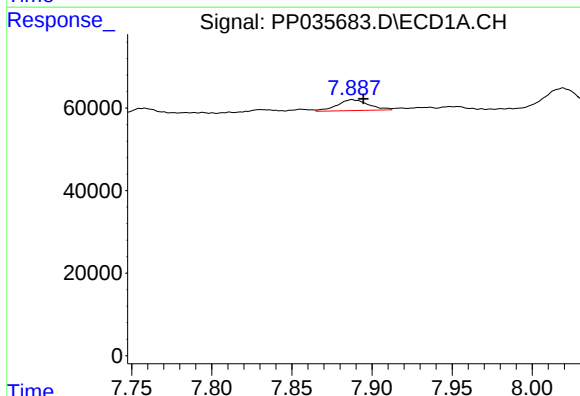


#29 AR-1254-4

R.T.: 7.887 min
Delta R.T.: -0.007 min
Response: 36232
Conc: 21.21 ng/ml m

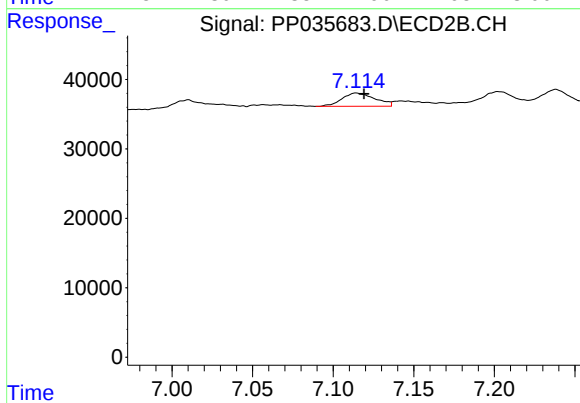

#29 AR-1254-4

R.T.: 7.114 min
Delta R.T.: -0.005 min
Response: 27505
Conc: 25.00 ng/ml m

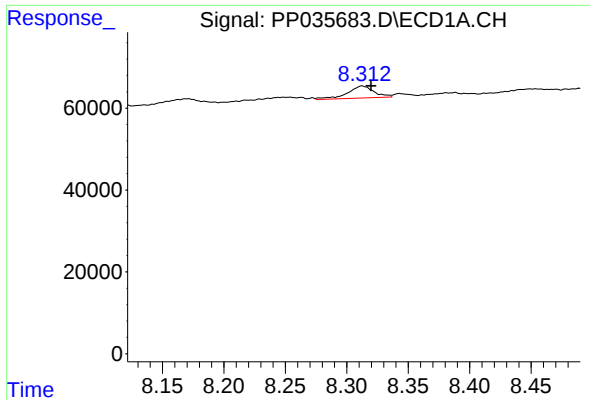


#30 AR-1254-5

R.T.: 8.312 min
Delta R.T.: -0.007 min
Response: 44590
Conc: 21.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MH-TP2

Manual Integrations
APPROVED

Ankita
5/10/2021 2:04:14 PM

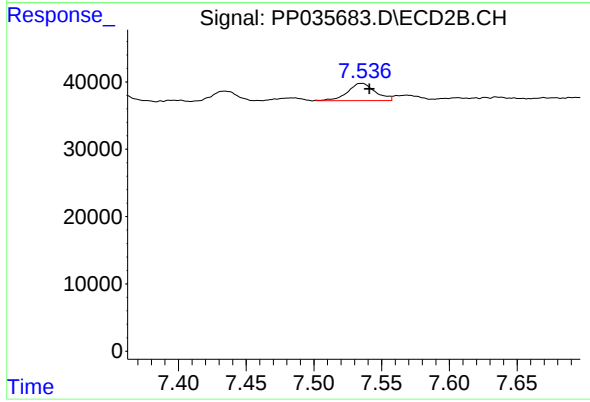

#30 AR-1254-5

R.T.: 7.536 min
Delta R.T.: -0.005 min
Response: 36611
Conc: 21.84 ng/ml m