

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
 Data File : PP035694.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2021 22:48
 Operator : DD\AJ
 Sample : M2317-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PE-6A-(0.5-1.0)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 00:52:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 06 11:27:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.199	772028	630725	17.646	20.792
2) SA Decachlor...	10.629	9.449	744677	412536	18.880	21.382

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050721\
Data File : PP035694.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2021 22:48
Operator : DD\AJ
Sample : M2317-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PE-6A-(0.5-1.0)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 00:52:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 06 11:27:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

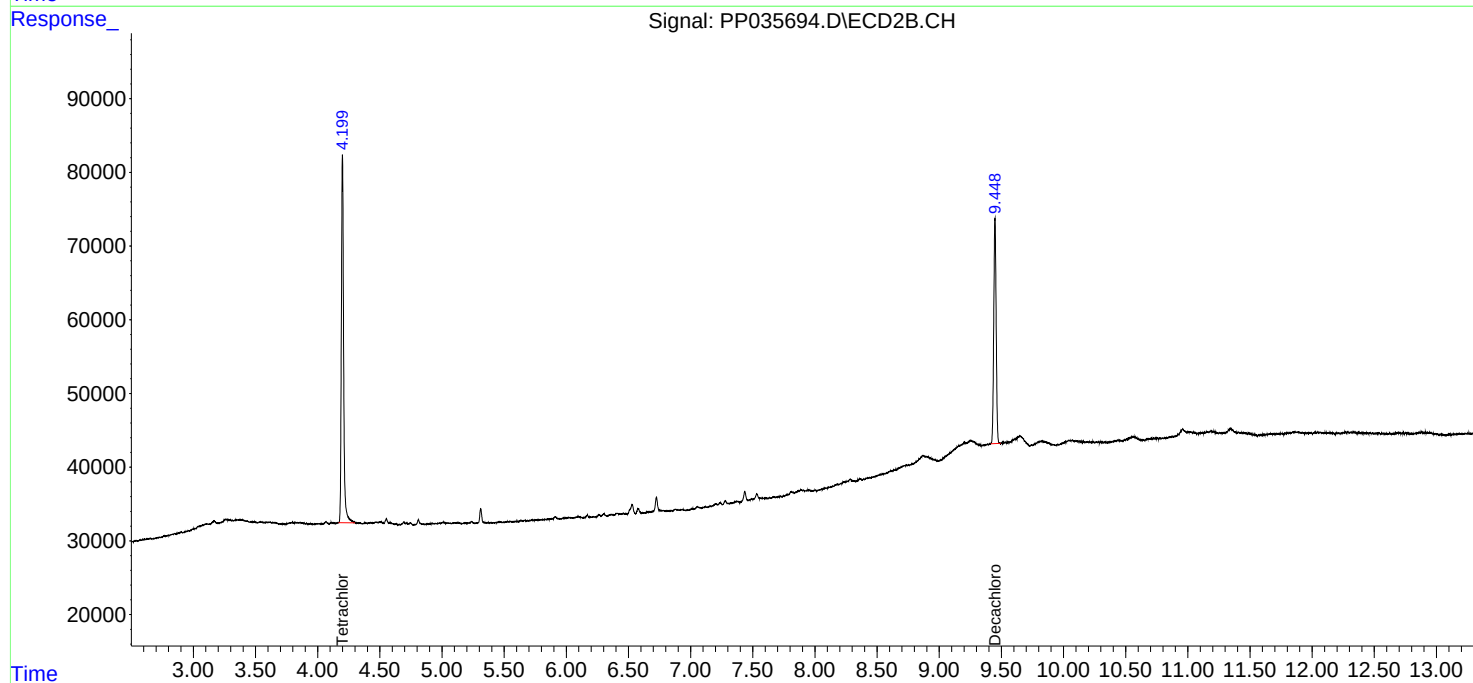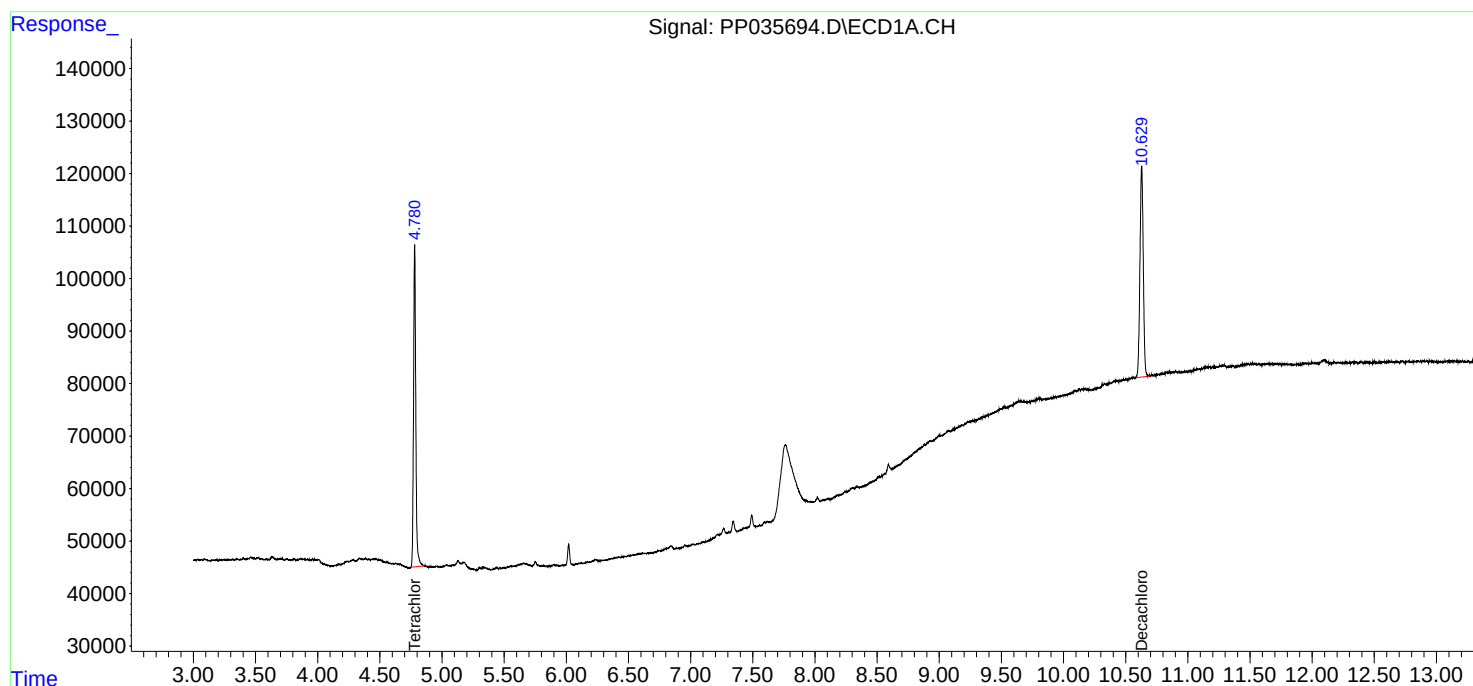


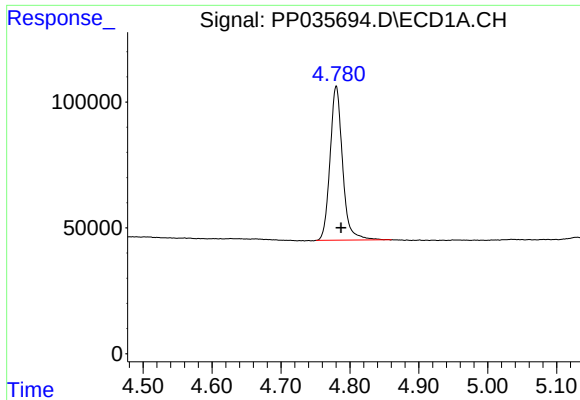

#1 Tetrachloro-m-xylene


R.T.: 4.780 min
Delta R.T.: -0.007 min
Response: 772028
Conc: 17.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
PE-6A-(0.5-1.0)

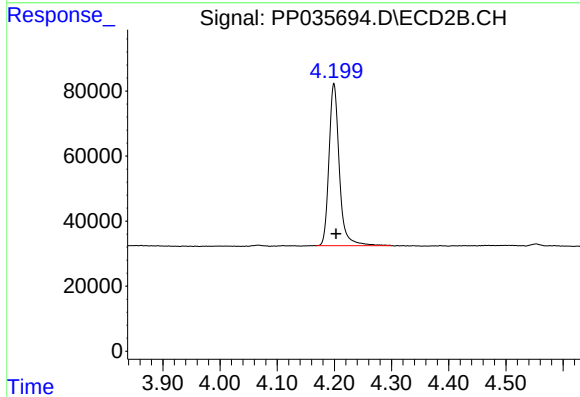


#1 Tetrachloro-m-xylene

R.T.: 4.199 min
Delta R.T.: -0.004 min
Response: 630725
Conc: 20.79 ng/ml

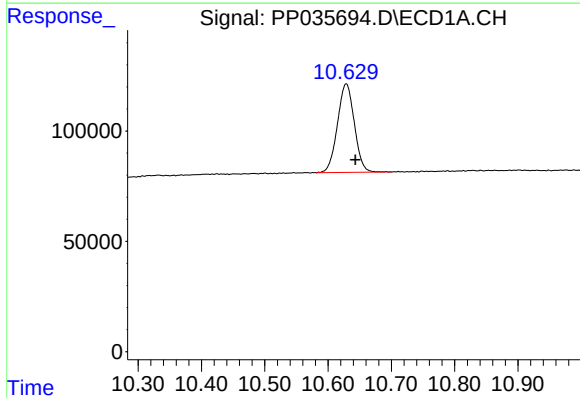

#2 Decachlorobiphenyl

R.T.: 10.629 min
Delta R.T.: -0.014 min
Response: 744677
Conc: 18.88 ng/ml

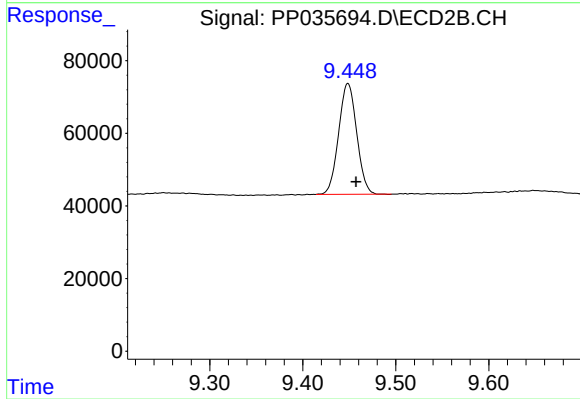

#2 Decachlorobiphenyl

R.T.: 9.449 min
Delta R.T.: -0.009 min
Response: 412536
Conc: 21.38 ng/ml