

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050922\
 Data File : PP047266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2022 14:59
 Operator : YP\AJ
 Sample : N2725-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-1284

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 16:36:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.858	3.127	21940712	39765090	9.089m	12.122 #
2) SA Decachlor...	9.970f	8.473f	13915742	26024950	9.457	10.911m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050922\
Data File : PP047266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2022 14:59
Operator : YP\AJ
Sample : N2725-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-1284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 16:36:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

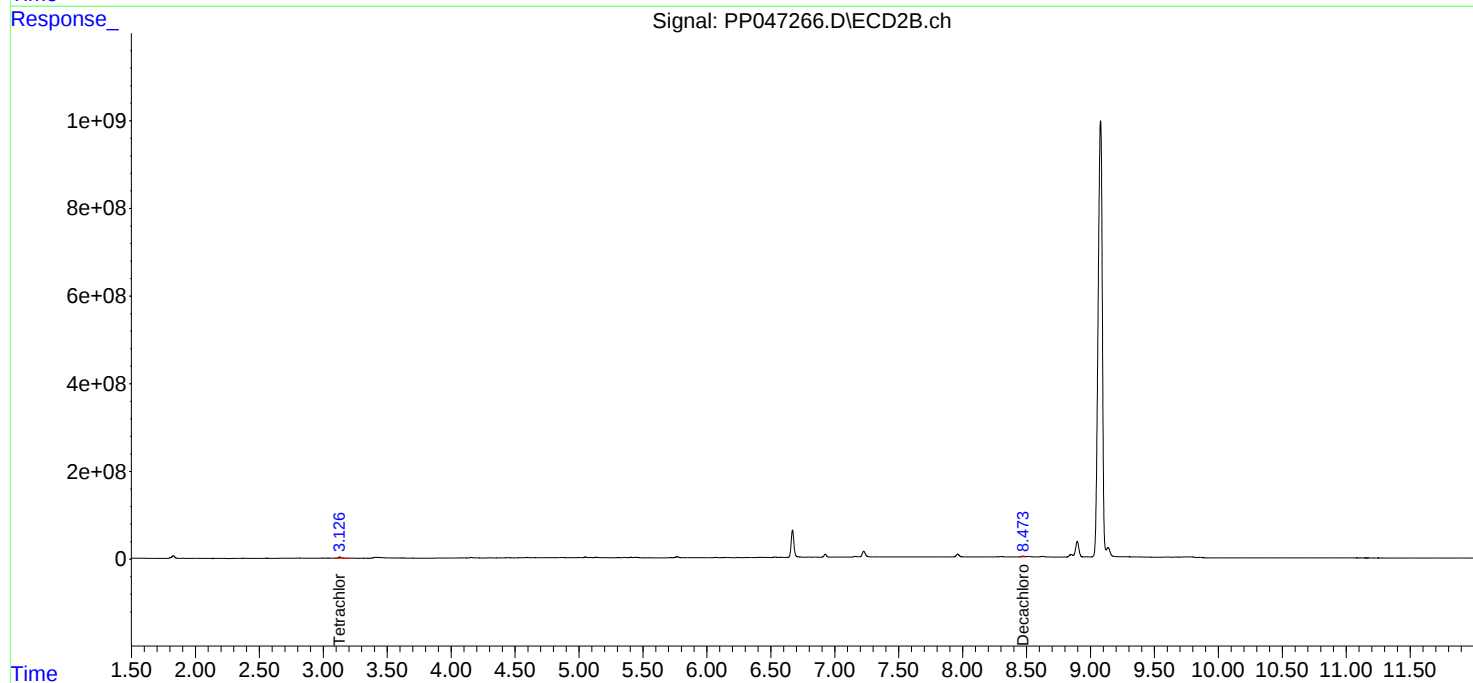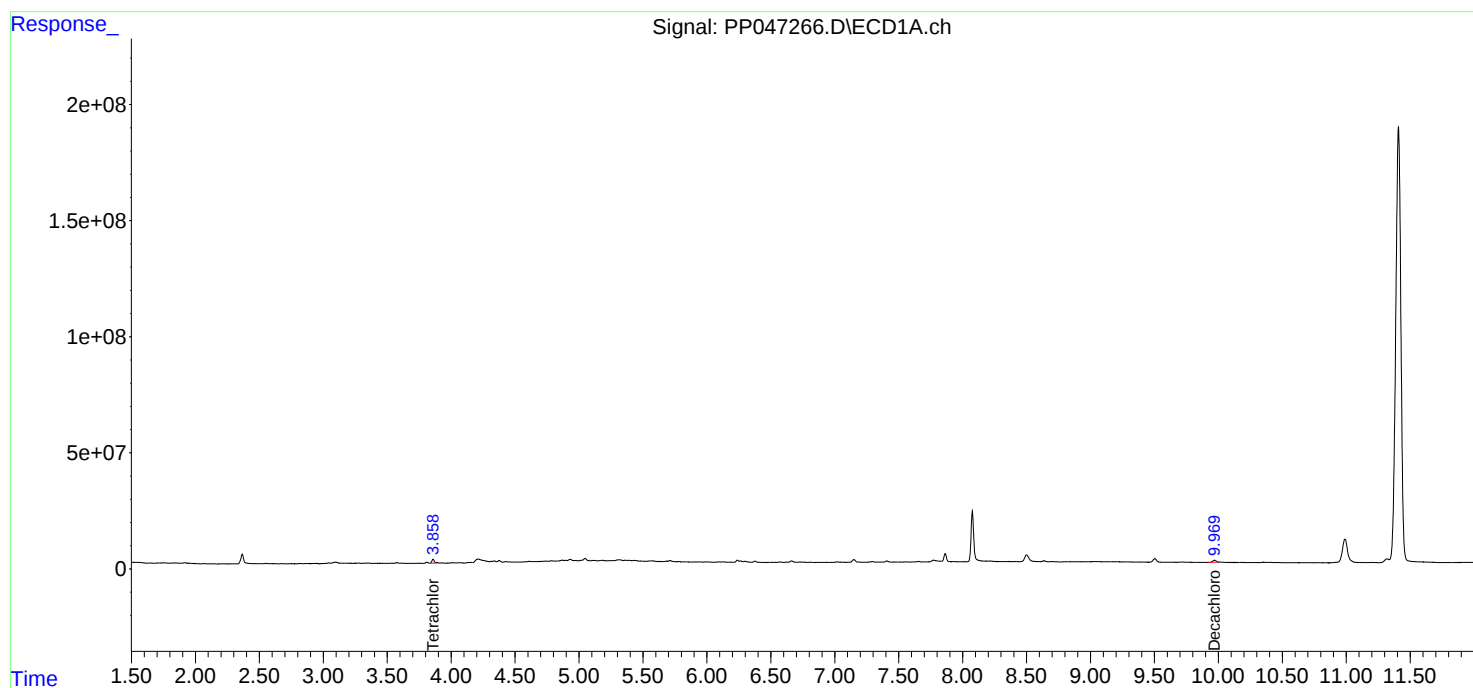

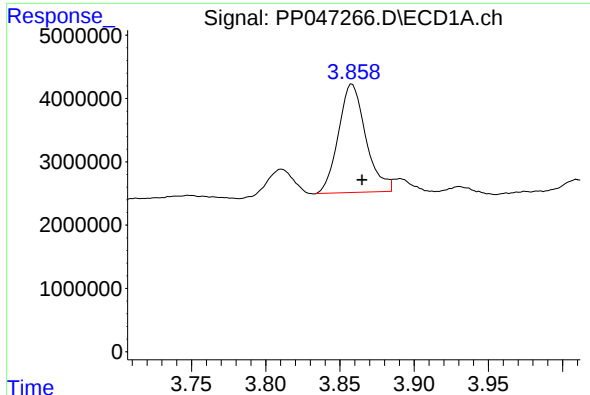


#1 Tetrachloro-m-xylene

R.T.: 3.858 min
Delta R.T.: -0.007 min
Response: 21940712
Conc: 9.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

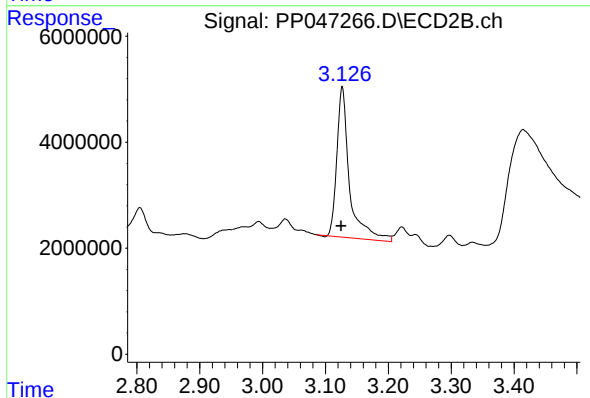


#1 Tetrachloro-m-xylene

R.T.: 3.127 min
Delta R.T.: 0.002 min
Response: 39765090
Conc: 12.12 ng/ml

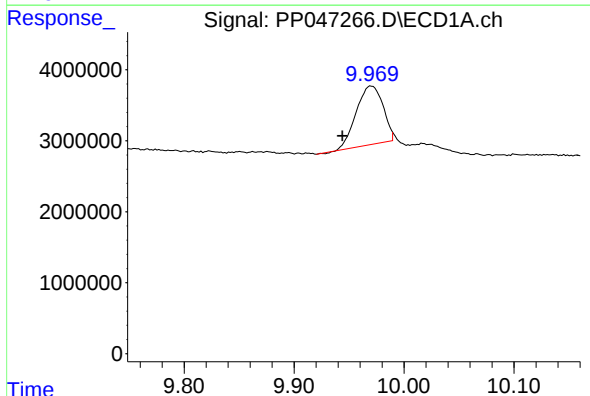

#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: 0.026 min
Response: 13915742
Conc: 9.46 ng/ml

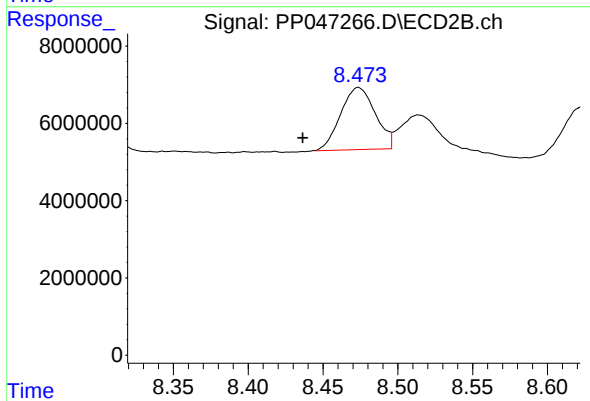

#2 Decachlorobiphenyl

R.T.: 8.473 min
Delta R.T.: 0.037 min
Response: 26024950
Conc: 10.91 ng/ml m