

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050922\
 Data File : PP047319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2022 06:27
 Operator : YP\AJ
 Sample : N2619-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB03-13-14-FT

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 07:55:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 06 10:17:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.849	3.116	45569163	51962185	18.878m	15.840m
2) SA Decachlor...	9.919	8.424	26464513	45553153	17.985	19.097

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050922\
Data File : PP047319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2022 06:27
Operator : YP\AJ
Sample : N2619-06
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB03-13-14-FT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 07:55:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 06 10:17:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

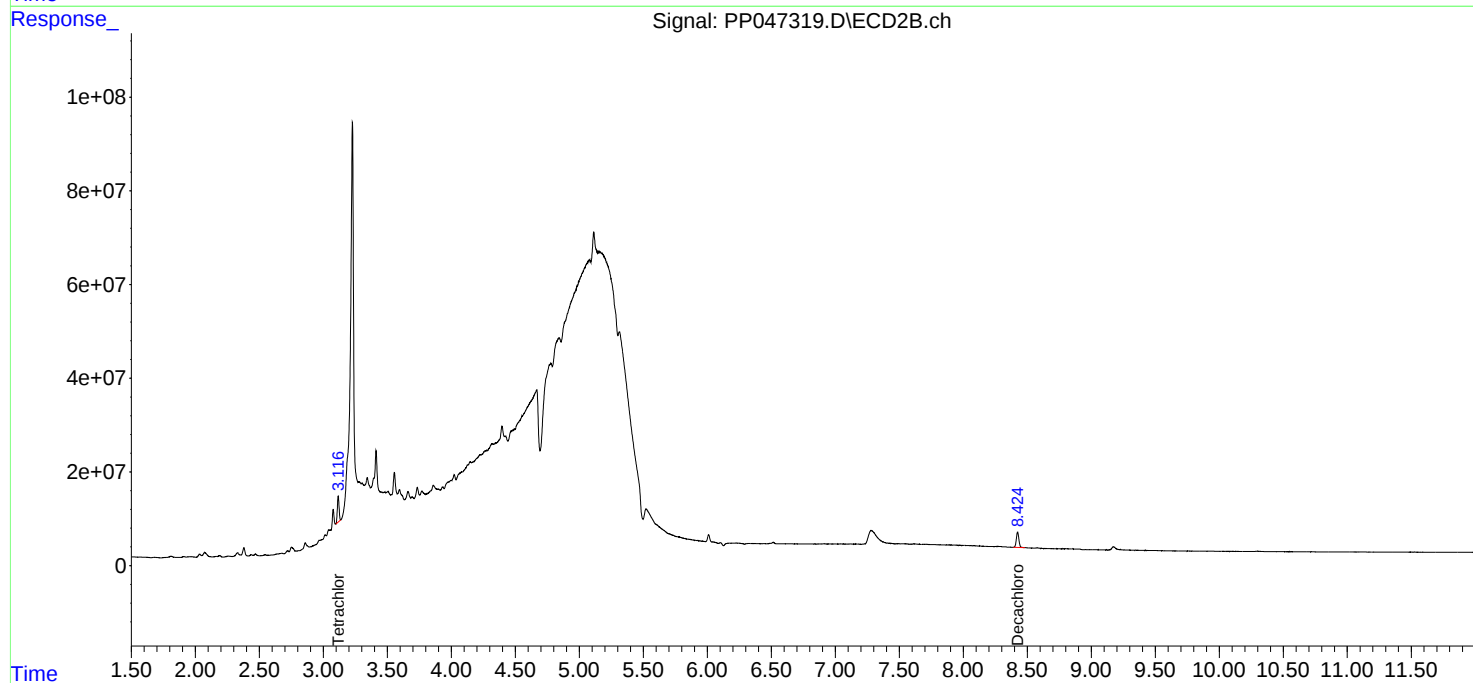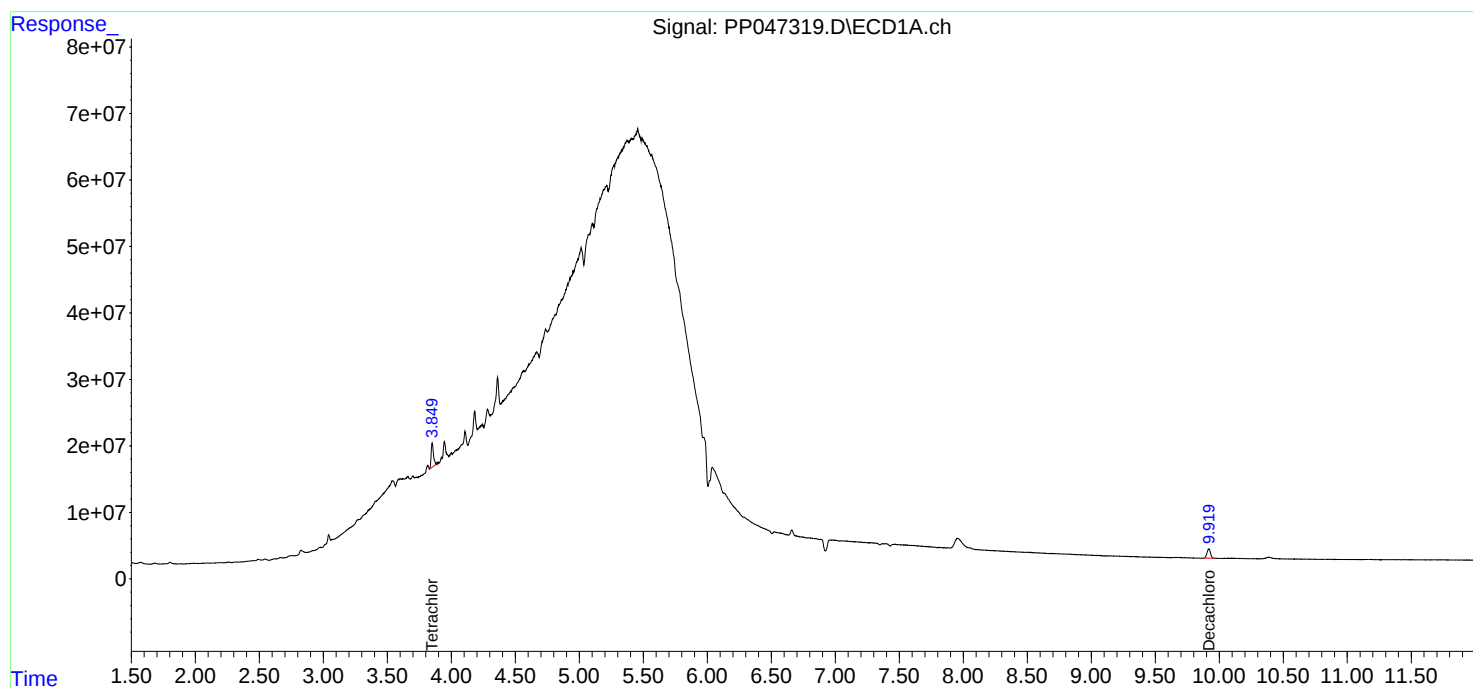

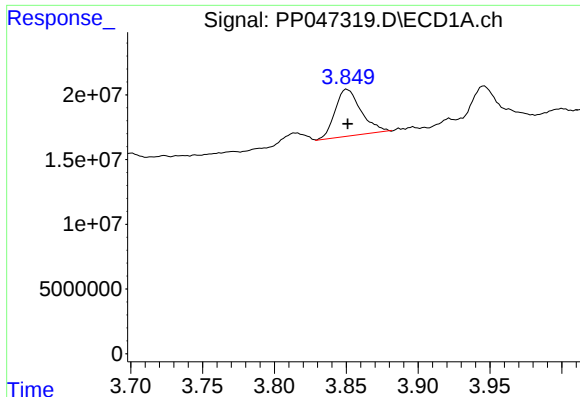


#1 Tetrachloro-m-xylene

R.T.: 3.849 min
Delta R.T.: -0.002 min
Response: 45569163
Conc: 18.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB03-13-14-FT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

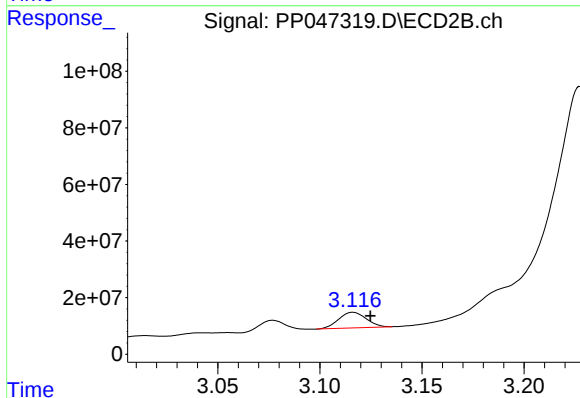


#1 Tetrachloro-m-xylene

R.T.: 3.116 min
Delta R.T.: -0.009 min
Response: 51962185
Conc: 15.84 ng/ml m

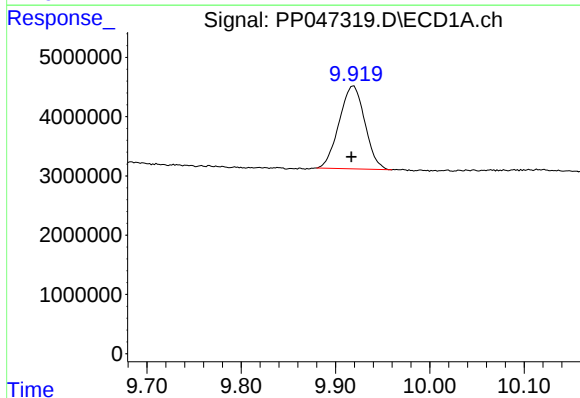

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: 0.002 min
Response: 26464513
Conc: 17.98 ng/ml

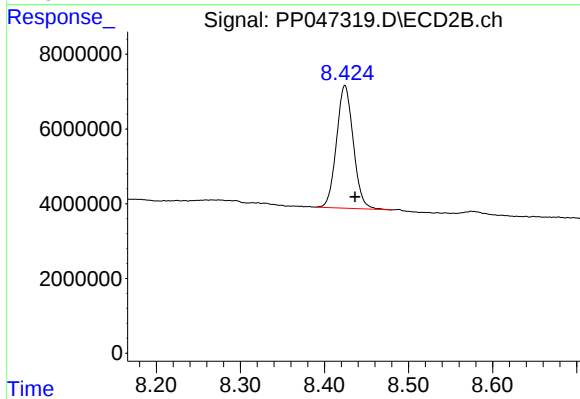

#2 Decachlorobiphenyl

R.T.: 8.424 min
Delta R.T.: -0.012 min
Response: 45553153
Conc: 19.10 ng/ml