

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
 Data File : PP035743.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2021 1:42
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 06:46:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.778	4.198	497696	696476	21.241	20.489
2)	SA Decachlor...	10.621	9.439	263826	467834	23.439	22.122
Target Compounds							
9)	L2 AR-1221-2	5.126	0.000	7468	0	33.278	N.D. #
29)	L6 AR-1254-4	7.895	0.000	94739	0	118.827	N.D. #
30)	L6 AR-1254-5	8.306	0.000	26665	0	28.259	N.D. #
33)	L7 AR-1260-3	8.374	0.000	8705	0	13.009	N.D. #
34)	L7 AR-1260-4	0.000	7.826	0	4237	N.D.	3.673 #
35)	L7 AR-1260-5	8.917	0.000	19418	0	14.722	N.D. #
36)	L8 AR-1262-1	8.374	0.000	8705	0	7.825	N.D. #
37)	L8 AR-1262-2	8.917	0.000	19418	0	11.014	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
Data File : PP035743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2021 1:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 06:46:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

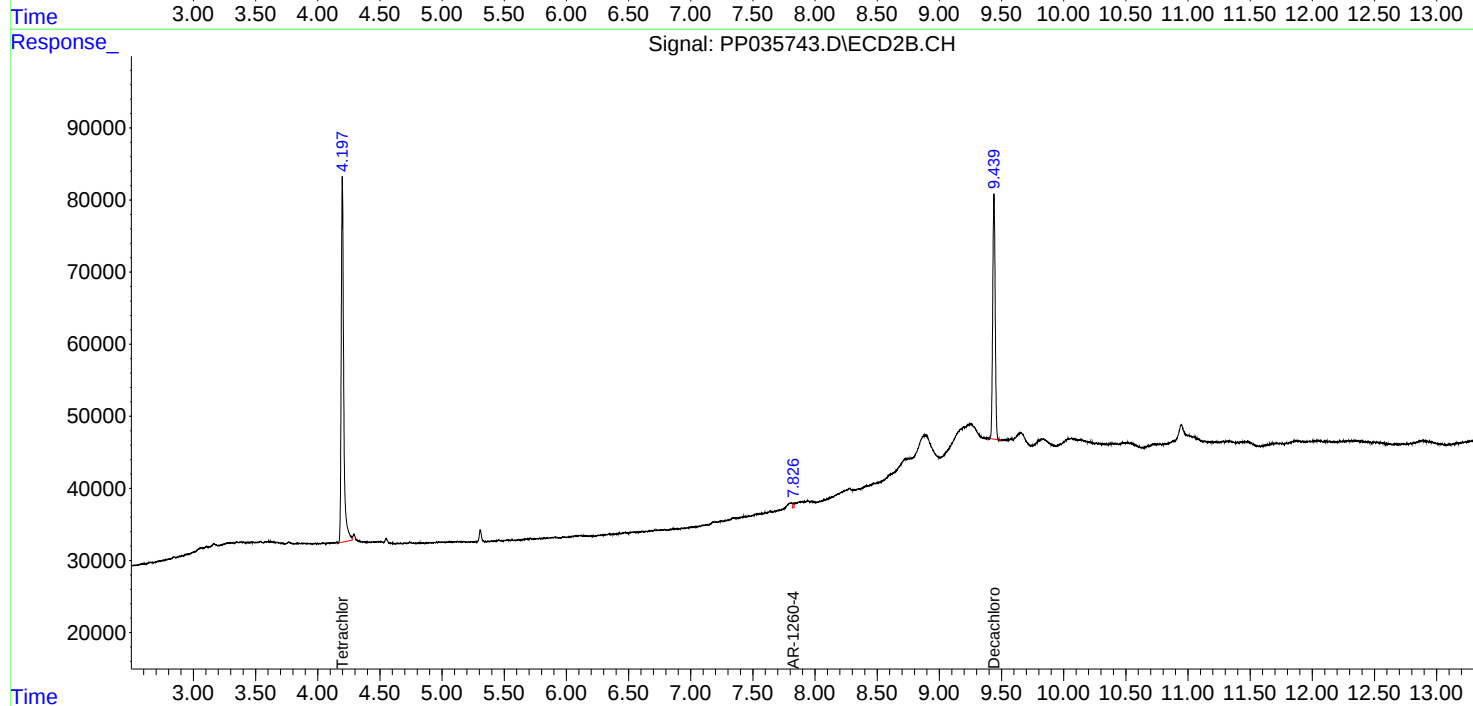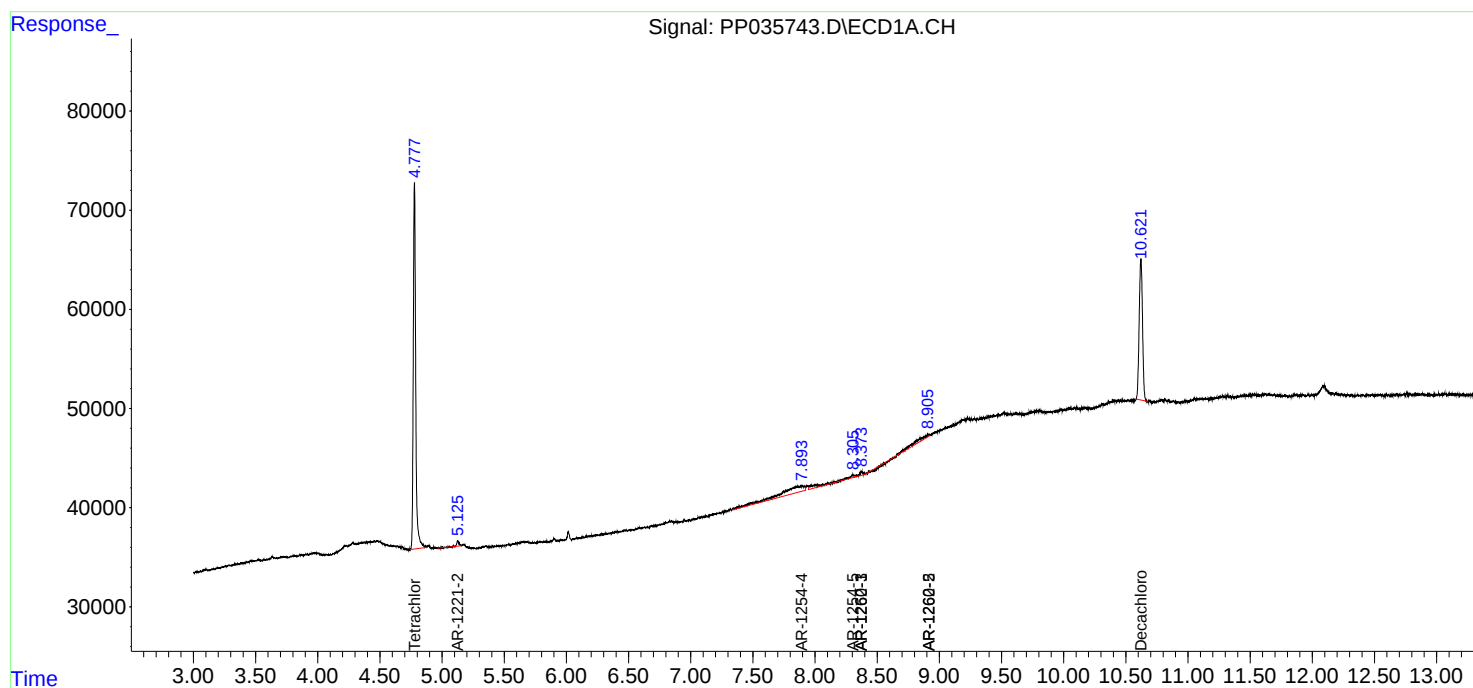


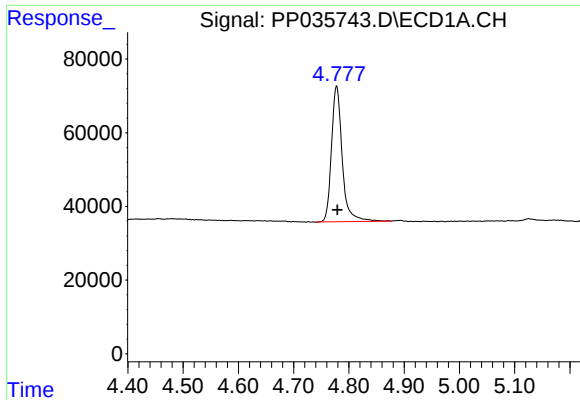

#1 Tetrachloro-m-xylene


R.T.: 4.778 min
Delta R.T.: -0.001 min
Response: 497696
Conc: 21.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

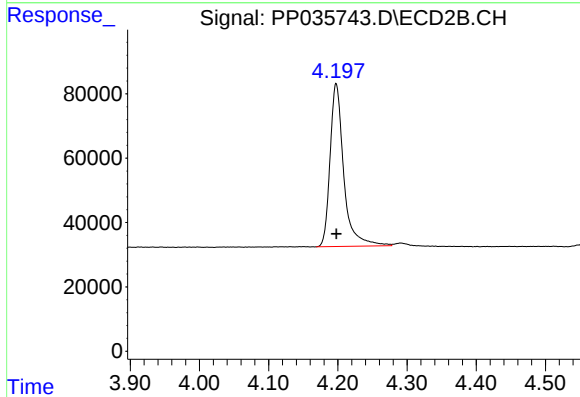


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: 0.000 min
Response: 696476
Conc: 20.49 ng/ml

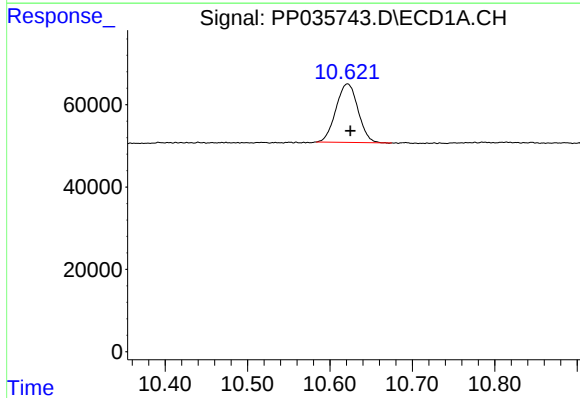


#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.003 min
Response: 263826
Conc: 23.44 ng/ml

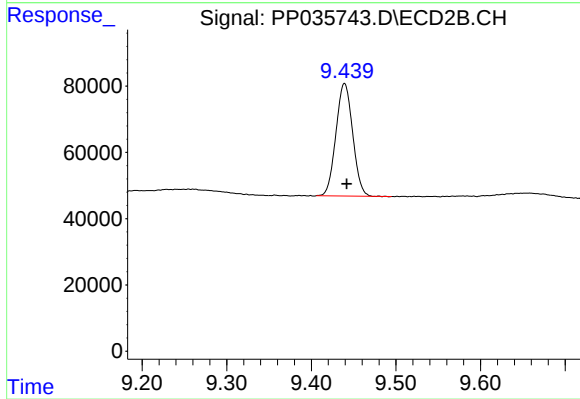

#2 Decachlorobiphenyl


R.T.: 9.439 min
Delta R.T.: -0.002 min
Response: 467834
Conc: 22.12 ng/ml

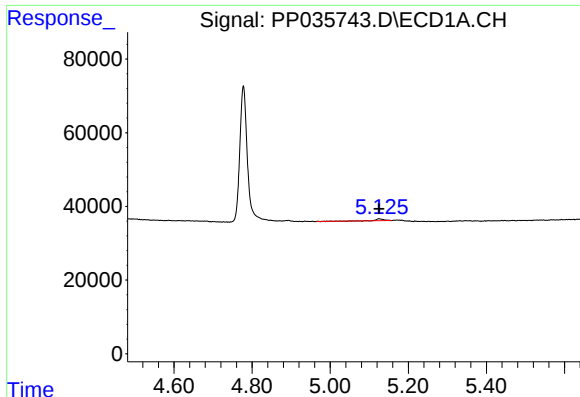

#9 AR-1221-2


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 7468
Conc: 33.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

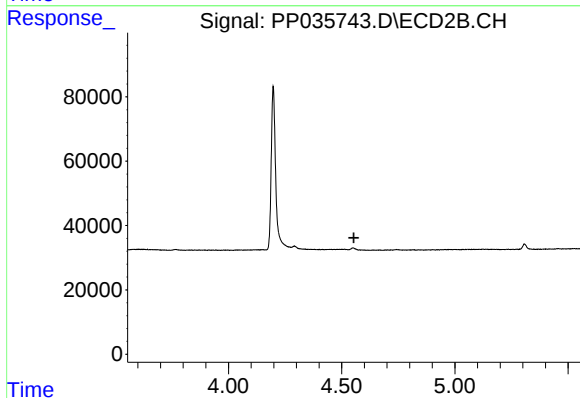


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

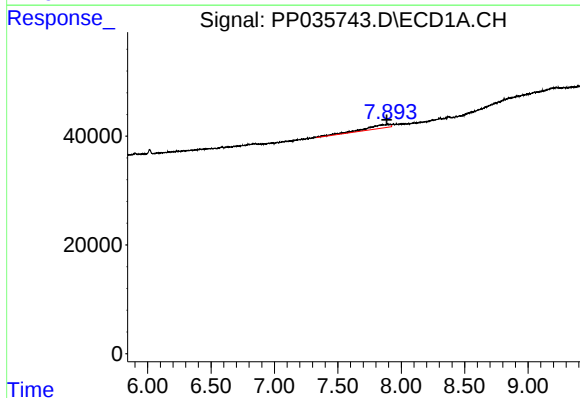


#29 AR-1254-4

R.T.: 7.895 min
Delta R.T.: 0.008 min
Response: 94739
Conc: 118.83 ng/ml

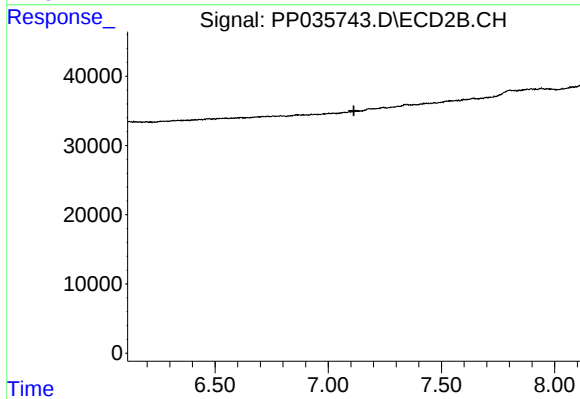

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

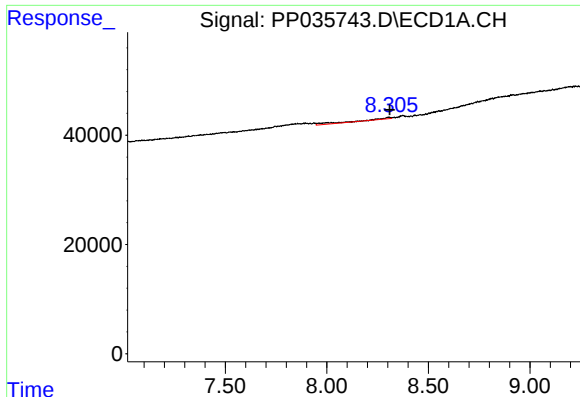

#30 AR-1254-5


R.T.: 8.306 min
Delta R.T.: -0.005 min
Response: 26665
Conc: 28.26 ng/ml

Instrument :
ECD_P
ClientSampleId :

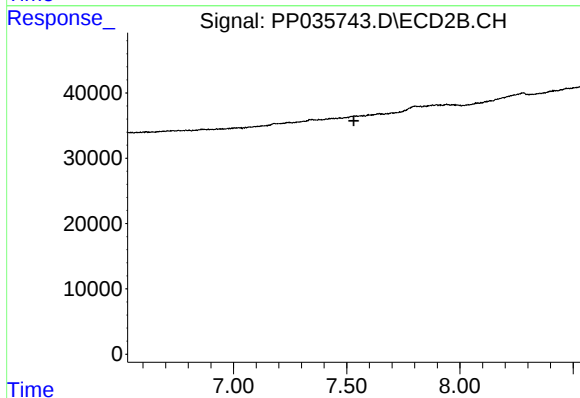


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.532 min
Response: 0
Conc: N.D.

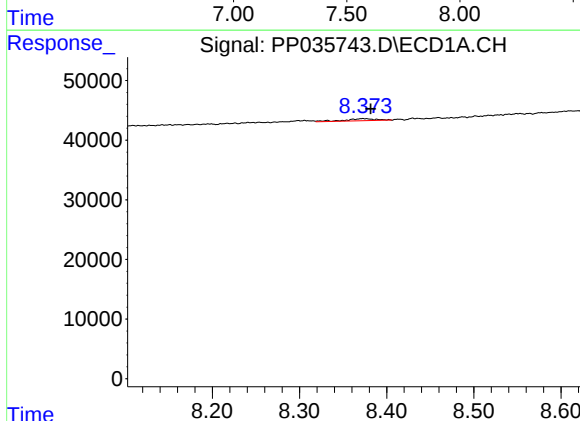


#33 AR-1260-3

R.T.: 8.374 min
Delta R.T.: -0.008 min
Response: 8705
Conc: 13.01 ng/ml

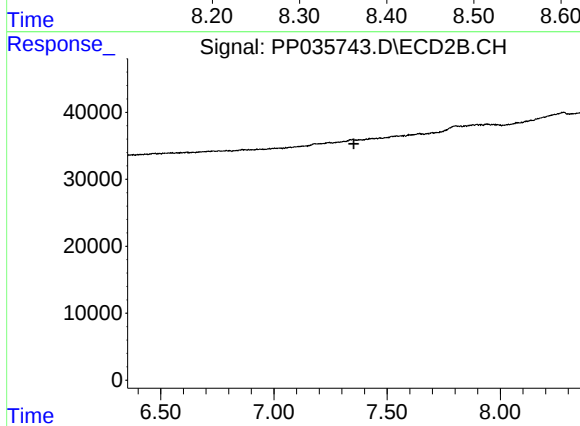

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.354 min
Response: 0
Conc: N.D.

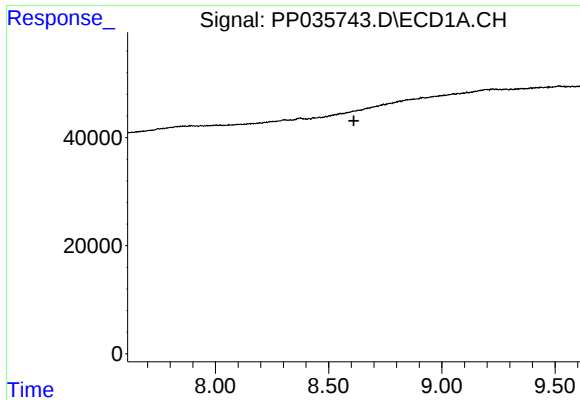


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :


Time

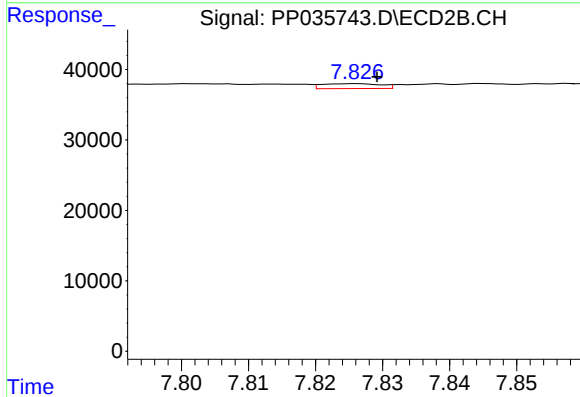

#34 AR-1260-4

R.T.: 7.826 min
Delta R.T.: -0.004 min
Response: 4237
Conc: 3.67 ng/ml


Time

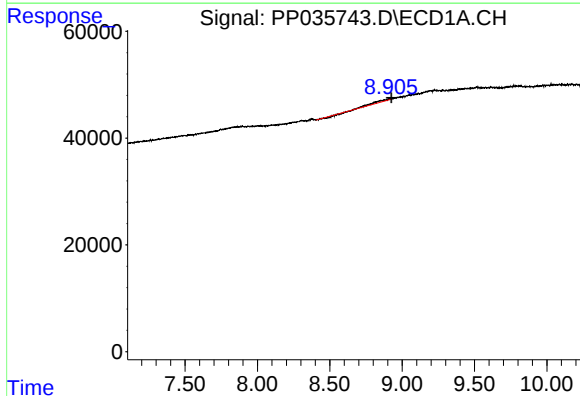

#35 AR-1260-5

R.T.: 8.917 min
Delta R.T.: -0.009 min
Response: 19418
Conc: 14.72 ng/ml


Time

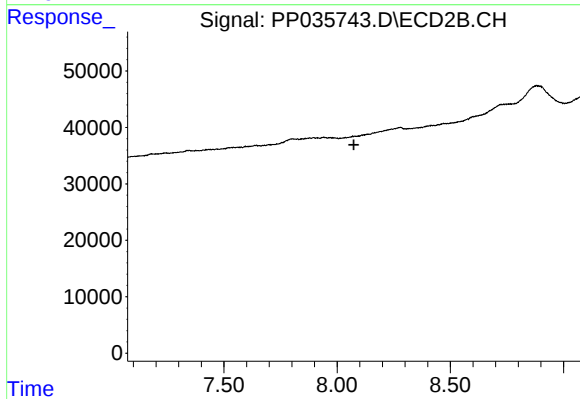

#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.074 min
Response: 0
Conc: N.D.


Time

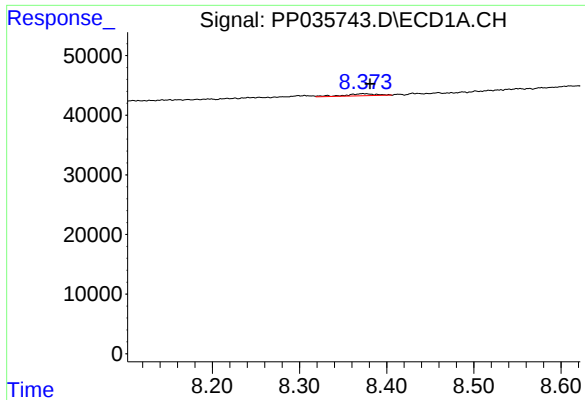

#36 AR-1262-1


R.T.: 8.374 min
Delta R.T.: -0.007 min
Response: 8705
Conc: 7.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

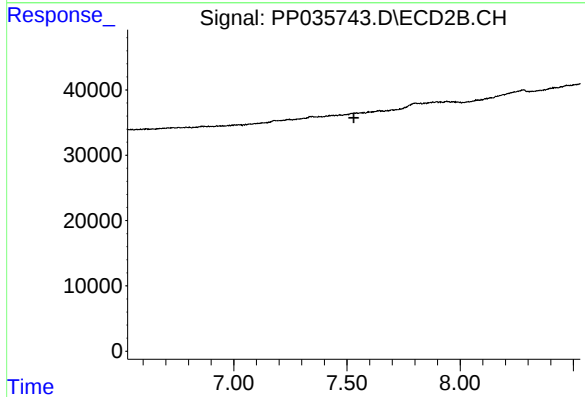


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.531 min
Response: 0
Conc: N.D.

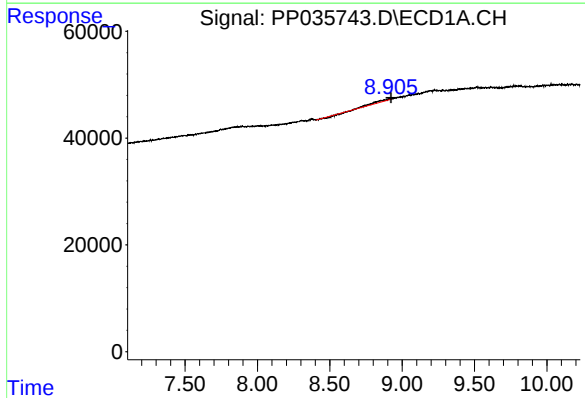

#37 AR-1262-2

R.T.: 8.917 min
Delta R.T.: -0.007 min
Response: 19418
Conc: 11.01 ng/ml

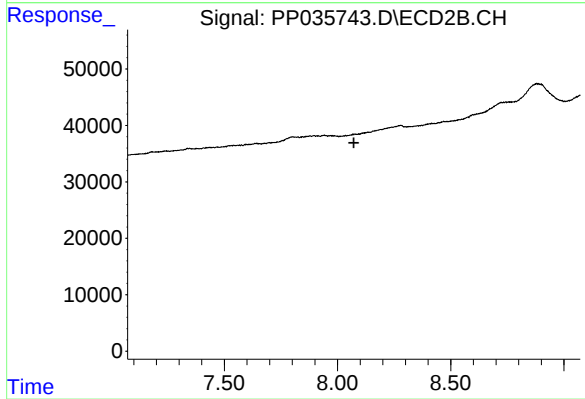

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.073 min
Response: 0
Conc: N.D.