

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
 Data File : PP035717.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2021 18:27
 Operator : DD\AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC750

Manual Integrations
 APPROVED

Ankita
 5/11/2021 4:08:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 05:20:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 05:17:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.779	4.197	1696061	2520813	74.978	75.858
2) SA Decachlor...	10.624	9.441	835101	1572314	74.564	74.500
Target Compounds						
21) L5 AR-1248-1	6.085	5.444	282910	356549	762.112	759.188
22) L5 AR-1248-2	6.374	5.697	392379	616404	748.943	750.790
23) L5 AR-1248-3	6.589	5.742	485429	647352	752.170	752.978
24) L5 AR-1248-4	7.016	5.926	486388	740676	742.032	748.919
25) L5 AR-1248-5	7.056	6.348	516930	837363	754.796	735.639m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
Data File : PP035717.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2021 18:27
Operator : DD\AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
AR1248ICC750


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 05:20:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 05:17:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

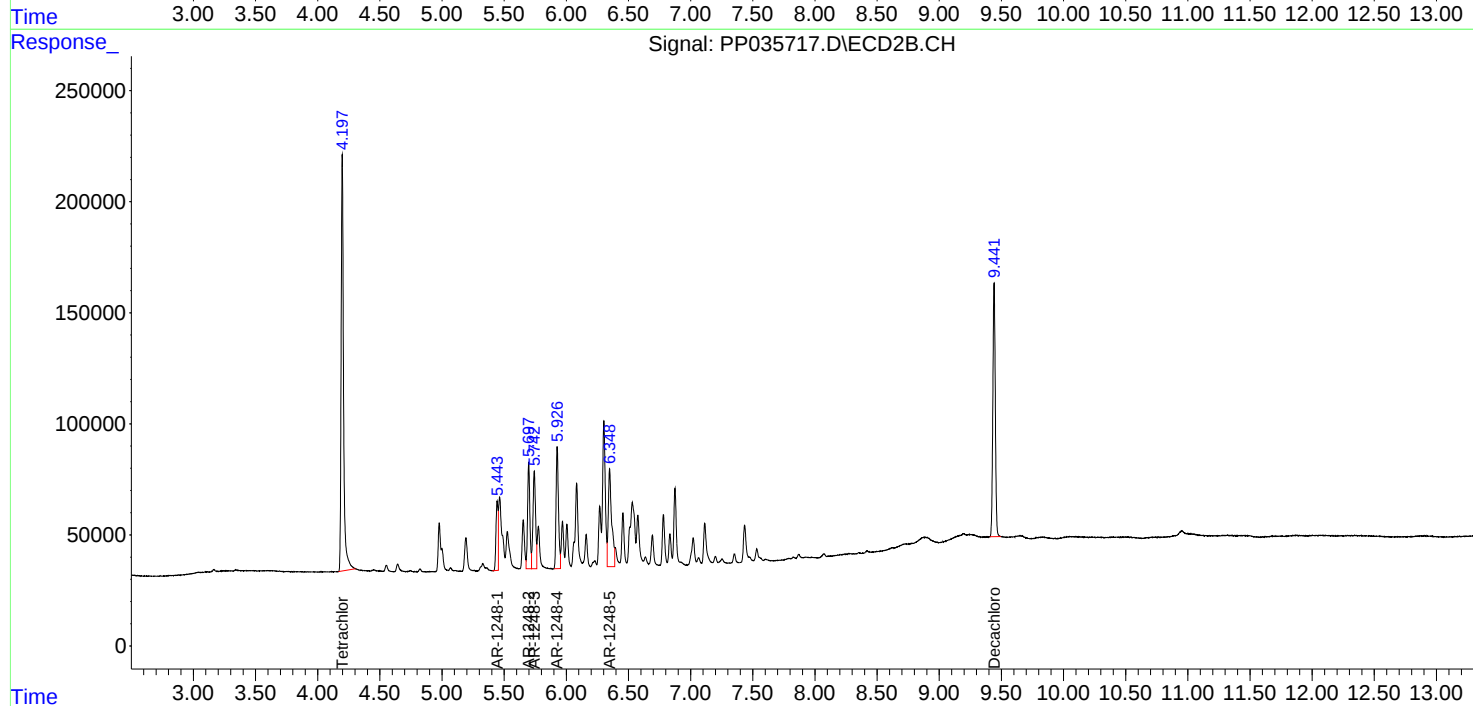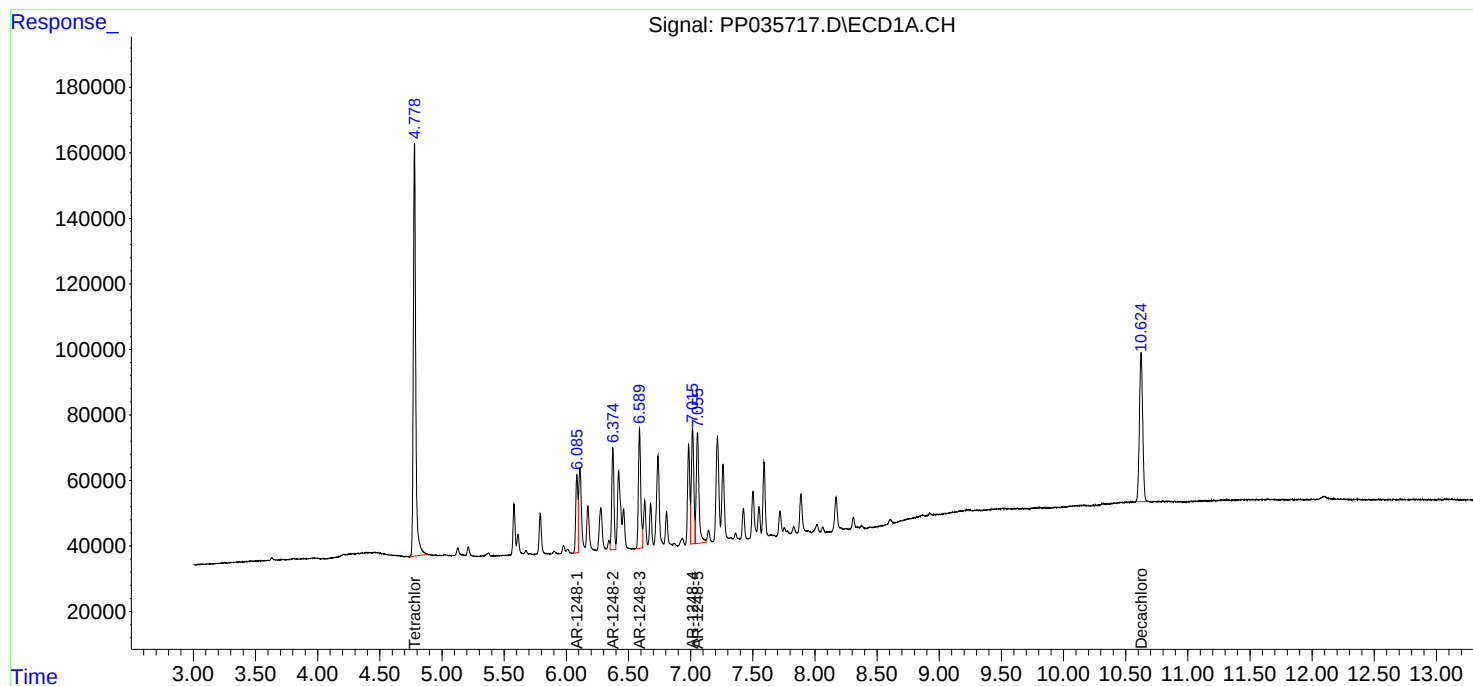

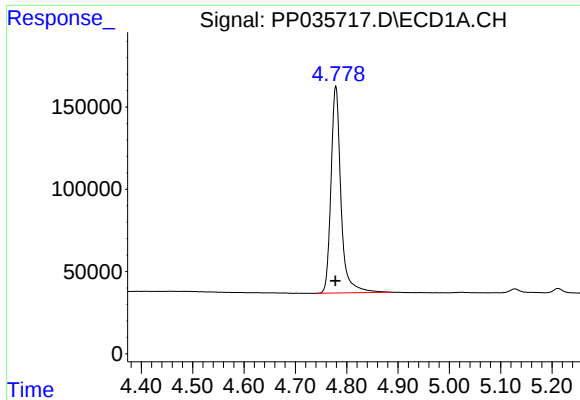


#1 Tetrachloro-m-xylene

R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 1696061
Conc: 74.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:41 PM

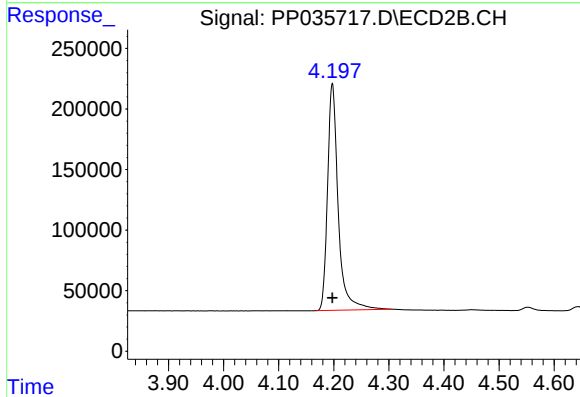


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: 0.000 min
Response: 2520813
Conc: 75.86 ng/ml

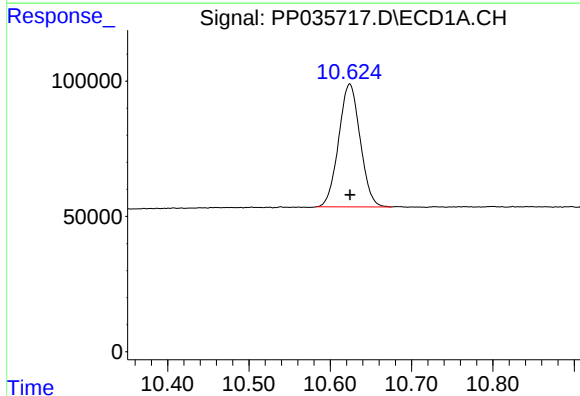


#2 Decachlorobiphenyl

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 835101
Conc: 74.56 ng/ml

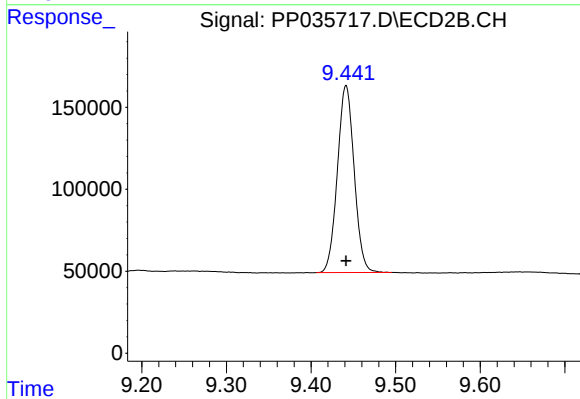

#2 Decachlorobiphenyl

R.T.: 9.441 min
Delta R.T.: 0.000 min
Response: 1572314
Conc: 74.50 ng/ml

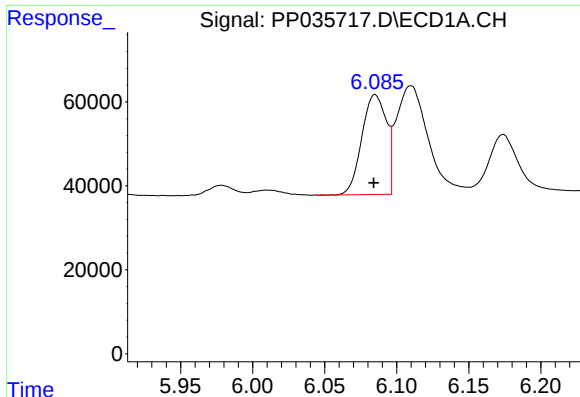


#21 AR-1248-1

R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 282910
Conc: 762.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:41 PM

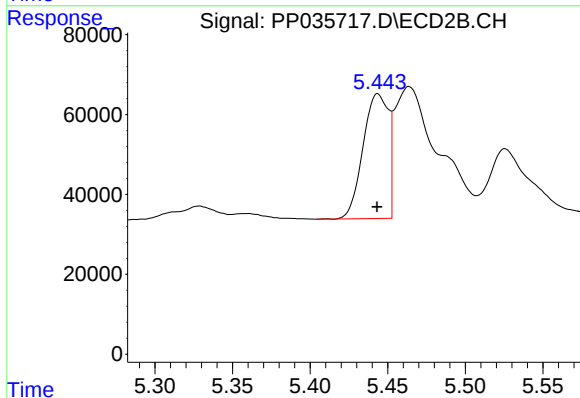


#21 AR-1248-1

R.T.: 5.444 min
Delta R.T.: 0.000 min
Response: 356549
Conc: 759.19 ng/ml

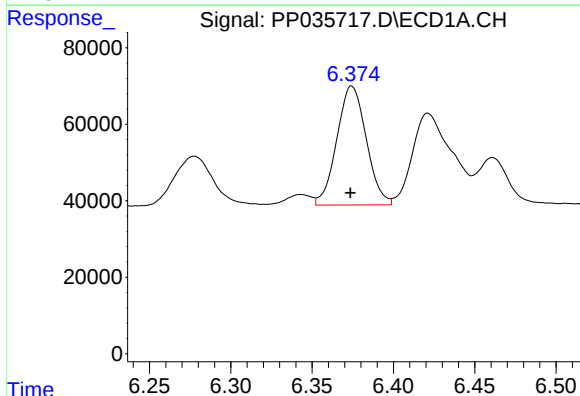


#22 AR-1248-2

R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 392379
Conc: 748.94 ng/ml

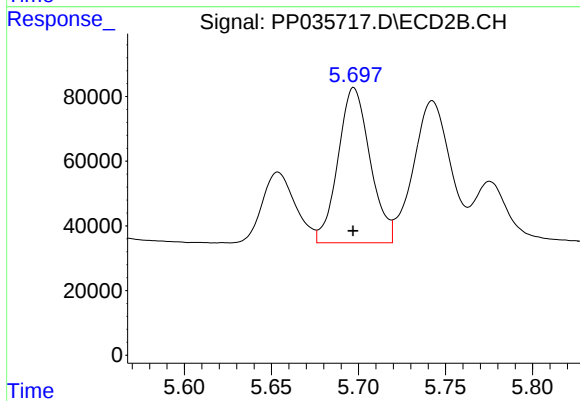

#22 AR-1248-2

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 616404
Conc: 750.79 ng/ml

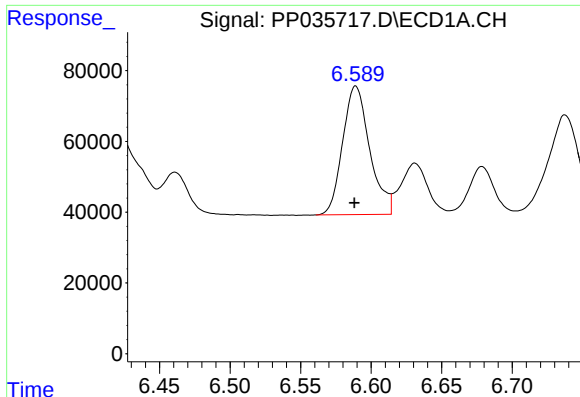


#23 AR-1248-3

R.T.: 6.589 min
Delta R.T.: 0.000 min
Response: 485429
Conc: 752.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:41 PM

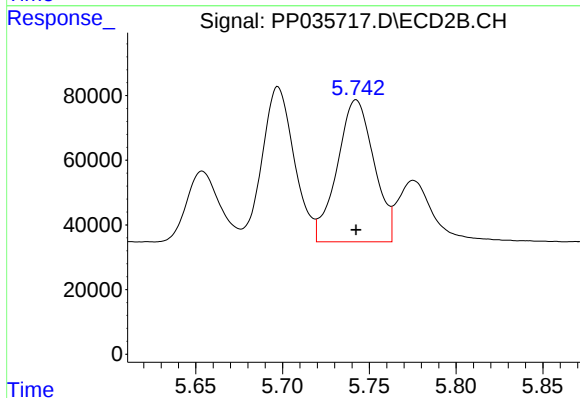


#23 AR-1248-3

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 647352
Conc: 752.98 ng/ml

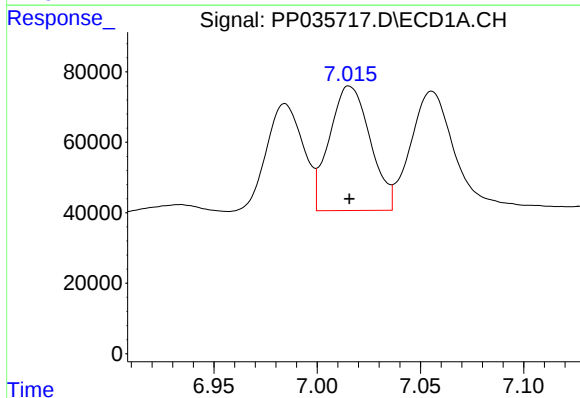


#24 AR-1248-4

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 486388
Conc: 742.03 ng/ml

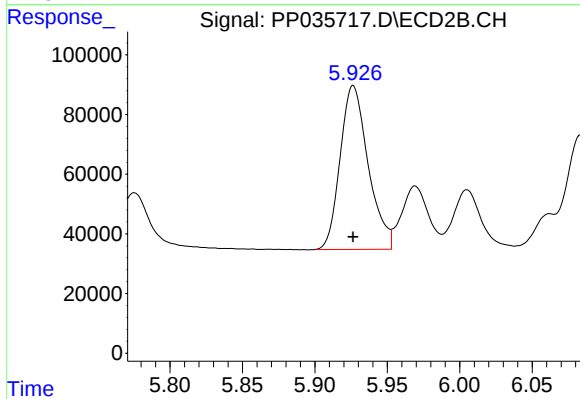

#24 AR-1248-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 740676
Conc: 748.92 ng/ml

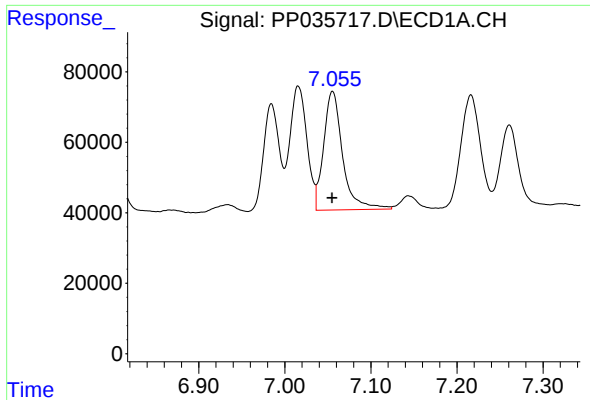


#25 AR-1248-5

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 516930
Conc: 754.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750

Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:41 PM

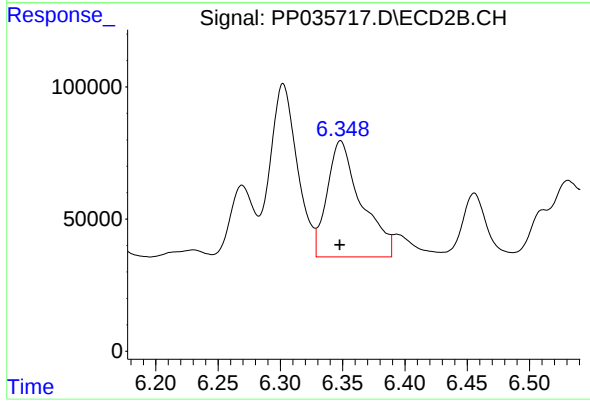

#25 AR-1248-5

R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 837363
Conc: 735.64 ng/ml m