

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
 Data File : PP035718.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2021 18:44
 Operator : DD\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC500

Manual Integrations
 APPROVED

Ankita
 5/11/2021 4:08:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 05:17:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 05:17:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.779	4.198	1180141	1713682	50.000	50.000
2) SA Decachlor...	10.625	9.442	589710	1103848	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	6.085	5.445	192888	238422	500.000	500.000
22) L5 AR-1248-2	6.375	5.697	275350	434389	500.000	500.000
23) L5 AR-1248-3	6.590	5.743	341109	454308	500.000	500.000
24) L5 AR-1248-4	7.016	5.927	345212	523399	500.000	500.000
25) L5 AR-1248-5	7.056	6.349	360365	591728	500.000	506.199m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
Data File : PP035718.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2021 18:44
Operator : DD\AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC500


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 05:17:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 05:17:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

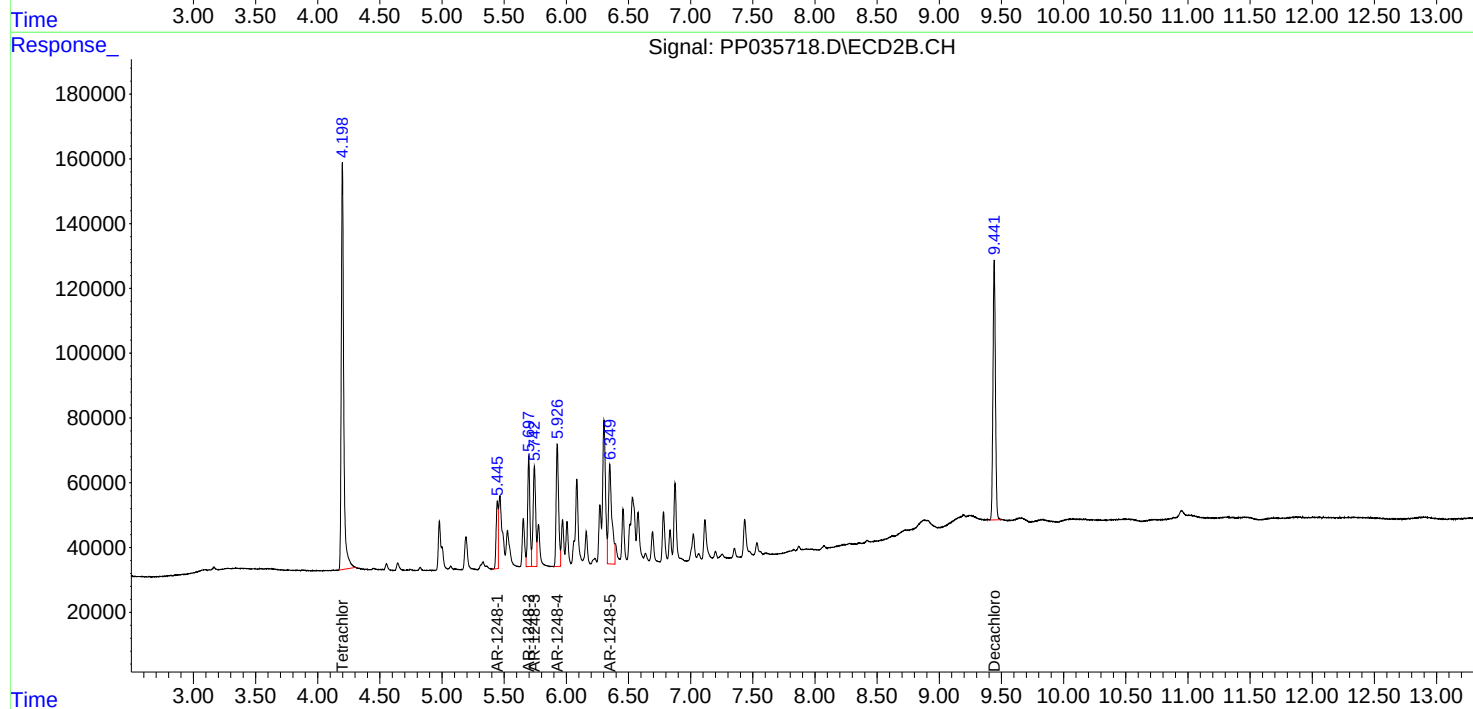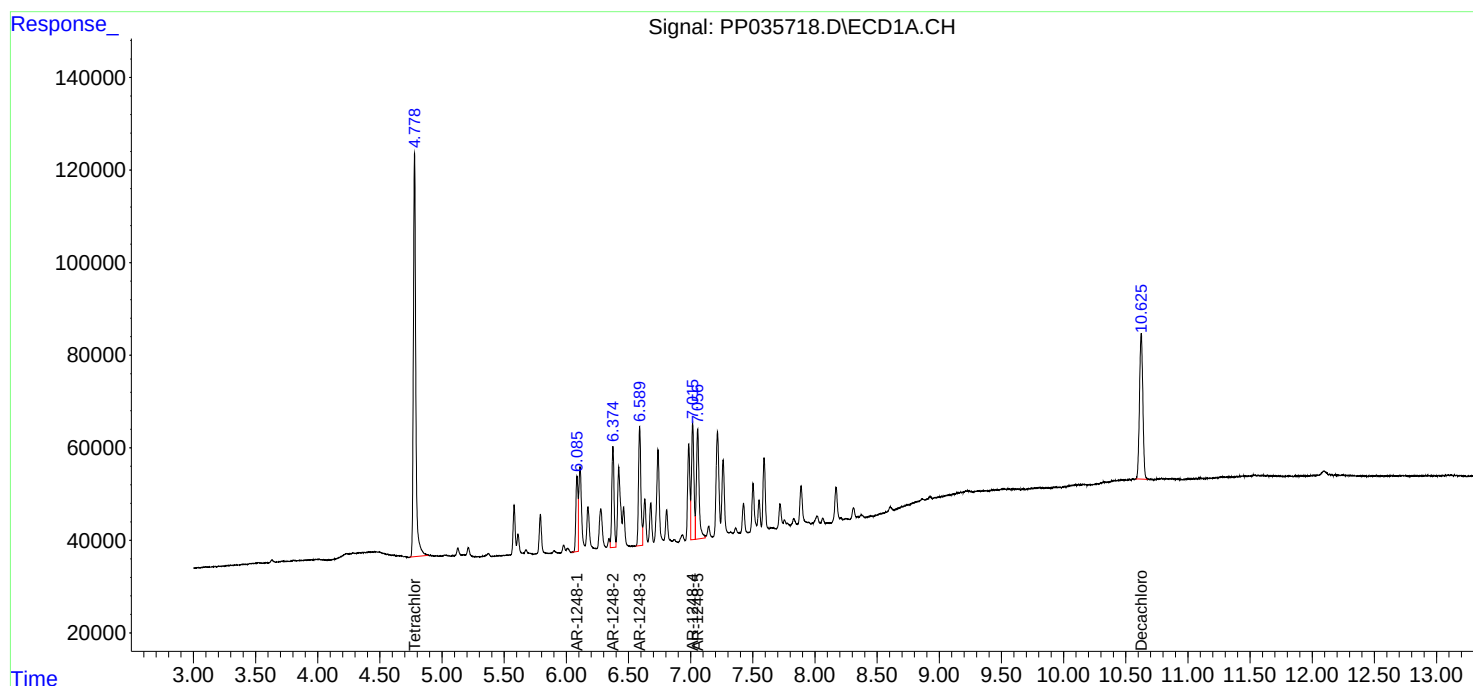

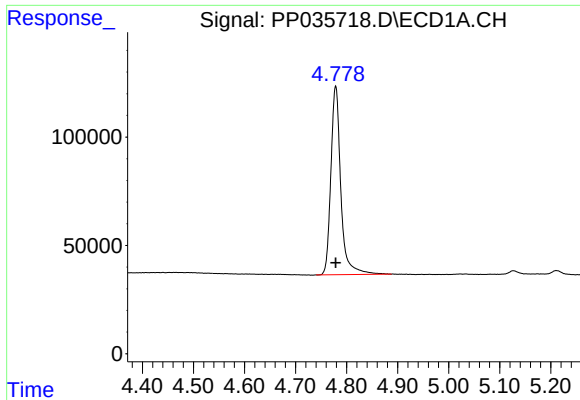


#1 Tetrachloro-m-xylene

R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 1180141
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:43 PM

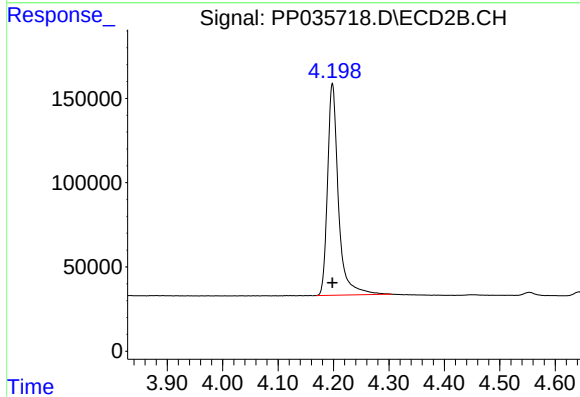


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: 0.000 min
Response: 1713682
Conc: 50.00 ng/ml

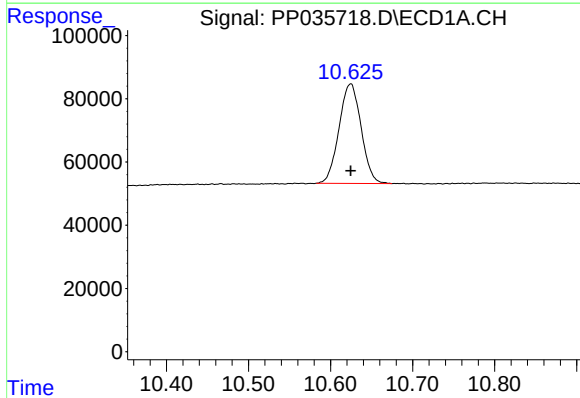


#2 Decachlorobiphenyl

R.T.: 10.625 min
Delta R.T.: 0.000 min
Response: 589710
Conc: 50.00 ng/ml

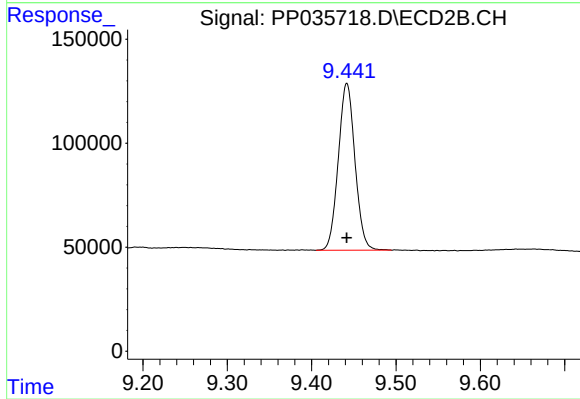

#2 Decachlorobiphenyl

R.T.: 9.442 min
Delta R.T.: 0.000 min
Response: 1103848
Conc: 50.00 ng/ml

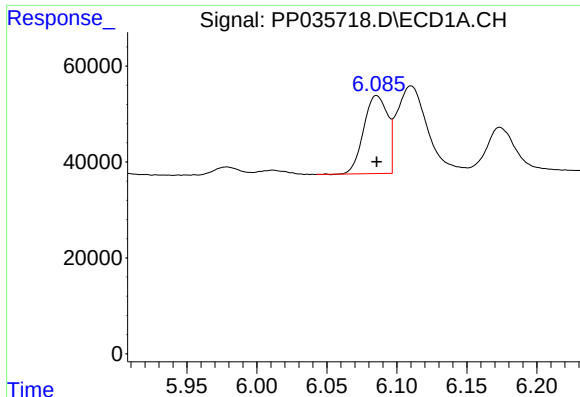


#21 AR-1248-1

R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 192888
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:43 PM

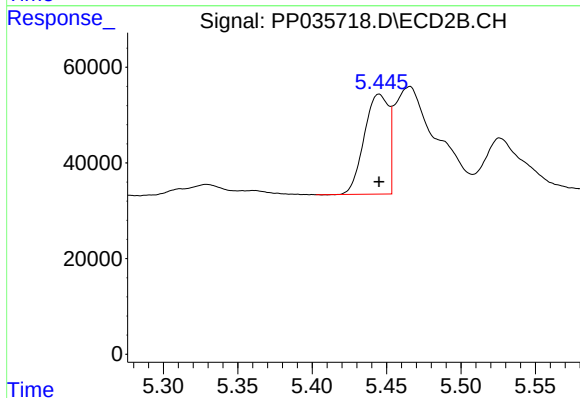


#21 AR-1248-1

R.T.: 5.445 min
Delta R.T.: 0.000 min
Response: 238422
Conc: 500.00 ng/ml

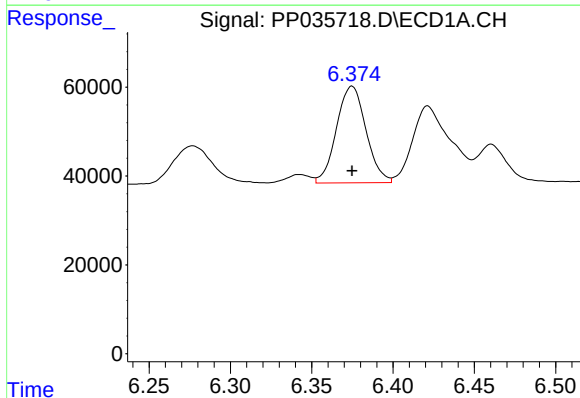


#22 AR-1248-2

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 275350
Conc: 500.00 ng/ml

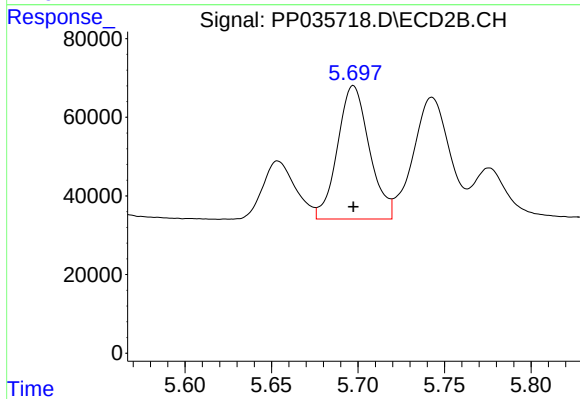

#22 AR-1248-2

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 434389
Conc: 500.00 ng/ml

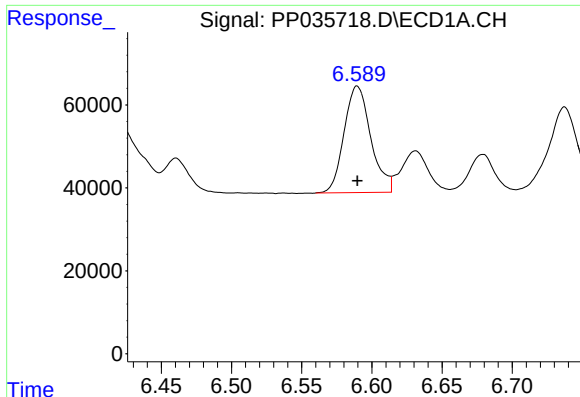


#23 AR-1248-3

R.T.: 6.590 min
Delta R.T.: 0.000 min
Response: 341109
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:43 PM

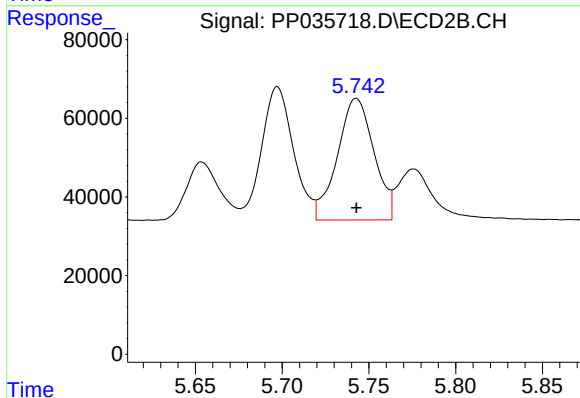


#23 AR-1248-3

R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 454308
Conc: 500.00 ng/ml

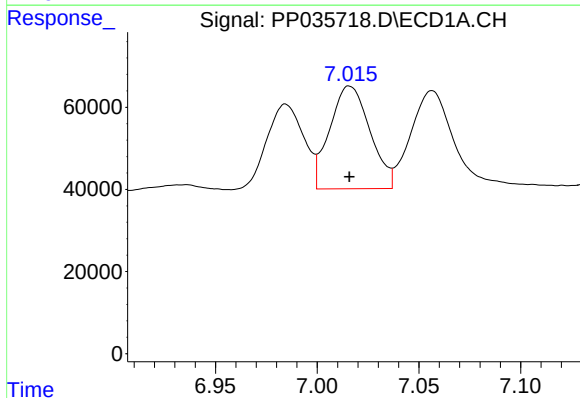


#24 AR-1248-4

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 345212
Conc: 500.00 ng/ml

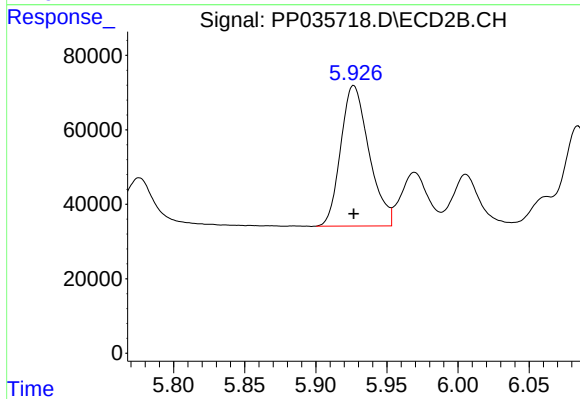

#24 AR-1248-4

R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 523399
Conc: 500.00 ng/ml

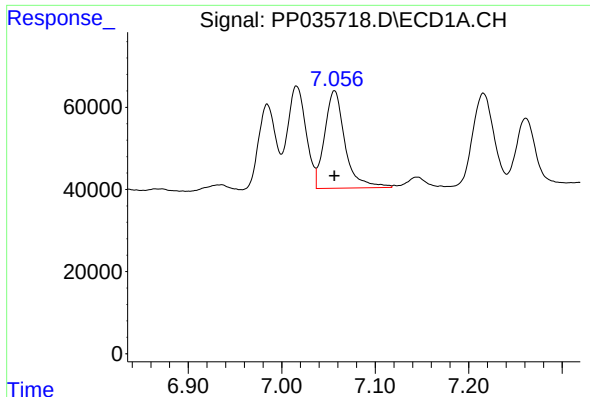


#25 AR-1248-5

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 360365
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:43 PM

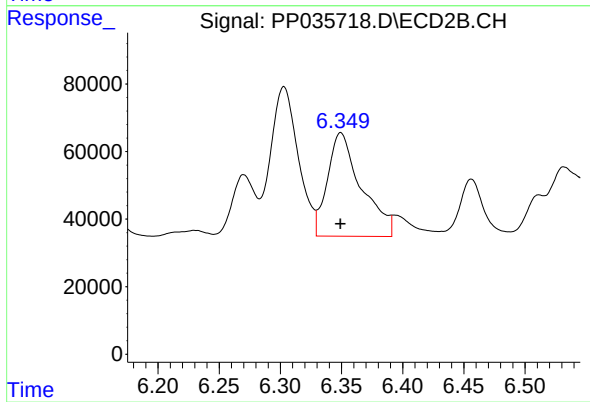

#25 AR-1248-5

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 591728
Conc: 506.20 ng/ml m