

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
 Data File : PP035719.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2021 19:01
 Operator : DD\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC250

Manual Integrations
 APPROVED

Ankita
 5/11/2021 4:08:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 05:22:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 05:17:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.779	4.198	630073	899014	27.083	26.435
2)	SA Decachlor...	10.623	9.442	310649	574877	27.036	26.686
Target Compounds							
21)	L5 AR-1248-1	6.087	5.446	95718	115458	254.819	246.111
22)	L5 AR-1248-2	6.375	5.698	145489	230643	270.306	272.429
23)	L5 AR-1248-3	6.590	5.743	180621	238063	271.563	269.391
24)	L5 AR-1248-4	7.017	5.927	176057	273535	264.378	269.513
25)	L5 AR-1248-5	7.057	6.350	178730	299725	257.733	257.474m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051021\
Data File : PP035719.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2021 19:01
Operator : DD\AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 05:22:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 05:17:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

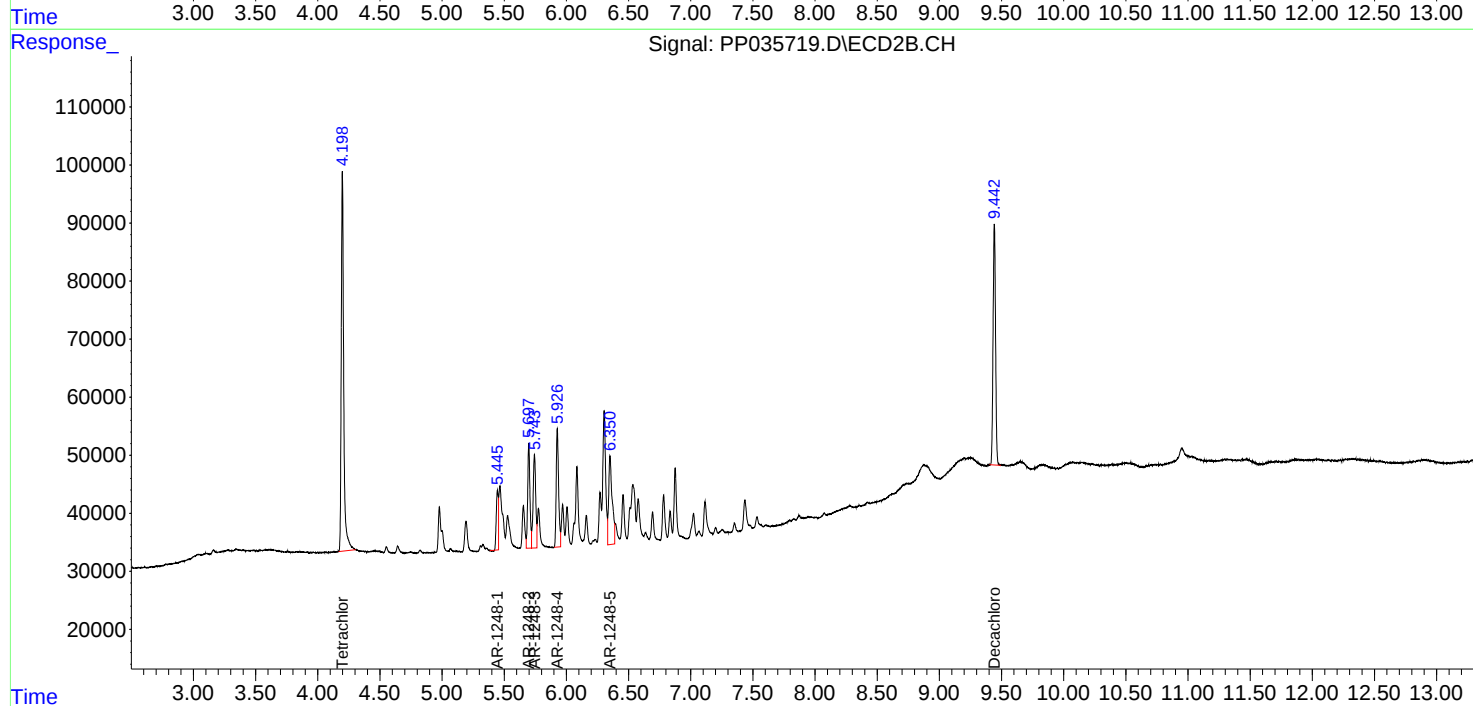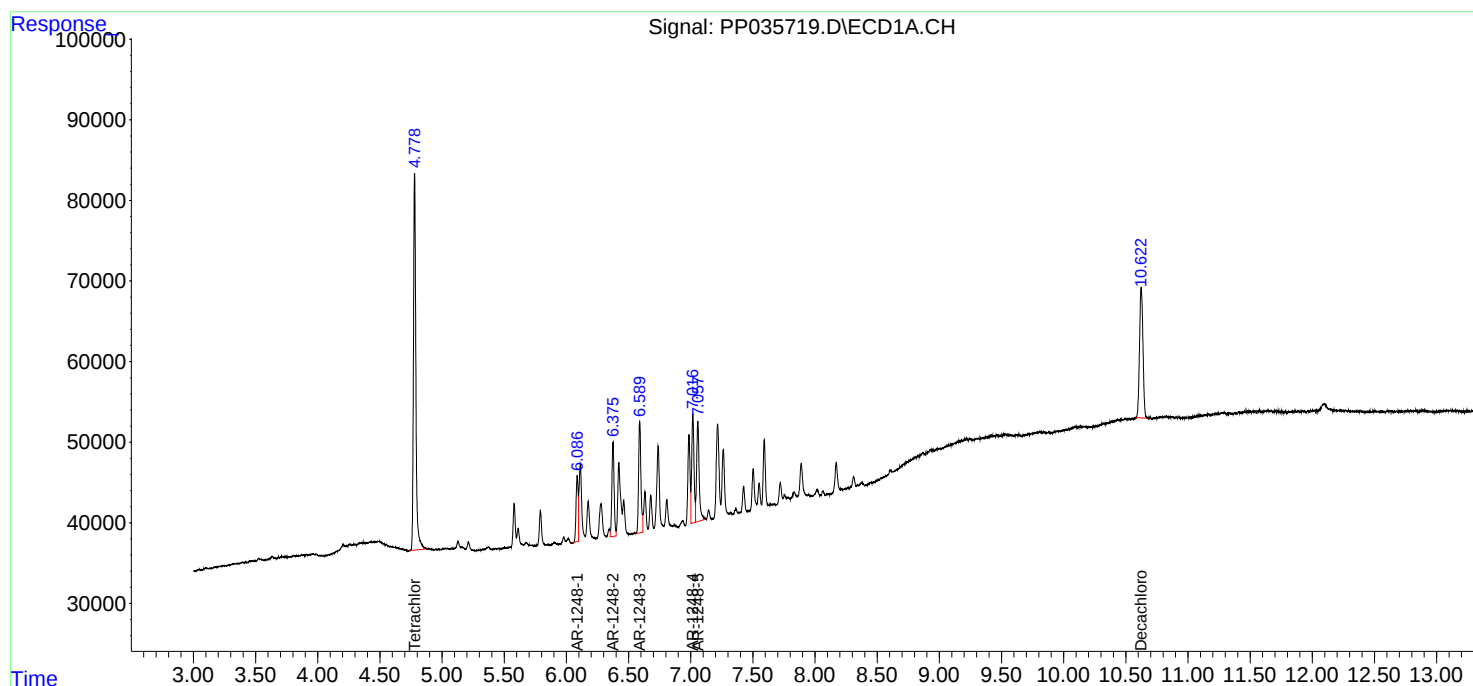

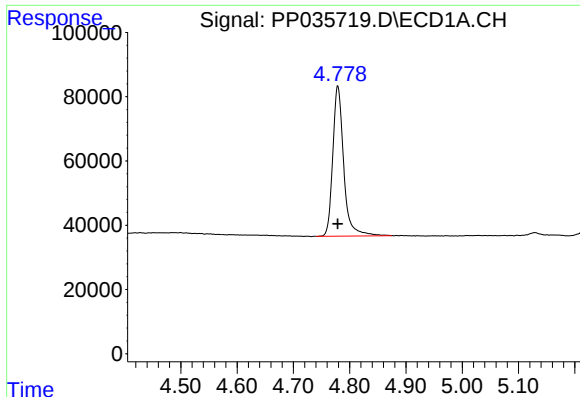


#1 Tetrachloro-m-xylene

R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 630073
Conc: 27.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:44 PM

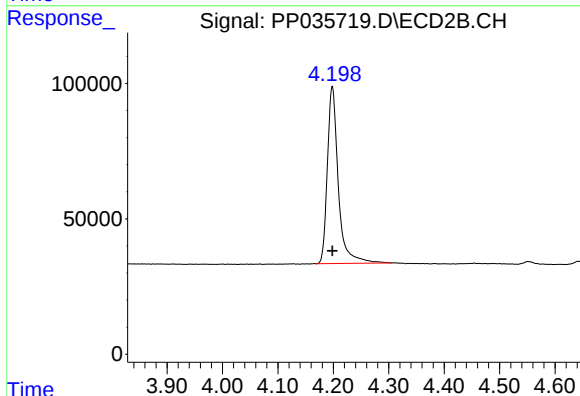


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: 0.000 min
Response: 899014
Conc: 26.44 ng/ml

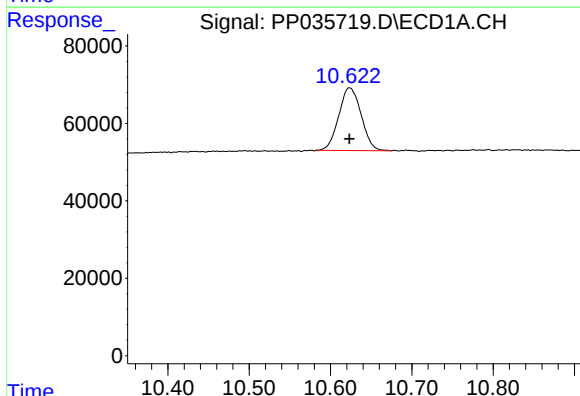


#2 Decachlorobiphenyl

R.T.: 10.623 min
Delta R.T.: 0.000 min
Response: 310649
Conc: 27.04 ng/ml

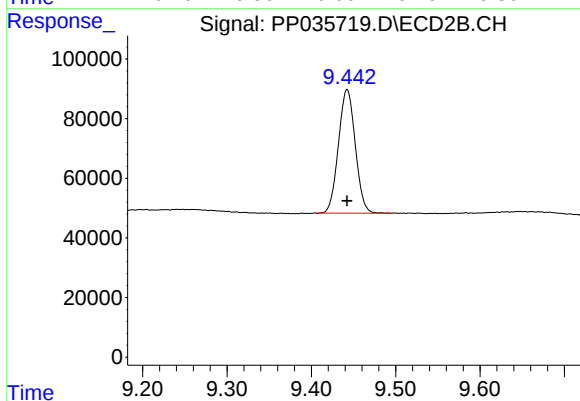

#2 Decachlorobiphenyl

R.T.: 9.442 min
Delta R.T.: 0.000 min
Response: 574877
Conc: 26.69 ng/ml

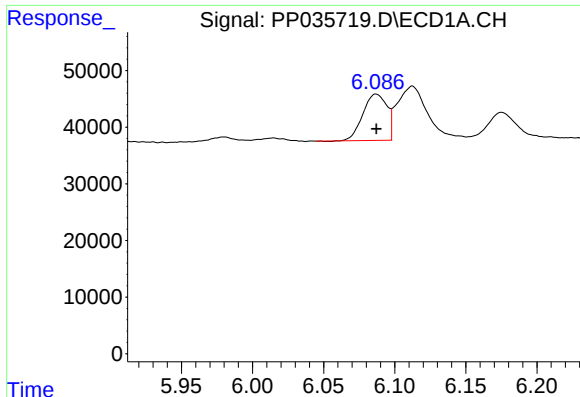


#21 AR-1248-1

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 95718
Conc: 254.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:44 PM

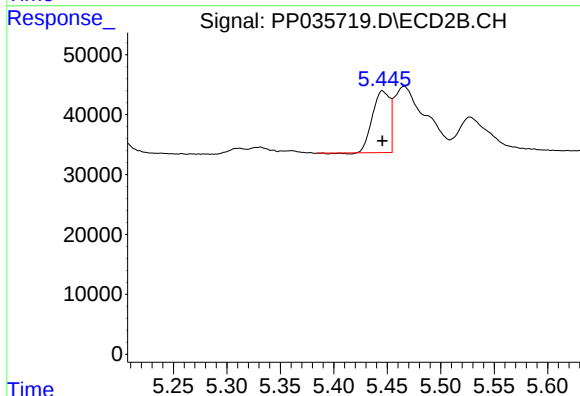


#21 AR-1248-1

R.T.: 5.446 min
Delta R.T.: 0.000 min
Response: 115458
Conc: 246.11 ng/ml

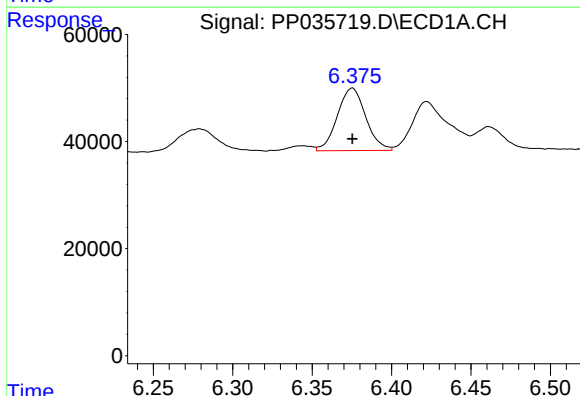


#22 AR-1248-2

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 145489
Conc: 270.31 ng/ml

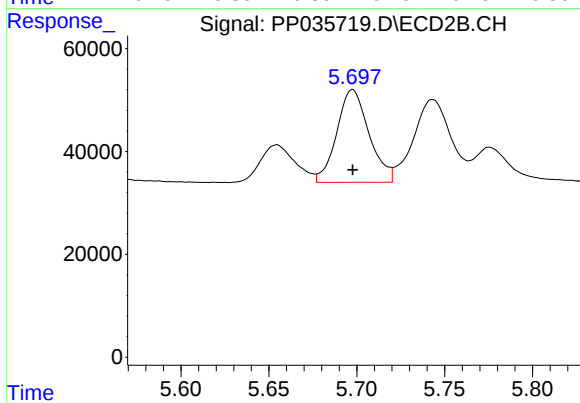

#22 AR-1248-2

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 230643
Conc: 272.43 ng/ml

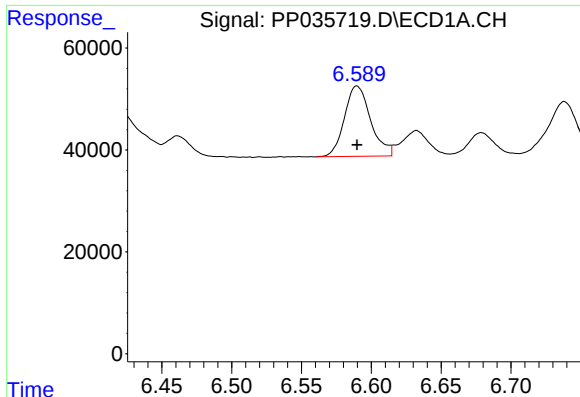


#23 AR-1248-3

R.T.: 6.590 min
Delta R.T.: 0.000 min
Response: 180621
Conc: 271.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:44 PM

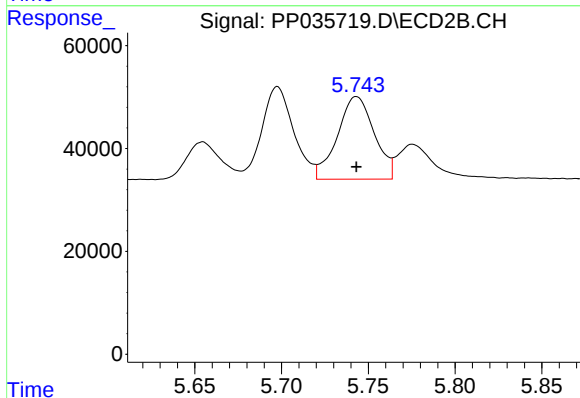


#23 AR-1248-3

R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 238063
Conc: 269.39 ng/ml

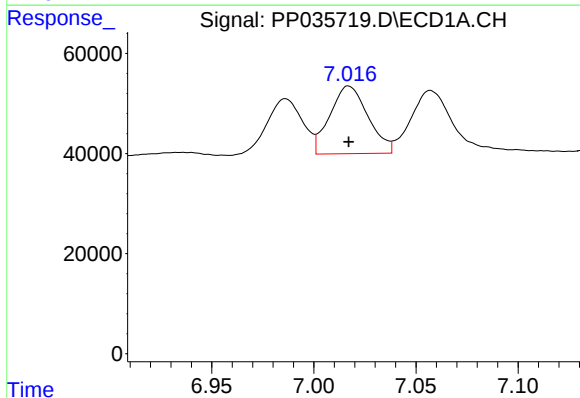


#24 AR-1248-4

R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 176057
Conc: 264.38 ng/ml

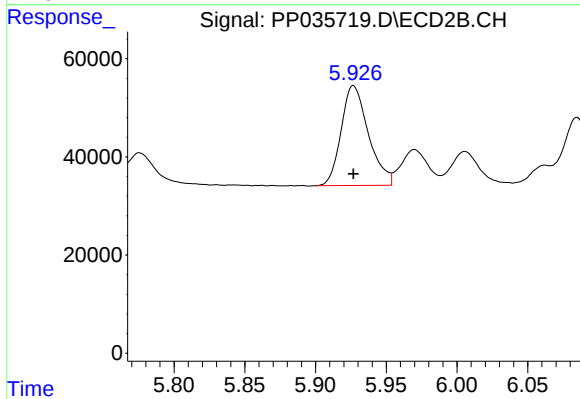

#24 AR-1248-4

R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 273535
Conc: 269.51 ng/ml

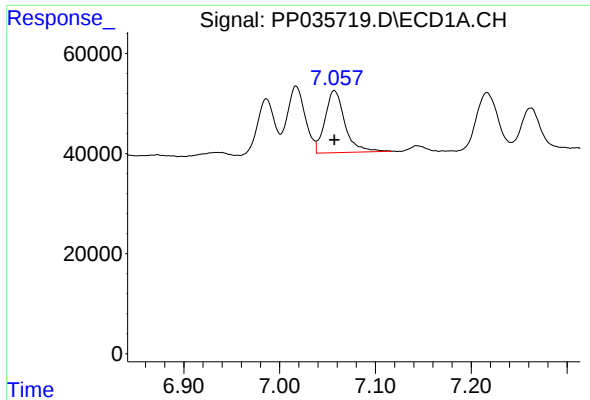


#25 AR-1248-5

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 178730
Conc: 257.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250

Manual Integrations
APPROVED

Ankita
5/11/2021 4:08:44 PM

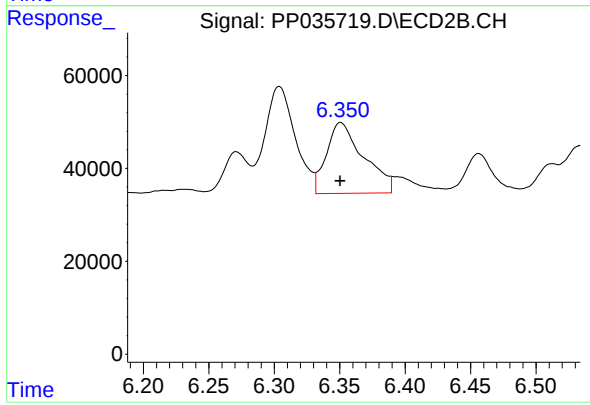

#25 AR-1248-5

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 299725
Conc: 257.47 ng/ml m