

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
 Data File : PP047360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2022 20:56
 Operator : YP\AJ
 Sample : N2725-02RE
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-1284RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/11/2022
 Supervised By :mohammad ahmed 05/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 01:36:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 10 18:34:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.854	3.123	23133875	36223310	9.099m	11.002m
2) SA Decachlor...	9.962f	8.469f	16899808	27819269	11.813m	10.220m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
Data File : PP047360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2022 20:56
Operator : YP\AJ
Sample : N2725-02RE
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-1284RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/11/2022
Supervised By :mohammad ahmed 05/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 01:36:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 10 18:34:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

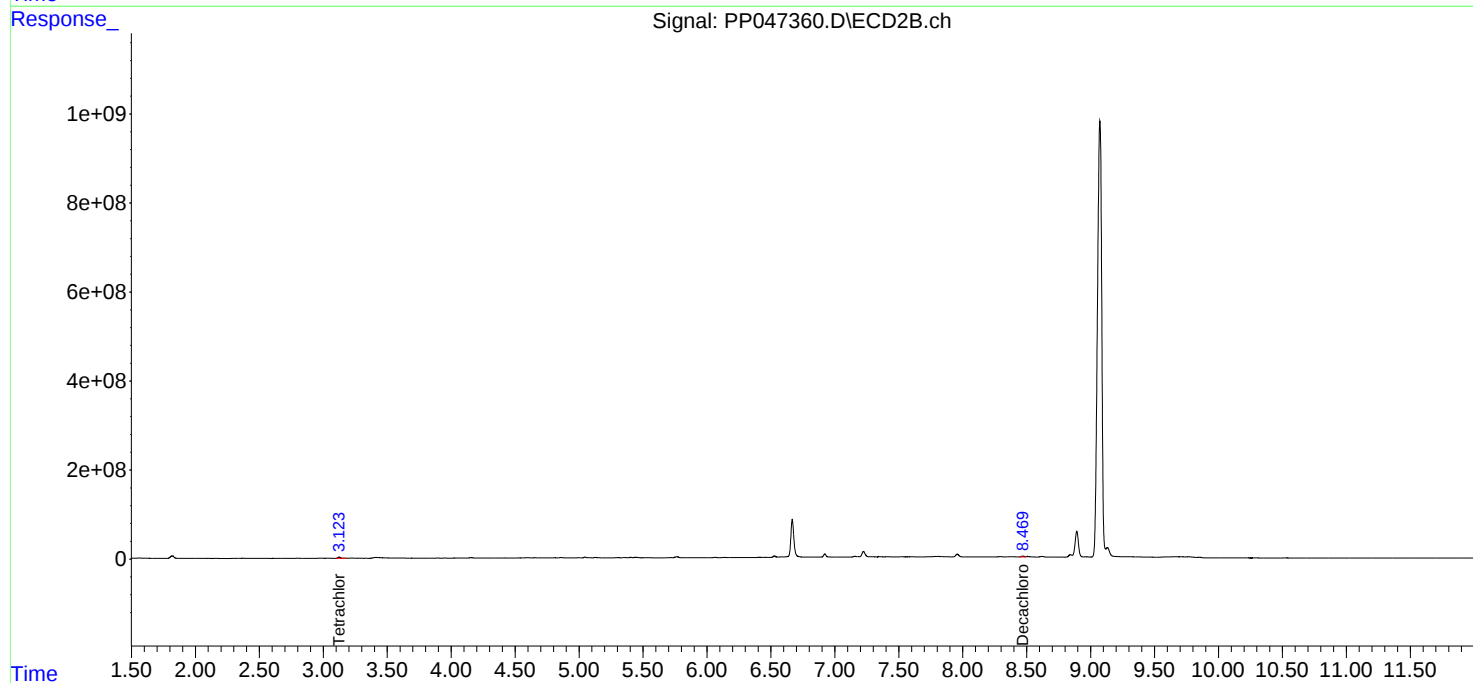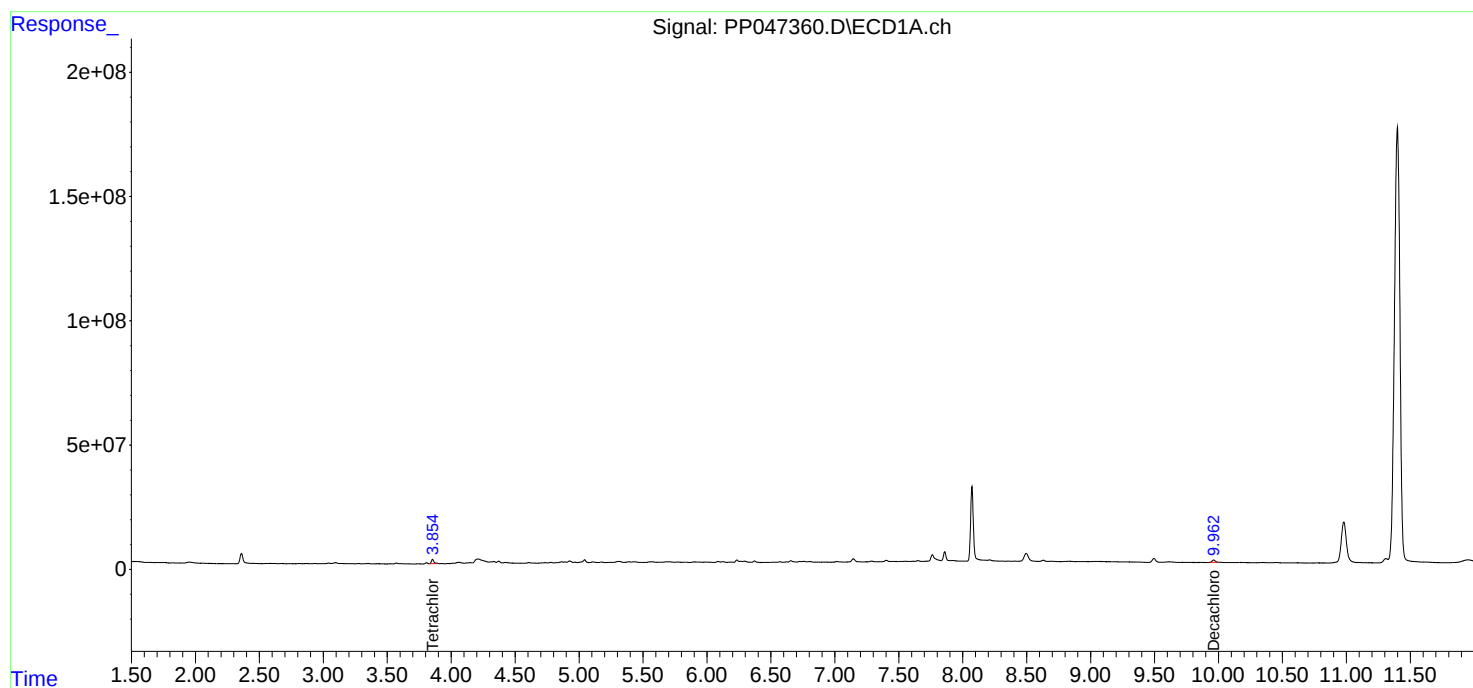

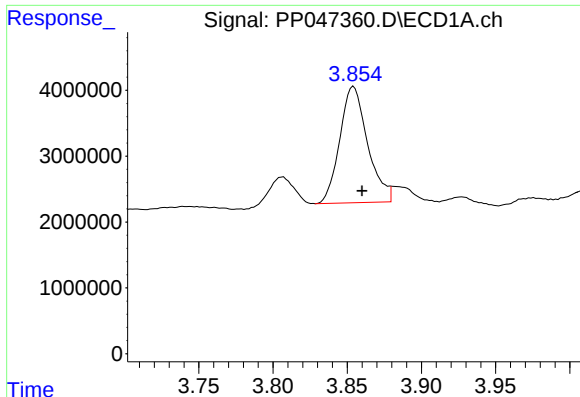


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.006 min
Response: 23133875
Conc: 9.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1284RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/11/2022
Supervised By :mohammad ahmed 05/11/2022

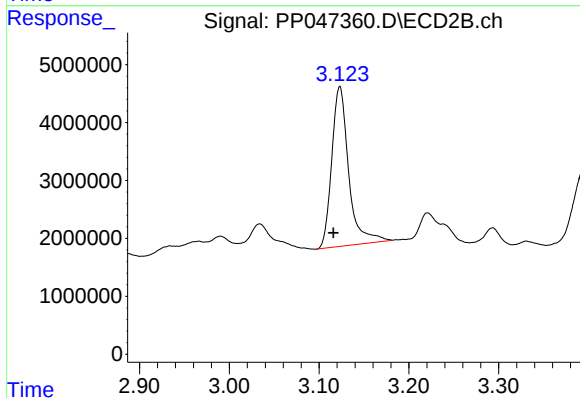


#1 Tetrachloro-m-xylene

R.T.: 3.123 min
Delta R.T.: 0.007 min
Response: 36223310
Conc: 11.00 ng/ml m

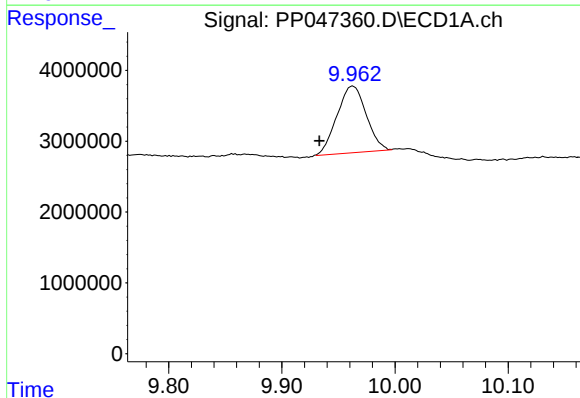

#2 Decachlorobiphenyl

R.T.: 9.962 min
Delta R.T.: 0.029 min
Response: 16899808
Conc: 11.81 ng/ml m

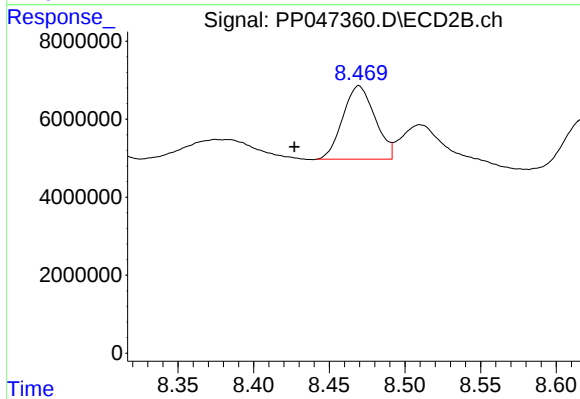

#2 Decachlorobiphenyl

R.T.: 8.469 min
Delta R.T.: 0.042 min
Response: 27819269
Conc: 10.22 ng/ml m