

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
 Data File : PP047365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2022 22:12
 Operator : YP\AJ
 Sample : N2742-01RE
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-1RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/12/2022
 Supervised By :mohammad ahmed 05/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 06:33:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 10 18:34:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.853	3.125	49712017	71901933	19.554m	21.838m
2) SA Decachlor...	9.936f	8.447f	31623681	46244170	22.106m	16.989

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
Data File : PP047365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2022 22:12
Operator : YP\AJ
Sample : N2742-01RE
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/12/2022
Supervised By :mohammad ahmed 05/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 06:33:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 10 18:34:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

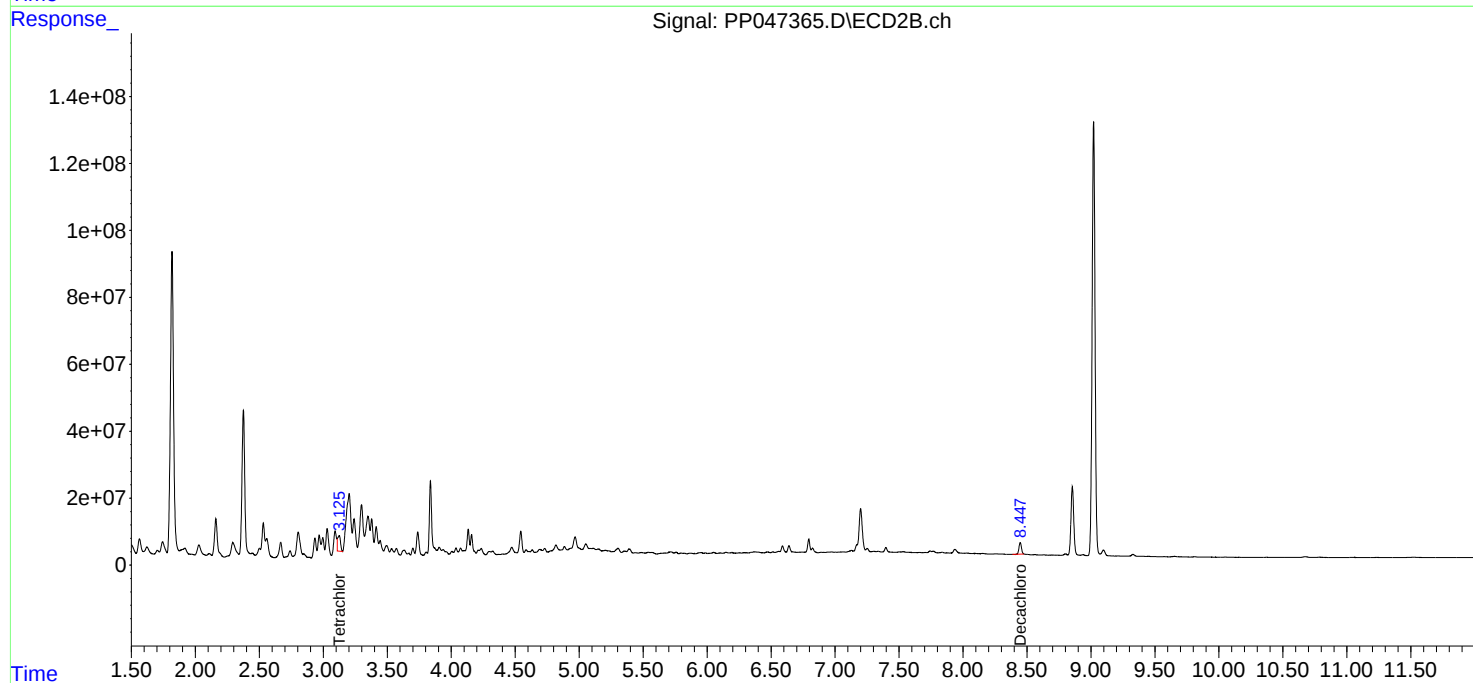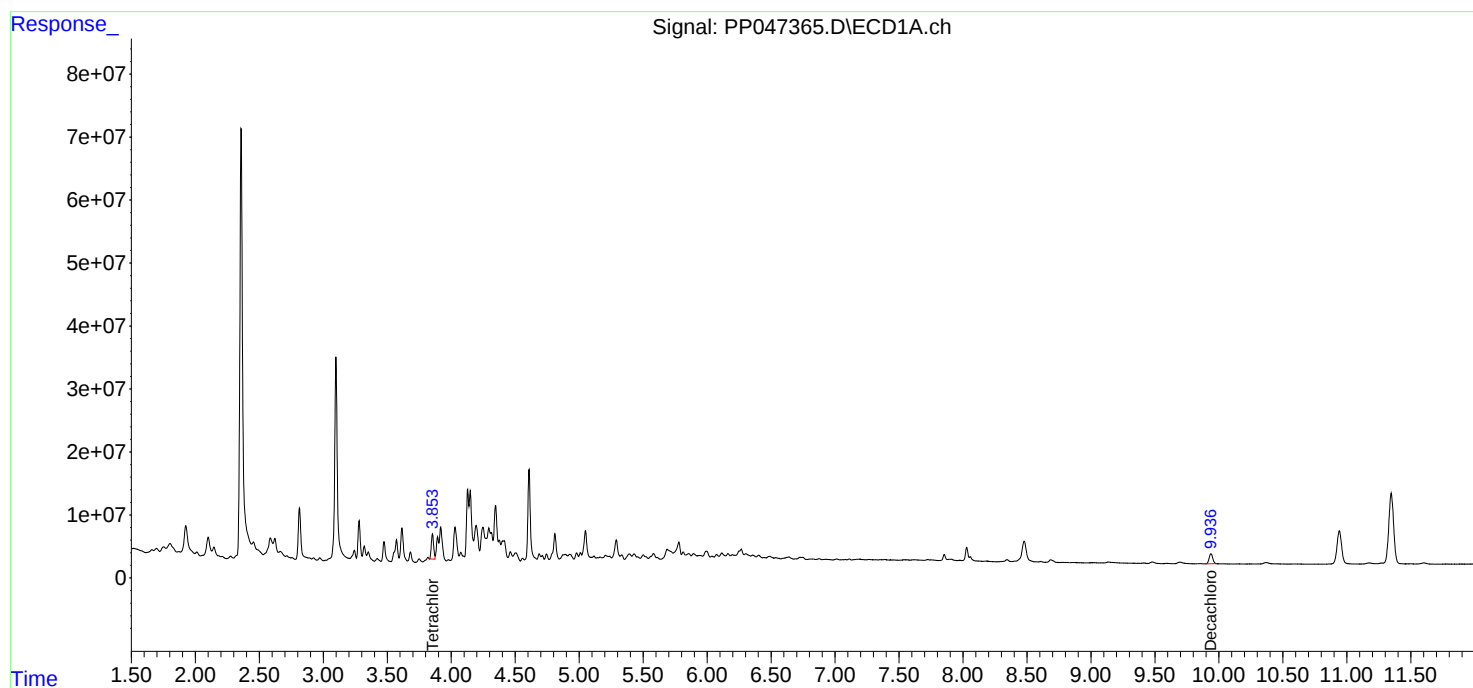

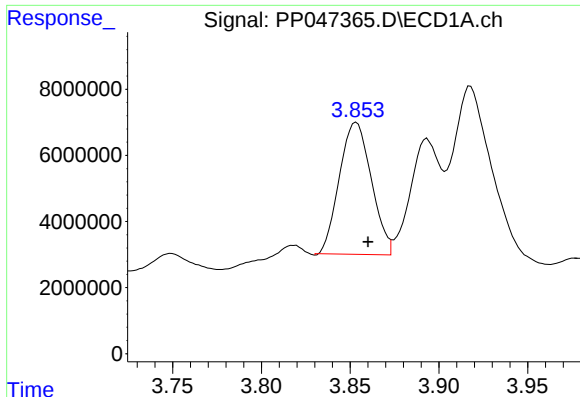


#1 Tetrachloro-m-xylene

R.T.: 3.853 min
Delta R.T.: -0.007 min
Response: 49712017
Conc: 19.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/12/2022
Supervised By :mohammad ahmed 05/12/2022

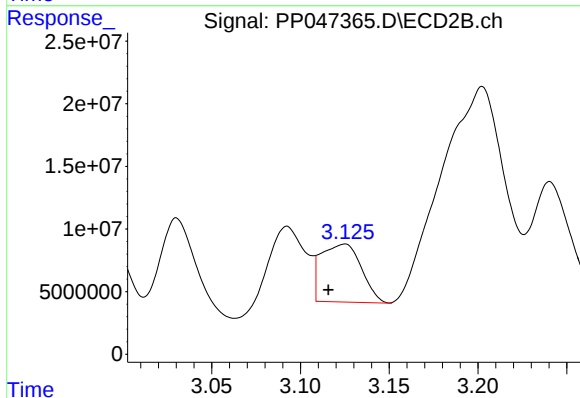


#1 Tetrachloro-m-xylene

R.T.: 3.125 min
Delta R.T.: 0.009 min
Response: 71901933
Conc: 21.84 ng/ml m

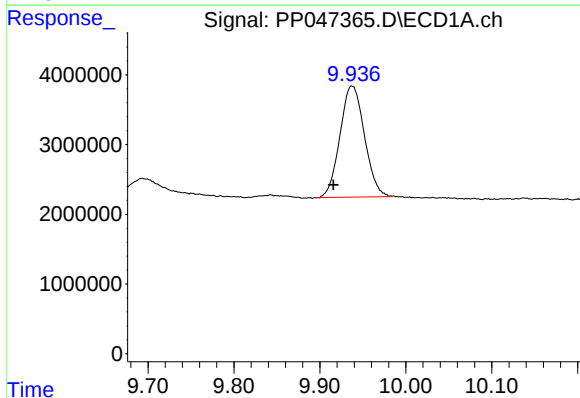

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.020 min
Response: 31623681
Conc: 22.11 ng/ml m

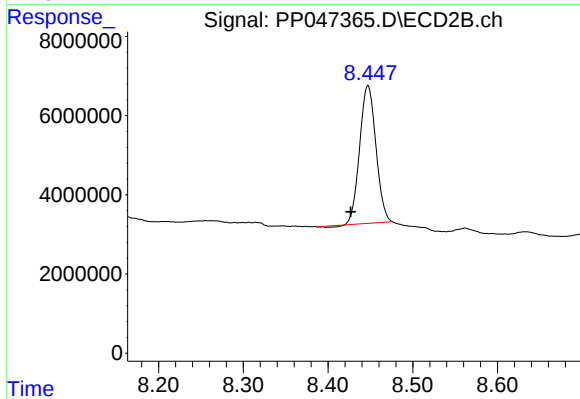

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: 0.020 min
Response: 46244170
Conc: 16.99 ng/ml