

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
 Data File : PP047388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 06:04
 Operator : YP\AJ
 Sample : N2743-10 10X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SOM-2022-32B

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 09:08:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 10 18:34:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

05/12/2022
 Supervised By :mohammad
 ahmed

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	05/12/2022
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	3.847	3.114	2780444	4877594	1.094m	1.481 #
2) SA Decachlor...	9.916	8.425	2601340	4081133	1.818	1.499

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051022\
Data File : PP047388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 06:04
Operator : YP\AJ
Sample : N2743-10 10X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SOM-2022-32B


Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 09:08:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 10 18:34:51 2022
Response via : Initial Calibration
Integrator: ChemStation

05/12/2022
Supervised By :mohammad
ahmed

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

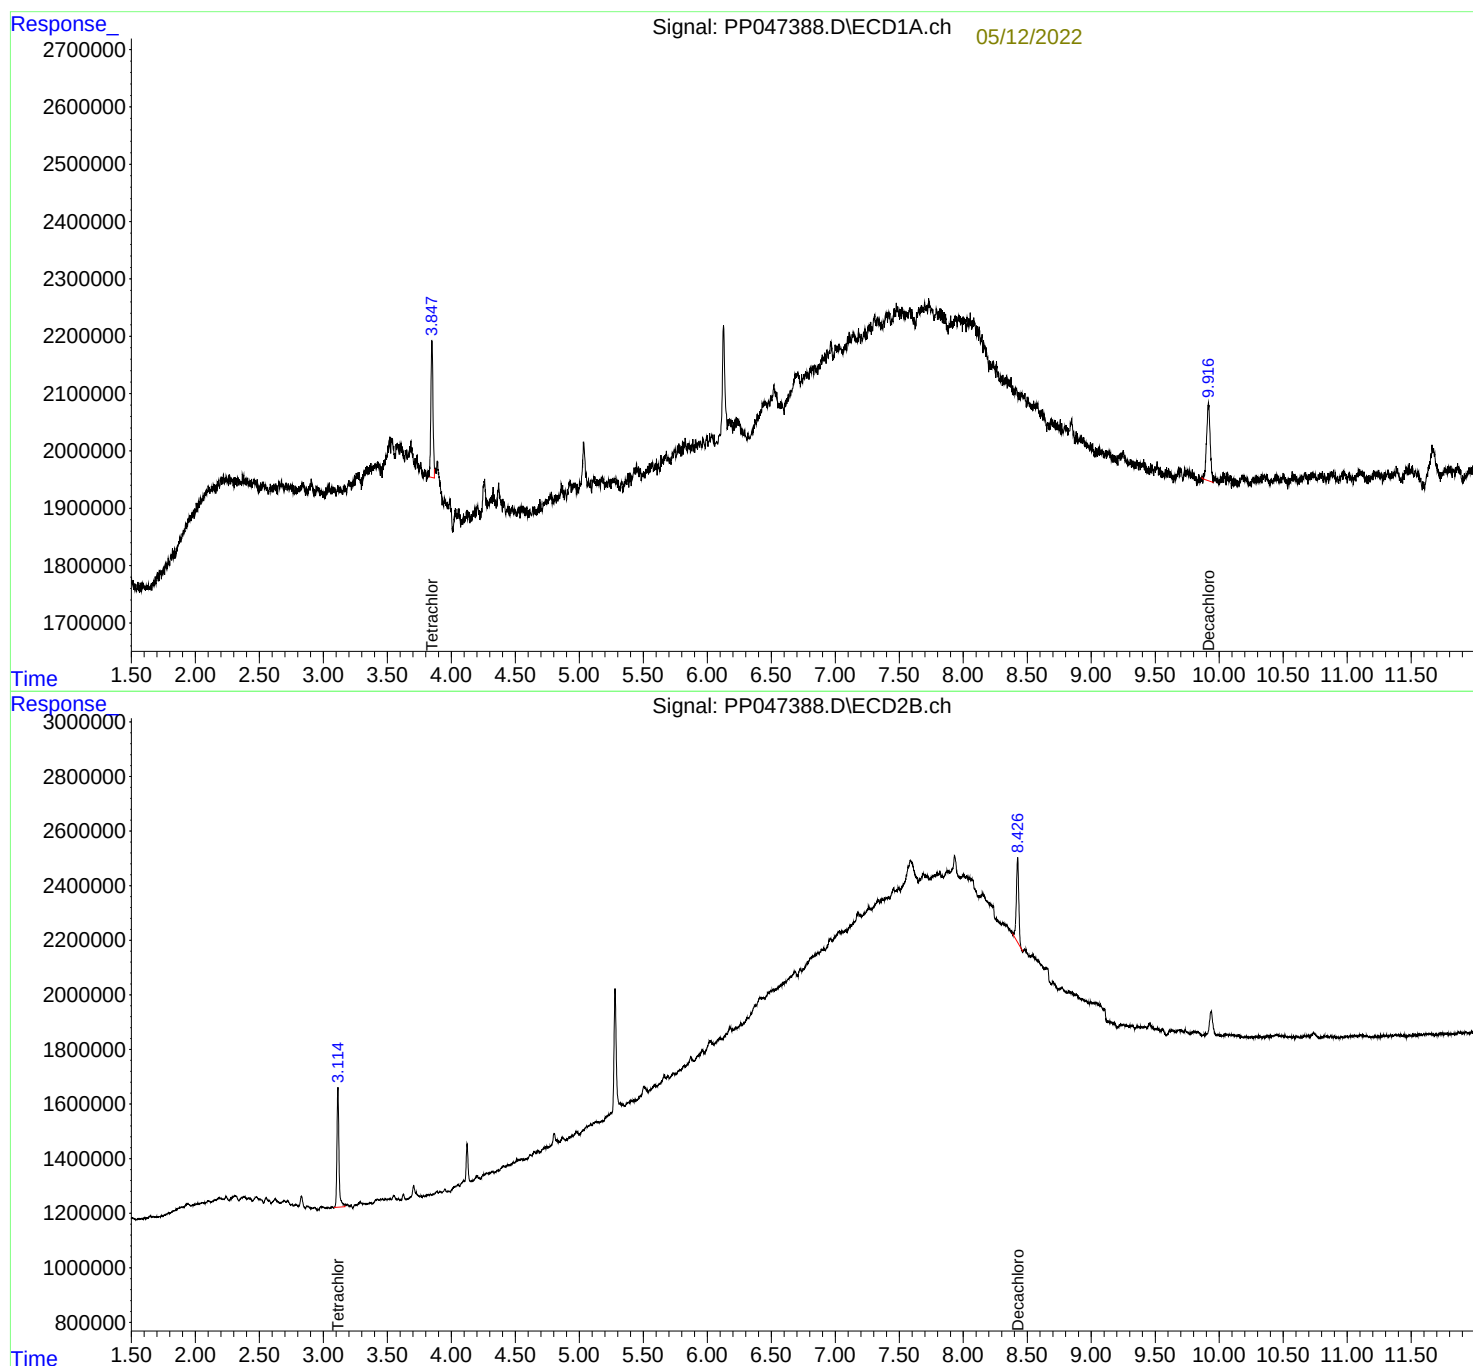

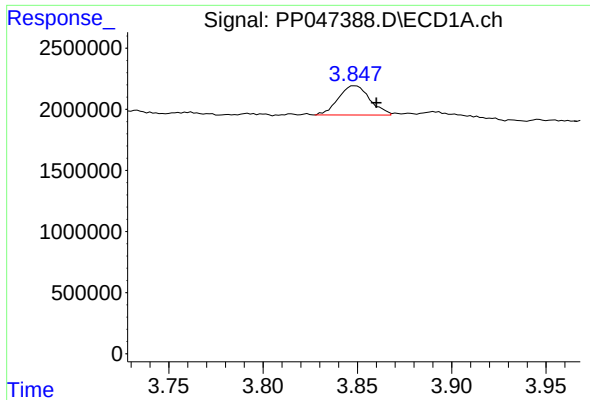


#1 Tetrachloro-m-xylene

R.T.: 3.847 min
Delta R.T.: -0.013 min
Response: 2780444
Conc: 1.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
SOM-2022-32B

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

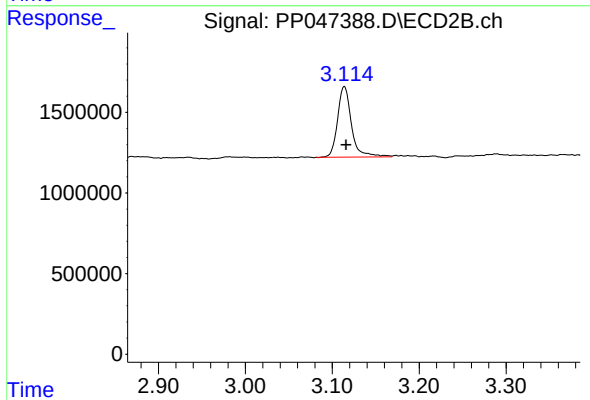


#1 Tetrachloro-m-xylene

R.T.: 3.114 min
Delta R.T.: -0.002 min
Response: 4877594
Conc: 1.48 ng/ml


05/12/2022
Supervised By :mohammad
ahmed

05/12/2022

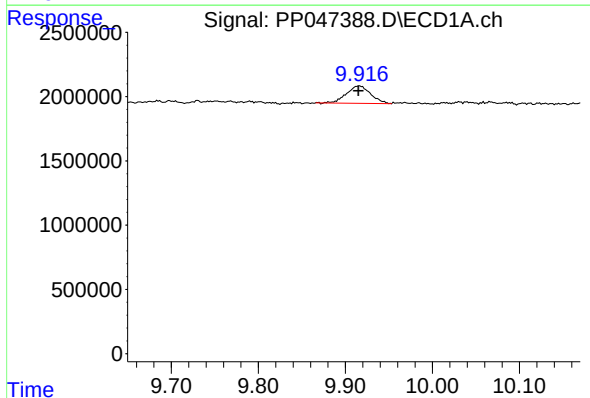

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: 0.001 min
Response: 2601340
Conc: 1.82 ng/ml

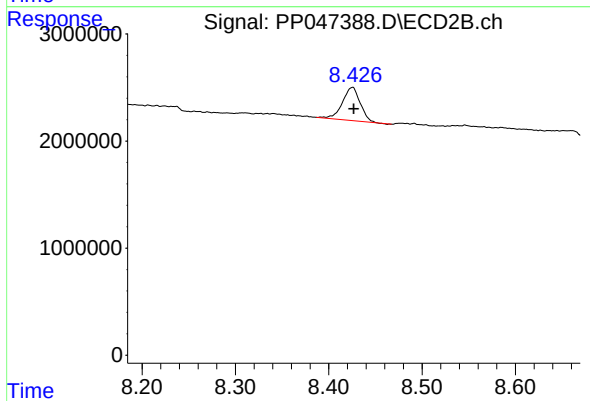

#2 Decachlorobiphenyl

R.T.: 8.425 min
Delta R.T.: -0.002 min
Response: 4081133
Conc: 1.50 ng/ml