

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
 Data File : PP035794.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2021 16:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 17:49:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.777	4.198	499459	731040	21.316	21.506
2)	SA Decachlor...	10.620	9.438	278947	433390	24.782	20.494
Target Compounds							
3)	L1 AR-1016-1	6.066f	0.000	1041	0	1.622	N.D. #
9)	L2 AR-1221-2	5.125	0.000	7225	0	32.193	N.D. #
16)	L4 AR-1242-1	6.066f	0.000	1041	0	2.116	N.D. #
21)	L5 AR-1248-1	6.066f	0.000	1041	0	2.773	N.D. #
29)	L6 AR-1254-4	7.874	0.000	18804	0	23.585	N.D. #
32)	L7 AR-1260-2	0.000	7.197	0	718	N.D.	0.416 #
33)	L7 AR-1260-3	8.372	0.000	2813	0	4.204	N.D. #
36)	L8 AR-1262-1	8.372	0.000	2813	0	2.529	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
Data File : PP035794.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2021 16:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 17:49:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

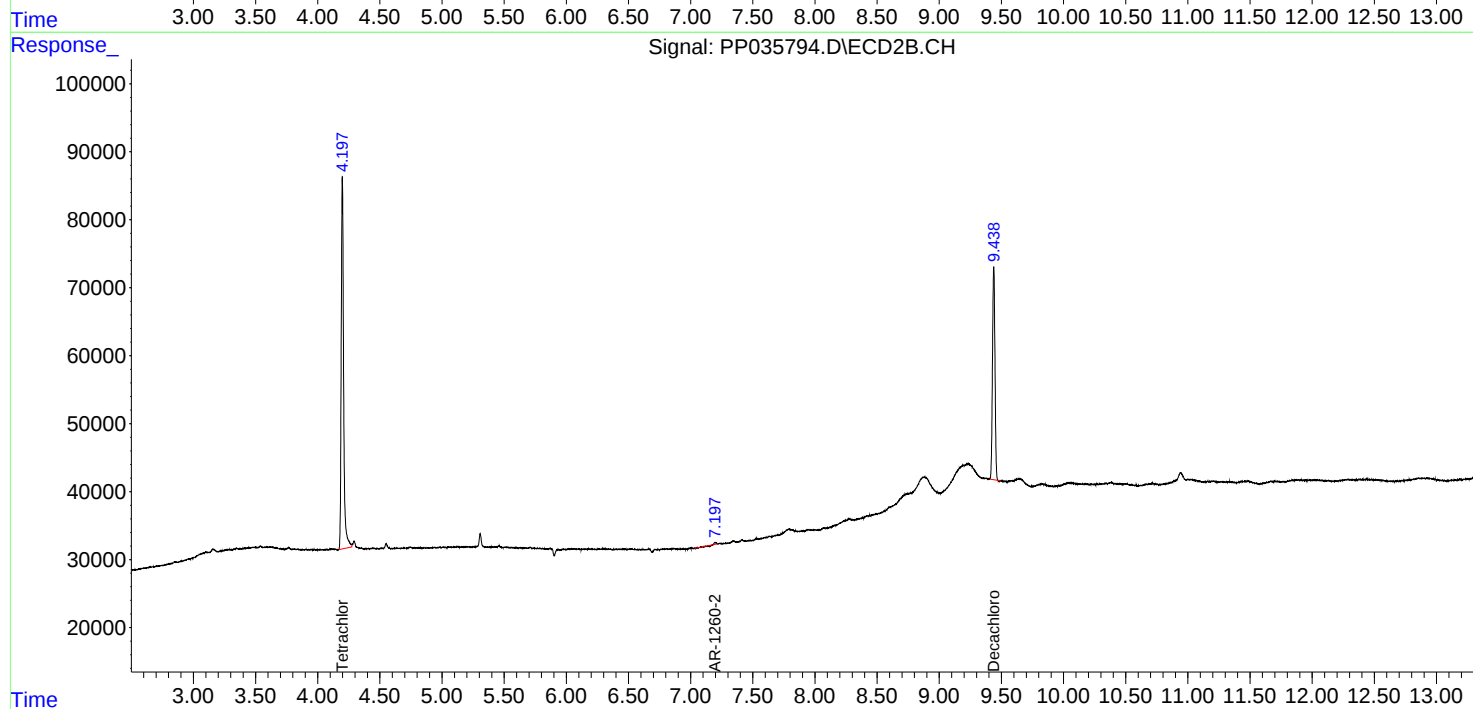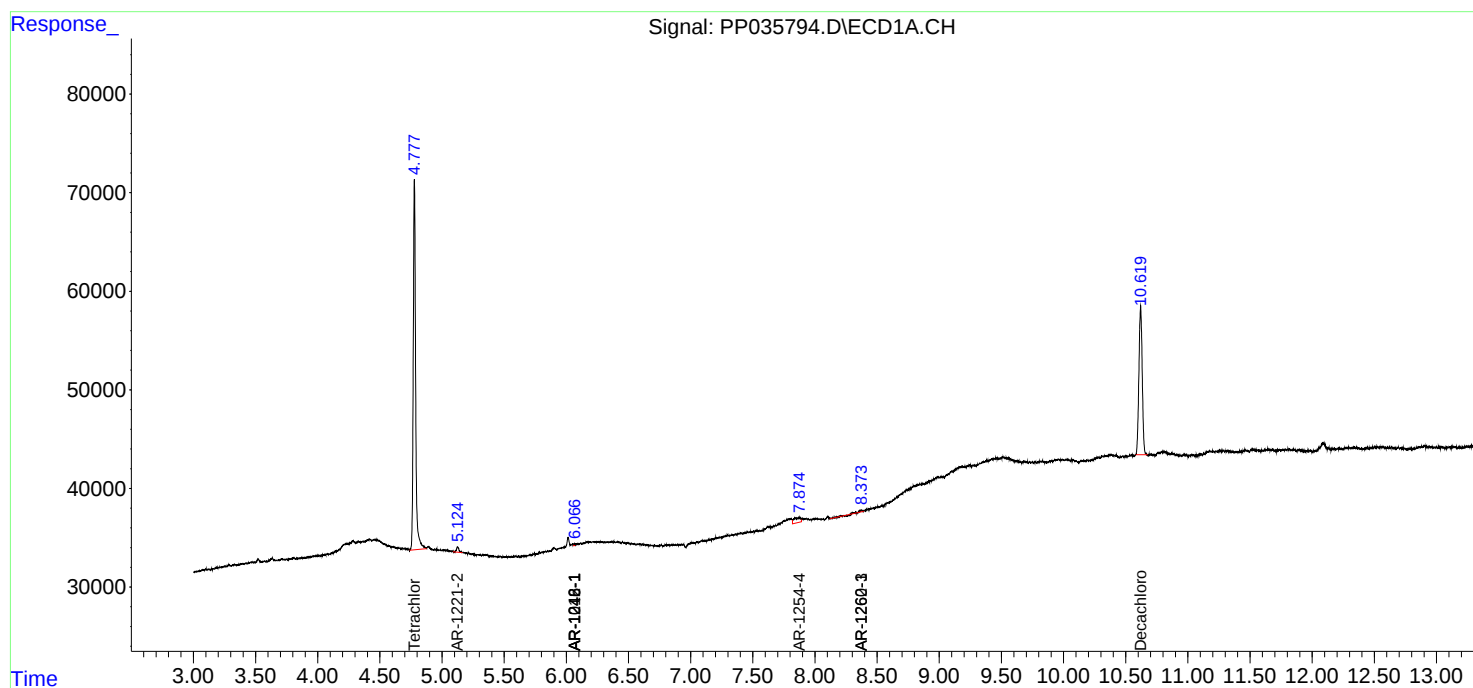


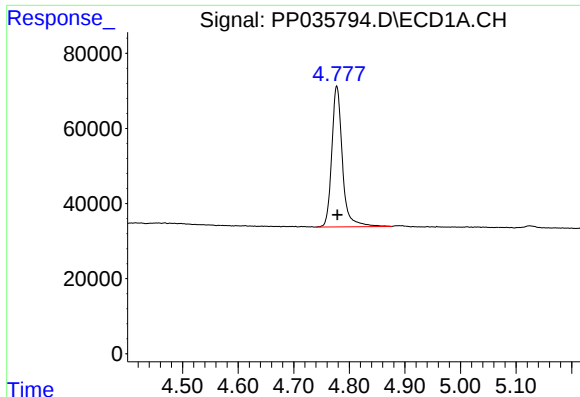

#1 Tetrachloro-m-xylene


R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 499459
Conc: 21.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

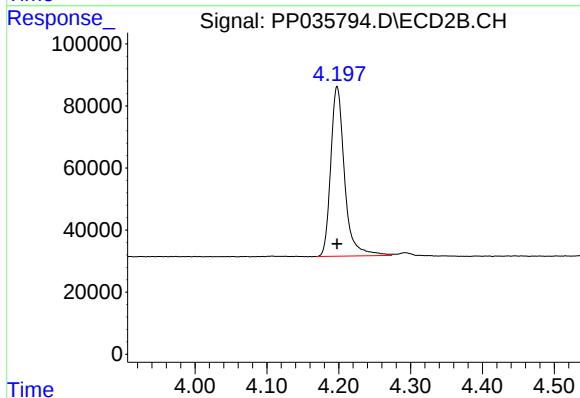


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: 0.000 min
Response: 731040
Conc: 21.51 ng/ml

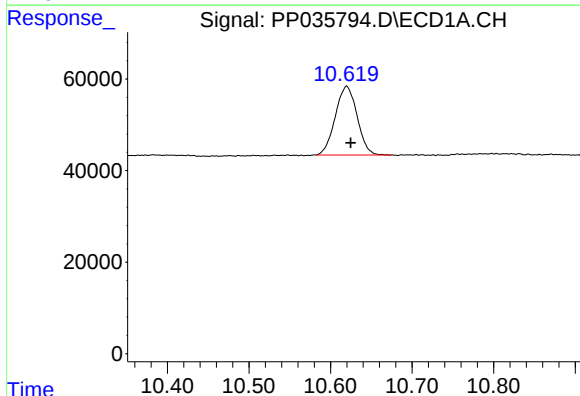


#2 Decachlorobiphenyl

R.T.: 10.620 min
Delta R.T.: -0.005 min
Response: 278947
Conc: 24.78 ng/ml

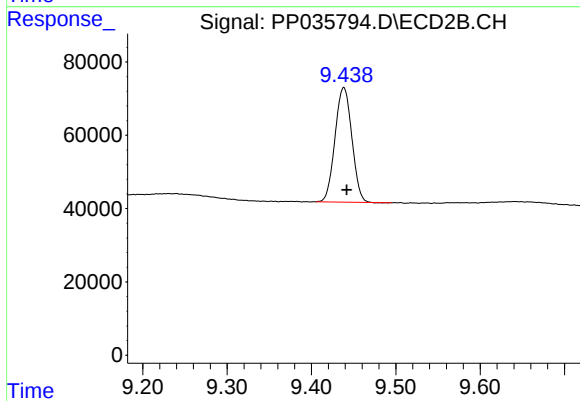

#2 Decachlorobiphenyl


R.T.: 9.438 min
Delta R.T.: -0.003 min
Response: 433390
Conc: 20.49 ng/ml

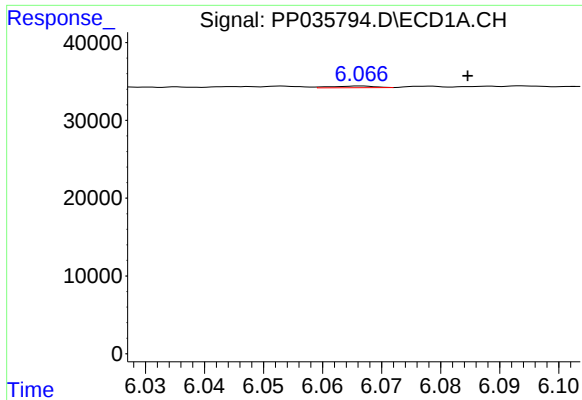

#3 AR-1016-1


R.T.: 6.066 min
Delta R.T.: -0.018 min
Response: 1041
Conc: 1.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

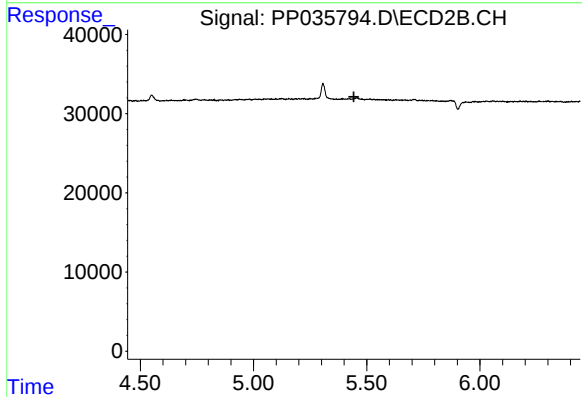


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

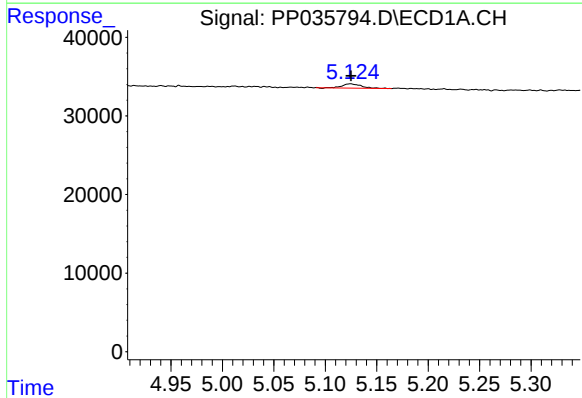


#9 AR-1221-2

R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 7225
Conc: 32.19 ng/ml

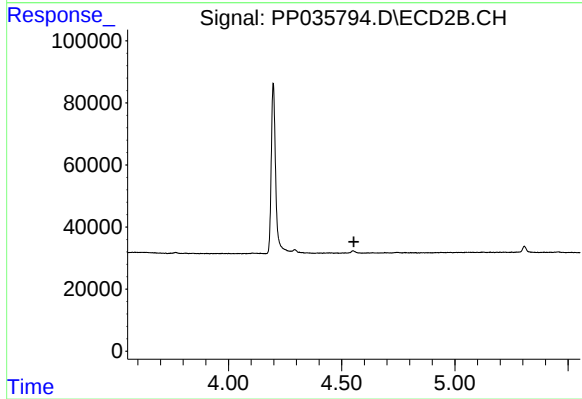

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

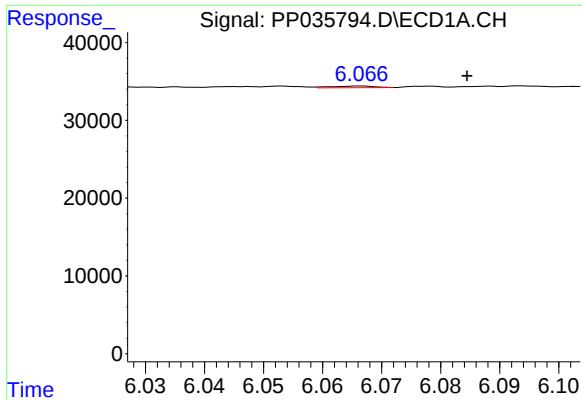

#16 AR-1242-1


R.T.: 6.066 min
Delta R.T.: -0.018 min
Response: 1041
Conc: 2.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

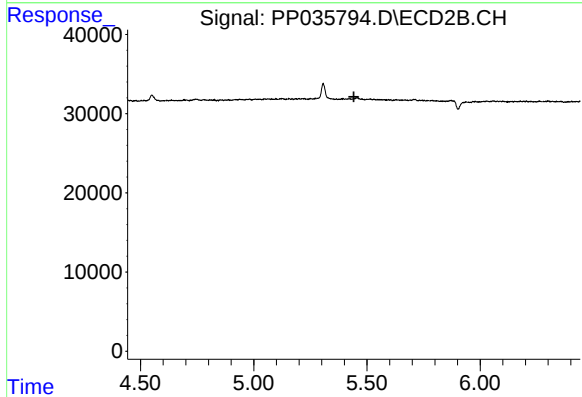


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.442 min
Response: 0
Conc: N.D.

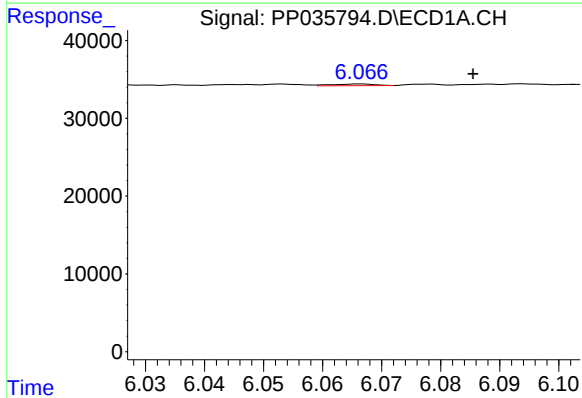


#21 AR-1248-1

R.T.: 6.066 min
Delta R.T.: -0.019 min
Response: 1041
Conc: 2.77 ng/ml

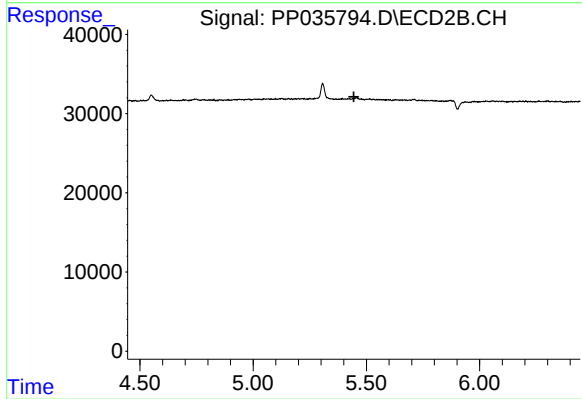

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 5.445 min
Response: 0
Conc: N.D.

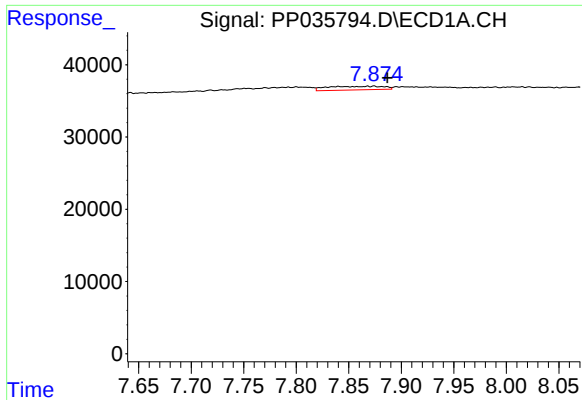

#29 AR-1254-4


R.T.: 7.874 min
Delta R.T.: -0.013 min
Response: 18804
Conc: 23.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

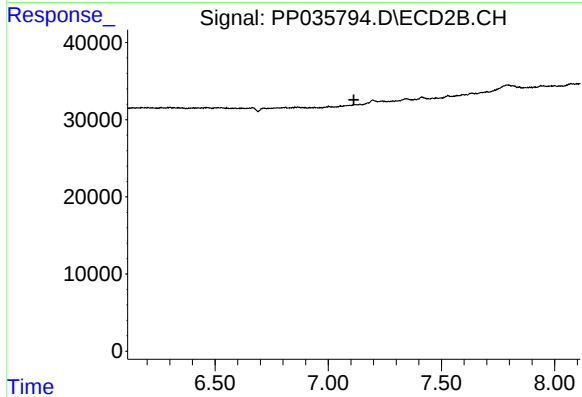


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

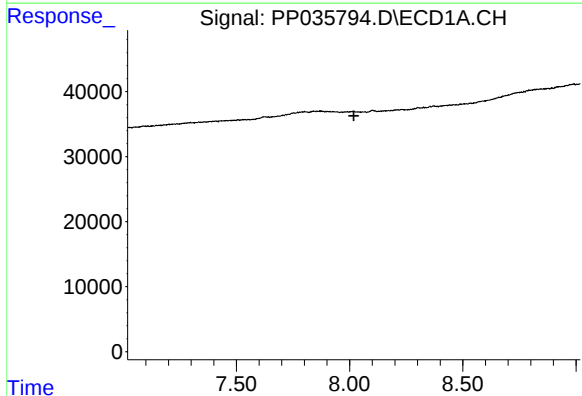


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.019 min
Response: 0
Conc: N.D.

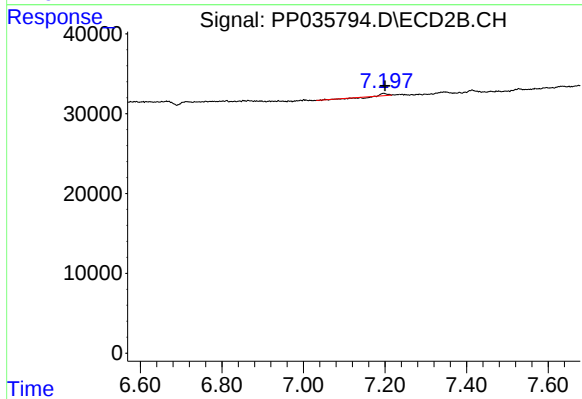

#32 AR-1260-2


R.T.: 7.197 min
Delta R.T.: -0.004 min
Response: 718
Conc: 0.42 ng/ml

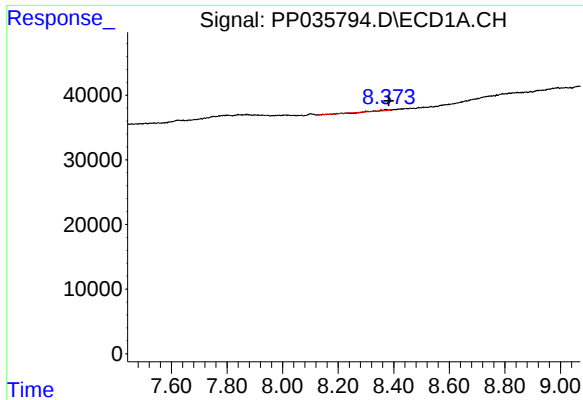

#33 AR-1260-3


R.T.: 8.372 min
Delta R.T.: -0.010 min
Response: 2813
Conc: 4.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

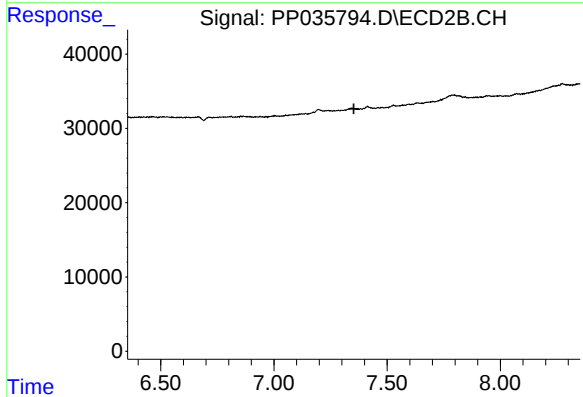


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.354 min
Response: 0
Conc: N.D.

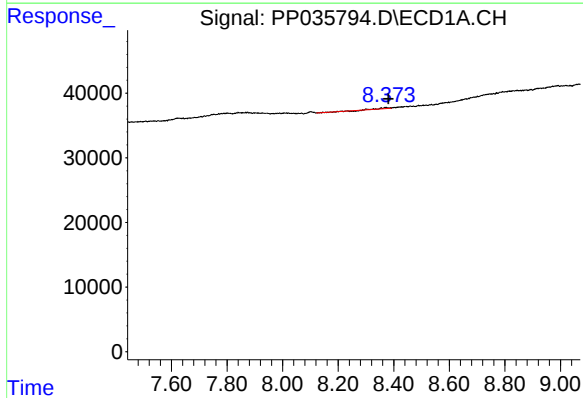

#36 AR-1262-1

R.T.: 8.372 min
Delta R.T.: -0.010 min
Response: 2813
Conc: 2.53 ng/ml

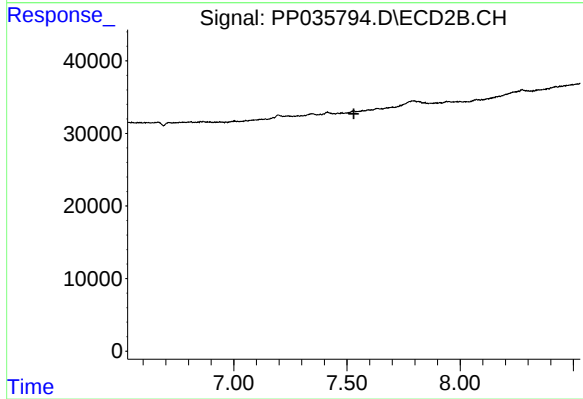

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.531 min
Response: 0
Conc: N.D.