

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
 Data File : PP035800.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2021 17:41
 Operator : DD\AJ
 Sample : M2348-04 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEH669L-2-2

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:48:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 17:55:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.777	4.197	39545	53795	1.688	1.583m
2) SA Decachlor...	10.620	9.439	21510	31105	1.911	1.471

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
Data File : PP035800.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2021 17:41
Operator : DD\AJ
Sample : M2348-04 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEH669L-2-2


Manual Integrations
APPROVED

Ankita
5/13/2021 10:48:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 17:55:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

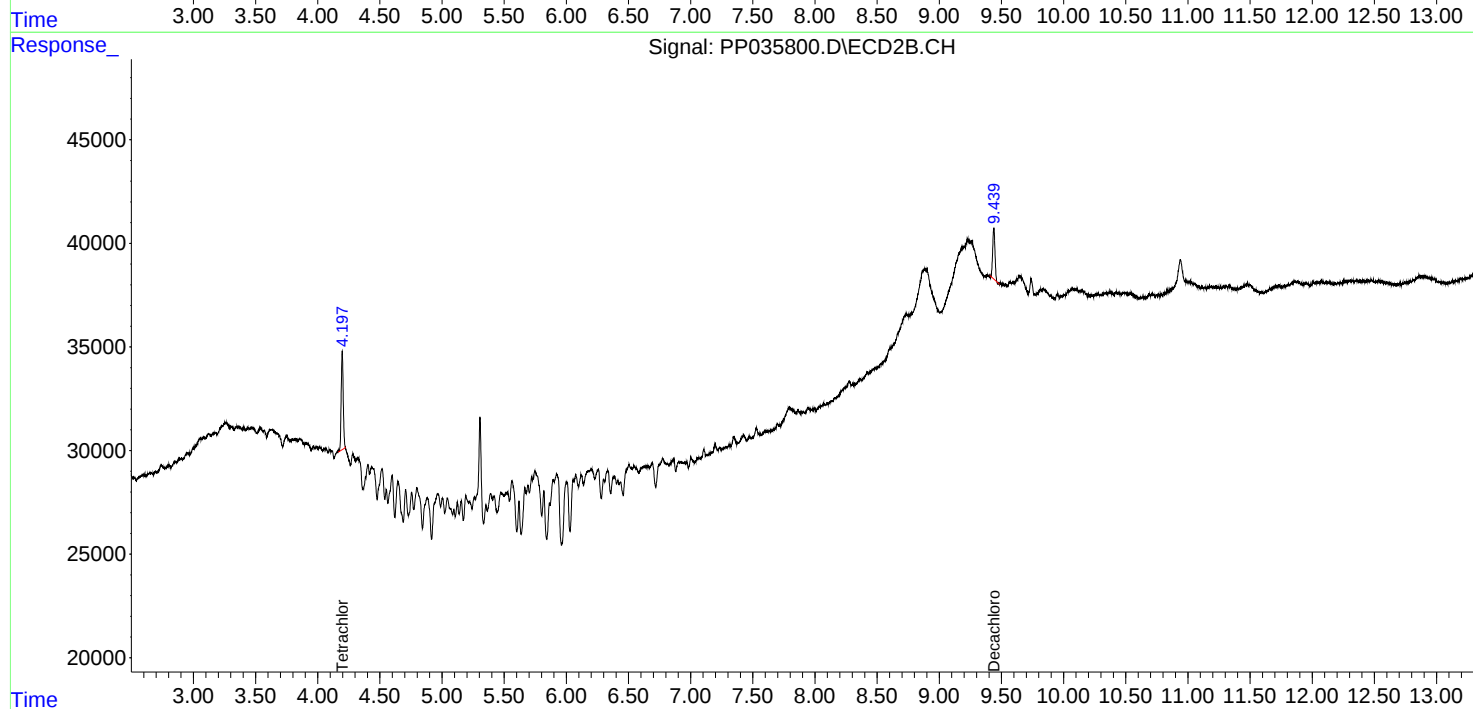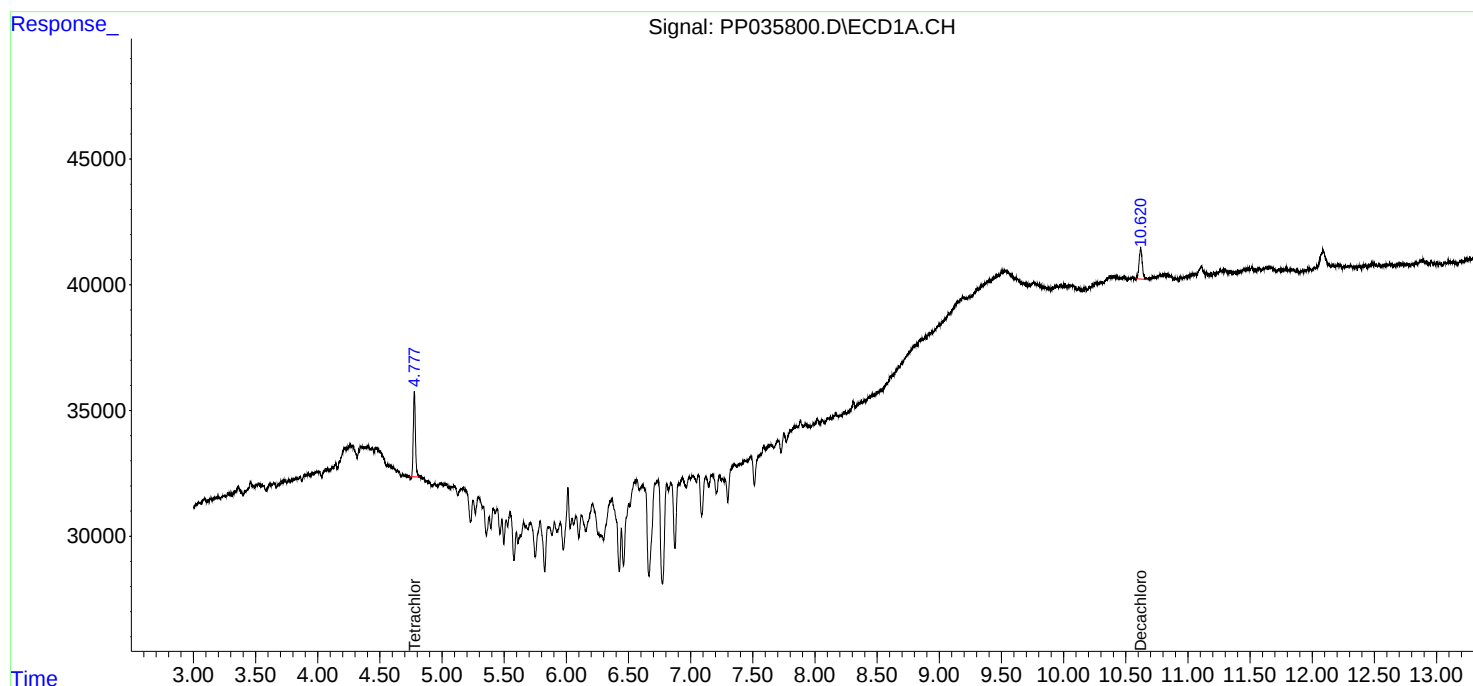

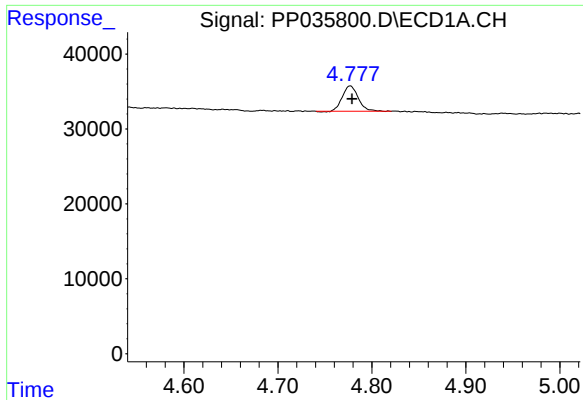


#1 Tetrachloro-m-xylene

R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 39545
Conc: 1.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEH669L-2-2


Manual Integrations
APPROVED

Ankita
5/13/2021 10:48:26 AM

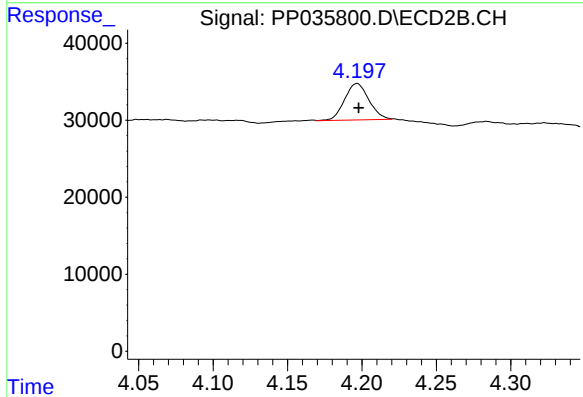


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.001 min
Response: 53795
Conc: 1.58 ng/ml m

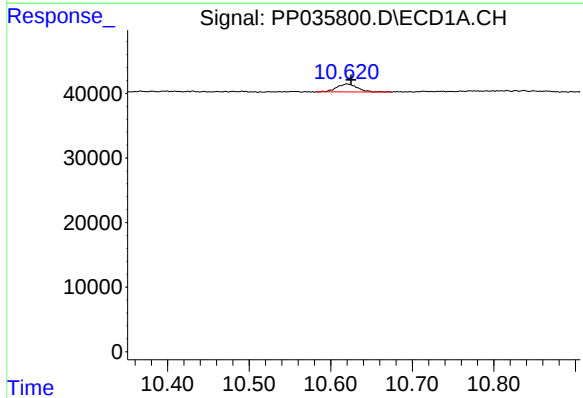

#2 Decachlorobiphenyl

R.T.: 10.620 min
Delta R.T.: -0.005 min
Response: 21510
Conc: 1.91 ng/ml

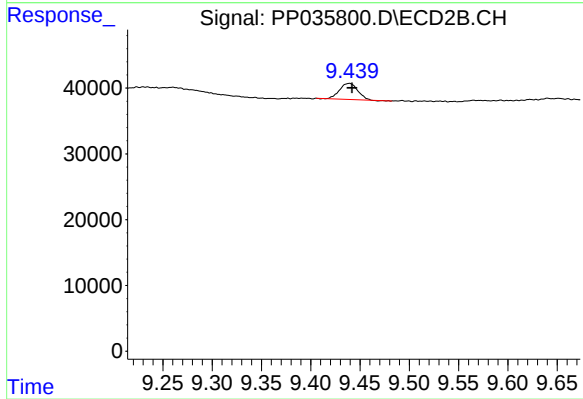

#2 Decachlorobiphenyl

R.T.: 9.439 min
Delta R.T.: -0.003 min
Response: 31105
Conc: 1.47 ng/ml