

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
 Data File : PP035804.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 May 2021 18:48
 Operator : DD\AJ
 Sample : M2351-03 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC260909-1-3

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:48:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 02:41:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.776	4.197	39063	60119	1.667	1.769
2) SA Decachlor...	10.617	9.438	25851	38374	2.297	1.815m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051121\
Data File : PP035804.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 May 2021 18:48
Operator : DD\AJ
Sample : M2351-03 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC260909-1-3


Manual Integrations
APPROVED

Ankita
5/13/2021 10:48:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 02:41:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

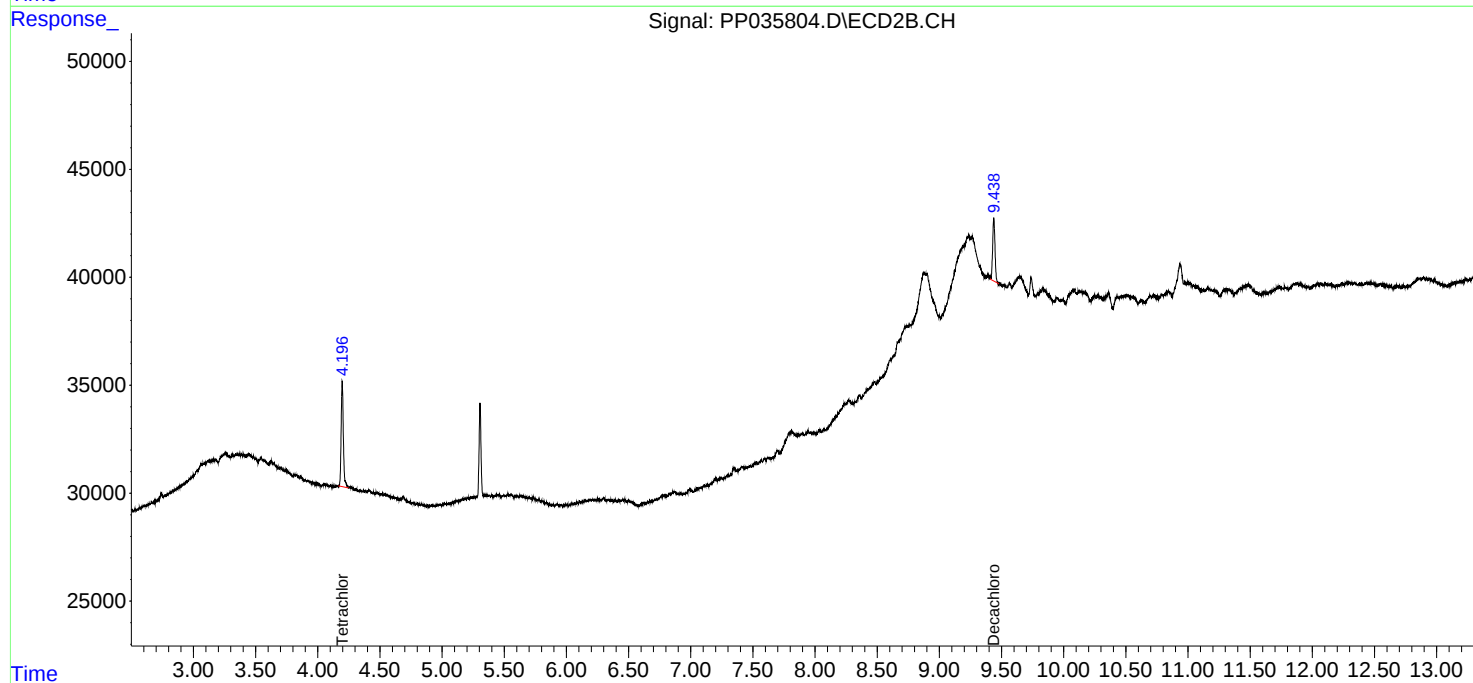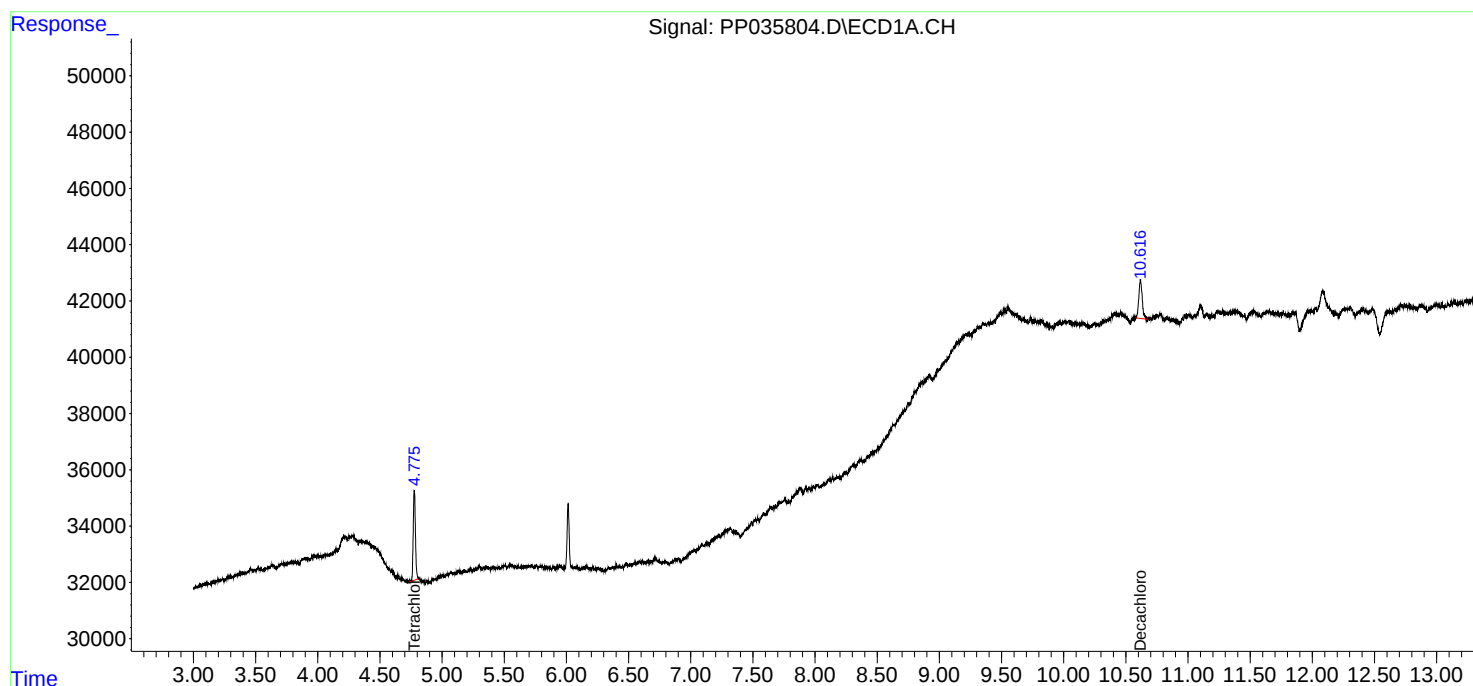

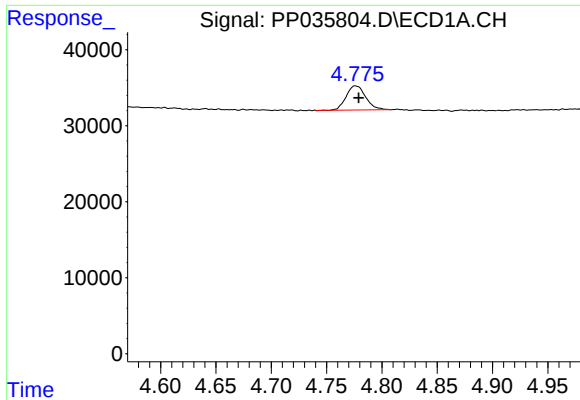


#1 Tetrachloro-m-xylene

R.T.: 4.776 min
Delta R.T.: -0.003 min
Response: 39063
Conc: 1.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC260909-1-3


Manual Integrations
APPROVED

Ankita
5/13/2021 10:48:30 AM

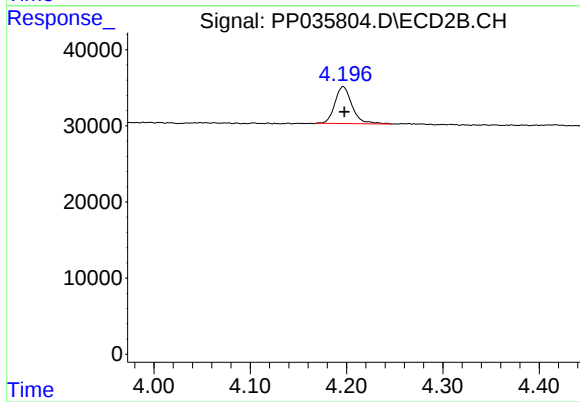


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.001 min
Response: 60119
Conc: 1.77 ng/ml

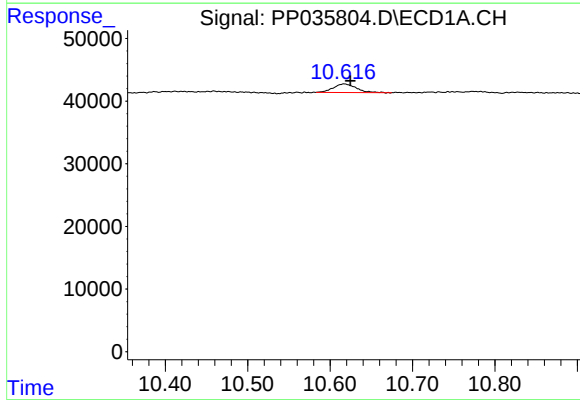

#2 Decachlorobiphenyl

R.T.: 10.617 min
Delta R.T.: -0.008 min
Response: 25851
Conc: 2.30 ng/ml

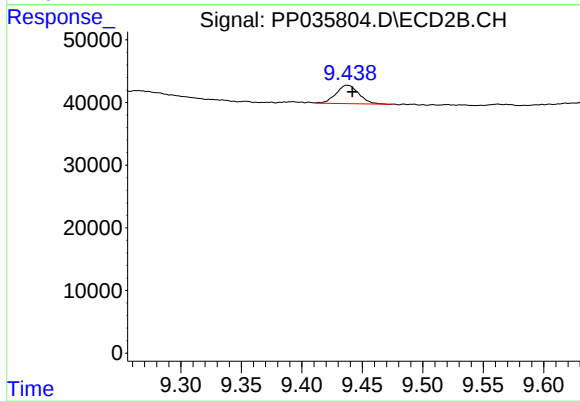

#2 Decachlorobiphenyl

R.T.: 9.438 min
Delta R.T.: -0.004 min
Response: 38374
Conc: 1.81 ng/ml m