

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051122\
 Data File : PP047429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 19:38
 Operator : YP\AJ
 Sample : N2755-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-221

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/12/2022
 Supervised By :mohammad ahmed 05/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 06:39:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 11 13:10:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.849	3.115	51642010	78836220	20.313	23.944
2) SA Decachlor...	9.910	8.419	35419593	64327657	24.759	23.633m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051122\
Data File : PP047429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 19:38
Operator : YP\AJ
Sample : N2755-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-221


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/12/2022
Supervised By :mohammad ahmed 05/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 06:39:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

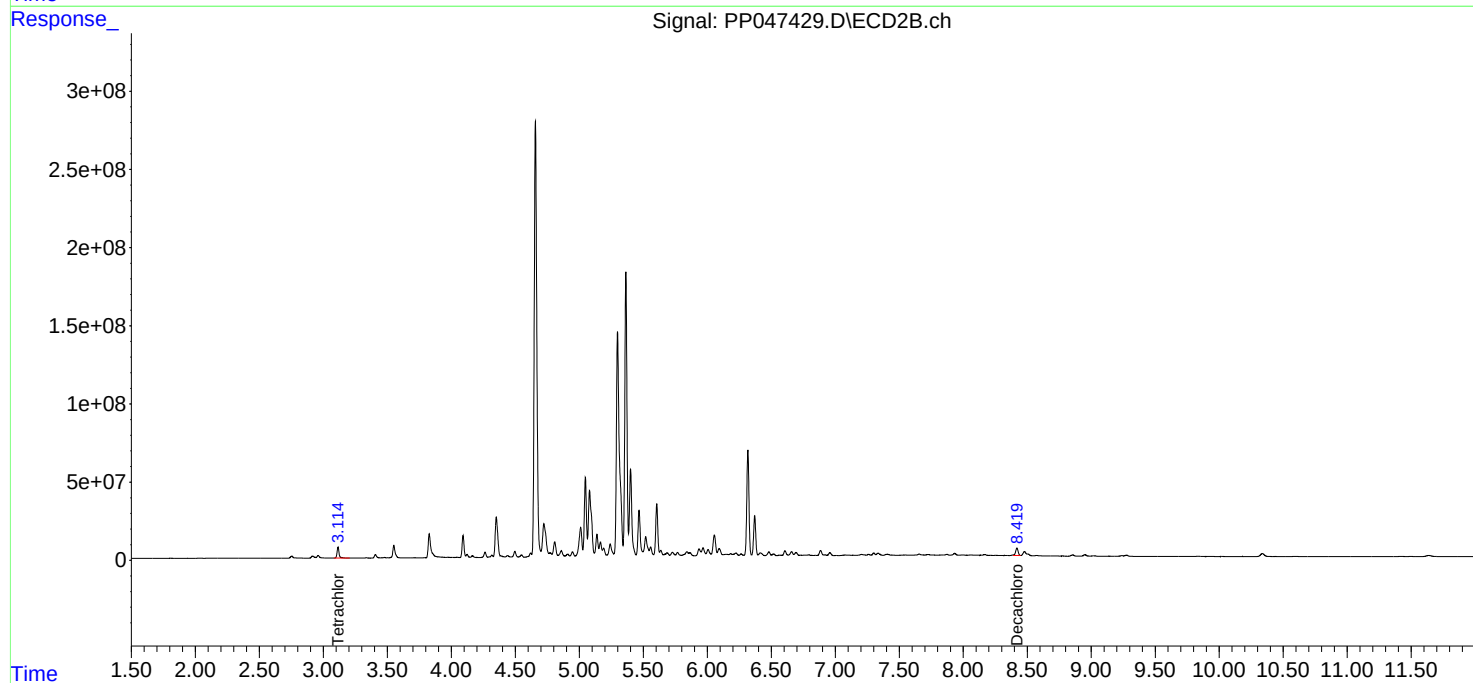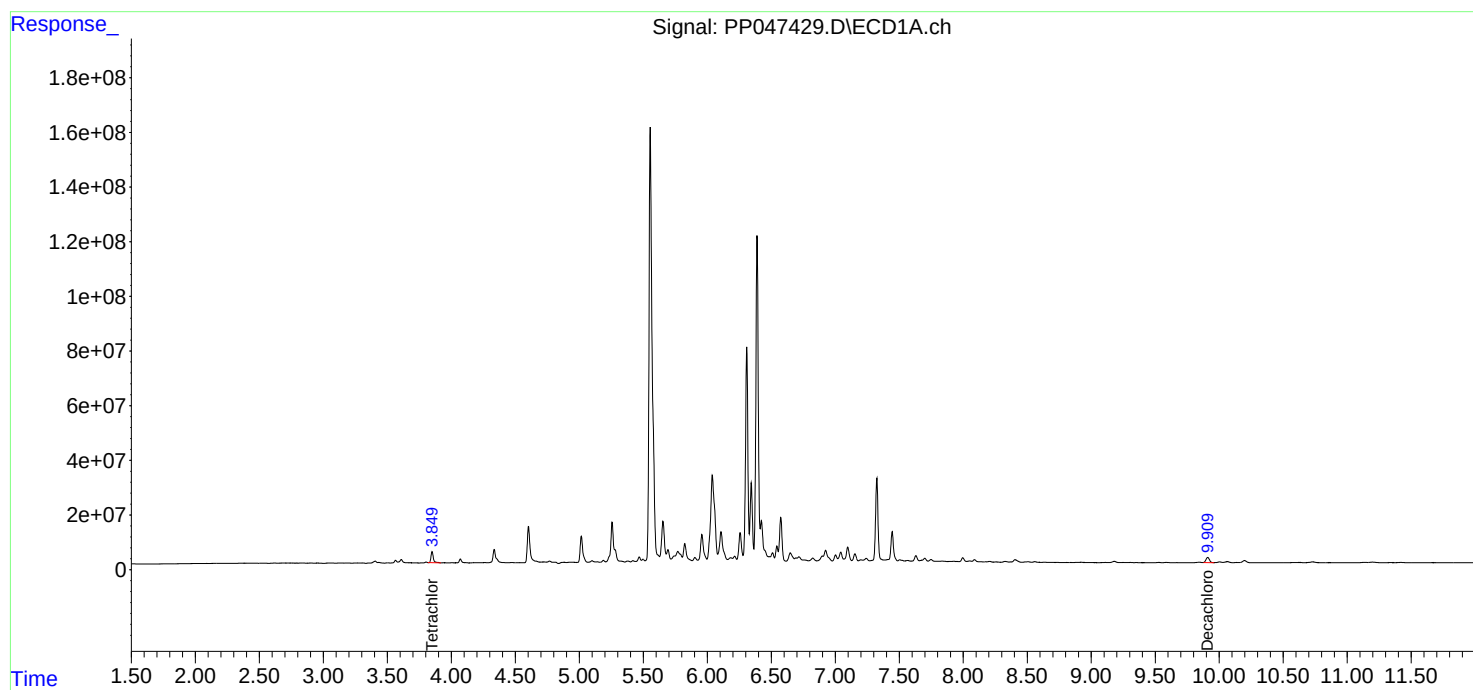

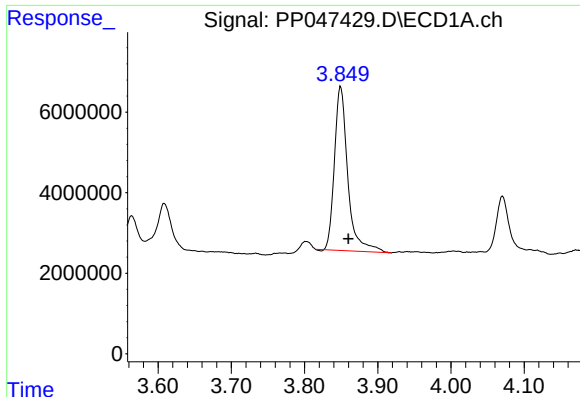


#1 Tetrachloro-m-xylene

R.T.: 3.849 min
Delta R.T.: -0.010 min
Response: 51642010
Conc: 20.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-221


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/12/2022
Supervised By :mohammad ahmed 05/12/2022

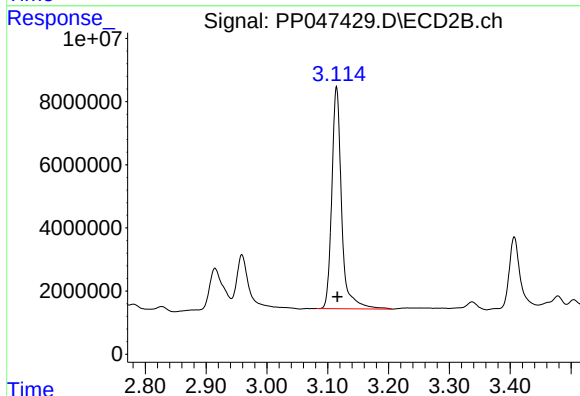


#1 Tetrachloro-m-xylene

R.T.: 3.115 min
Delta R.T.: -0.001 min
Response: 78836220
Conc: 23.94 ng/ml

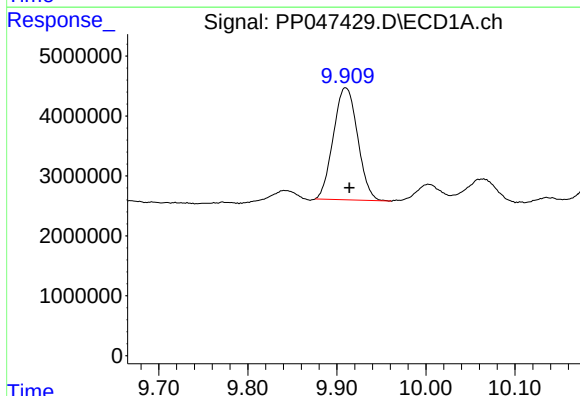

#2 Decachlorobiphenyl

R.T.: 9.910 min
Delta R.T.: -0.004 min
Response: 35419593
Conc: 24.76 ng/ml

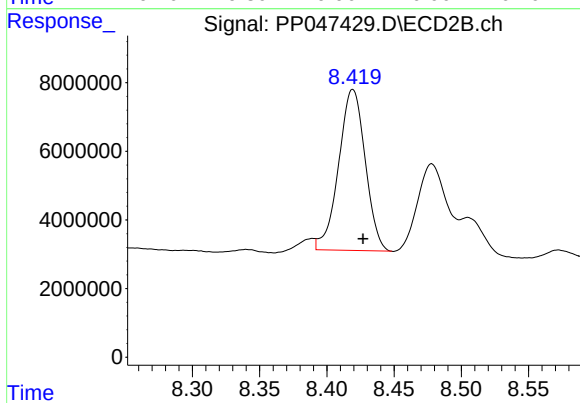

#2 Decachlorobiphenyl

R.T.: 8.419 min
Delta R.T.: -0.008 min
Response: 64327657
Conc: 23.63 ng/ml m