

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051222\
Data File : PP047519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 00:29
Operator : YP\AJ
Sample : N2780-16 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KMA964P-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2022
Supervised By :mohammad ahmed 05/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:38:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.850	3.114	2488960	2958831	0.979	0.899
2) SA Decachlor...	9.907	8.416	2727858	4189707	1.907m	1.539

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051222\
Data File : PP047519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 00:29
Operator : YP\AJ
Sample : N2780-16 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMA964P-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2022
Supervised By :mohammad ahmed 05/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 03:38:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

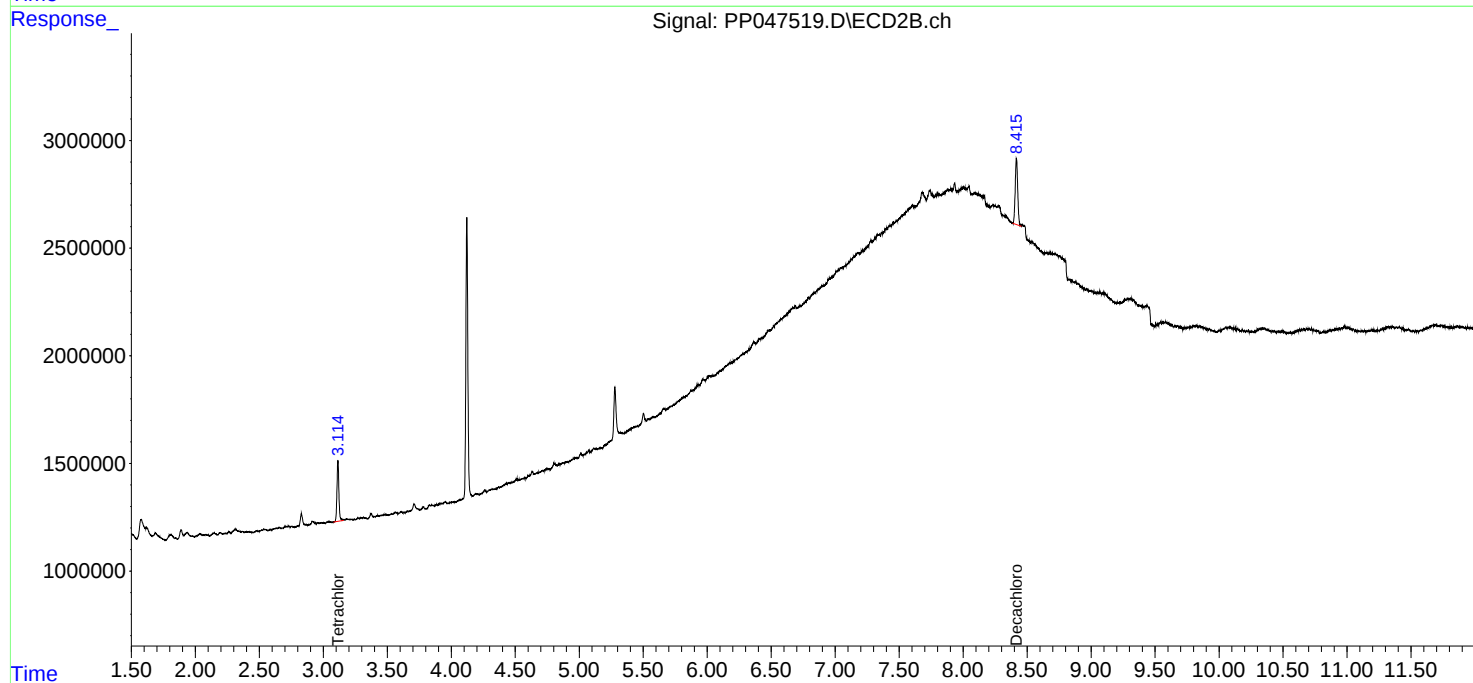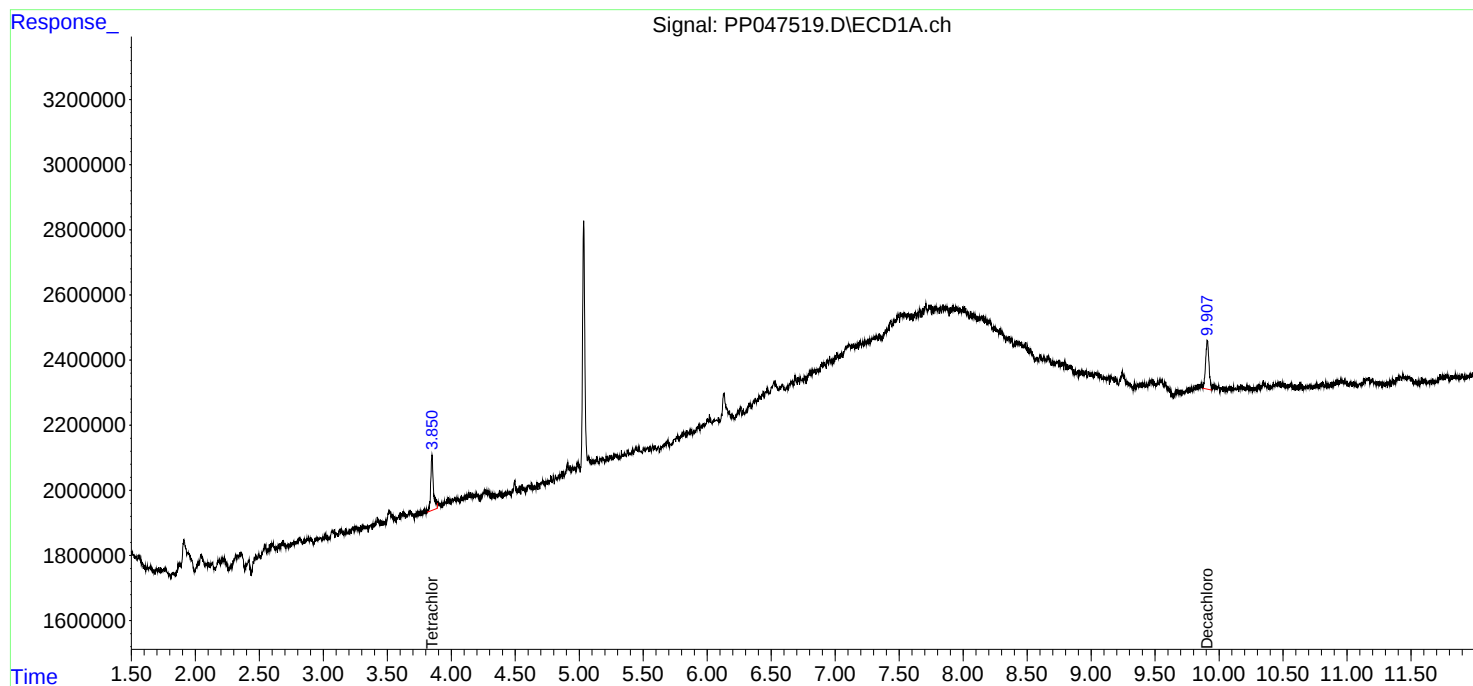

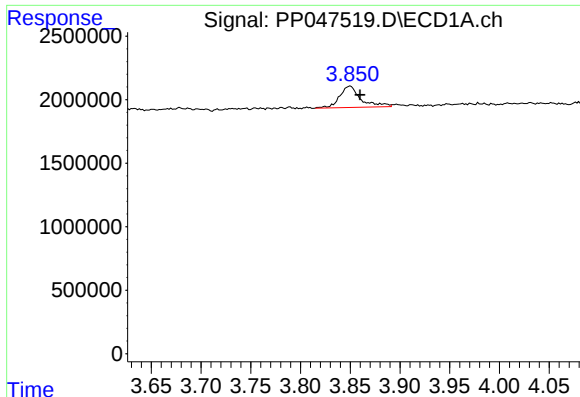


#1 Tetrachloro-m-xylene

R.T.: 3.850 min
Delta R.T.: -0.010 min
Response: 2488960
Conc: 0.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMA964P-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2022
Supervised By :mohammad ahmed 05/13/2022

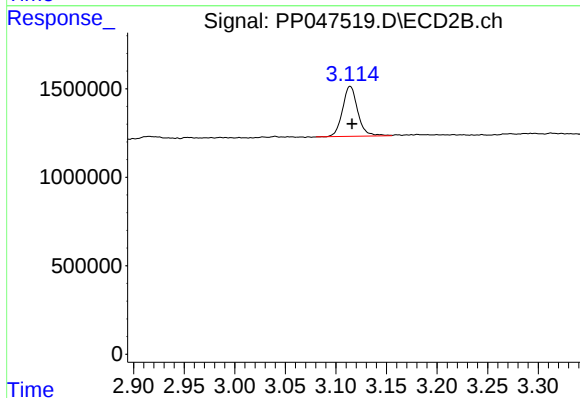


#1 Tetrachloro-m-xylene

R.T.: 3.114 min
Delta R.T.: -0.002 min
Response: 2958831
Conc: 0.90 ng/ml

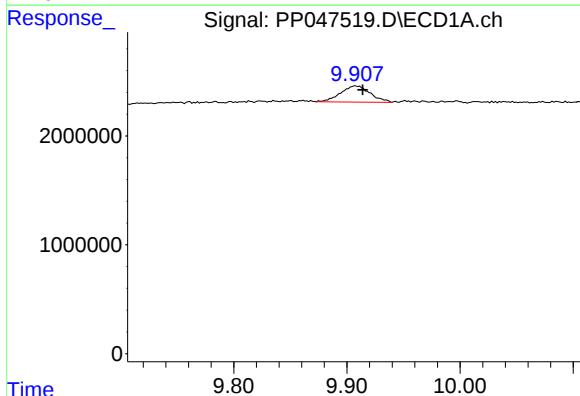

#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.007 min
Response: 2727858
Conc: 1.91 ng/ml m

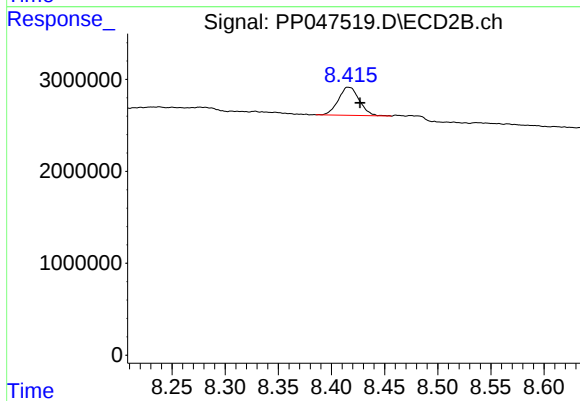

#2 Decachlorobiphenyl

R.T.: 8.416 min
Delta R.T.: -0.011 min
Response: 4189707
Conc: 1.54 ng/ml