

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035819.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 10:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 11:29:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.776	4.197	458165	674124	19.554	19.831
2)	SA Decachlor...	10.614	9.435	261526	431165	23.235	20.388
Target Compounds							
9)	L2 AR-1221-2	5.125	0.000	5046	0	22.484	N.D. #
27)	L6 AR-1254-2	7.195f	0.000	3471	0	3.154	N.D. #
28)	L6 AR-1254-3	7.598	0.000	2021	0	1.708	N.D. #
31)	L7 AR-1260-1	7.753	0.000	11335	0	12.573	N.D. #
32)	L7 AR-1260-2	8.018	0.000	3497	0	3.590	N.D. #
33)	L7 AR-1260-3	8.362f	0.000	8947	0	13.370	N.D. #
36)	L8 AR-1262-1	8.362f	0.000	8947	0	8.042	N.D. #
45)	L9 AR-1268-5	0.000	9.224f	0	18741	N.D.	2.374 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035819.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 10:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 11:29:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

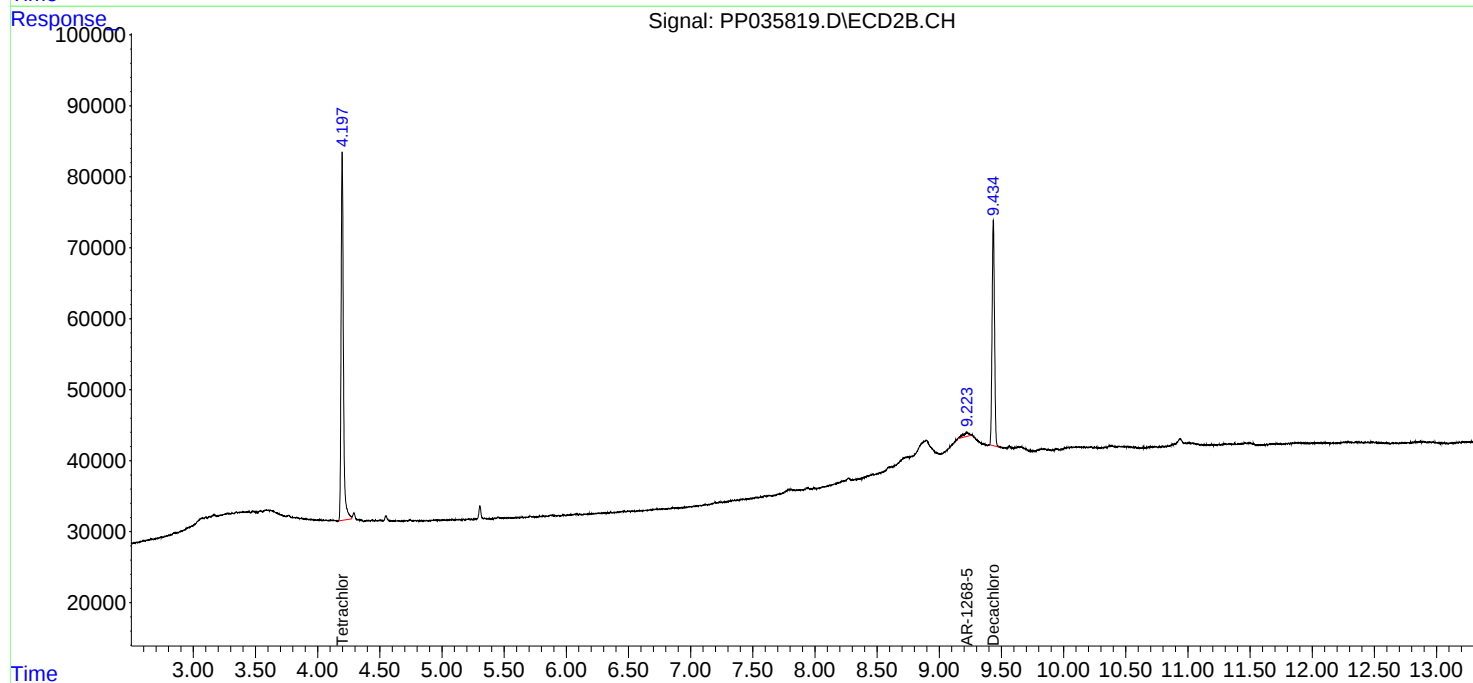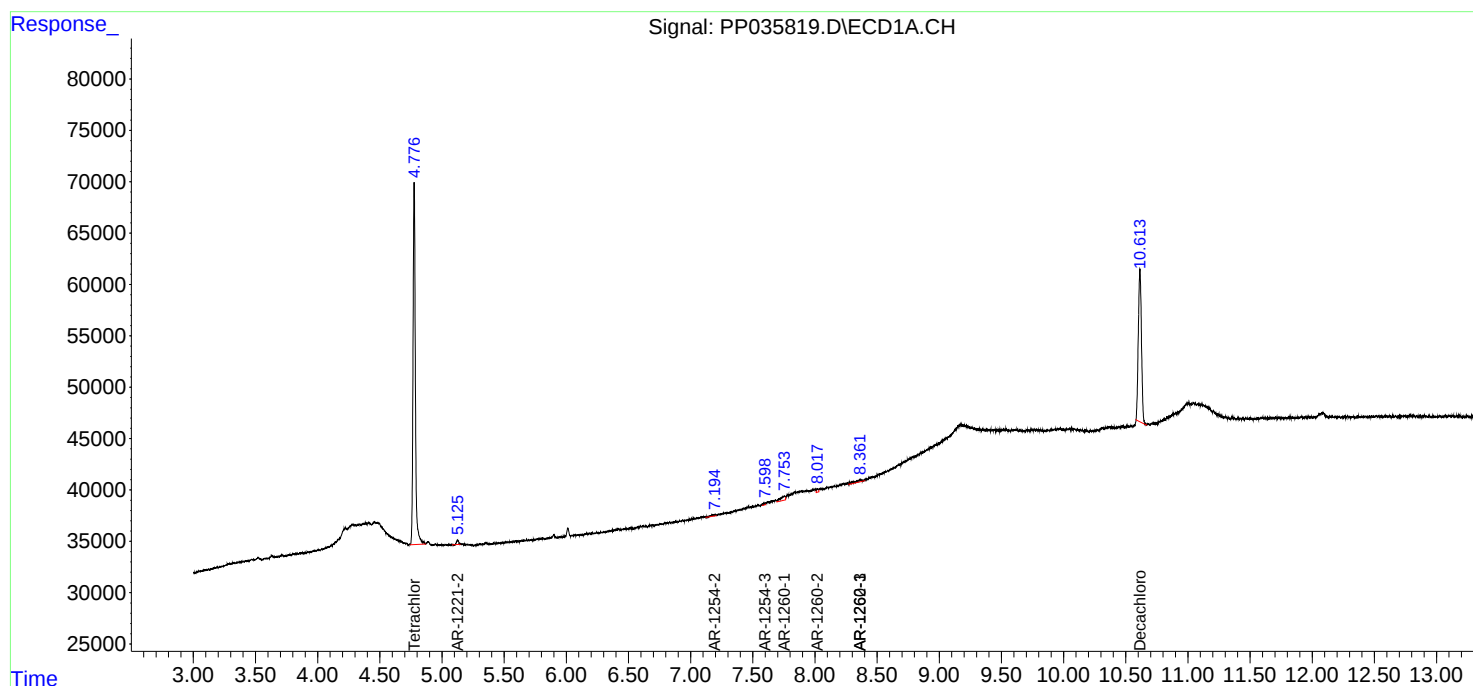


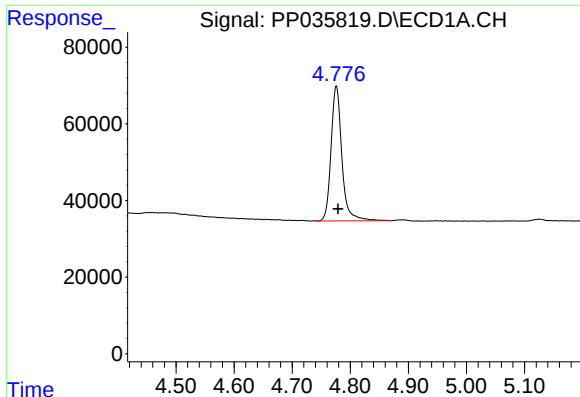

#1 Tetrachloro-m-xylene


R.T.: 4.776 min
Delta R.T.: -0.003 min
Response: 458165
Conc: 19.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

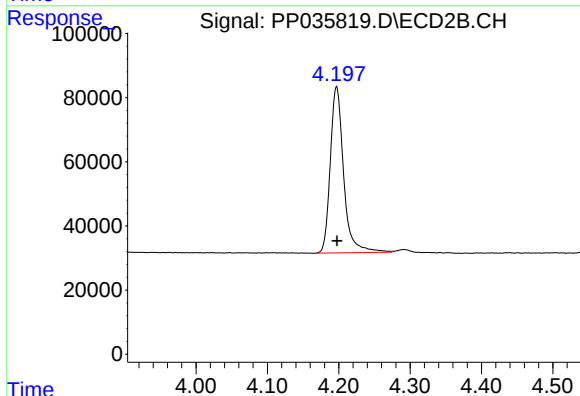


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: 0.000 min
Response: 674124
Conc: 19.83 ng/ml

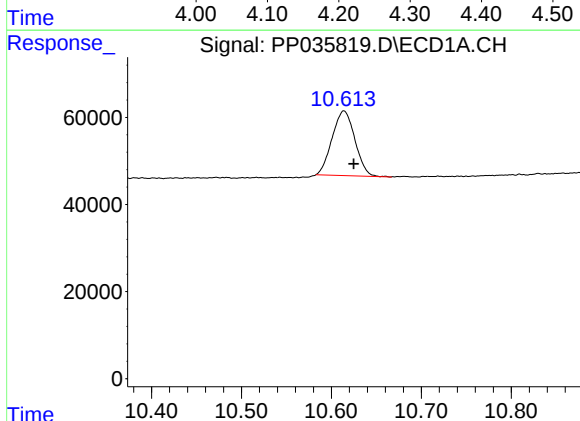


#2 Decachlorobiphenyl

R.T.: 10.614 min
Delta R.T.: -0.011 min
Response: 261526
Conc: 23.23 ng/ml

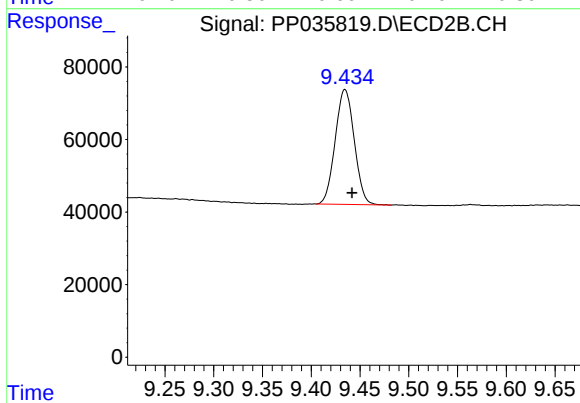

#2 Decachlorobiphenyl


R.T.: 9.435 min
Delta R.T.: -0.007 min
Response: 431165
Conc: 20.39 ng/ml

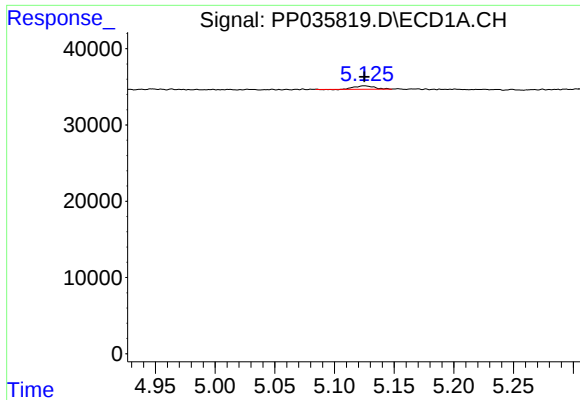

#9 AR-1221-2


R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 5046
Conc: 22.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

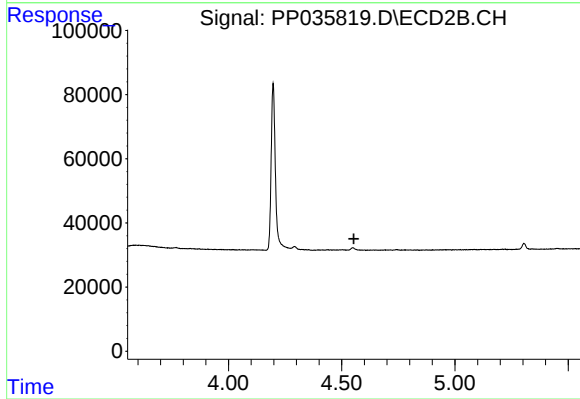


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

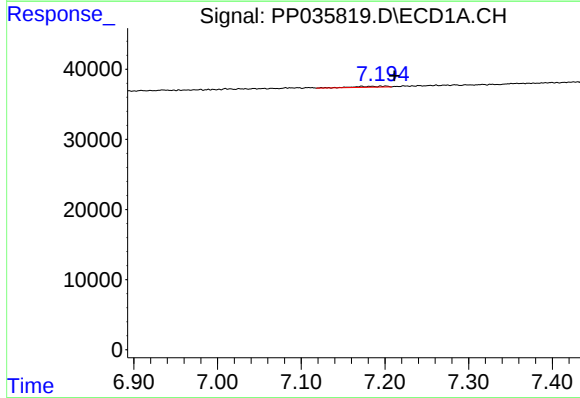


#27 AR-1254-2

R.T.: 7.195 min
Delta R.T.: -0.017 min
Response: 3471
Conc: 3.15 ng/ml

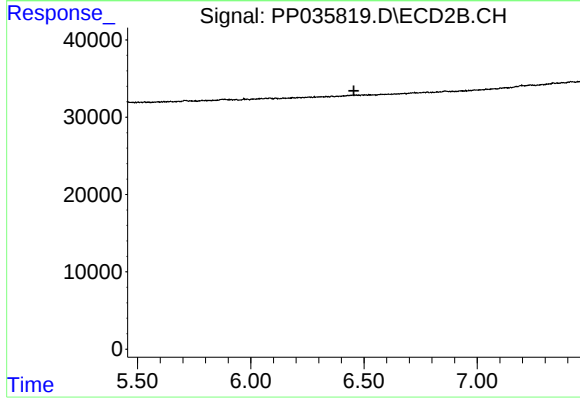

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

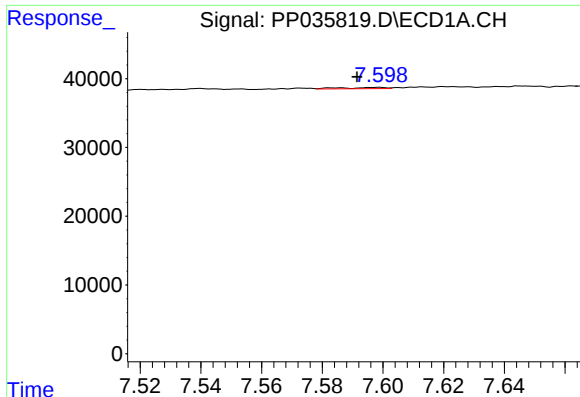

#28 AR-1254-3


R.T.: 7.598 min
Delta R.T.: 0.007 min
Response: 2021
Conc: 1.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

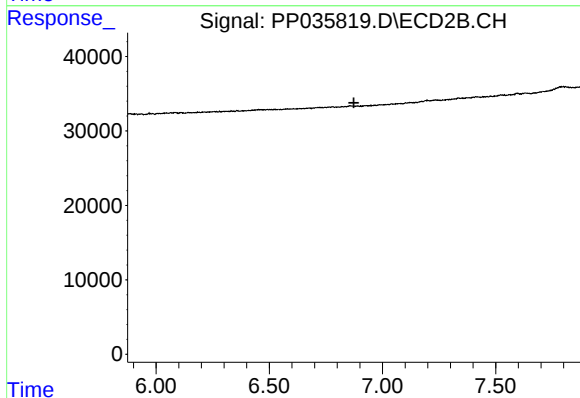


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.874 min
Response: 0
Conc: N.D.

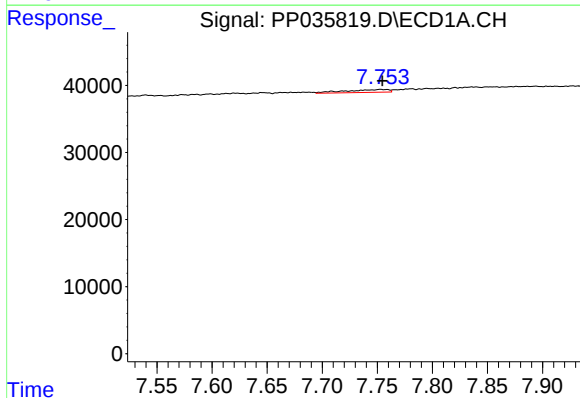


#31 AR-1260-1

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 11335
Conc: 12.57 ng/ml

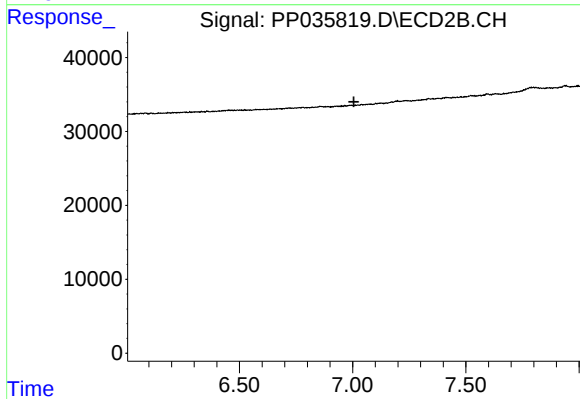

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.005 min
Response: 0
Conc: N.D.

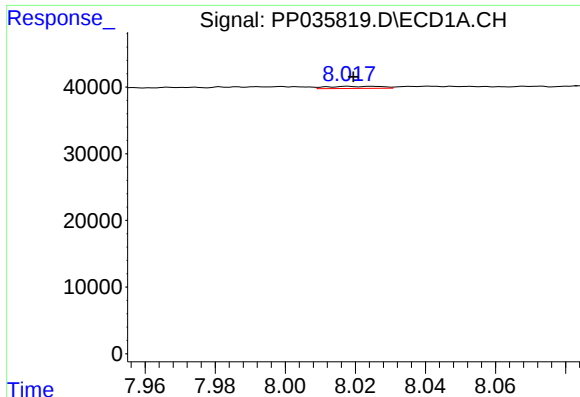

#32 AR-1260-2


R.T.: 8.018 min
Delta R.T.: -0.001 min
Response: 3497
Conc: 3.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

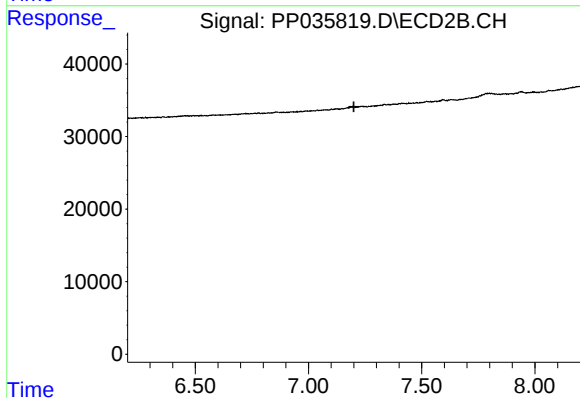


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

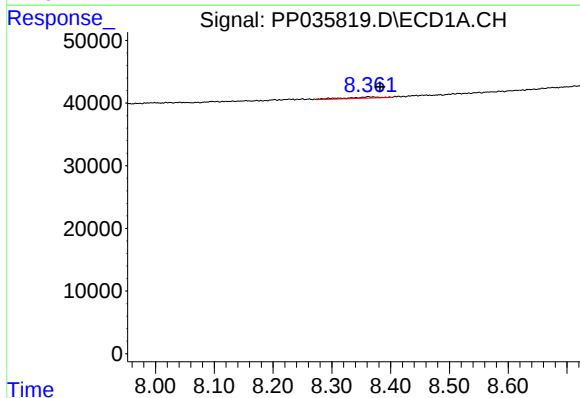


#33 AR-1260-3

R.T.: 8.362 min
Delta R.T.: -0.020 min
Response: 8947
Conc: 13.37 ng/ml

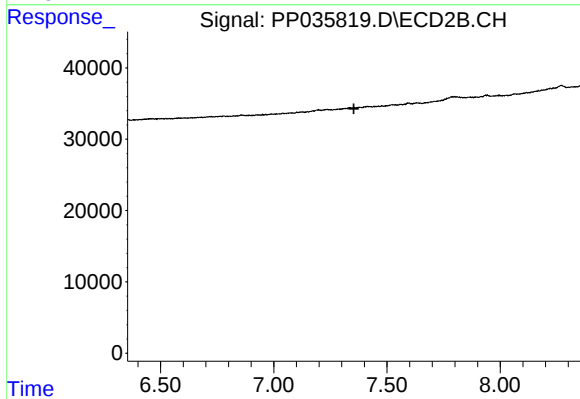

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.354 min
Response: 0
Conc: N.D.

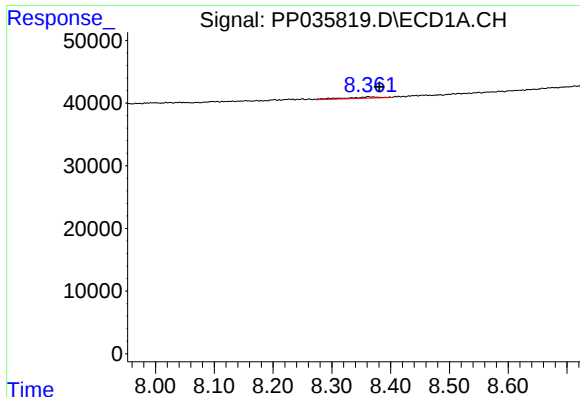

#36 AR-1262-1


R.T.: 8.362 min
Delta R.T.: -0.019 min
Response: 8947
Conc: 8.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

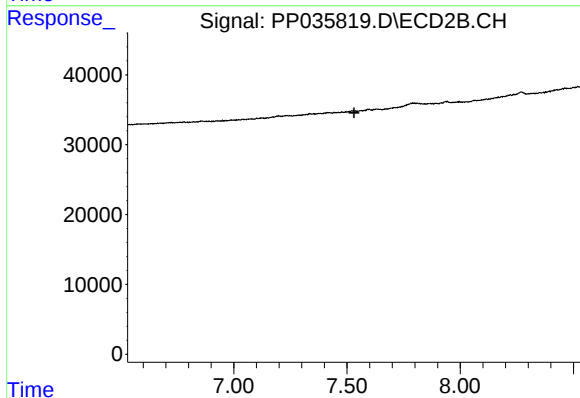


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.531 min
Response: 0
Conc: N.D.

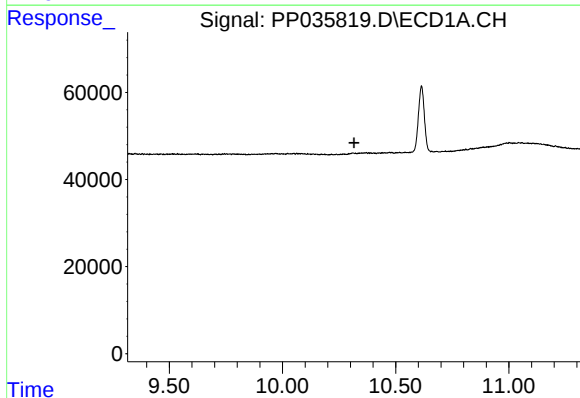

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.316 min
Response: 0
Conc: N.D.

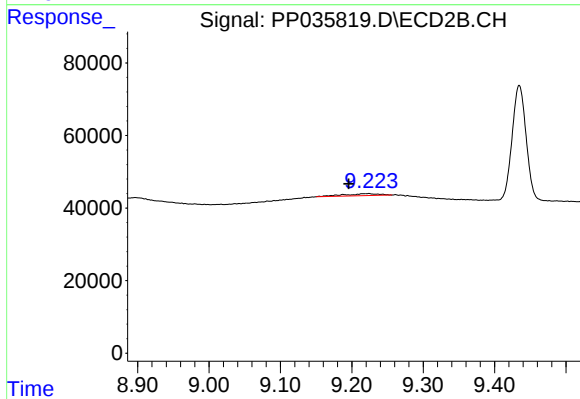

#45 AR-1268-5

R.T.: 9.224 min
Delta R.T.: 0.029 min
Response: 18741
Conc: 2.37 ng/ml