

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035890.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 6:55
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 13:00:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.774	4.195	462274	686761	19.729	20.203
2)	SA Decachlor...	10.609	9.431	234541	411380	20.837	19.453
Target Compounds							
9)	L2 AR-1221-2	5.121	0.000	7062	0	31.467	N.D. #
24)	L5 AR-1248-4	7.020	0.000	893	0	1.330	N.D. #
26)	L6 AR-1254-1	6.998	0.000	7037	0	10.047	N.D. #
28)	L6 AR-1254-3	7.619f	0.000	10733	0	9.070	N.D. #
29)	L6 AR-1254-4	7.877	0.000	1780	0	2.232	N.D. #
30)	L6 AR-1254-5	8.293f	0.000	1716	0	1.819	N.D. #
31)	L7 AR-1260-1	7.751	0.000	4862	0	5.393	N.D. #
35)	L7 AR-1260-5	8.914	0.000	12268	0	9.301	N.D. #
37)	L8 AR-1262-2	8.914	0.000	12268	0	6.958	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035890.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 6:55
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 13:00:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

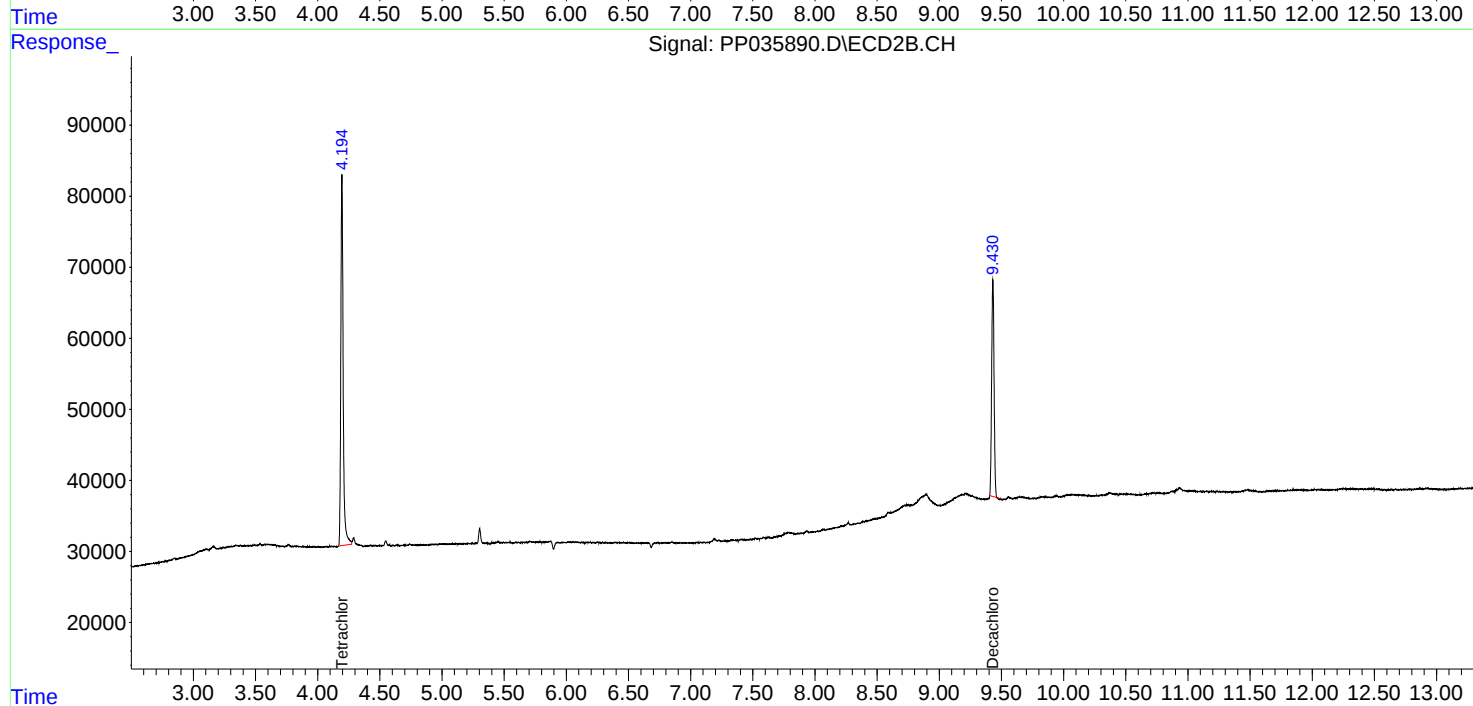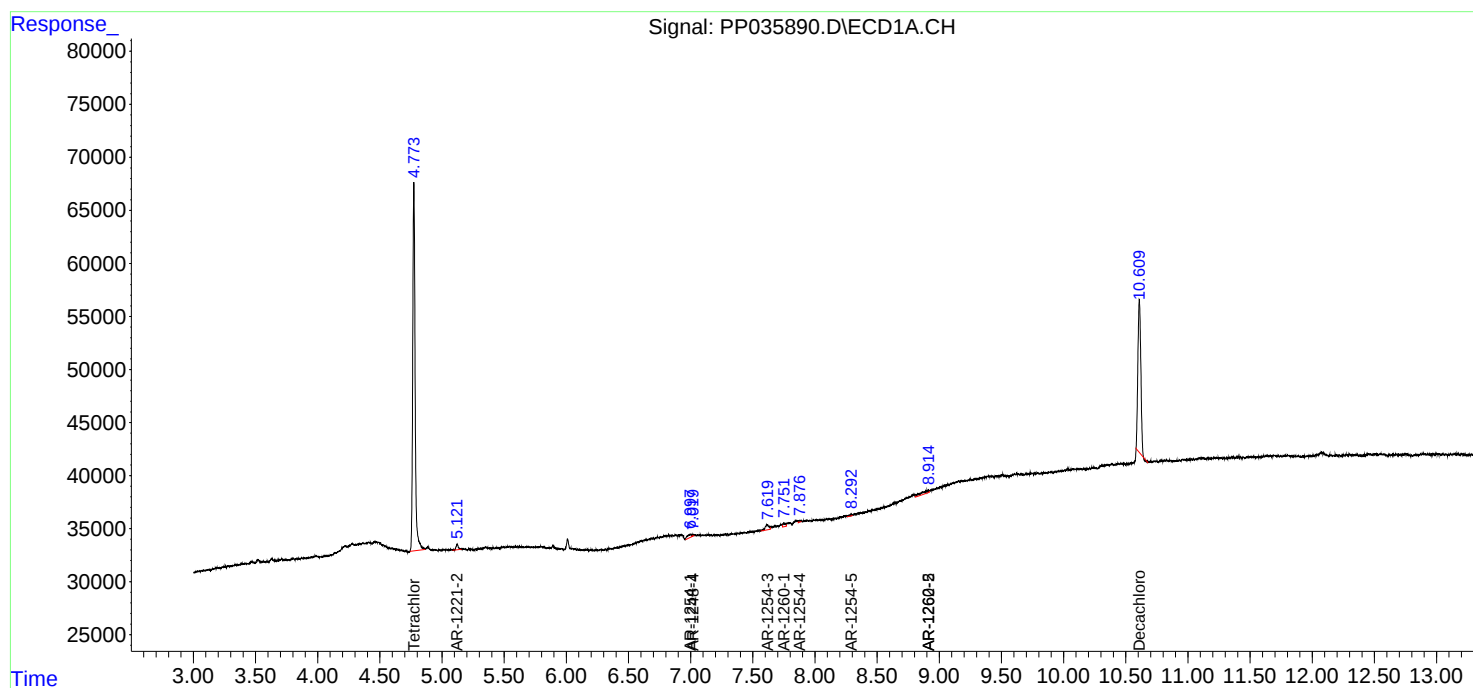


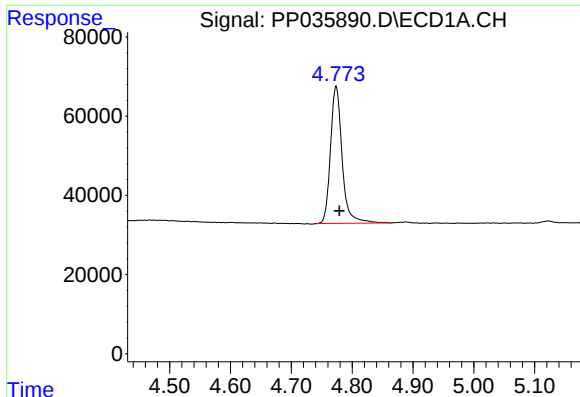

#1 Tetrachloro-m-xylene


R.T.: 4.774 min
Delta R.T.: -0.005 min
Response: 462274
Conc: 19.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

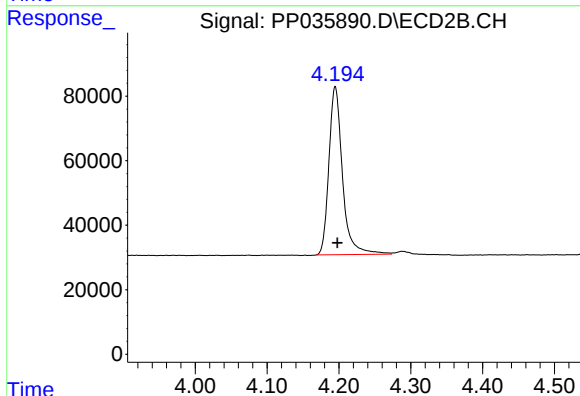


#1 Tetrachloro-m-xylene

R.T.: 4.195 min
Delta R.T.: -0.003 min
Response: 686761
Conc: 20.20 ng/ml

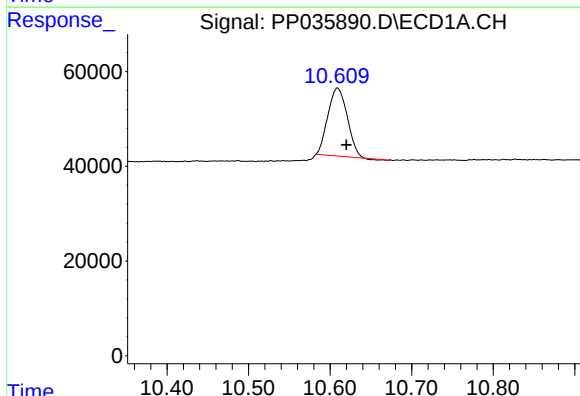


#2 Decachlorobiphenyl

R.T.: 10.609 min
Delta R.T.: -0.011 min
Response: 234541
Conc: 20.84 ng/ml

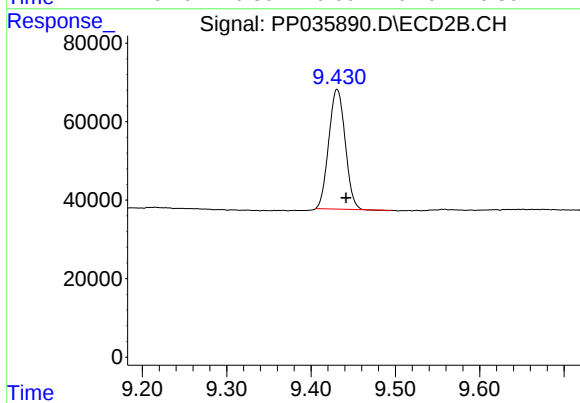

#2 Decachlorobiphenyl


R.T.: 9.431 min
Delta R.T.: -0.011 min
Response: 411380
Conc: 19.45 ng/ml

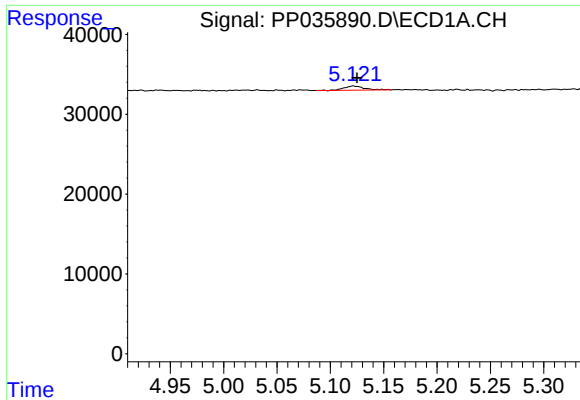

#9 AR-1221-2


R.T.: 5.121 min
Delta R.T.: -0.003 min
Response: 7062
Conc: 31.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

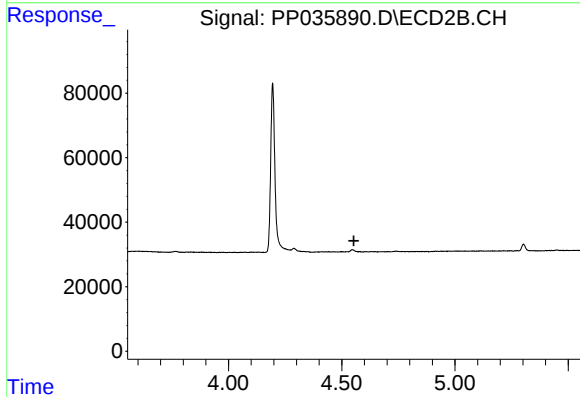


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

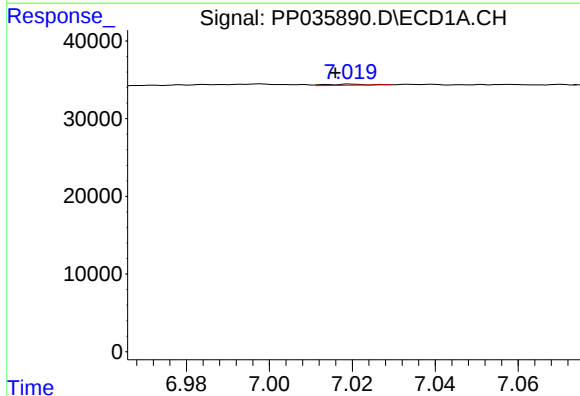


#24 AR-1248-4

R.T.: 7.020 min
Delta R.T.: 0.004 min
Response: 893
Conc: 1.33 ng/ml

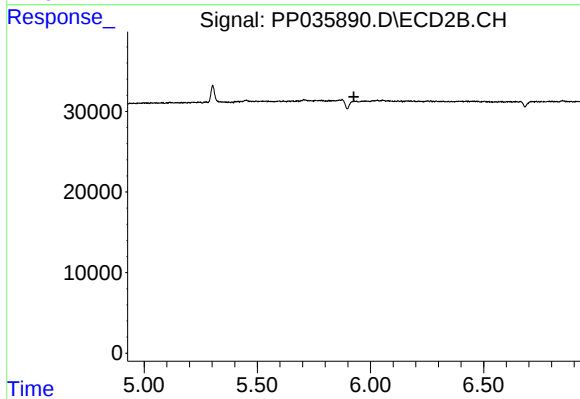

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.927 min
Response: 0
Conc: N.D.

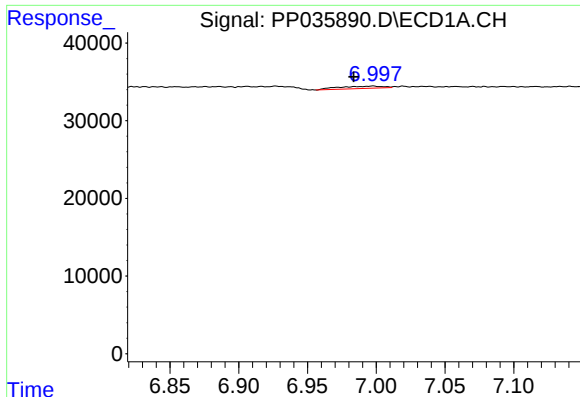

#26 AR-1254-1


R.T.: 6.998 min
Delta R.T.: 0.014 min
Response: 7037
Conc: 10.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

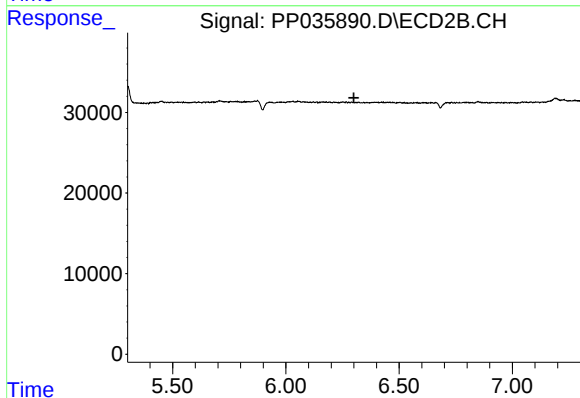


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.300 min
Response: 0
Conc: N.D.

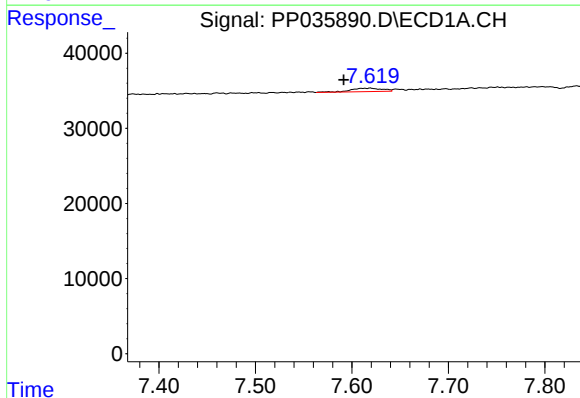


#28 AR-1254-3

R.T.: 7.619 min
Delta R.T.: 0.028 min
Response: 10733
Conc: 9.07 ng/ml

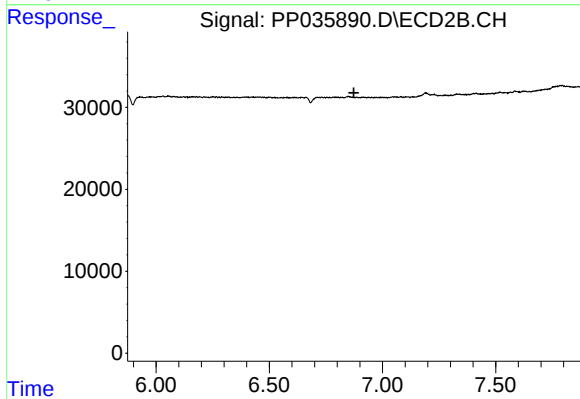

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.874 min
Response: 0
Conc: N.D.

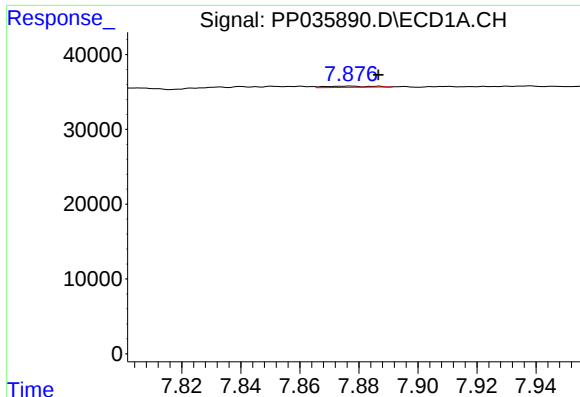

#29 AR-1254-4


R.T.: 7.877 min
Delta R.T.: -0.010 min
Response: 1780
Conc: 2.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

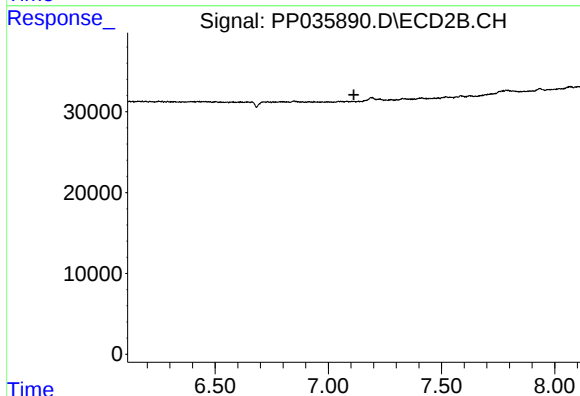


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

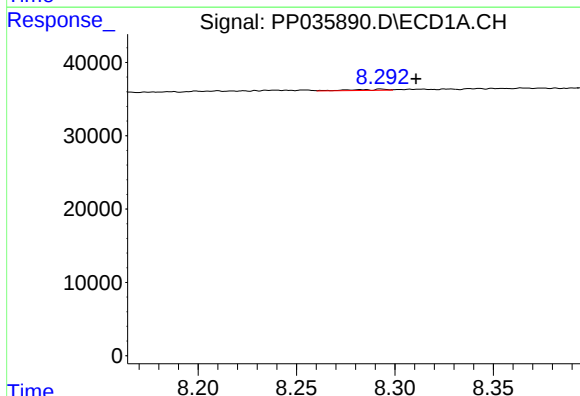


#30 AR-1254-5

R.T.: 8.293 min
Delta R.T.: -0.018 min
Response: 1716
Conc: 1.82 ng/ml

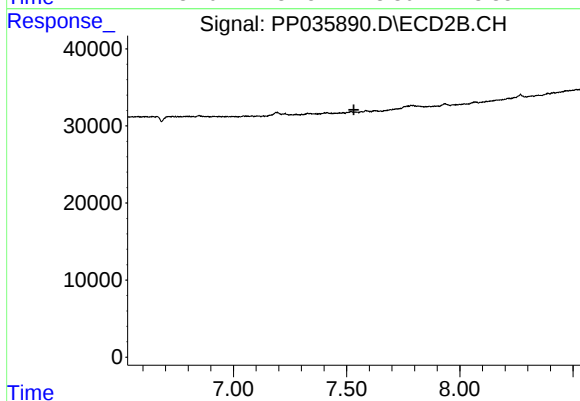

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.532 min
Response: 0
Conc: N.D.

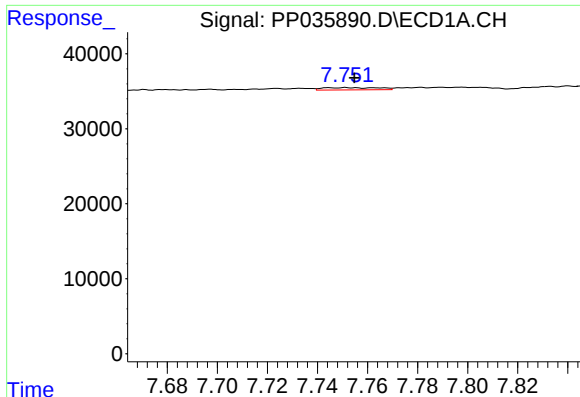

#31 AR-1260-1


R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 4862
Conc: 5.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

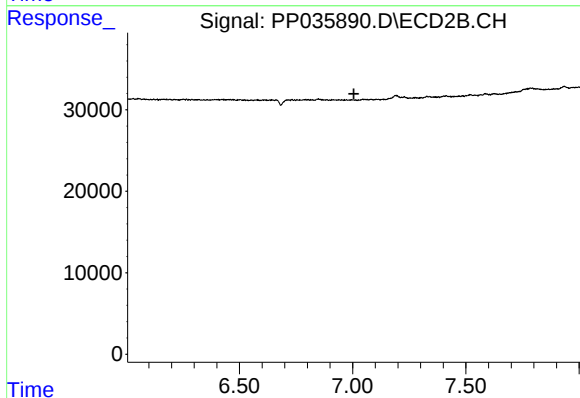


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.005 min
Response: 0
Conc: N.D.

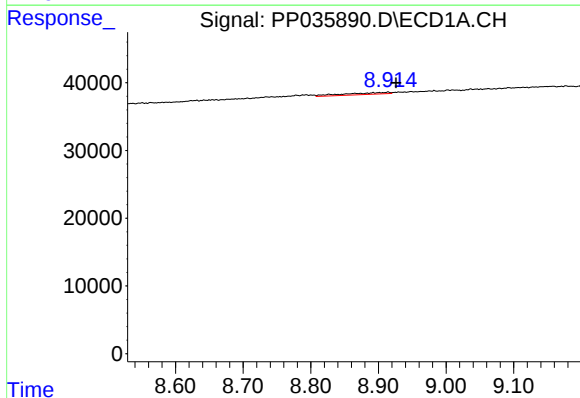


#35 AR-1260-5

R.T.: 8.914 min
Delta R.T.: -0.012 min
Response: 12268
Conc: 9.30 ng/ml

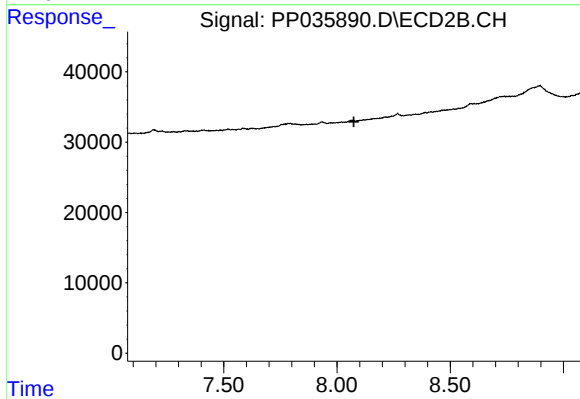

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.074 min
Response: 0
Conc: N.D.

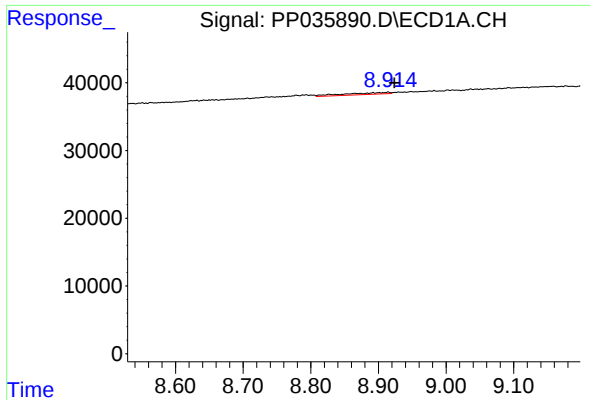

#37 AR-1262-2

R.T.: 8.914 min
Delta R.T.: -0.010 min
Response: 12268
Conc: 6.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

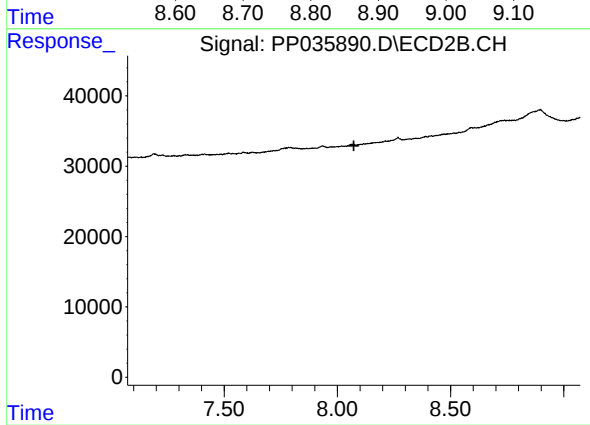

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.073 min
Response: 0
Conc: N.D.