

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035824.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 11:54
 Operator : DD\AJ
 Sample : M2362-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 149TH-ST-DRUM-1-PPE

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:07:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 13:14:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.776	4.196	344720	435195	14.712	12.803
2) SA Decachlor...	10.614	9.437	195898	283941	17.404m	13.427

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035824.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 11:54
Operator : DD\AJ
Sample : M2362-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
149TH-ST-DRUM-1-PPE


Manual Integrations
APPROVED

Ankita
5/14/2021 2:07:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 13:14:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

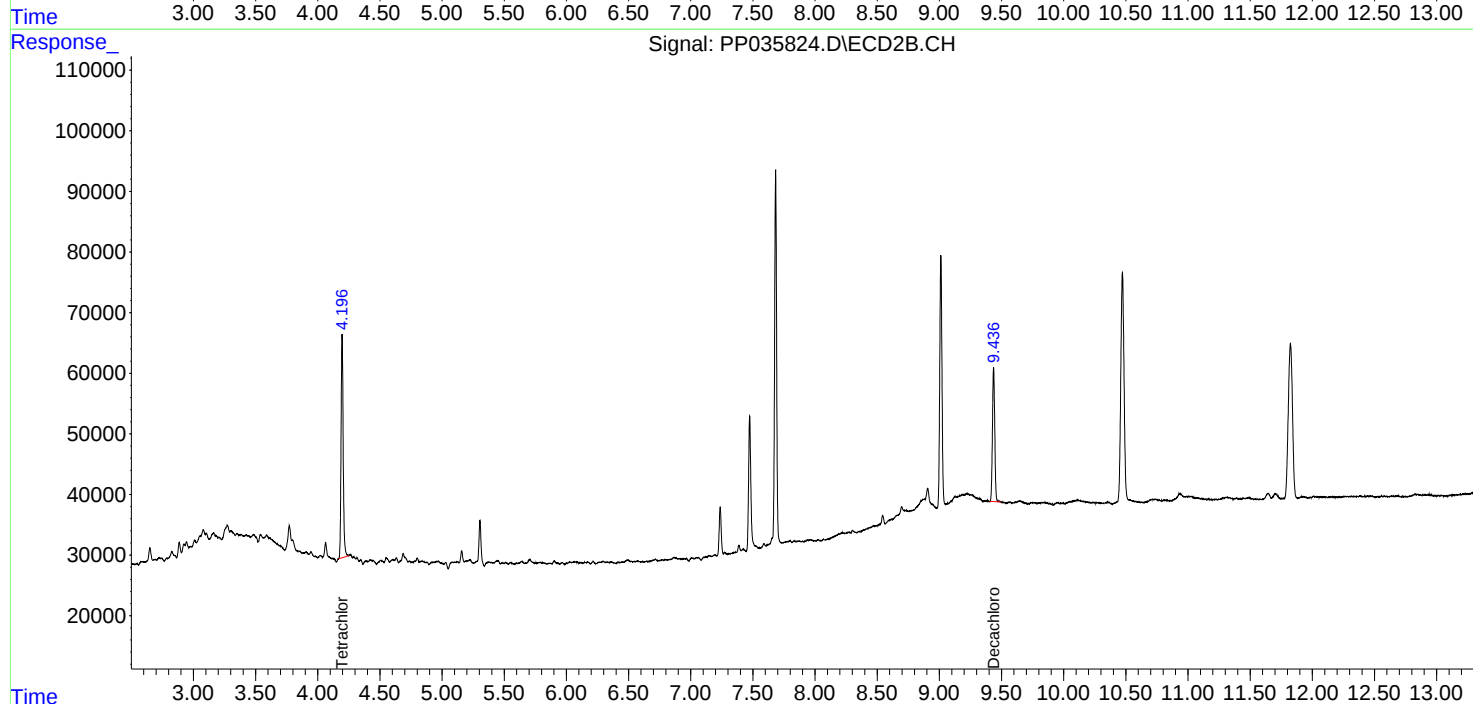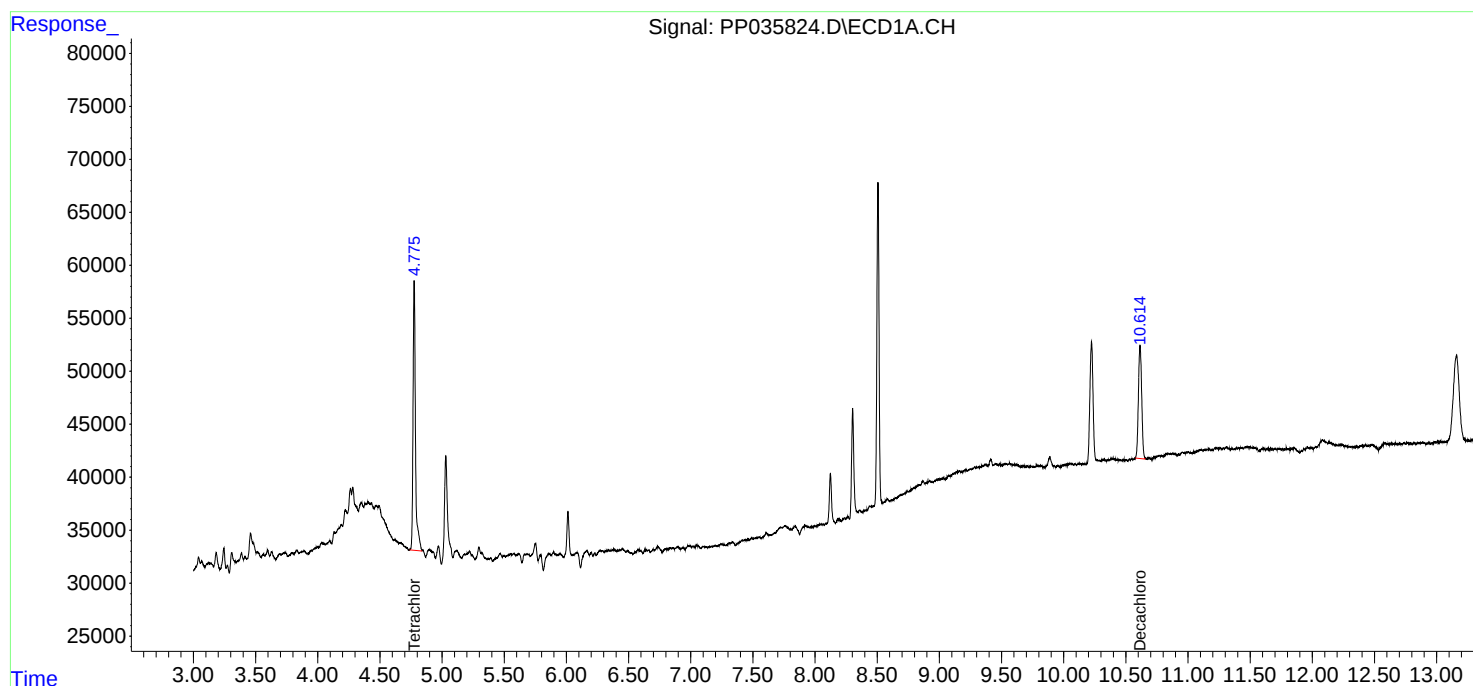

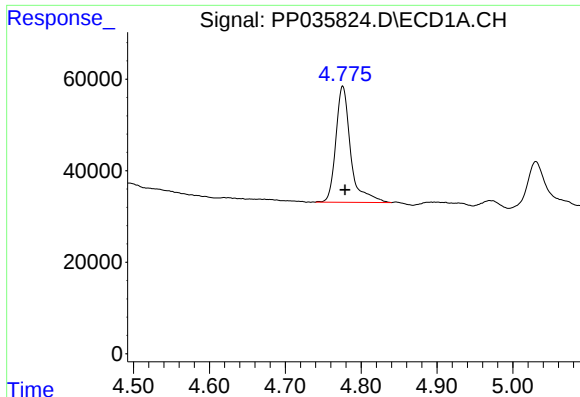


#1 Tetrachloro-m-xylene

R.T.: 4.776 min
Delta R.T.: -0.003 min
Response: 344720
Conc: 14.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
149TH-ST-DRUM-1-PPE


Manual Integrations
APPROVED

Ankita
5/14/2021 2:07:57 PM

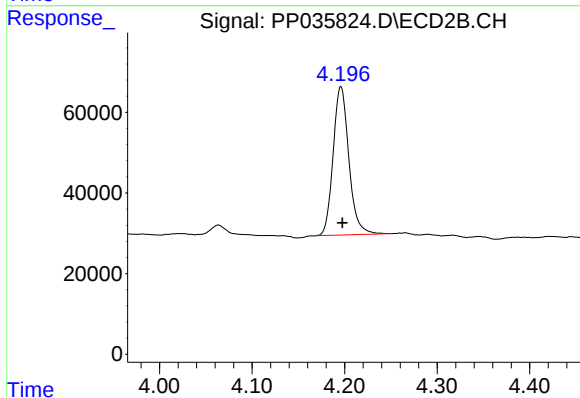


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.002 min
Response: 435195
Conc: 12.80 ng/ml

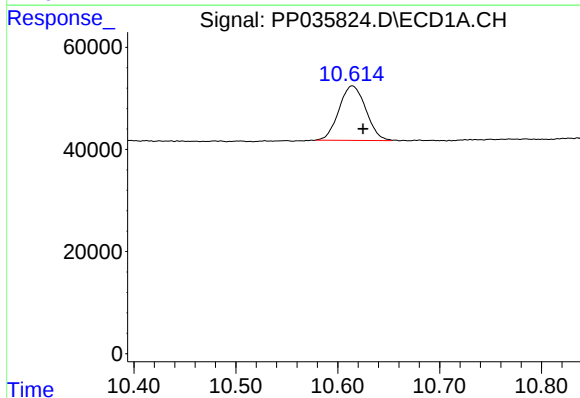

#2 Decachlorobiphenyl

R.T.: 10.614 min
Delta R.T.: -0.011 min
Response: 195898
Conc: 17.40 ng/ml m

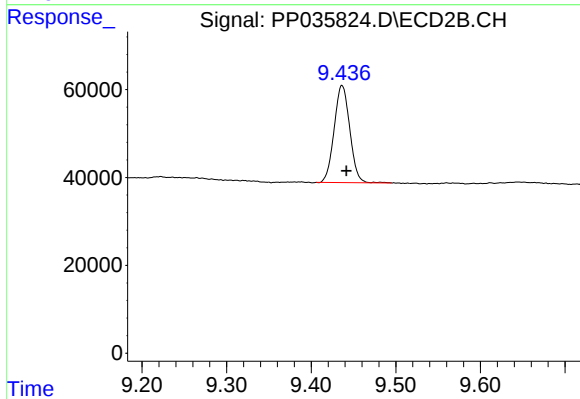

#2 Decachlorobiphenyl

R.T.: 9.437 min
Delta R.T.: -0.005 min
Response: 283941
Conc: 13.43 ng/ml