

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035826.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 12:27
 Operator : DD\AJ
 Sample : M2362-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TREMONT-AVE-DRUM-9-POLY

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:08:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 13:15:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.777	4.197	498708	708213	21.284	20.834
2) SA Decachlor...	10.616	9.436	296091	453287	26.306m	21.435

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035826.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 12:27
Operator : DD\AJ
Sample : M2362-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-DRUM-9-POLY


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 13:15:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

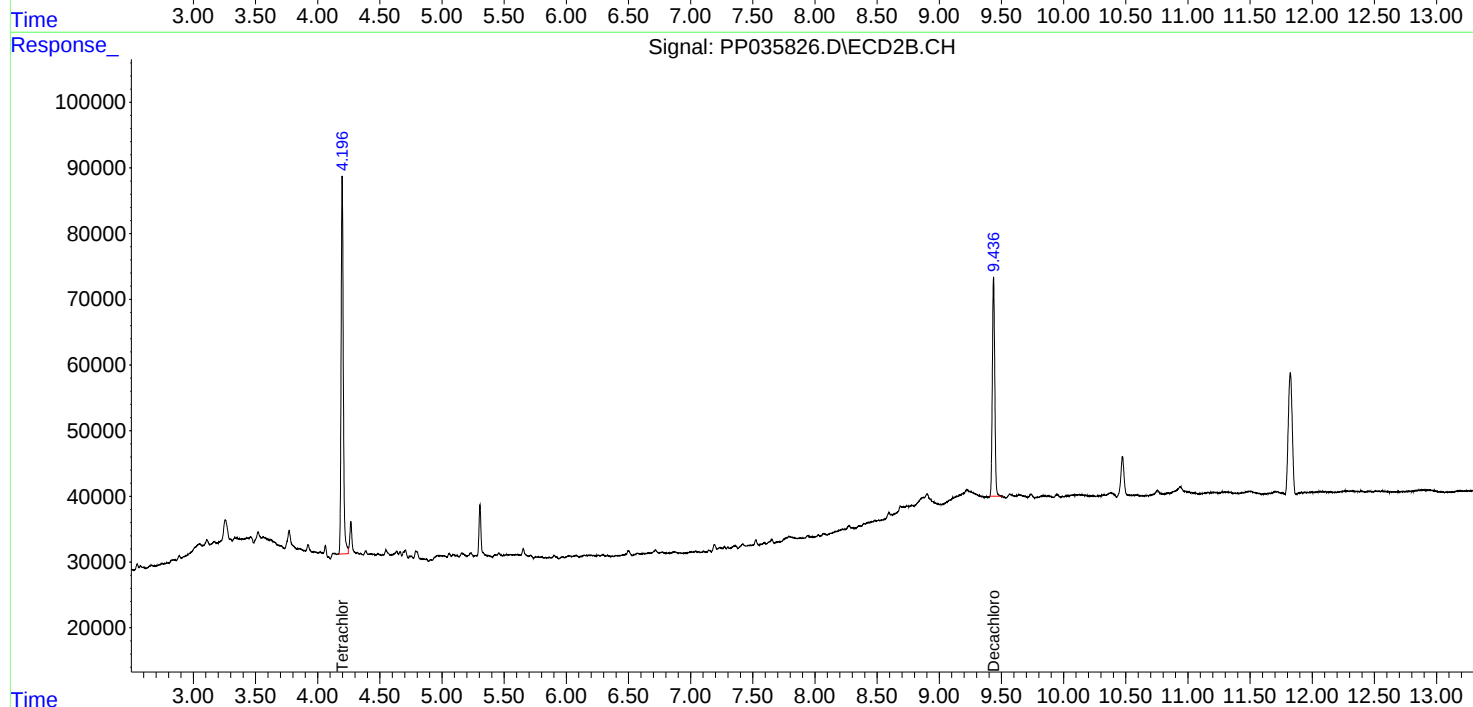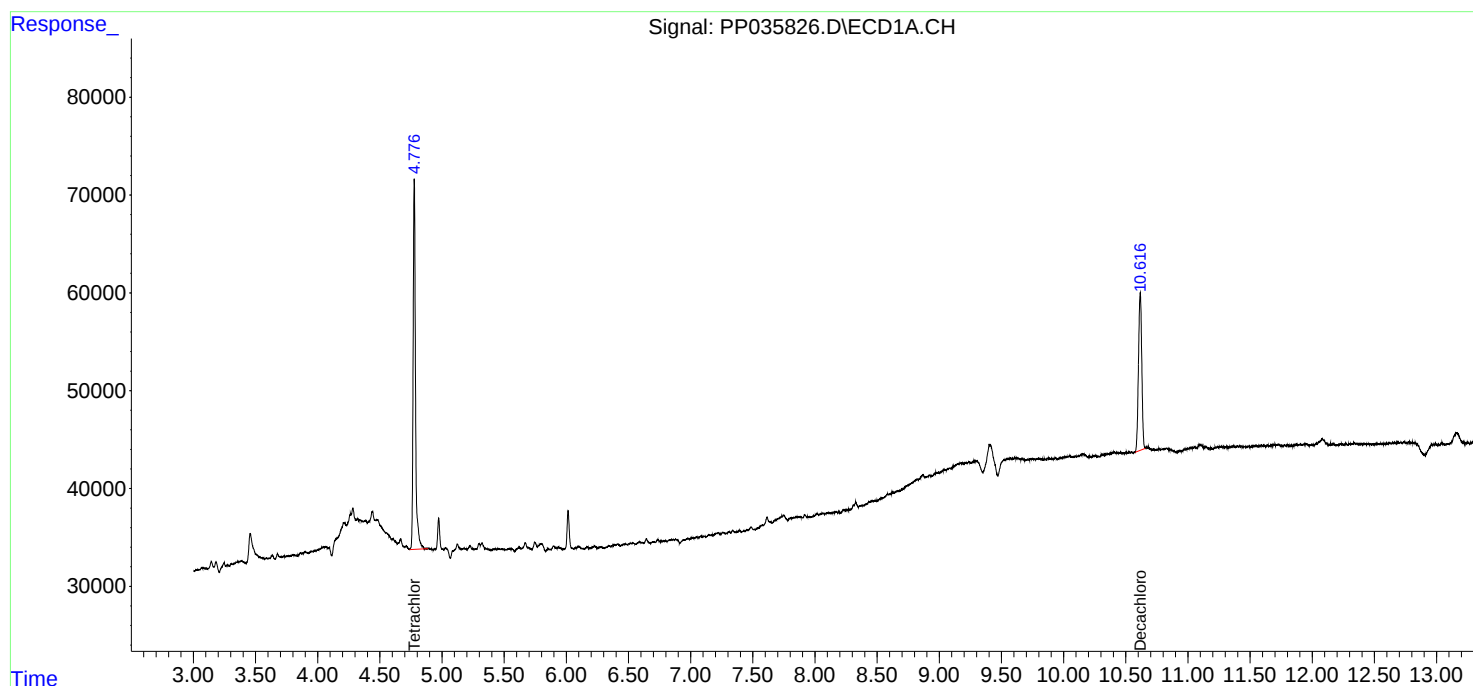

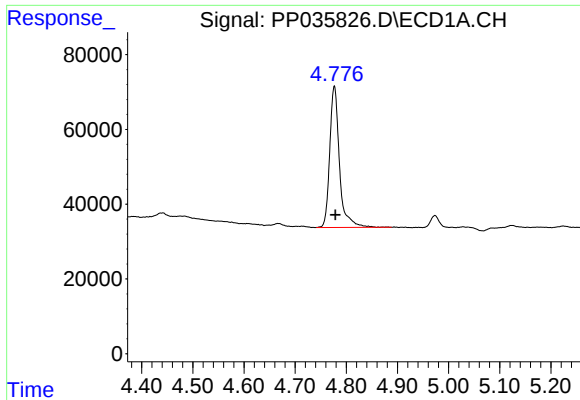


#1 Tetrachloro-m-xylene

R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 498708
Conc: 21.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-DRUM-9-POLY


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:01 PM

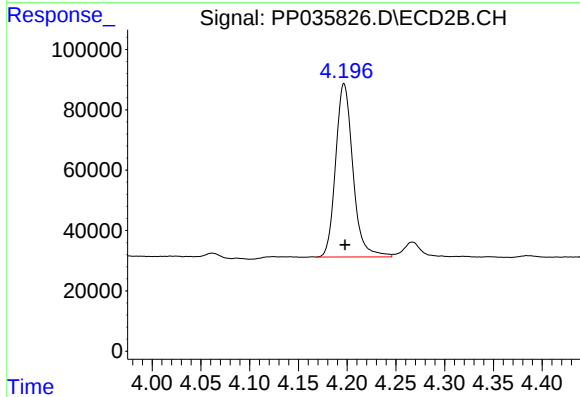


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: 0.000 min
Response: 708213
Conc: 20.83 ng/ml

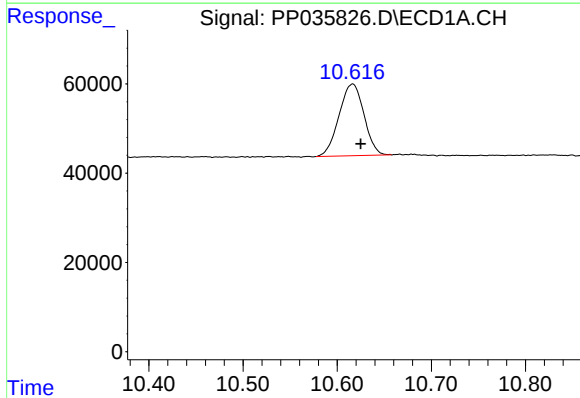

#2 Decachlorobiphenyl

R.T.: 10.616 min
Delta R.T.: -0.009 min
Response: 296091
Conc: 26.31 ng/ml m

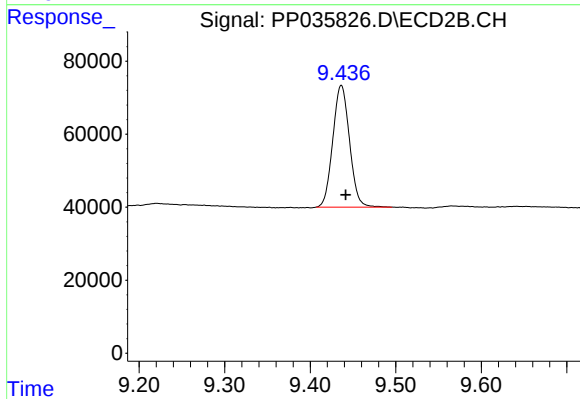

#2 Decachlorobiphenyl

R.T.: 9.436 min
Delta R.T.: -0.005 min
Response: 453287
Conc: 21.43 ng/ml