

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035832.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 14:26
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:08:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 17:14:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.776	4.196	1094869	1690310	46.728	49.726
2) SA Decachlor...	10.613	9.435	647438	1015800	57.520m	48.034
Target Compounds						
26) L6 AR-1254-1	6.977	6.295	345144	755230	492.797	463.143
27) L6 AR-1254-2	7.205	6.451	529787	665337	481.388	483.924
28) L6 AR-1254-3	7.585	6.869	576513	1001151	487.190	482.356
29) L6 AR-1254-4	7.879	7.106	426114	743891	534.453	511.822
30) L6 AR-1254-5	8.304	7.527	468763	886227	496.781	461.904

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035832.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 14:26
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 17:14:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

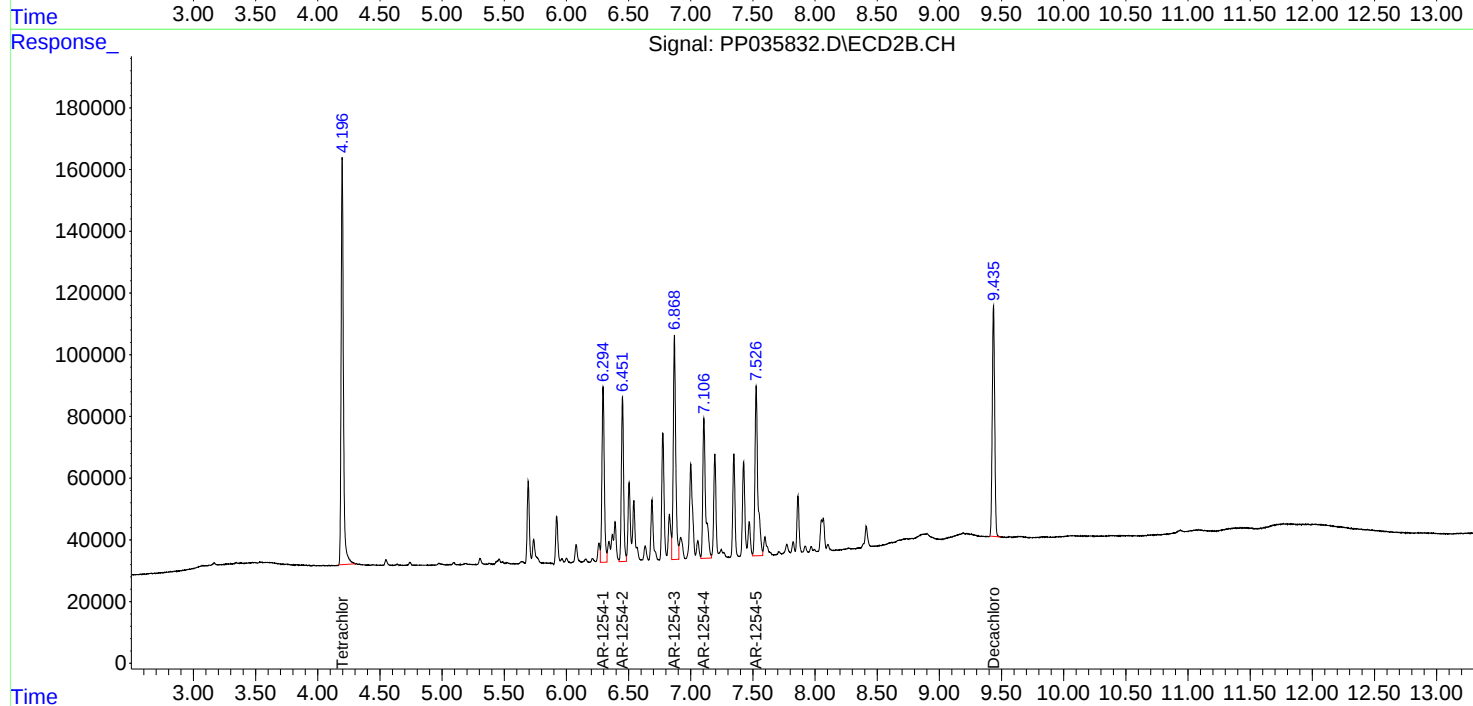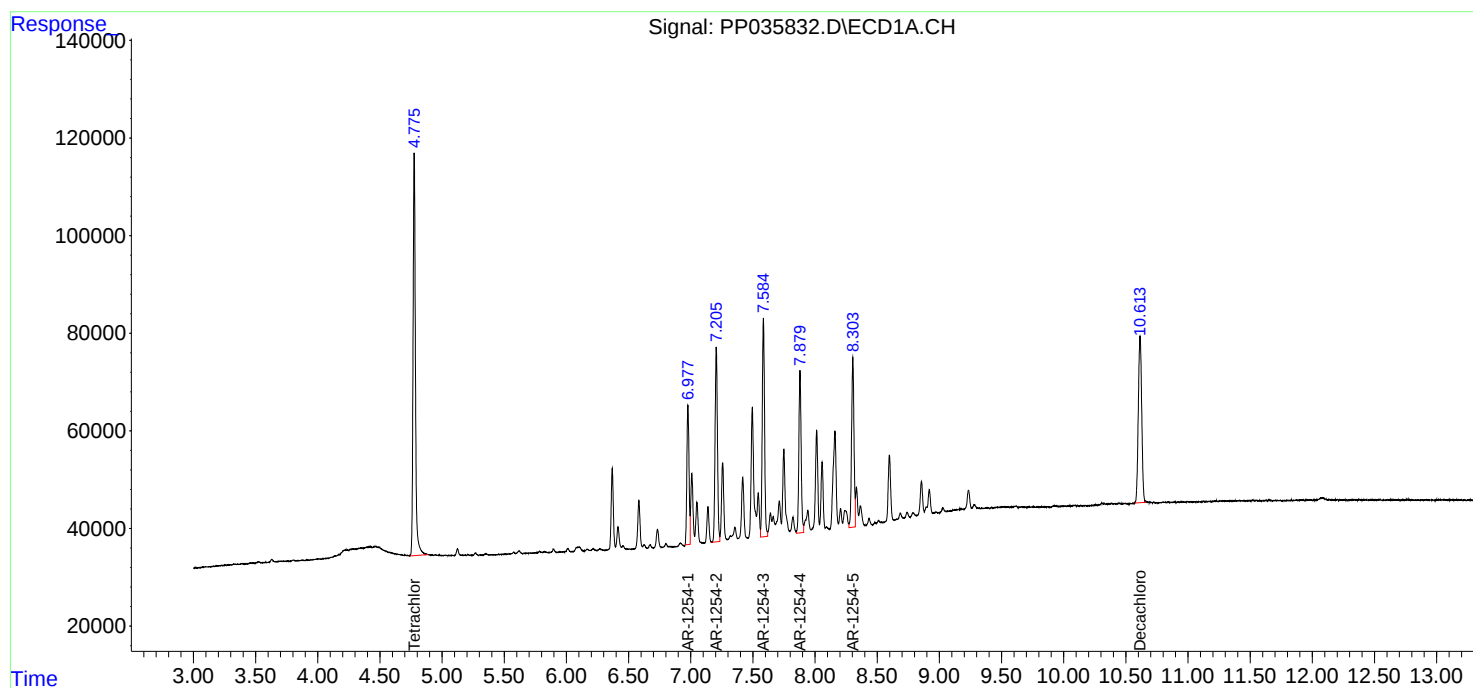

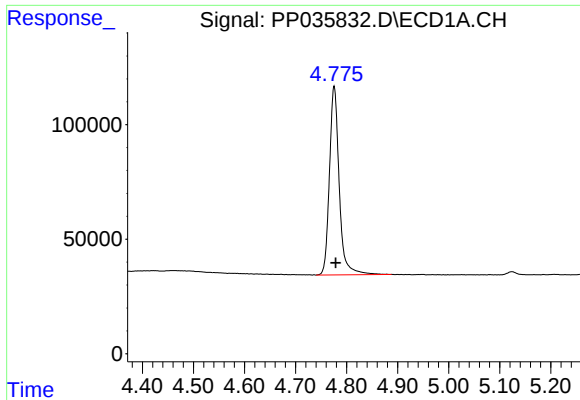


#1 Tetrachloro-m-xylene

R.T.: 4.776 min
Delta R.T.: -0.003 min
Response: 1094869
Conc: 46.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:11 PM

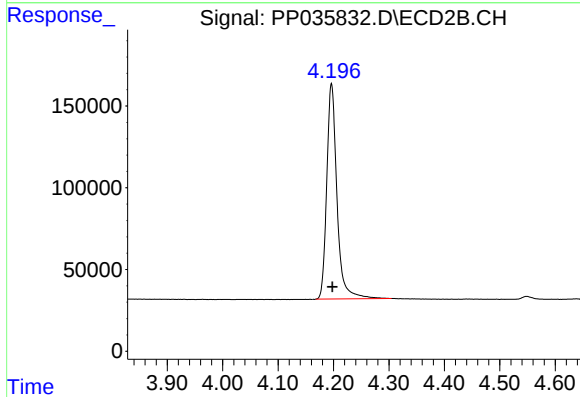


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.001 min
Response: 1690310
Conc: 49.73 ng/ml

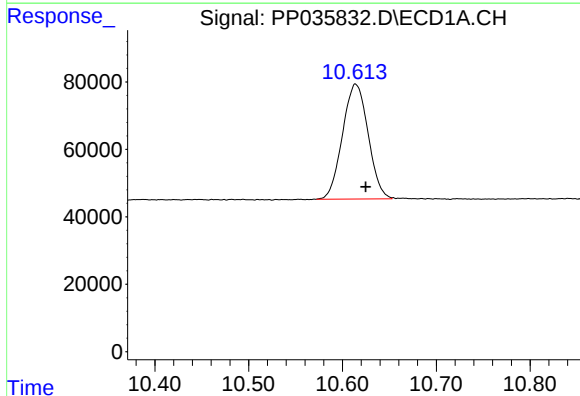


#2 Decachlorobiphenyl

R.T.: 10.613 min
Delta R.T.: -0.012 min
Response: 647438
Conc: 57.52 ng/ml m

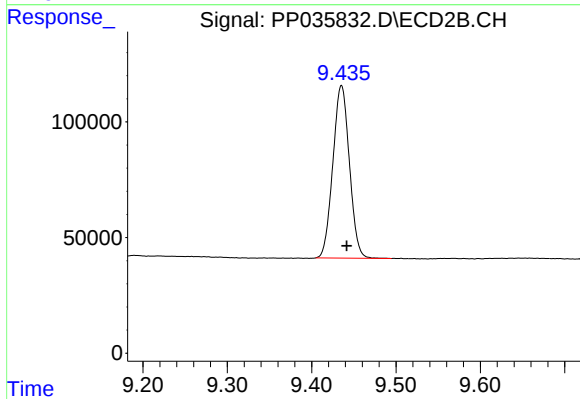

#2 Decachlorobiphenyl

R.T.: 9.435 min
Delta R.T.: -0.006 min
Response: 1015800
Conc: 48.03 ng/ml

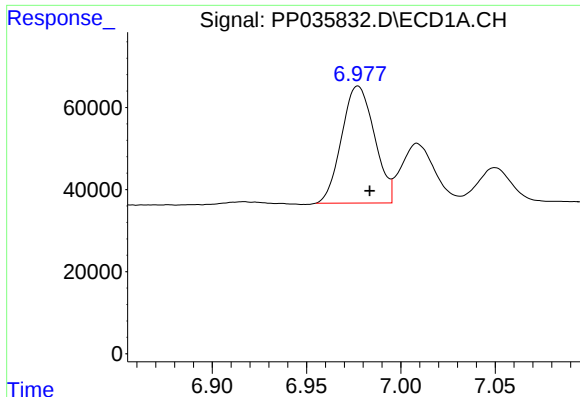


#26 AR-1254-1

R.T.: 6.977 min
Delta R.T.: -0.006 min
Response: 345144
Conc: 492.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:11 PM

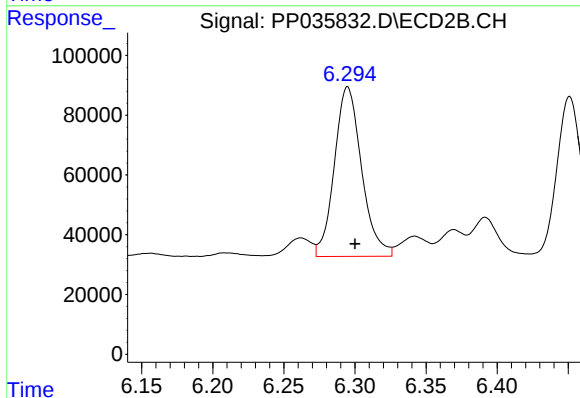


#26 AR-1254-1

R.T.: 6.295 min
Delta R.T.: -0.005 min
Response: 755230
Conc: 463.14 ng/ml

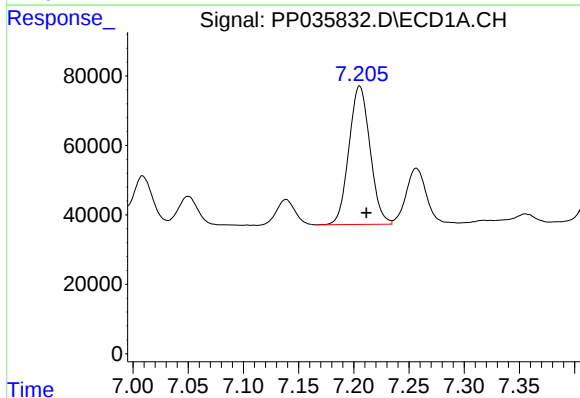


#27 AR-1254-2

R.T.: 7.205 min
Delta R.T.: -0.006 min
Response: 529787
Conc: 481.39 ng/ml

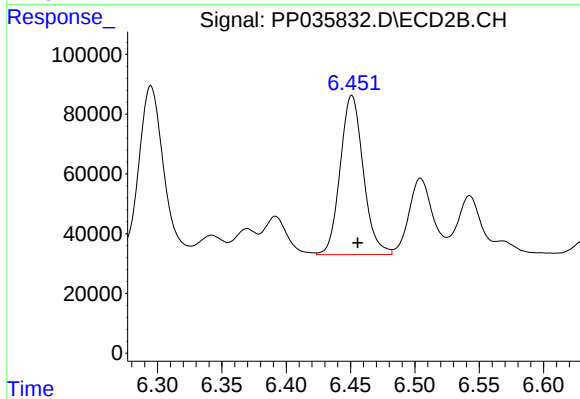

#27 AR-1254-2

R.T.: 6.451 min
Delta R.T.: -0.005 min
Response: 665337
Conc: 483.92 ng/ml

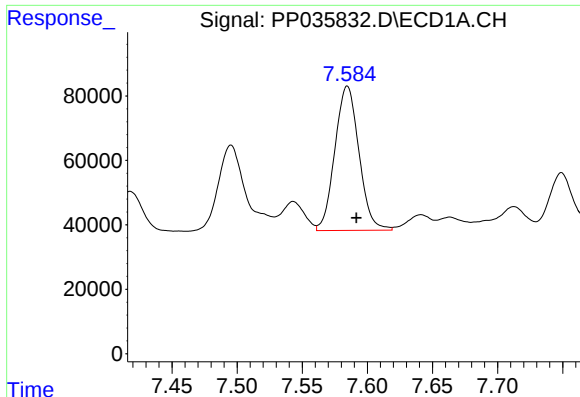


#28 AR-1254-3

R.T.: 7.585 min
Delta R.T.: -0.007 min
Response: 576513
Conc: 487.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:11 PM

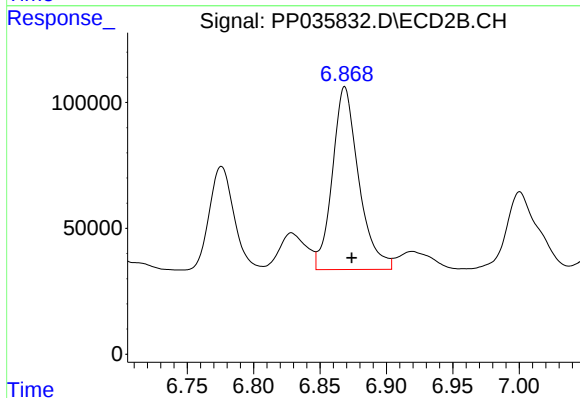


#28 AR-1254-3

R.T.: 6.869 min
Delta R.T.: -0.005 min
Response: 1001151
Conc: 482.36 ng/ml

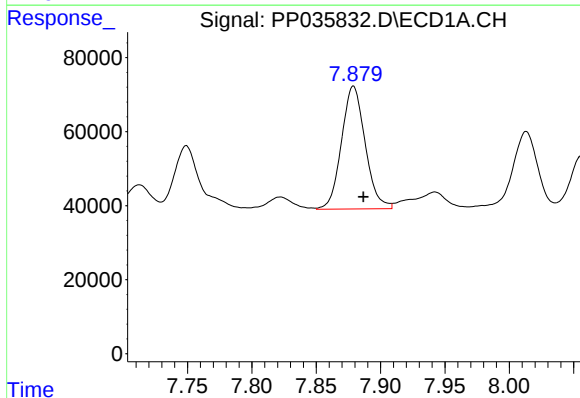


#29 AR-1254-4

R.T.: 7.879 min
Delta R.T.: -0.008 min
Response: 426114
Conc: 534.45 ng/ml

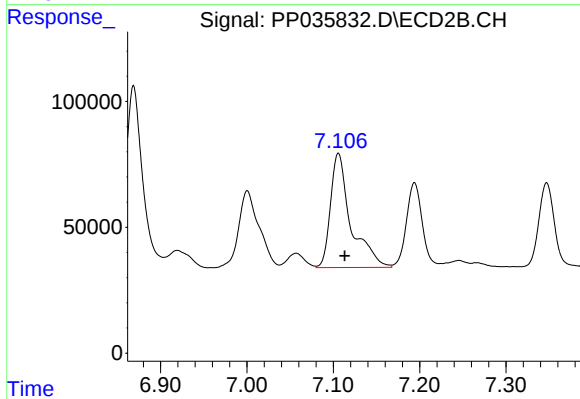

#29 AR-1254-4

R.T.: 7.106 min
Delta R.T.: -0.007 min
Response: 743891
Conc: 511.82 ng/ml

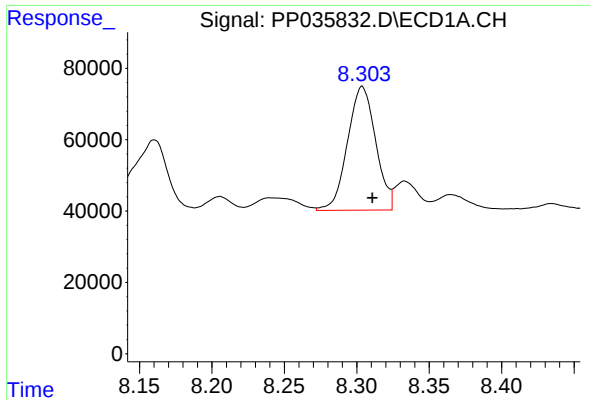


#30 AR-1254-5

R.T.: 8.304 min
Delta R.T.: -0.007 min
Response: 468763
Conc: 496.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
5/14/2021 2:08:11 PM

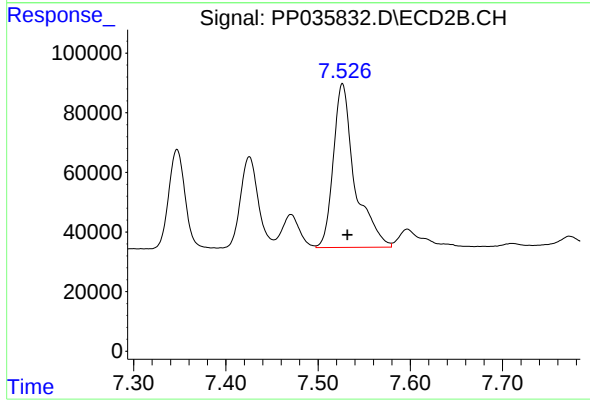

#30 AR-1254-5

R.T.: 7.527 min
Delta R.T.: -0.005 min
Response: 886227
Conc: 461.90 ng/ml