

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035853.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 20:36
 Operator : DD\AJ
 Sample : M2372-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-26855

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:09:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 02:05:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.773	4.194	413890	565394	17.664	16.633
2) SA Decachlor...	10.611	9.432	153225	231025	13.613	10.924
Target Compounds						
31) L7 AR-1260-1	7.746	6.998	25536	28638	28.325m	19.975m#
32) L7 AR-1260-2	8.006	7.192	68207	28804	70.018	16.687 #
33) L7 AR-1260-3	8.369	7.346	26160	26805	39.095	16.612 #
34) L7 AR-1260-4	8.601	7.822	16441	26067	20.980m	22.596
35) L7 AR-1260-5	8.917	8.066	24715	43998	18.738m	17.147

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035853.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 20:36
Operator : DD\AJ
Sample : M2372-11
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
CHRT-26855


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 02:05:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

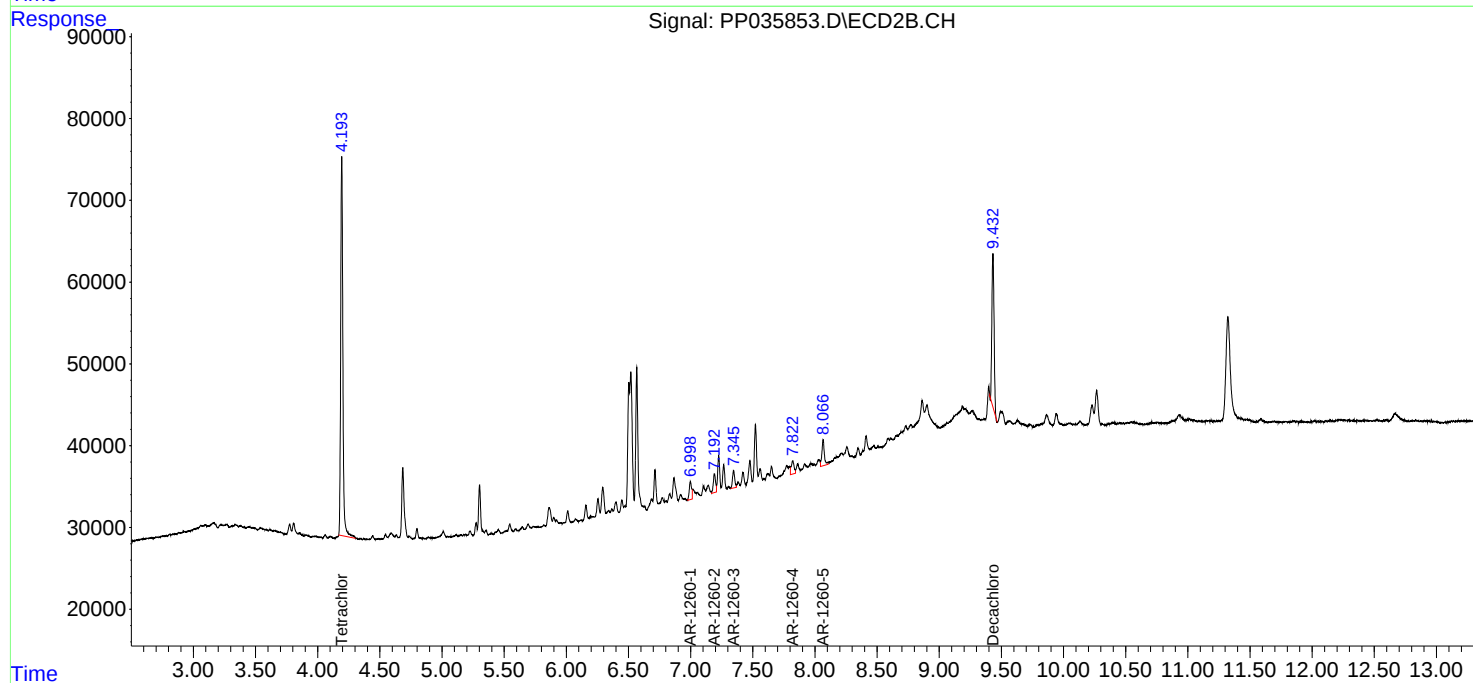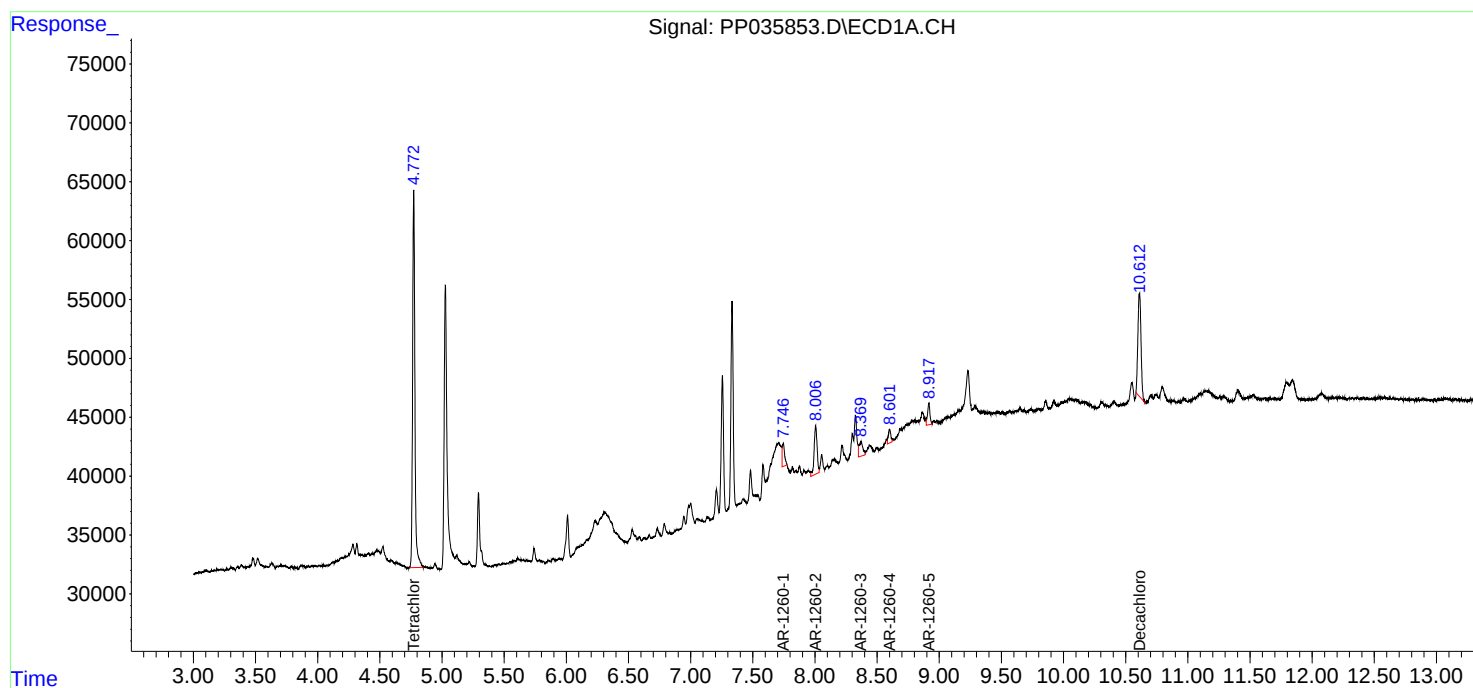

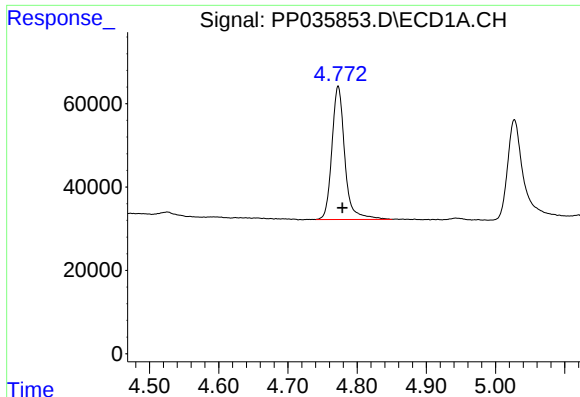


#1 Tetrachloro-m-xylene

R.T.: 4.773 min
Delta R.T.: -0.006 min
Response: 413890
Conc: 17.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26855


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:07 PM

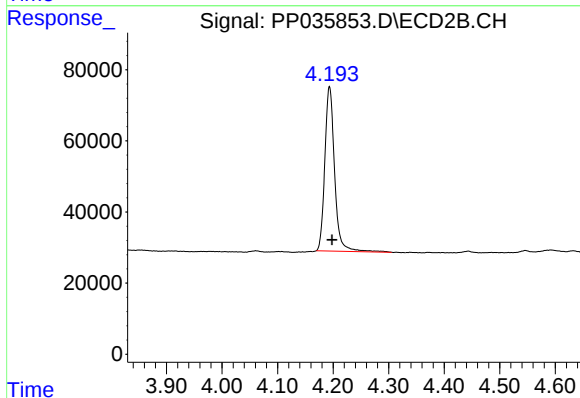


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.004 min
Response: 565394
Conc: 16.63 ng/ml

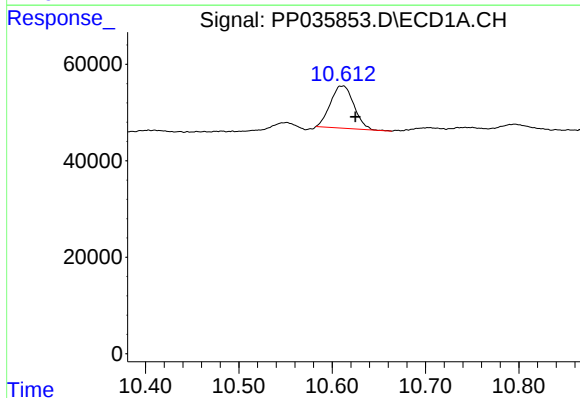


#2 Decachlorobiphenyl

R.T.: 10.611 min
Delta R.T.: -0.014 min
Response: 153225
Conc: 13.61 ng/ml

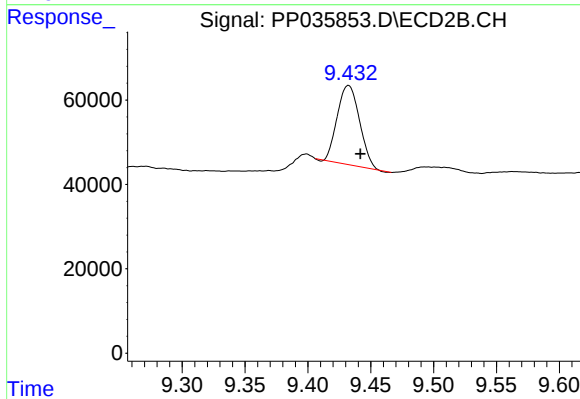

#2 Decachlorobiphenyl

R.T.: 9.432 min
Delta R.T.: -0.009 min
Response: 231025
Conc: 10.92 ng/ml

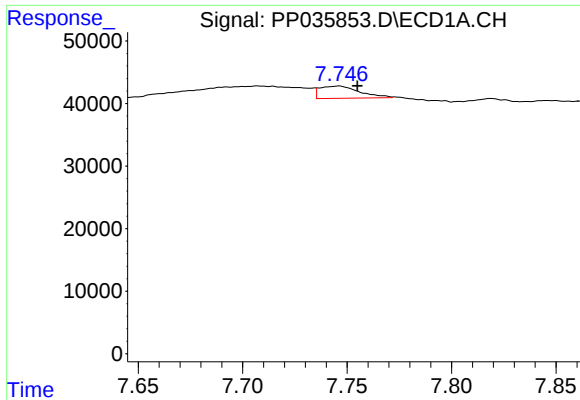


#31 AR-1260-1

R.T.: 7.746 min
Delta R.T.: -0.009 min
Response: 25536
Conc: 28.32 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CHRT-26855


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:07 PM

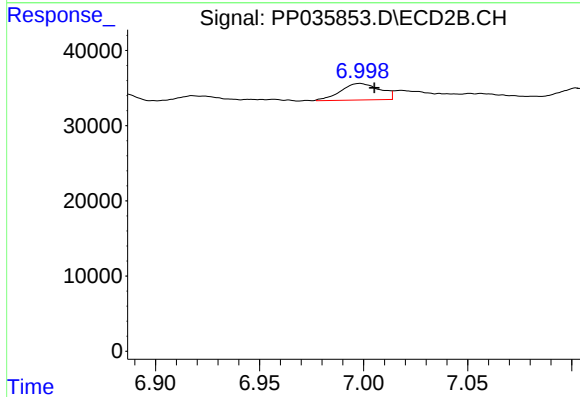


#31 AR-1260-1

R.T.: 6.998 min
Delta R.T.: -0.007 min
Response: 28638
Conc: 19.97 ng/ml m

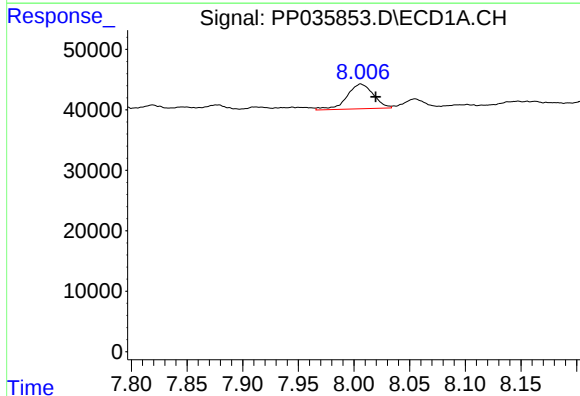


#32 AR-1260-2

R.T.: 8.006 min
Delta R.T.: -0.013 min
Response: 68207
Conc: 70.02 ng/ml

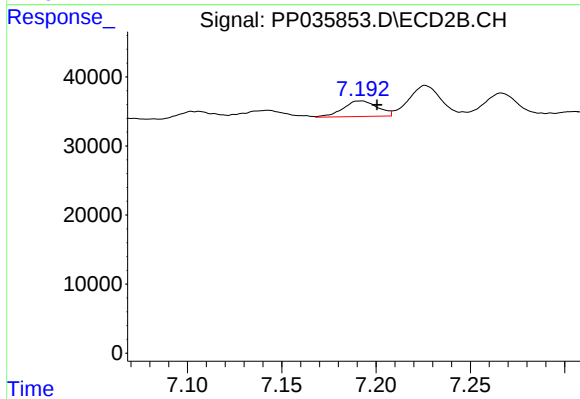

#32 AR-1260-2

R.T.: 7.192 min
Delta R.T.: -0.009 min
Response: 28804
Conc: 16.69 ng/ml

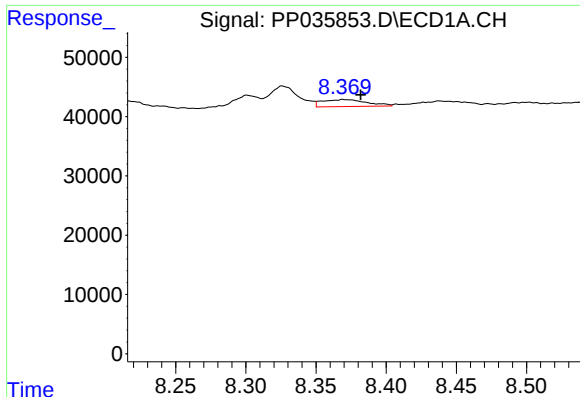


#33 AR-1260-3

R.T.: 8.369 min
Delta R.T.: -0.012 min
Response: 26160
Conc: 39.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26855


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:07 PM

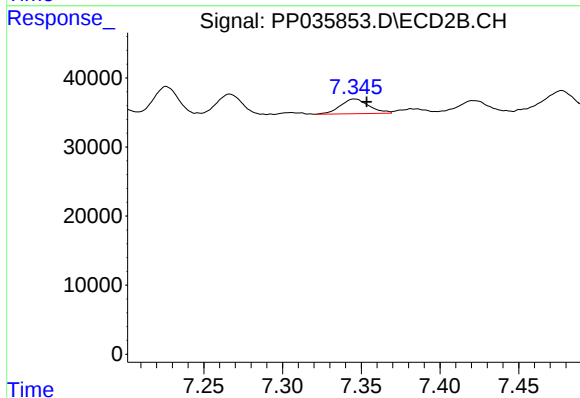


#33 AR-1260-3

R.T.: 7.346 min
Delta R.T.: -0.008 min
Response: 26805
Conc: 16.61 ng/ml

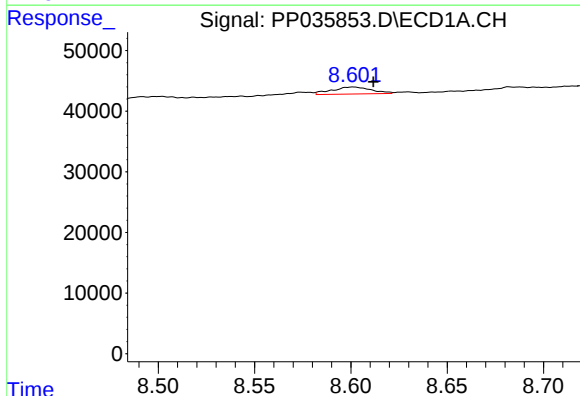


#34 AR-1260-4

R.T.: 8.601 min
Delta R.T.: -0.011 min
Response: 16441
Conc: 20.98 ng/ml m

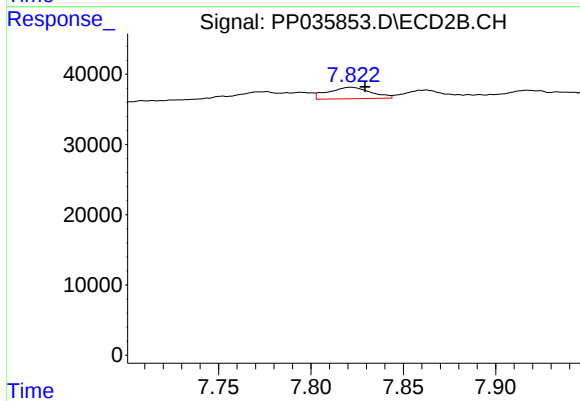

#34 AR-1260-4

R.T.: 7.822 min
Delta R.T.: -0.007 min
Response: 26067
Conc: 22.60 ng/ml

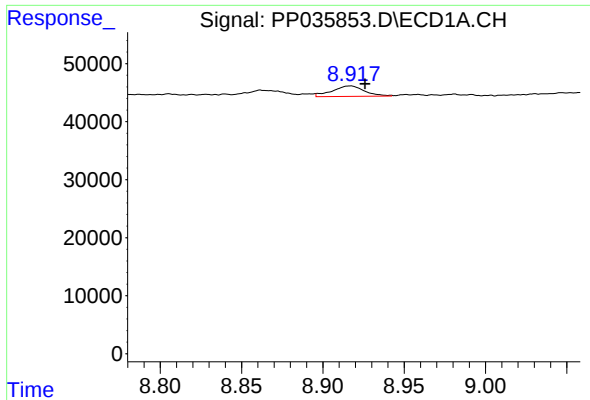


#35 AR-1260-5

R.T.: 8.917 min
Delta R.T.: -0.009 min
Response: 24715
Conc: 18.74 ng/ml m

Instrument :
ECD_P
ClientSampleId :
CHRT-26855

Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:07 PM

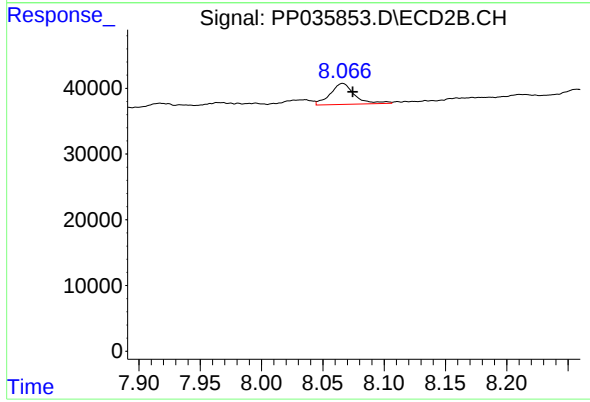

#35 AR-1260-5

R.T.: 8.066 min
Delta R.T.: -0.008 min
Response: 43998
Conc: 17.15 ng/ml