

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035862.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2021 23:07
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:09:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 04:08:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.775	4.196	1107939	1721059	47.285	50.630
2) SA Decachlor...	10.611	9.433	667143	1060851	59.271m	50.164
Target Compounds						
26) L6 AR-1254-1	6.977	6.294	351574	777535	501.979	476.821
27) L6 AR-1254-2	7.205	6.450	542412	683486	492.860	497.124
28) L6 AR-1254-3	7.584	6.868	589097	1024750	497.825	493.726
29) L6 AR-1254-4	7.879	7.105	434569	771607	545.058	530.891
30) L6 AR-1254-5	8.302	7.525	478411	924776	507.005	481.996

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035862.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2021 23:07
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 04:08:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

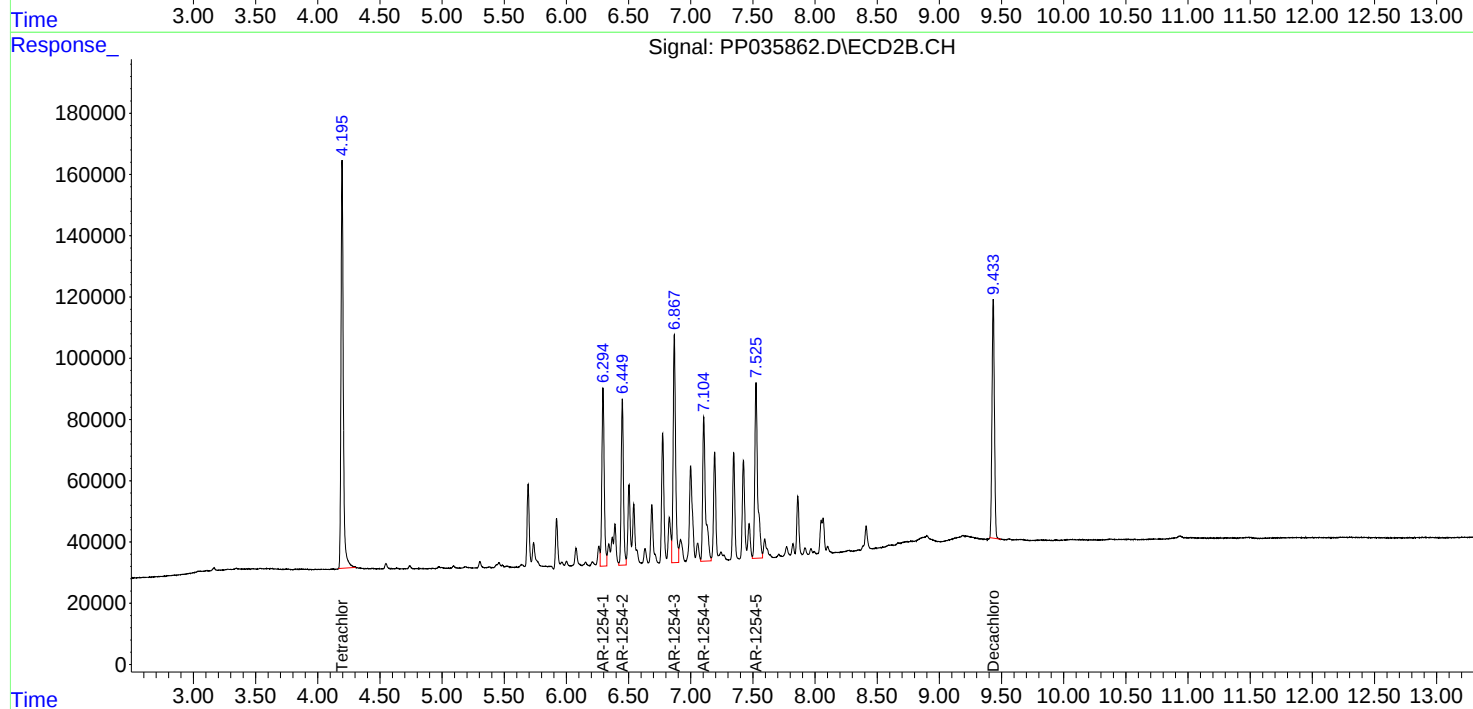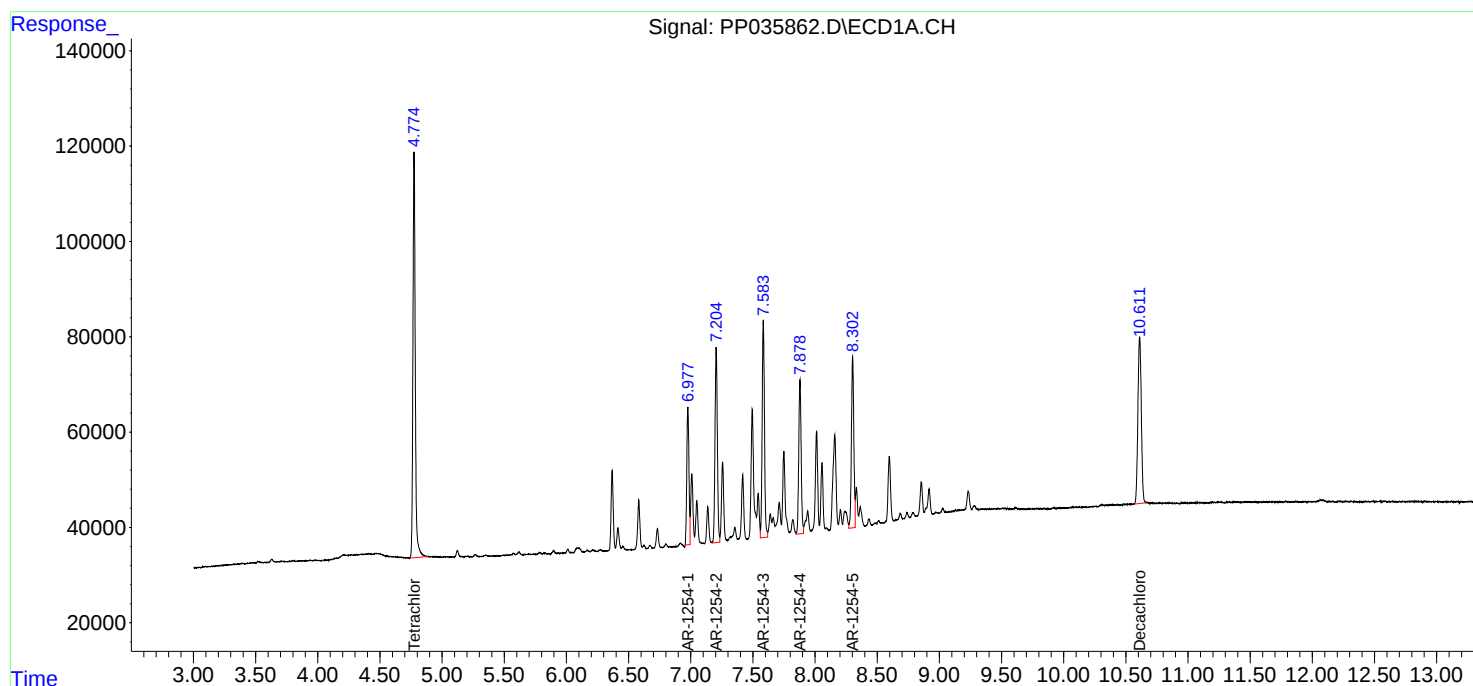

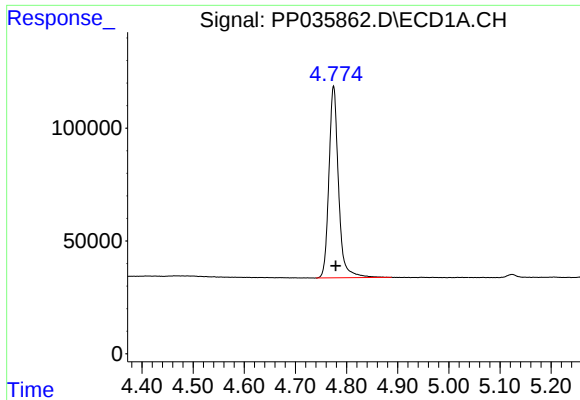


#1 Tetrachloro-m-xylene

R.T.: 4.775 min
Delta R.T.: -0.004 min
Response: 1107939
Conc: 47.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:25 PM

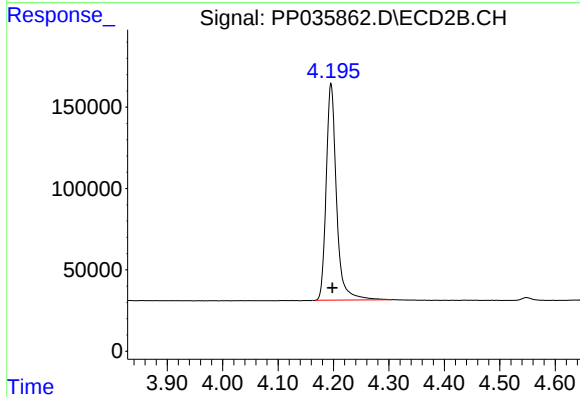


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.002 min
Response: 1721059
Conc: 50.63 ng/ml

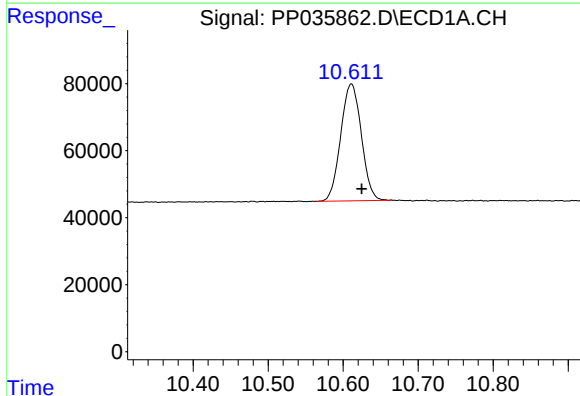


#2 Decachlorobiphenyl

R.T.: 10.611 min
Delta R.T.: -0.014 min
Response: 667143
Conc: 59.27 ng/ml m

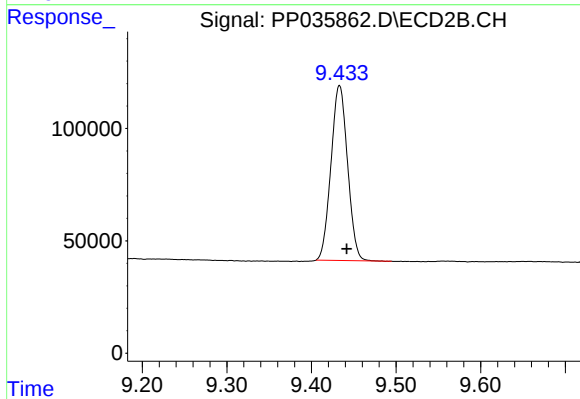

#2 Decachlorobiphenyl

R.T.: 9.433 min
Delta R.T.: -0.009 min
Response: 1060851
Conc: 50.16 ng/ml

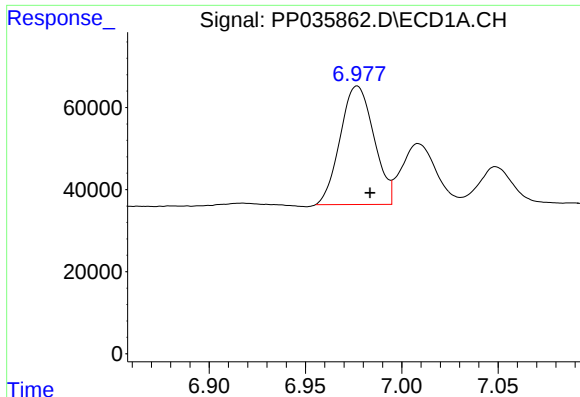


#26 AR-1254-1

R.T.: 6.977 min
Delta R.T.: -0.007 min
Response: 351574
Conc: 501.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:25 PM

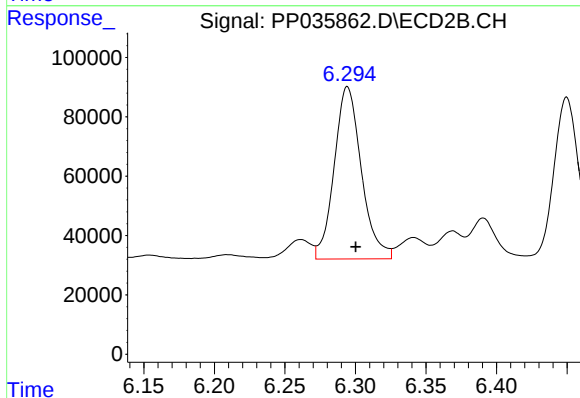


#26 AR-1254-1

R.T.: 6.294 min
Delta R.T.: -0.006 min
Response: 777535
Conc: 476.82 ng/ml

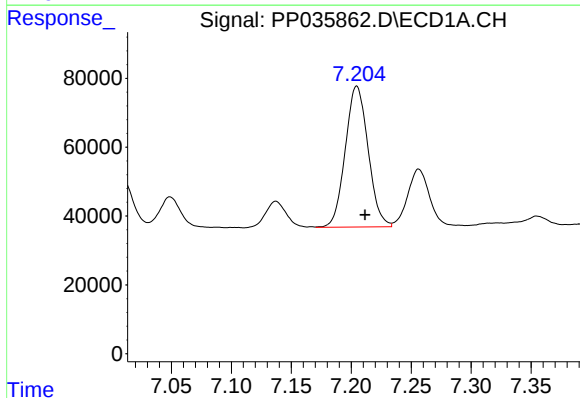


#27 AR-1254-2

R.T.: 7.205 min
Delta R.T.: -0.007 min
Response: 542412
Conc: 492.86 ng/ml

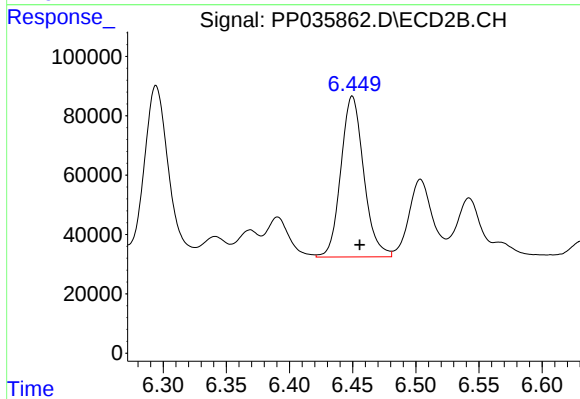

#27 AR-1254-2

R.T.: 6.450 min
Delta R.T.: -0.006 min
Response: 683486
Conc: 497.12 ng/ml

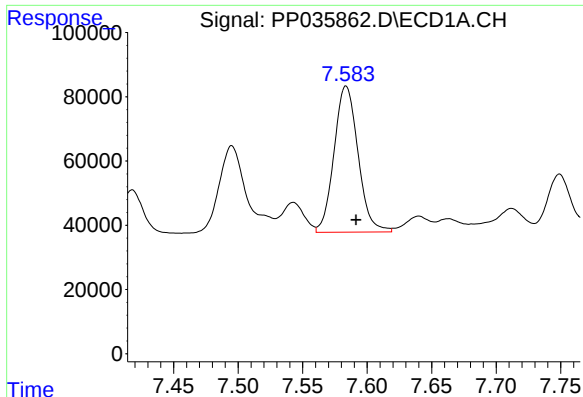


#28 AR-1254-3

R.T.: 7.584 min
Delta R.T.: -0.008 min
Response: 589097
Conc: 497.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:25 PM

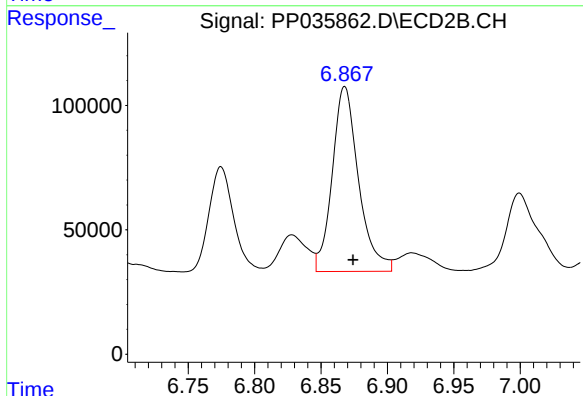


#28 AR-1254-3

R.T.: 6.868 min
Delta R.T.: -0.006 min
Response: 1024750
Conc: 493.73 ng/ml

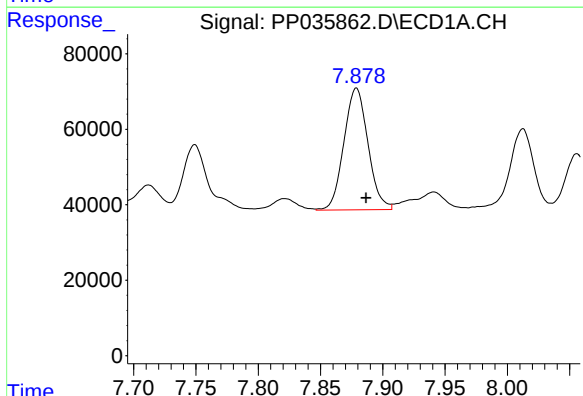


#29 AR-1254-4

R.T.: 7.879 min
Delta R.T.: -0.008 min
Response: 434569
Conc: 545.06 ng/ml

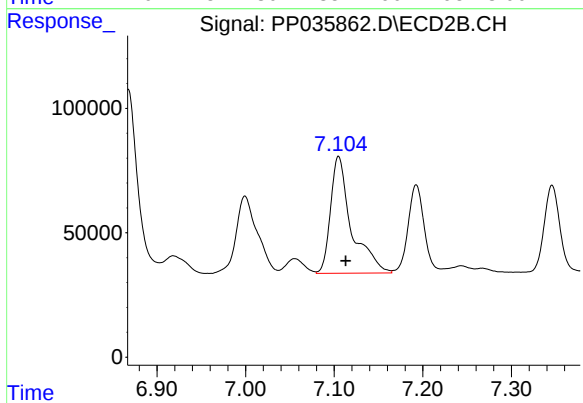

#29 AR-1254-4

R.T.: 7.105 min
Delta R.T.: -0.008 min
Response: 771607
Conc: 530.89 ng/ml

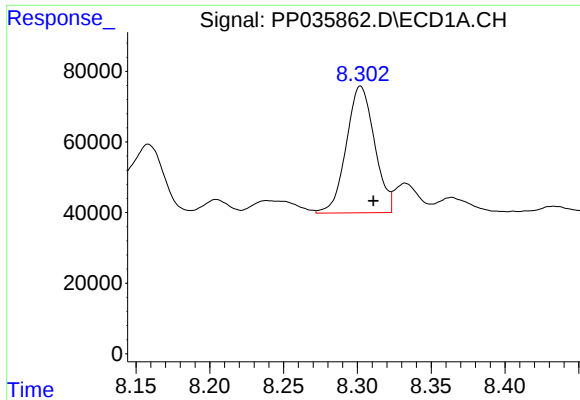


#30 AR-1254-5

R.T.: 8.302 min
Delta R.T.: -0.009 min
Response: 478411
Conc: 507.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
5/14/2021 2:09:25 PM

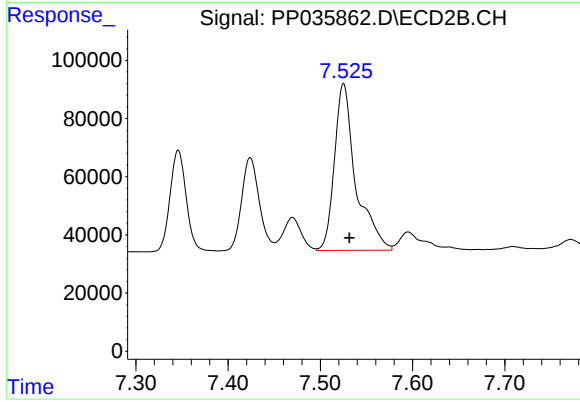

#30 AR-1254-5

R.T.: 7.525 min
Delta R.T.: -0.006 min
Response: 924776
Conc: 482.00 ng/ml